

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040922\
 Data File : PD069042.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 18:46
 Operator : AR\AJ
 Sample : N2284-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/09/2022
 Supervised By : mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 23:24:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 03:30:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.443	4.173	75273801	236.7E6	61.996m	24.762m#
28) SA Decachlor...	8.202	9.376	5526456	53254213	4.374m	9.398m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD040922\
Data File : PD069042.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 18:46
Operator : AR\AJ
Sample : N2284-04
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/09/2022
Supervised By : mohammad ahmed 04/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 23:24:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031222.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 03:30:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

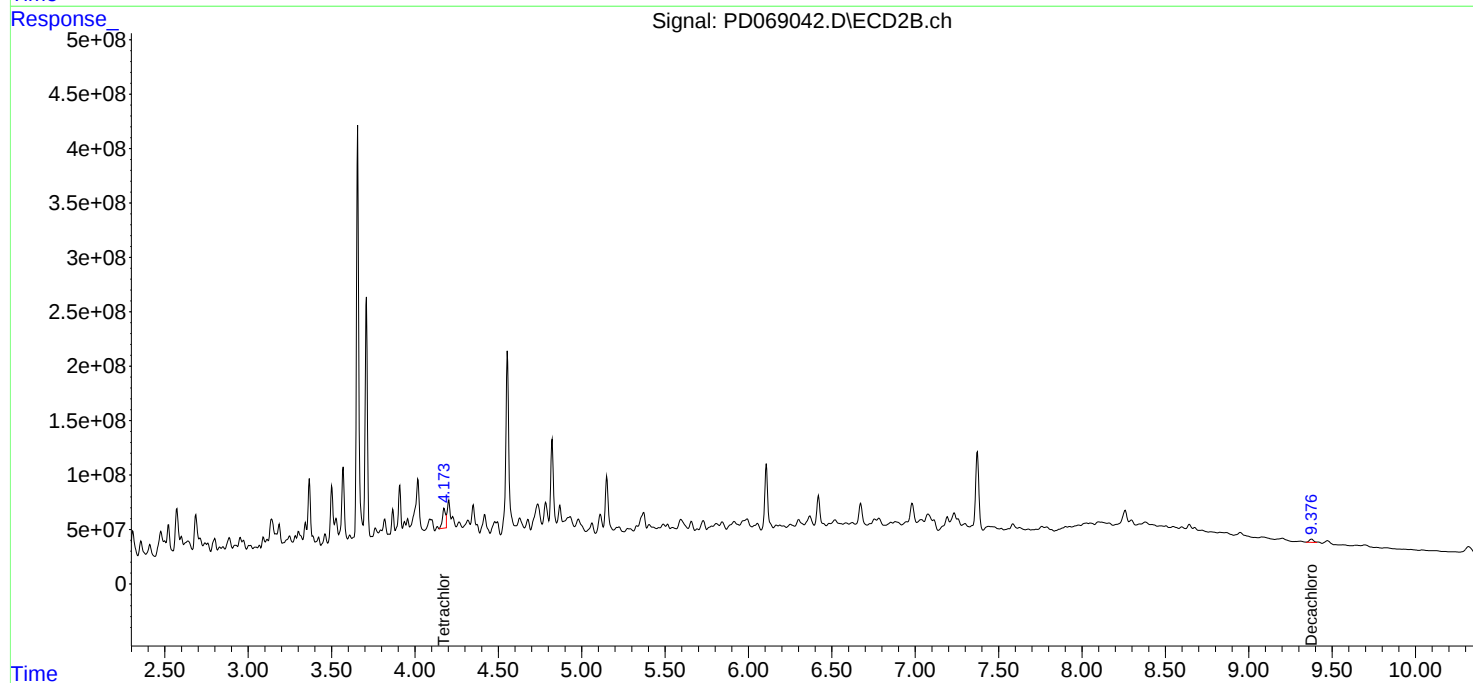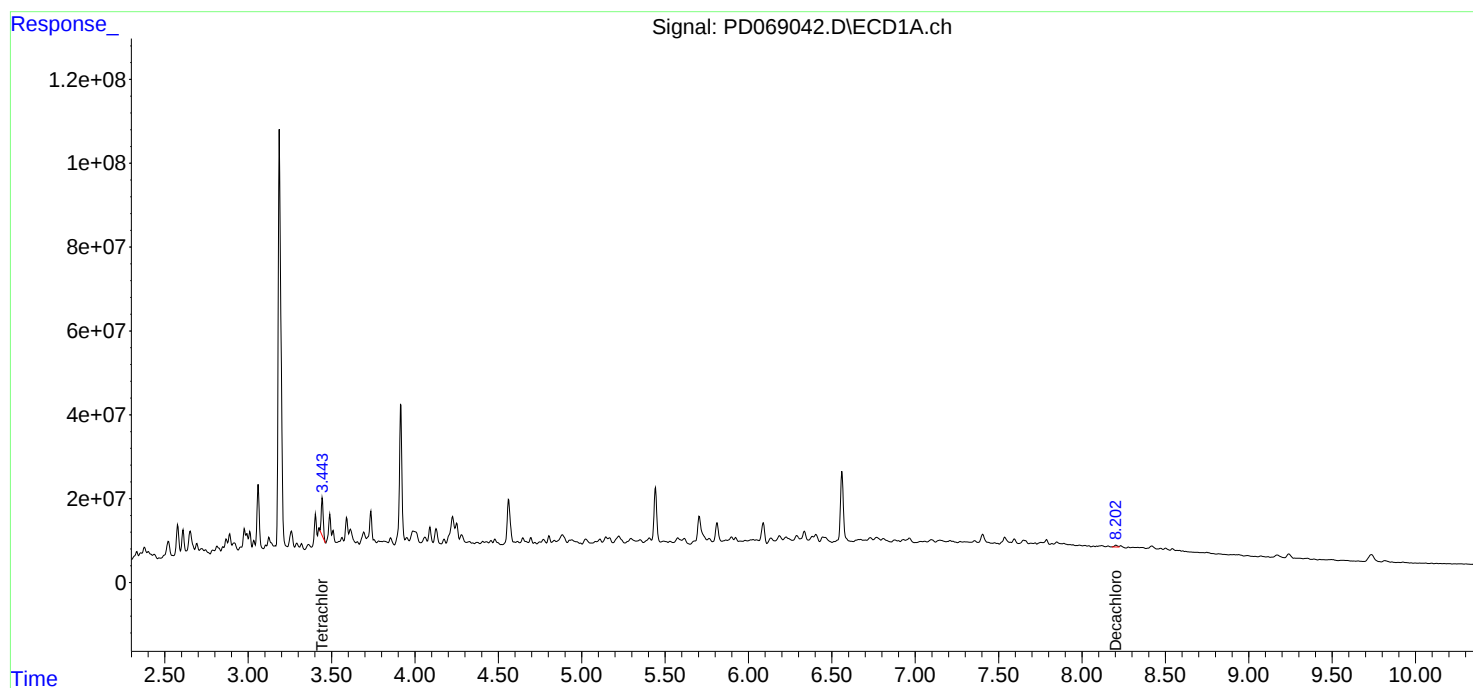

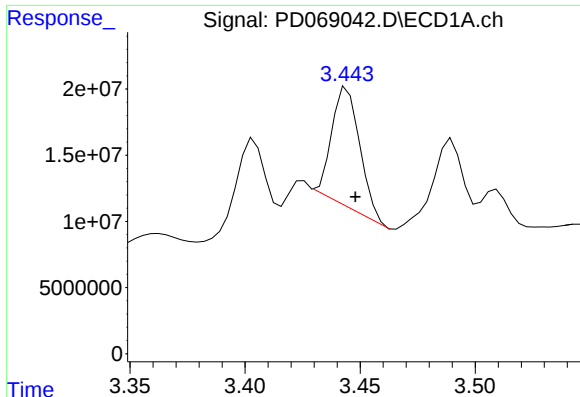


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: -0.005 min
Response: 75273801
Conc: 62.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/09/2022
Supervised By :mohammad ahmed 04/11/2022

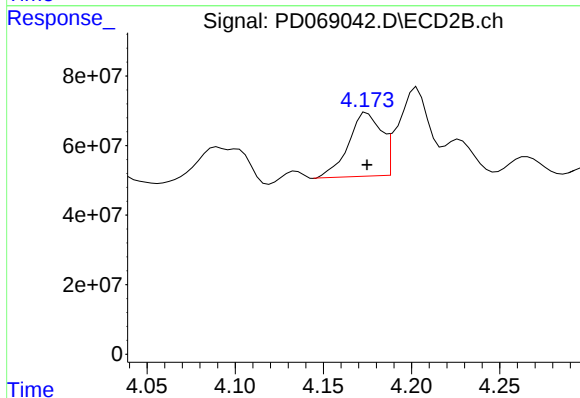


#1 Tetrachloro-m-xylene

R.T.: 4.173 min
Delta R.T.: -0.001 min
Response: 236740083
Conc: 24.76 ng/ml m

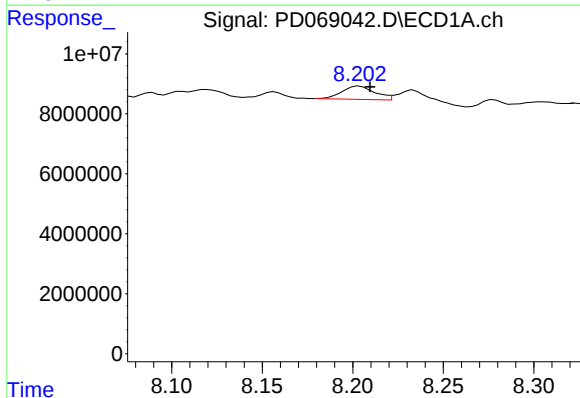

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.007 min
Response: 5526456
Conc: 4.37 ng/ml m

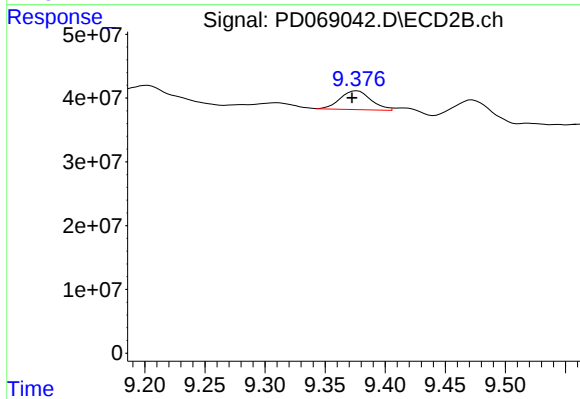

#28 Decachlorobiphenyl

R.T.: 9.376 min
Delta R.T.: 0.003 min
Response: 53254213
Conc: 9.40 ng/ml m