

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041019\
 Data File : PD052835.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Apr 2019 18:06
 Operator : AJ\SJ
 Sample : K2255-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFC54

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 06:53:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.043	10695193	214.5E6	7.025	6.779
27)	SA Decachlor...	7.815	9.162	14681587	150.2E6	10.413	10.418
Target Compounds							
2)	A alpha-BHC	0.000	4.407f	0 12945936	N.D.	0.272	
6)	B beta-BHC	0.000	4.937f	0 10570292	N.D.	0.541	
7)	B delta-BHC	0.000	5.083f	0 55226510	N.D.	1.532	
8)	B Heptachlo...	0.000	5.913	0 66621234	N.D.	1.881	
10)	B trans-Chl...	0.000	6.218f	0 12485023	N.D.	0.348	
11)	B cis-Chlor...	0.000	6.218	0 12485023	N.D.	0.363	
15)	B Endosulfa...	0.000	6.985	0 26391636	N.D.	1.002	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041019\
Data File : PD052835.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Apr 2019 18:06
Operator : AJ\SJ
Sample : K2255-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BFC54

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 06:53:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

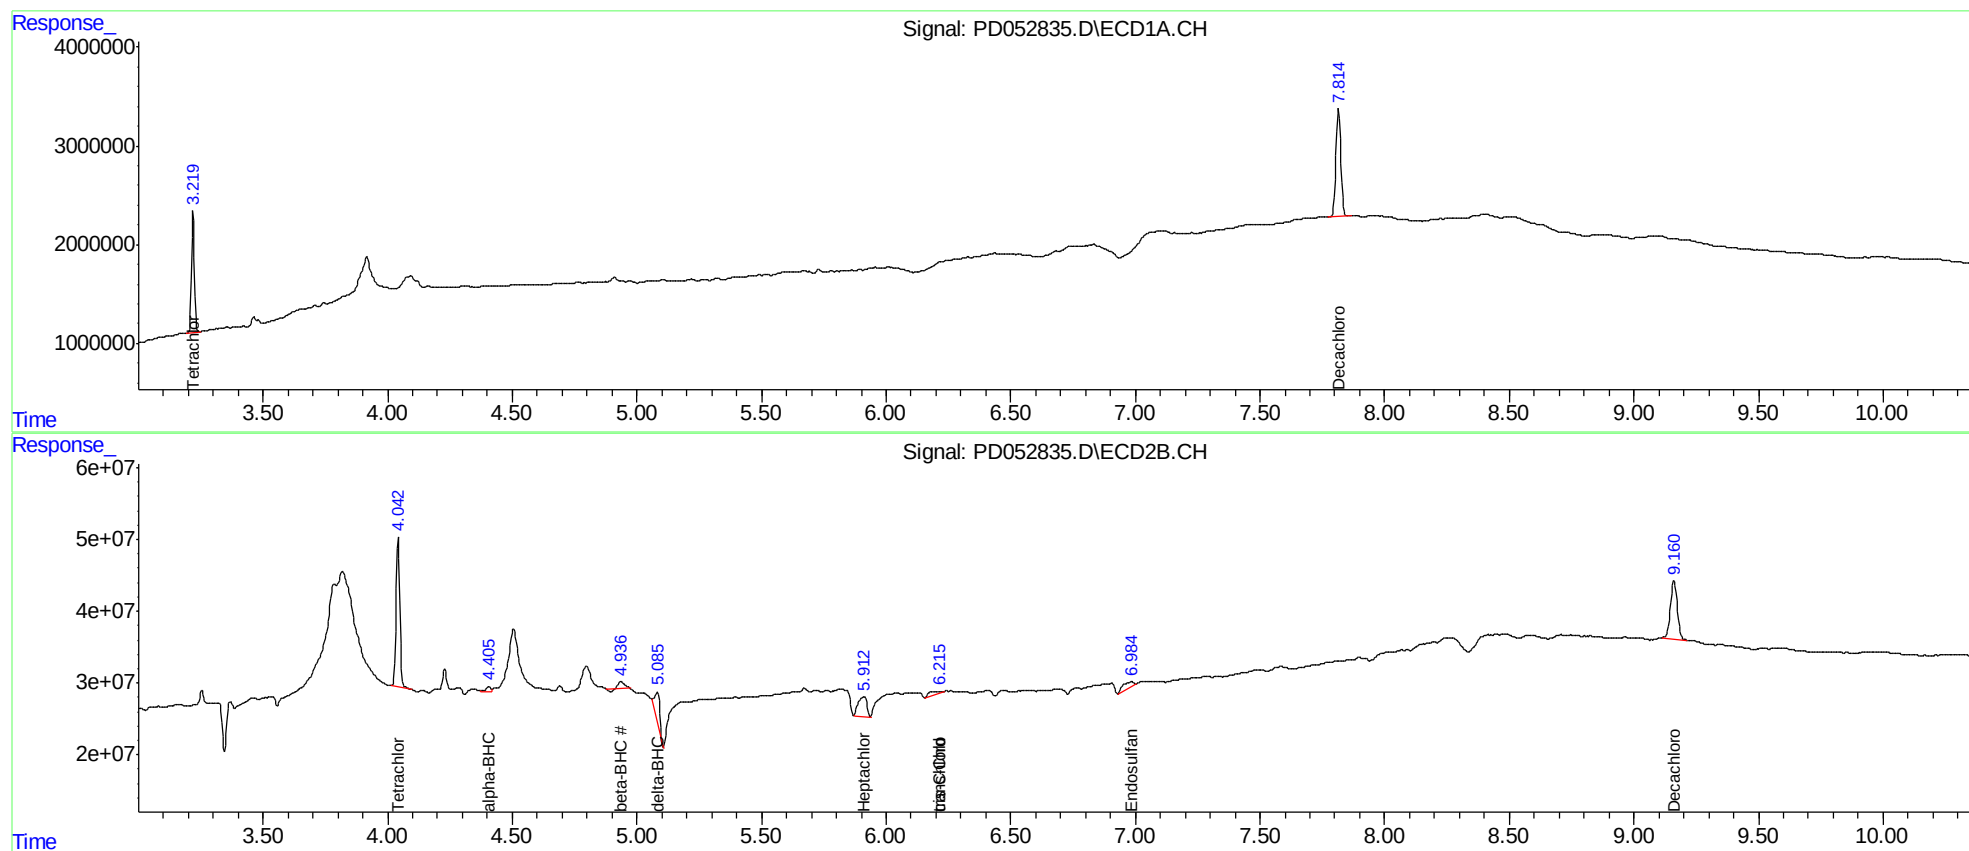


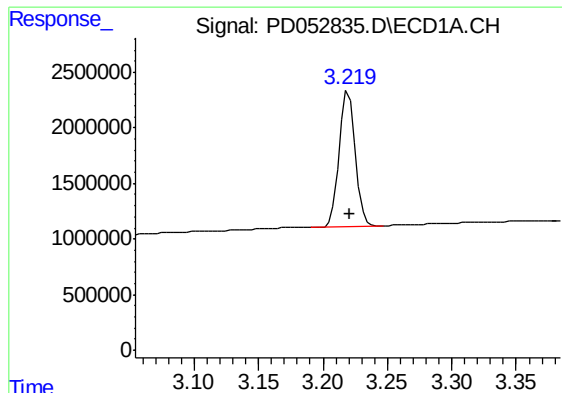

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: -0.001 min
Response: 10695193
Conc: 7.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC54

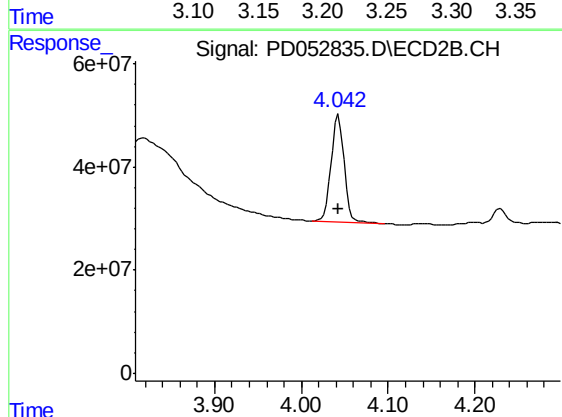


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 214523340
Conc: 6.78 ng/ml

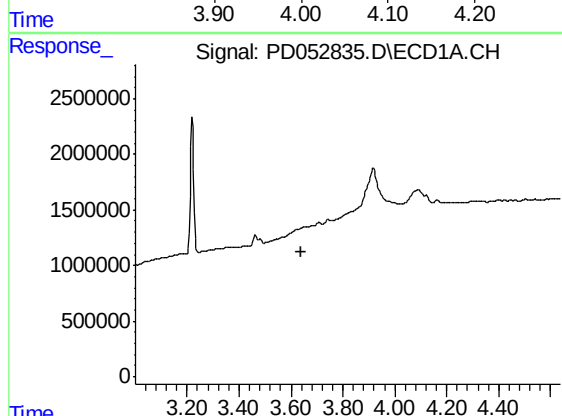


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.640 min
Response: 0
Conc: N.D.

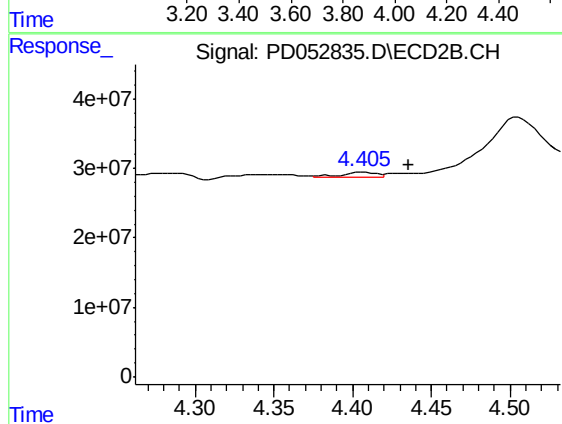

#2 alpha-BHC


R.T.: 4.407 min
Delta R.T.: -0.028 min
Response: 12945936
Conc: 0.27 ng/ml

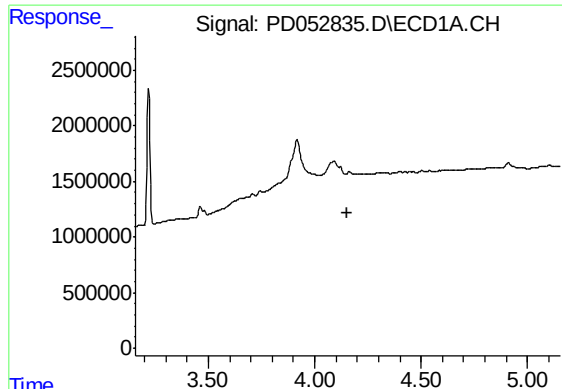

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC54

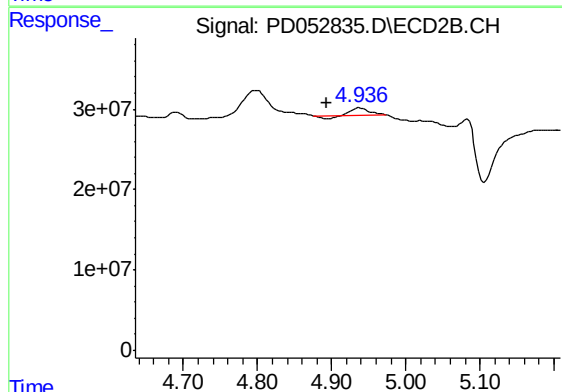


#6 beta-BHC

R.T.: 4.937 min
Delta R.T.: 0.044 min
Response: 10570292
Conc: 0.54 ng/ml

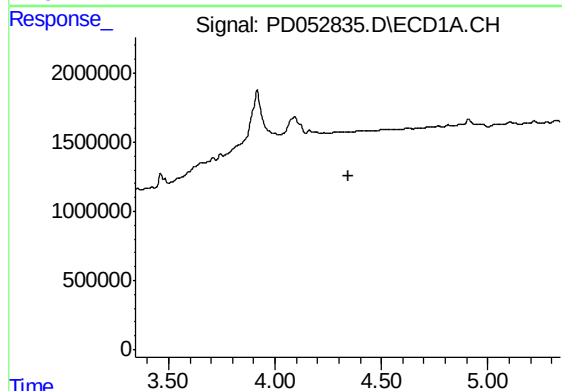


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.343 min
Response: 0
Conc: N.D.

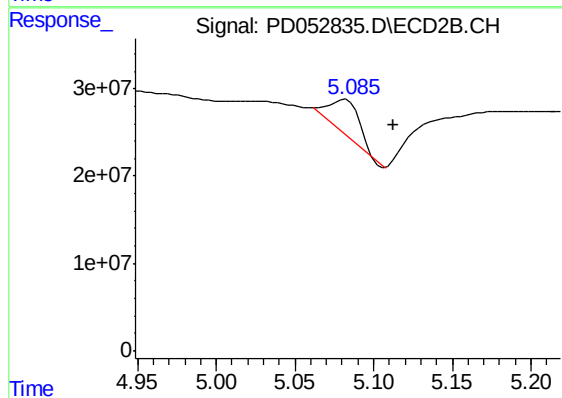

#7 delta-BHC


R.T.: 5.083 min
Delta R.T.: -0.030 min
Response: 55226510
Conc: 1.53 ng/ml

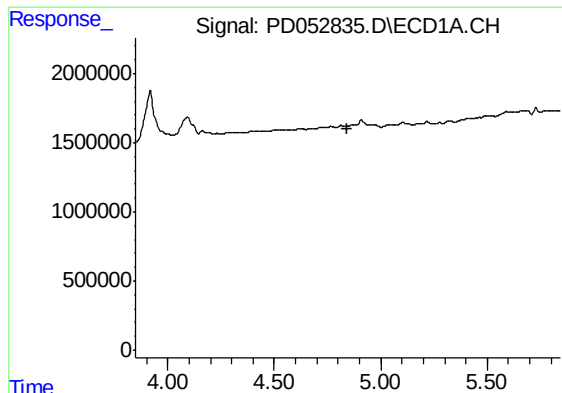

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC54

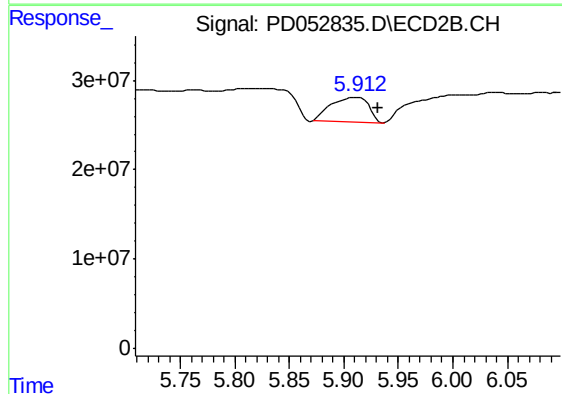


#8 Heptachlor epoxide

R.T.: 5.913 min
Delta R.T.: -0.019 min
Response: 66621234
Conc: 1.88 ng/ml

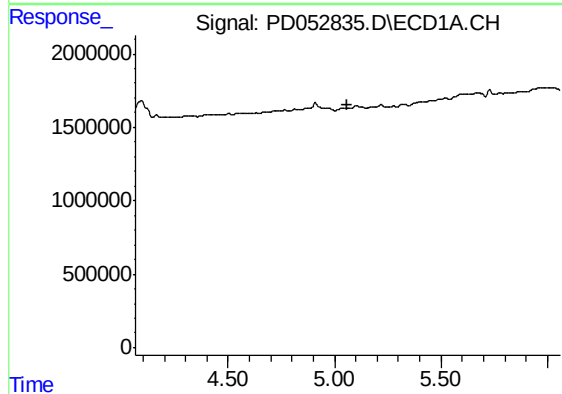


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.061 min
Response: 0
Conc: N.D.

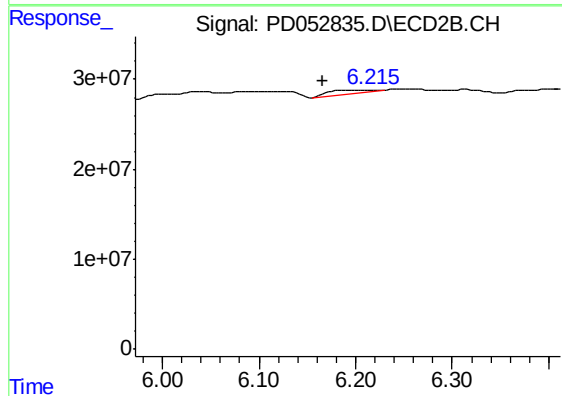

#10 trans-Chlordane


R.T.: 6.218 min
Delta R.T.: 0.051 min
Response: 12485023
Conc: 0.35 ng/ml

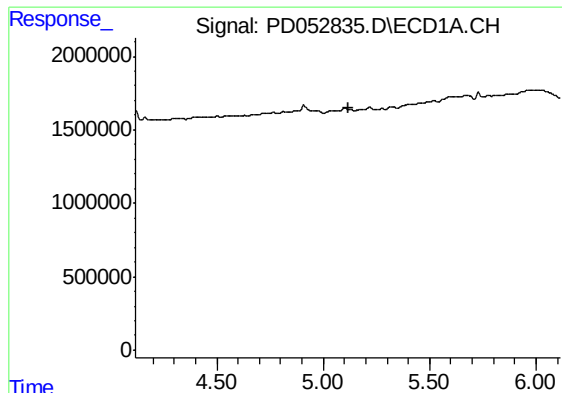

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC54

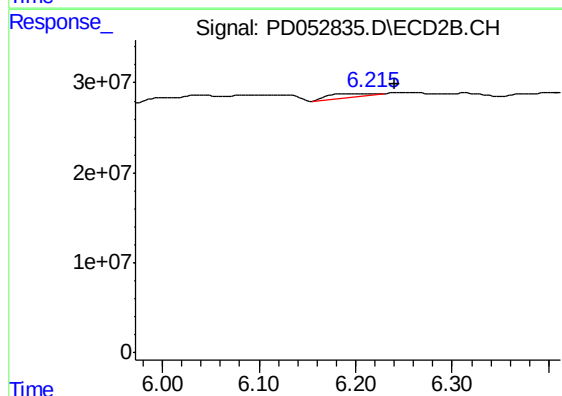


#11 cis-Chlordane

R.T.: 6.218 min
Delta R.T.: -0.022 min
Response: 12485023
Conc: 0.36 ng/ml

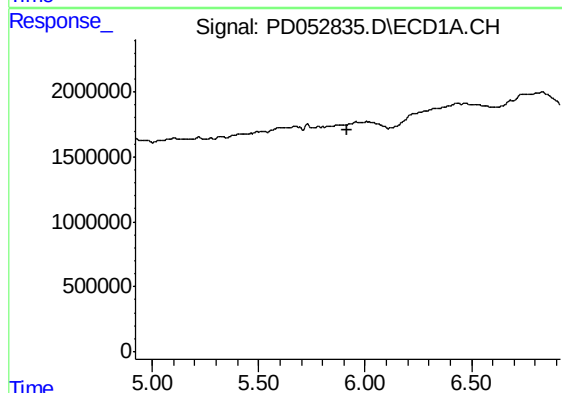


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.919 min
Response: 0
Conc: N.D.

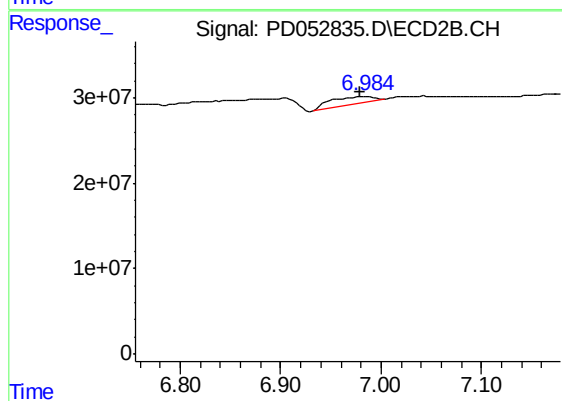

#15 Endosulfan II


R.T.: 6.985 min
Delta R.T.: 0.006 min
Response: 26391636
Conc: 1.00 ng/ml

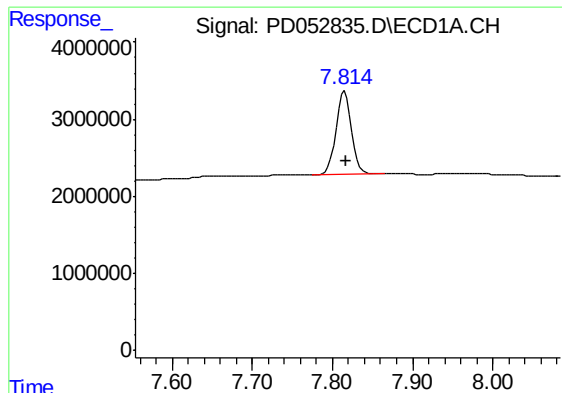

#27 Decachlorobiphenyl

R.T.: 7.815 min
Delta R.T.: -0.002 min
Response: 14681587
Conc: 10.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC54

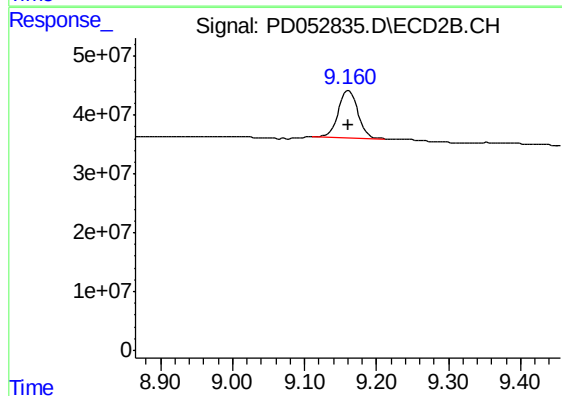

#27 Decachlorobiphenyl

R.T.: 9.162 min
Delta R.T.: 0.000 min
Response: 150214273
Conc: 10.42 ng/ml