

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041023\
 Data File : PD074639.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2023 16:14
 Operator : AR\AJ
 Sample : 02213-08
 Misc : CHLOR LOQ 50PPB
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOQ-WATER-02-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 22:44:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:23:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.554	2.768	41136912	22888827	17.636	18.808
28) SA Decachlor...	9.099	7.923	56343884	25367174	21.066	20.675
Target Compounds						
23) Chlordane-1	4.720	3.769	5861238	2326068	49.155m	46.159
24) Chlordane-2	5.252	4.348	7262545	2900019	54.202	49.759
25) Chlordane-3	5.963	4.978	22944028	7899684	46.380m	47.062
26) Chlordane-4	6.047	5.043	29062576	7877749	48.378	48.829
27) Chlordane-5	6.897	5.939	5833818	2740786	56.616m	45.405



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041023\
Data File : PD074639.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2023 16:14
Operator : AR\AJ
Sample : 02213-08
Misc : CHLOR LOQ 50PPB
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 22:44:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:23:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

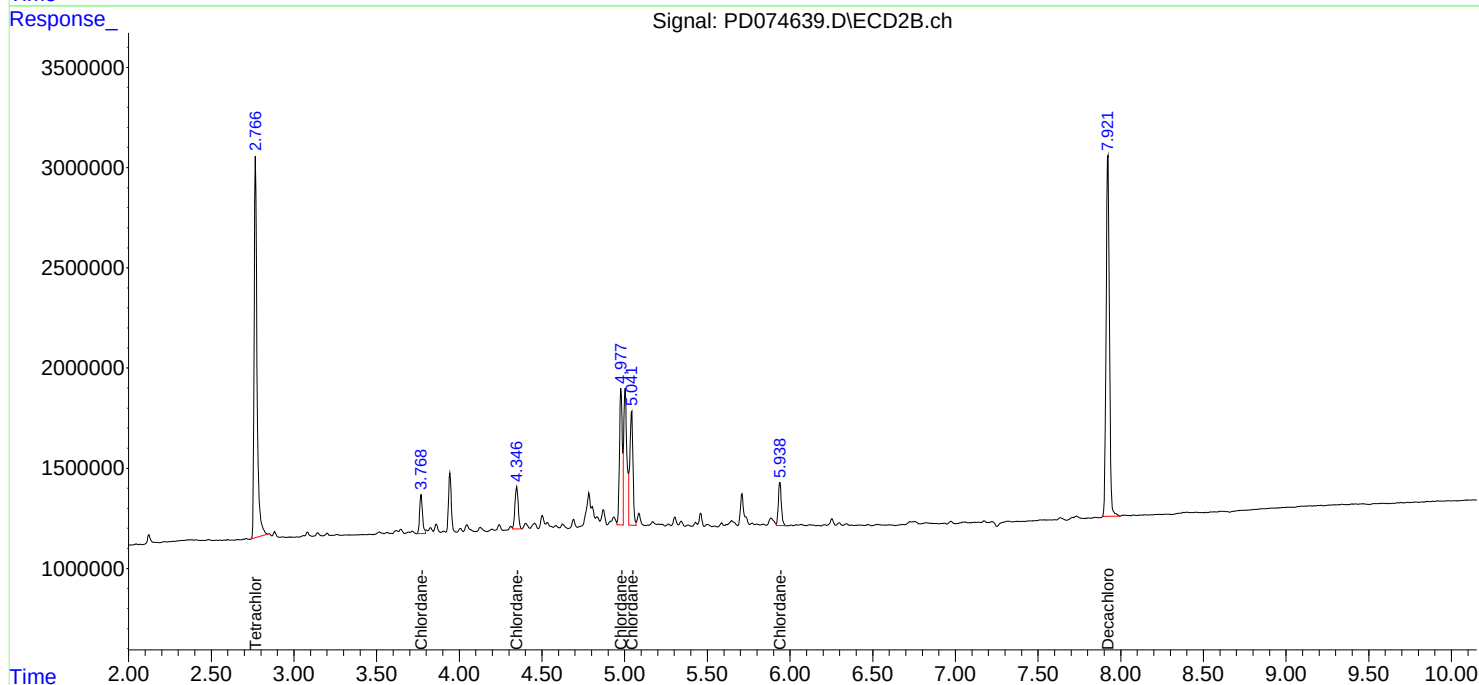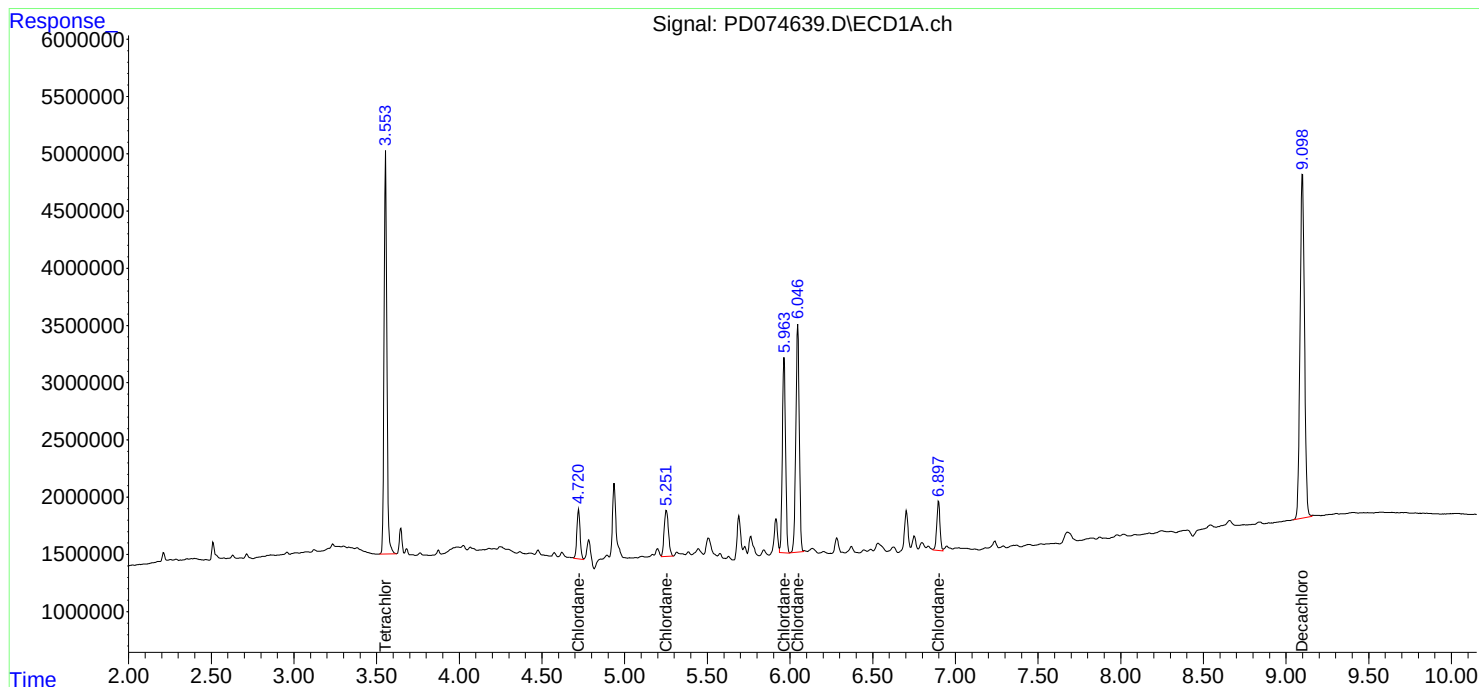


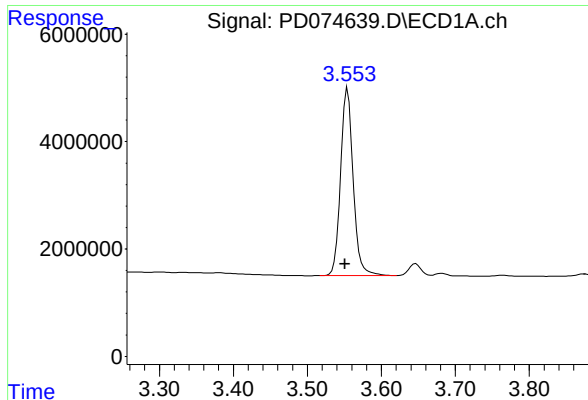

#1 Tetrachloro-m-xylene


R.T.: 3.554 min
Delta R.T.: 0.003 min
Response: 41136912
Conc: 17.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT2-2023

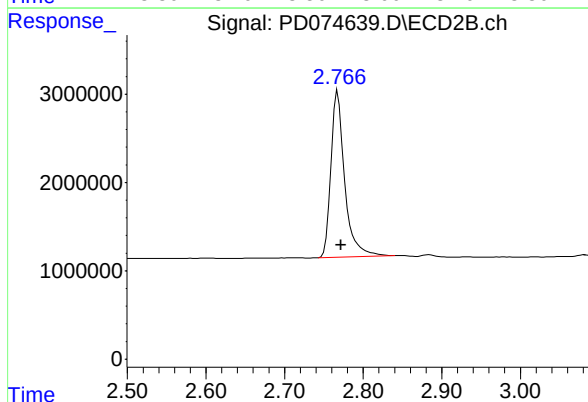


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: -0.004 min
Response: 22888827
Conc: 18.81 ng/ml

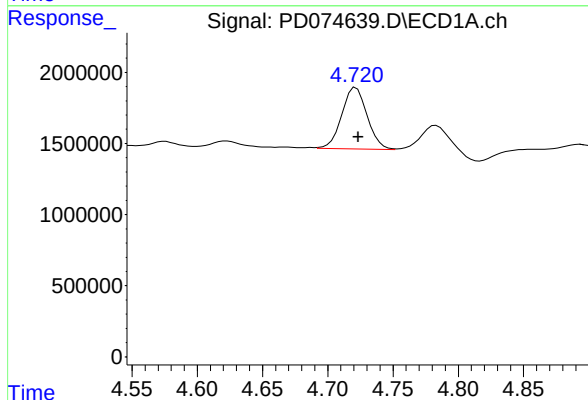


#23 Chlordane-1

R.T.: 4.720 min
Delta R.T.: -0.003 min
Response: 5861238
Conc: 49.16 ng/ml m

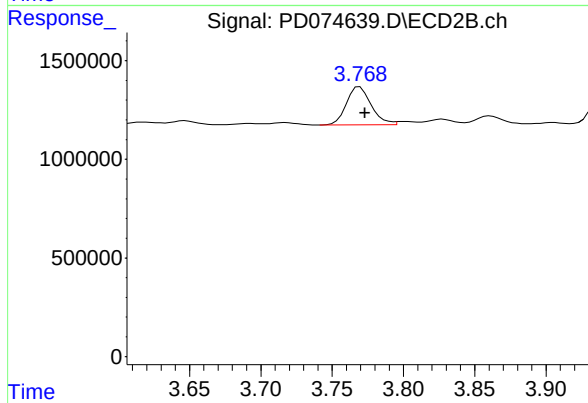

#23 Chlordane-1


R.T.: 3.769 min
Delta R.T.: -0.003 min
Response: 2326068
Conc: 46.16 ng/ml

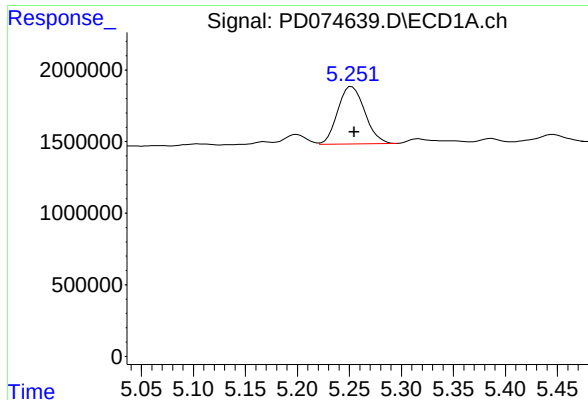

#24 Chlordane-2


R.T.: 5.252 min
Delta R.T.: -0.003 min
Response: 7262545
Conc: 54.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT2-2023

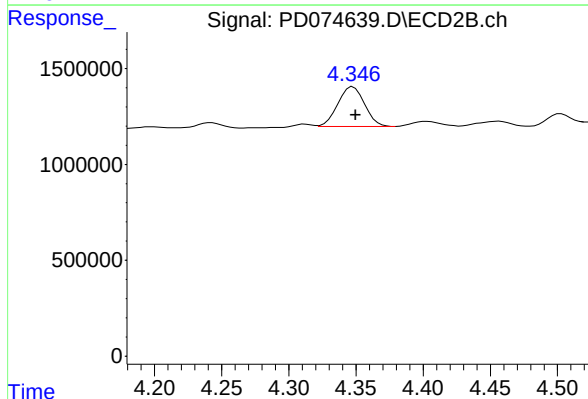


#24 Chlordane-2

R.T.: 4.348 min
Delta R.T.: -0.002 min
Response: 2900019
Conc: 49.76 ng/ml

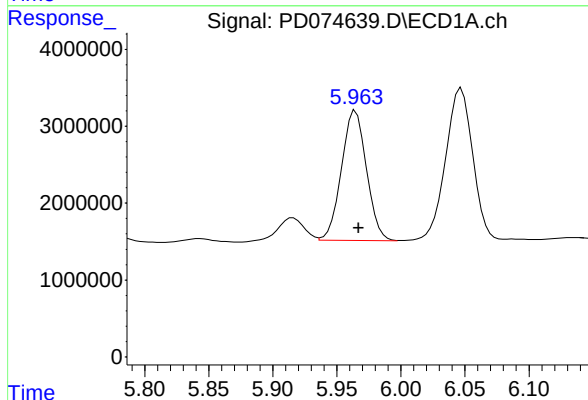


#25 Chlordane-3

R.T.: 5.963 min
Delta R.T.: -0.004 min
Response: 22944028
Conc: 46.38 ng/ml m

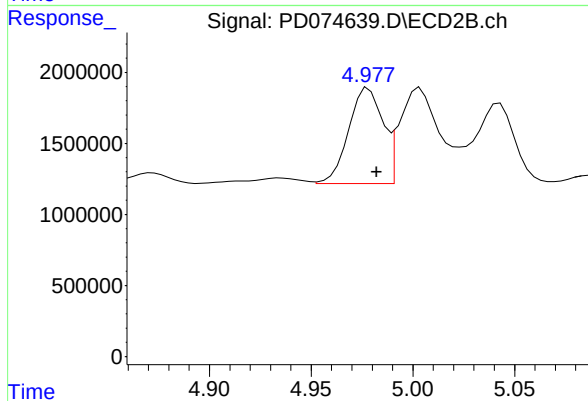

#25 Chlordane-3


R.T.: 4.978 min
Delta R.T.: -0.004 min
Response: 7899684
Conc: 47.06 ng/ml

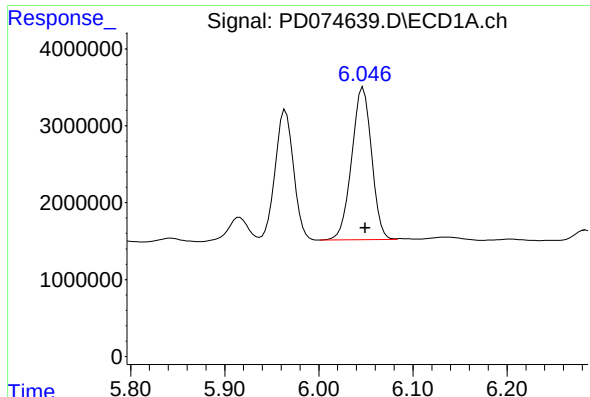

#26 Chlordane-4


R.T.: 6.047 min
Delta R.T.: -0.002 min
Response: 29062576
Conc: 48.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT2-2023

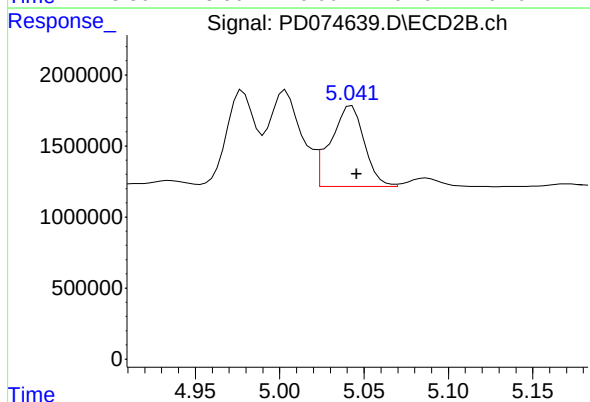


#26 Chlordane-4

R.T.: 5.043 min
Delta R.T.: -0.003 min
Response: 7877749
Conc: 48.83 ng/ml

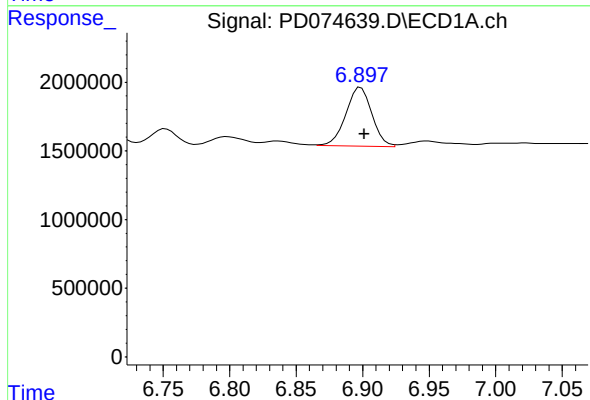


#27 Chlordane-5

R.T.: 6.897 min
Delta R.T.: -0.004 min
Response: 5833818
Conc: 56.62 ng/ml m

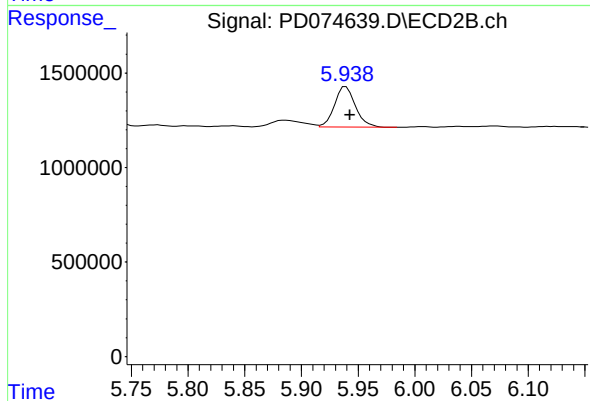

#27 Chlordane-5


R.T.: 5.939 min
Delta R.T.: -0.004 min
Response: 2740786
Conc: 45.41 ng/ml

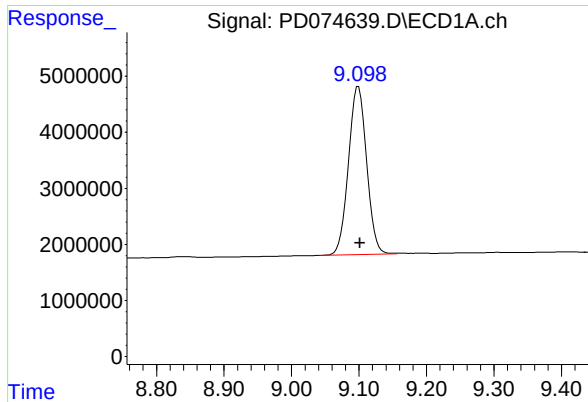

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.002 min
Response: 56343884
Conc: 21.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
LOQ-WATER-02-QT2-2023

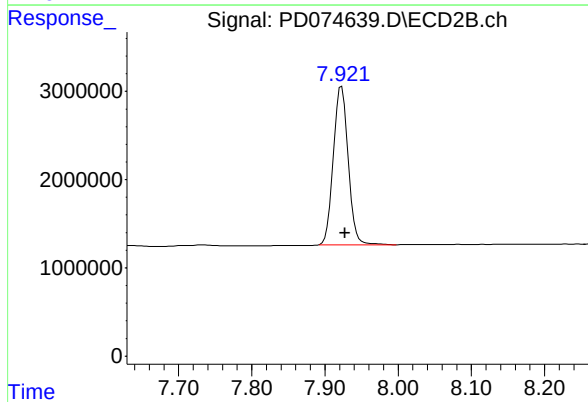

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: -0.005 min
Response: 25367174
Conc: 20.68 ng/ml