

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
 Data File : PD082337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 19:43
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA1003

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:54:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 01:51:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.565	2.777	7775217	17158030	5.315	4.923
27) SA Decachlor...	9.118	7.910	20919515	32558974	10.652	9.803
Target Compounds						
2) A alpha-BHC	4.023	3.277	12219316	24909813	5.123	4.603
3) MA gamma-BHC...	4.357	3.606	11925865	23400987	5.032	4.628
4) MA Heptachlor	4.950	3.945	12573016	22274924	5.177	4.733
9) A Endosulfan I	6.107	5.095	11392263	18426419	5.301	4.756
13) MA Dieldrin	6.383	5.360	21808293	39299843	10.137	9.194
14) MA Endrin	6.614	5.635	18418143	33977482	10.344	9.203
16) A 4,4'-DDD	6.746	5.782	15430444	28752315	9.946	9.207
17) MA 4,4'-DDT	7.062	6.033	15803180	29515795	9.813	8.876
20) A Methoxychlor	7.537	6.609	47259426	86212971	54.578	49.513


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 19:43
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:54:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 01:51:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

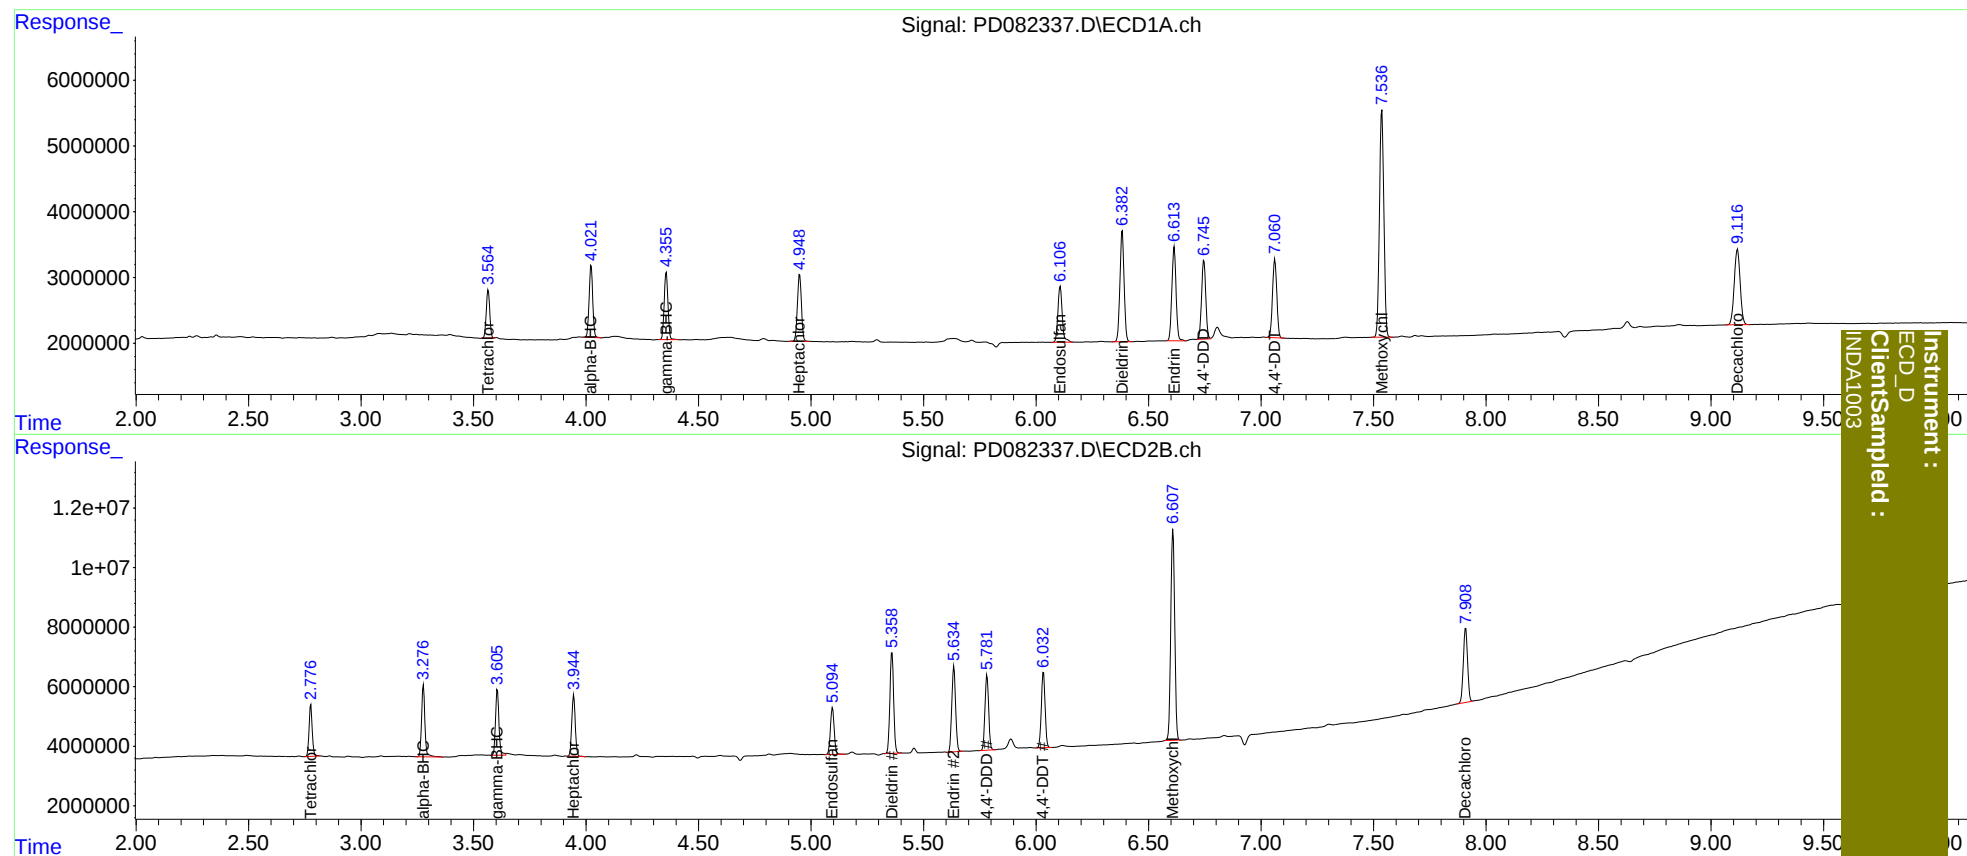


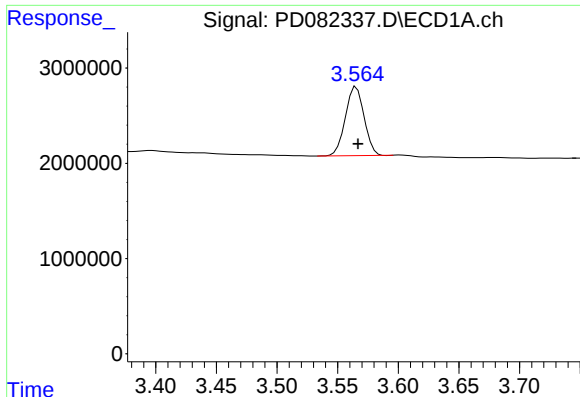

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: -0.002 min
Response: 7775217
Conc: 5.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1003

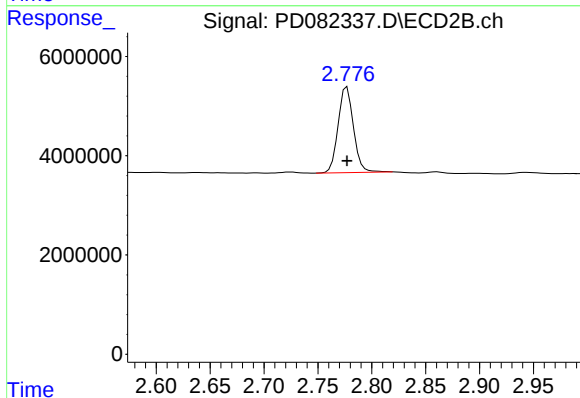


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 17158030
Conc: 4.92 ng/ml

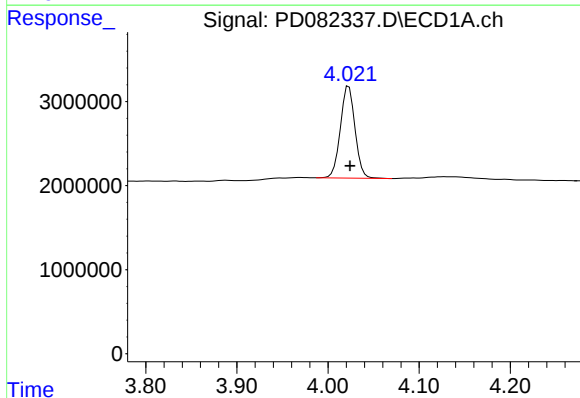


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: -0.001 min
Response: 12219316
Conc: 5.12 ng/ml

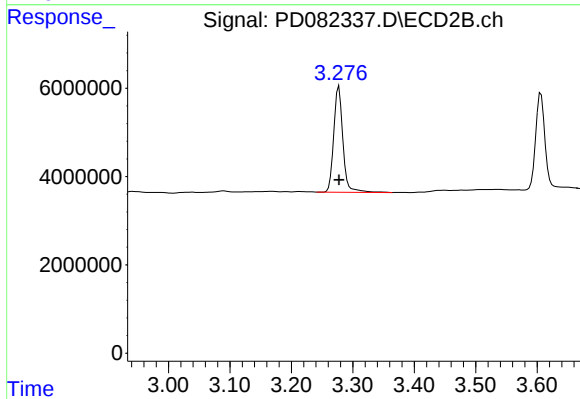

#2 alpha-BHC


R.T.: 3.277 min
Delta R.T.: 0.000 min
Response: 24909813
Conc: 4.60 ng/ml

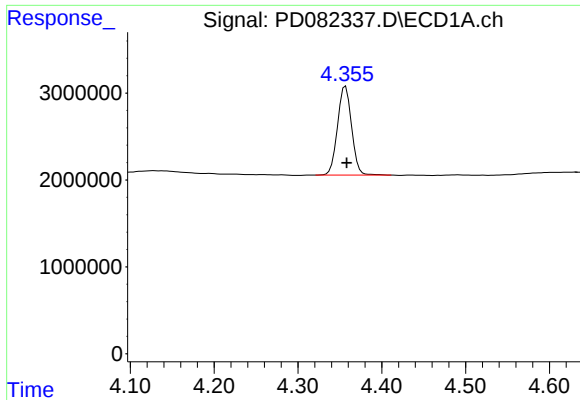

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: -0.001 min
Response: 11925865
Conc: 5.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1003

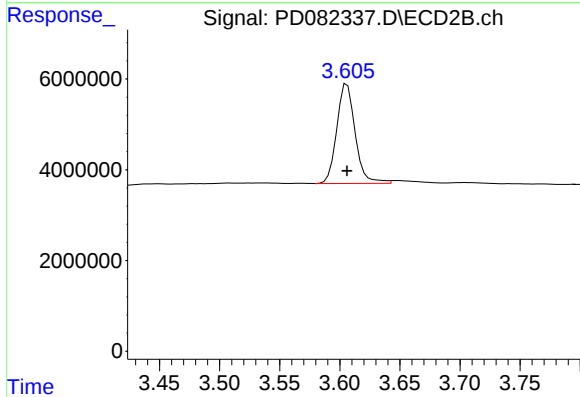


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 23400987
Conc: 4.63 ng/ml

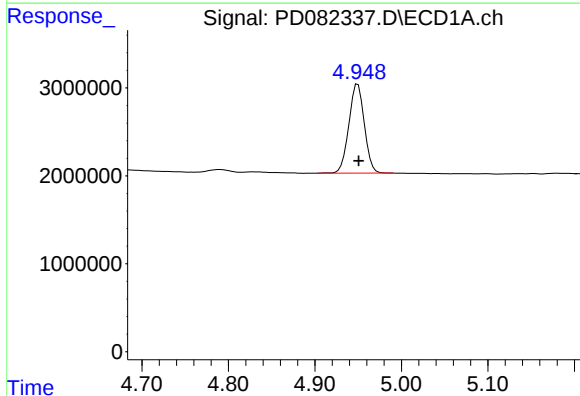


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: -0.001 min
Response: 12573016
Conc: 5.18 ng/ml

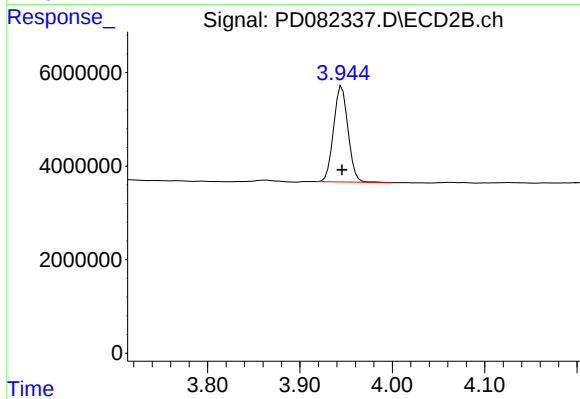

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 22274924
Conc: 4.73 ng/ml

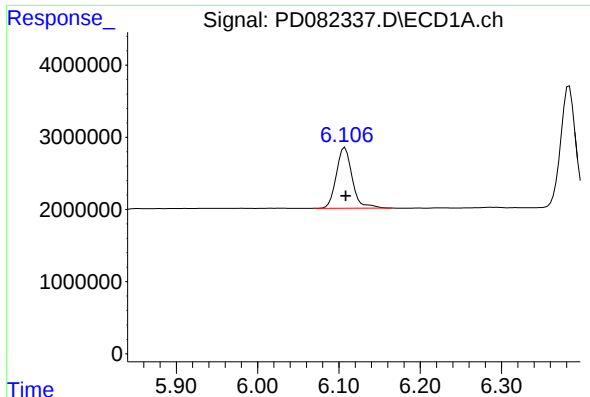

#9 Endosulfan I


R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 11392263
Conc: 5.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1003

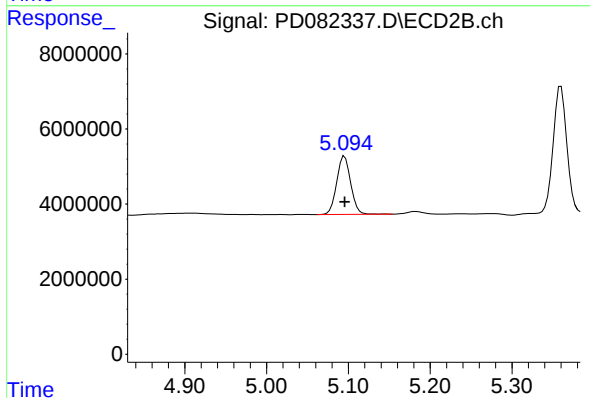


#9 Endosulfan I

R.T.: 5.095 min
Delta R.T.: 0.000 min
Response: 18426419
Conc: 4.76 ng/ml

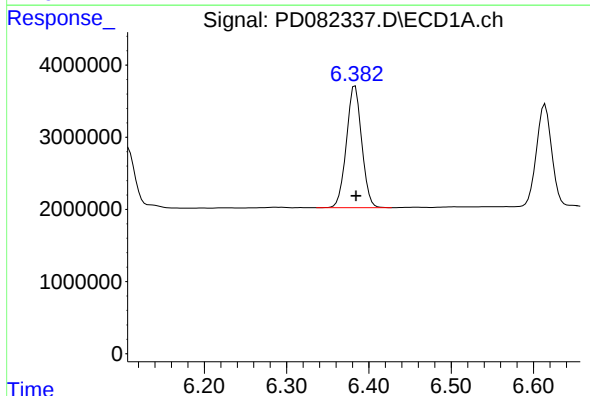


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: -0.001 min
Response: 21808293
Conc: 10.14 ng/ml

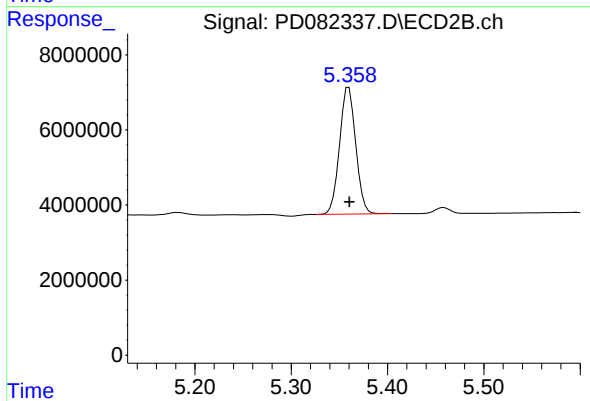

#13 Dieldrin


R.T.: 5.360 min
Delta R.T.: 0.000 min
Response: 39299843
Conc: 9.19 ng/ml

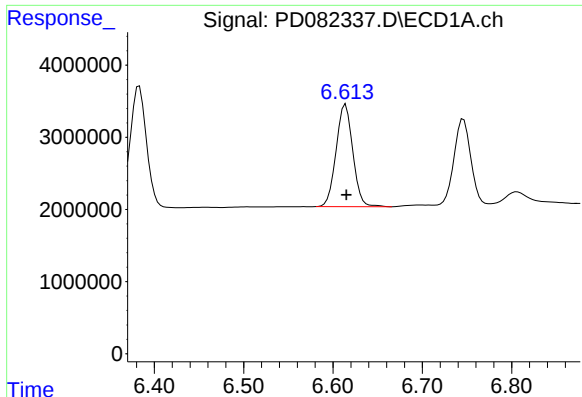

#14 Endrin


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 18418143
Conc: 10.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1003

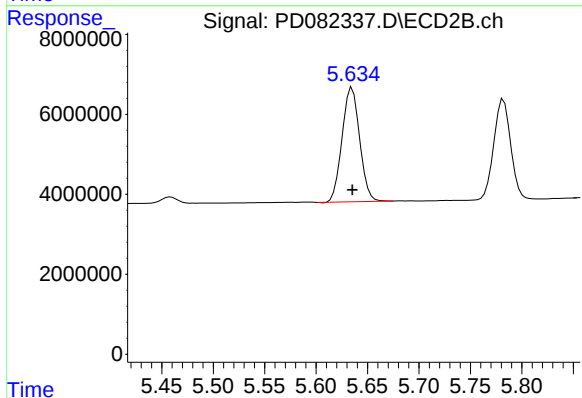


#14 Endrin

R.T.: 5.635 min
Delta R.T.: 0.000 min
Response: 33977482
Conc: 9.20 ng/ml

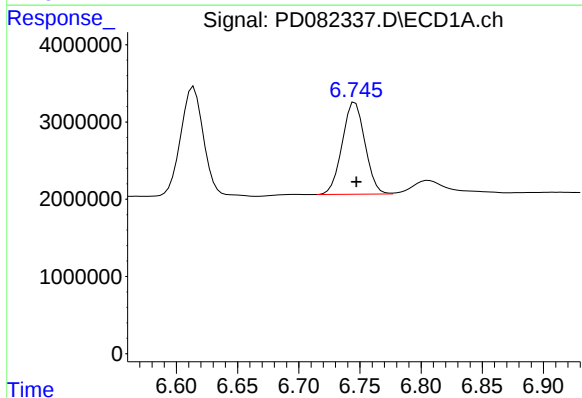


#16 4,4'-DDD

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 15430444
Conc: 9.95 ng/ml

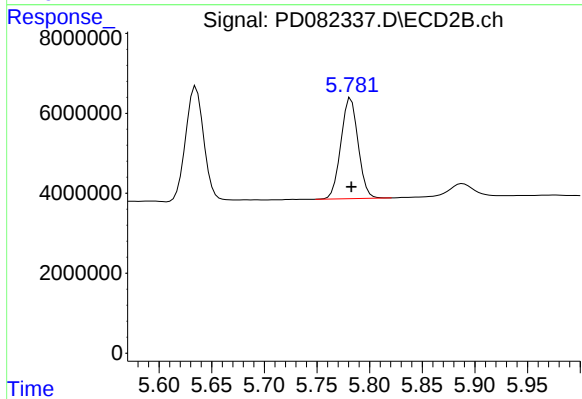

#16 4,4'-DDD


R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 28752315
Conc: 9.21 ng/ml

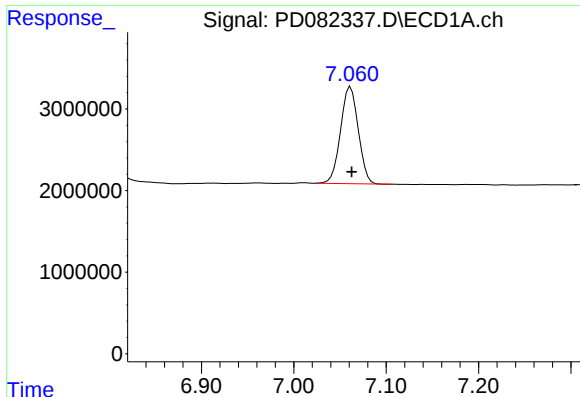

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: -0.001 min
Response: 15803180
Conc: 9.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1003

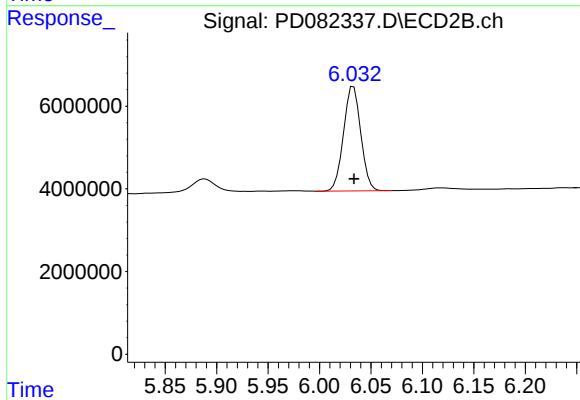


#17 4,4'-DDT

R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 29515795
Conc: 8.88 ng/ml

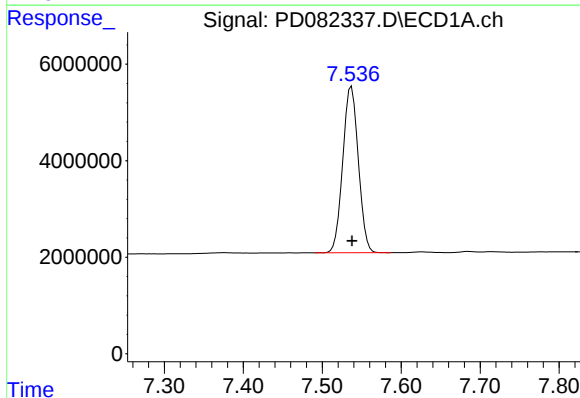


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 47259426
Conc: 54.58 ng/ml

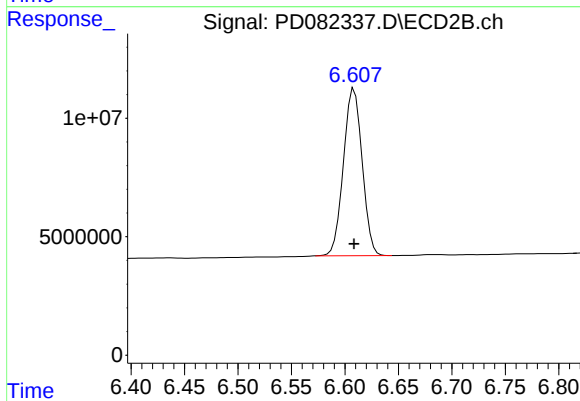

#20 Methoxychlor


R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 86212971
Conc: 49.51 ng/ml

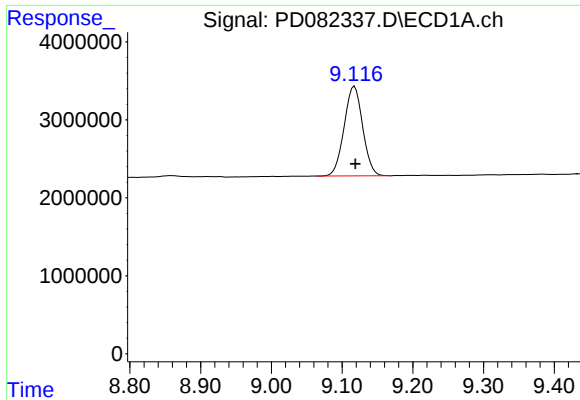

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.001 min
Response: 20919515
Conc: 10.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1003

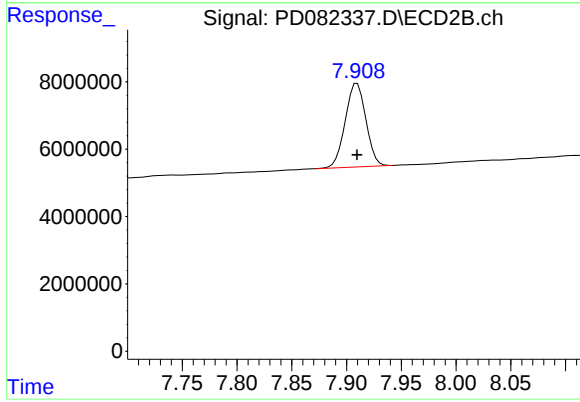

#27 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.000 min
Response: 32558974
Conc: 9.80 ng/ml