

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
 Data File : PD082341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 20:37
 Operator : AR\AJ
 Sample : INDA3007
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3007

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:54:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 01:51:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.567	2.777	29260305	69703786	20.000	20.000
27)	SA Decachlor...	9.119	7.910	78553556	132.8E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.024	3.277	47699469	108.2E6	20.000	20.000
3)	MA gamma-BHC...	4.358	3.606	47402865	101.1E6	20.000	20.000
4)	MA Heptachlor	4.951	3.946	48574304	94118037	20.000	20.000
9)	A Endosulfan I	6.108	5.096	42983949	77484890	20.000	20.000
13)	MA Dieldrin	6.384	5.360	86056509	171.0E6	40.000	40.000
14)	MA Endrin	6.615	5.635	71219799	147.7E6	40.000	40.000
16)	A 4,4'-DDD	6.747	5.783	62056933	124.9E6	40.000	40.000
17)	MA 4,4'-DDT	7.063	6.033	64420582	133.0E6	40.000	40.000
20)	A Methoxychlor	7.538	6.609	173.2E6	348.2E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 20:37
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:54:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 01:51:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

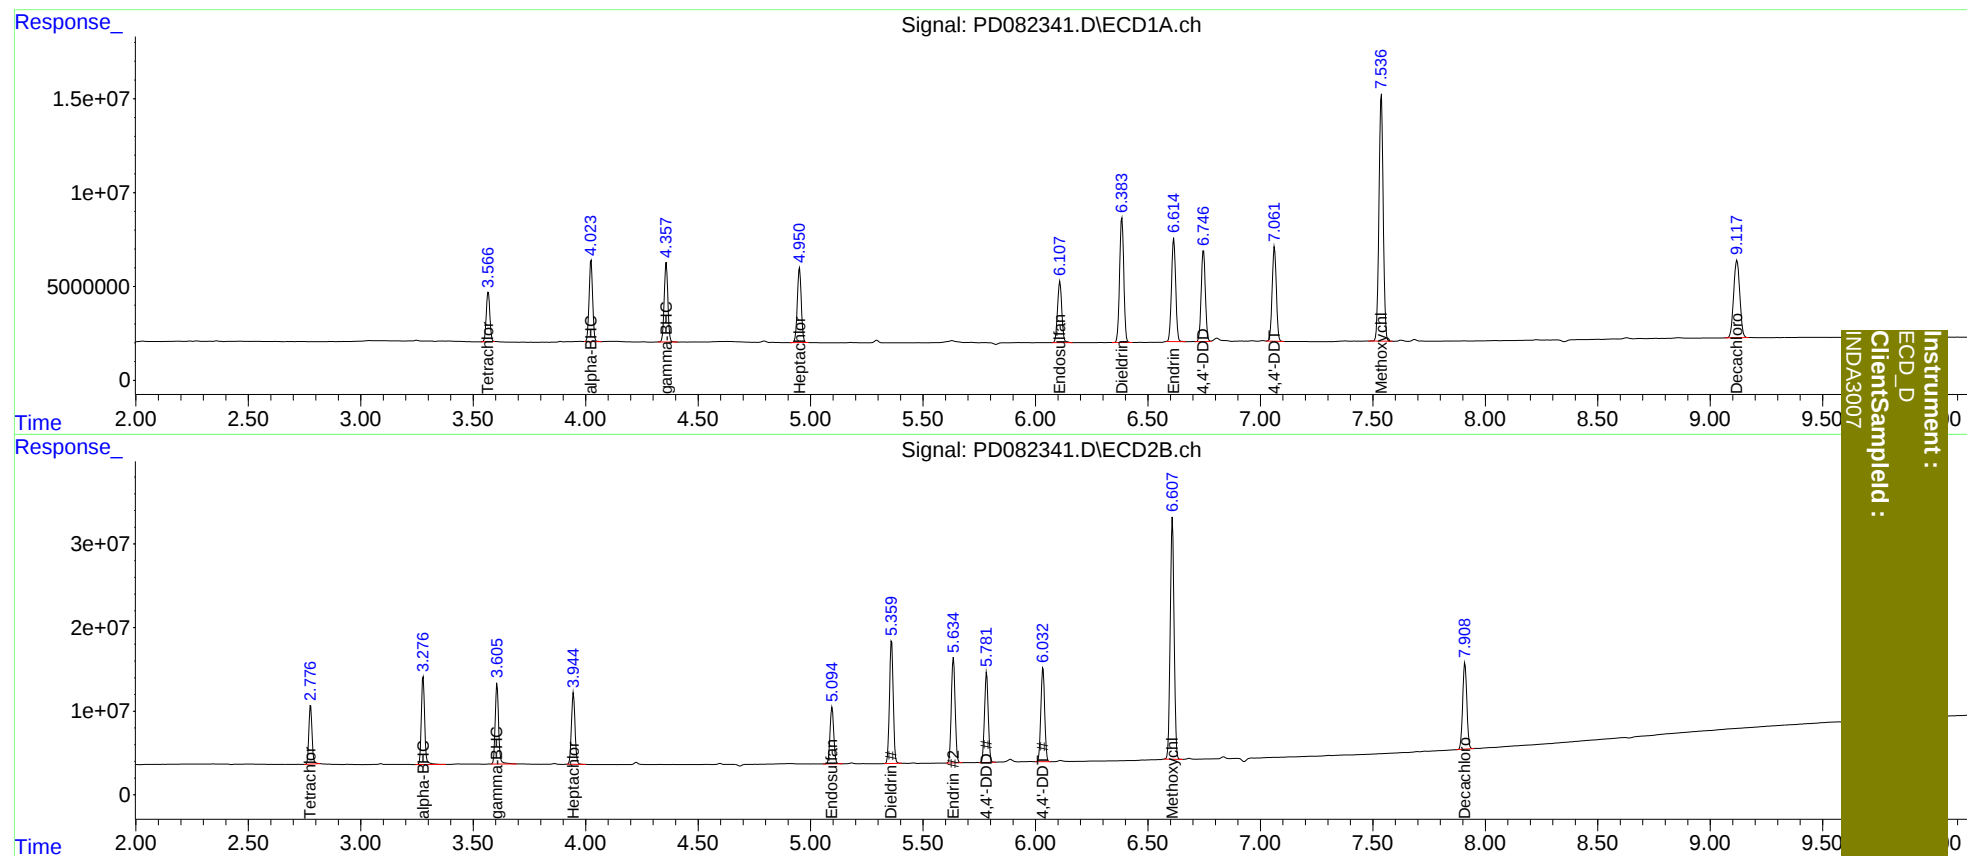


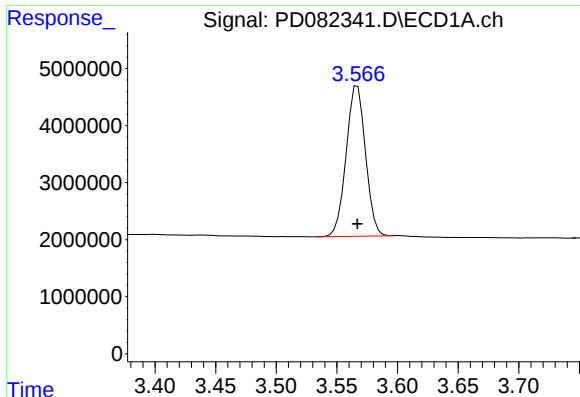

#1 Tetrachloro-m-xylene


R.T.: 3.567 min
Delta R.T.: 0.000 min
Response: 29260305
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3007

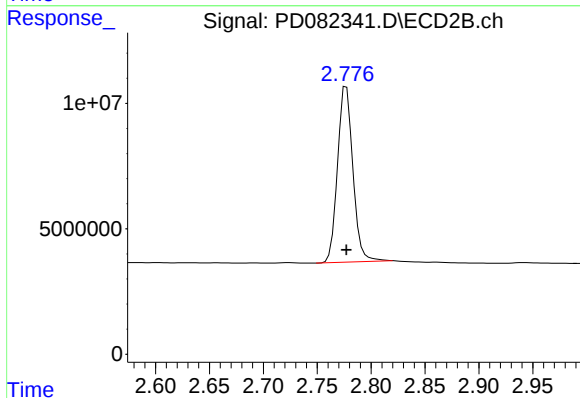


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 69703786
Conc: 20.00 ng/ml

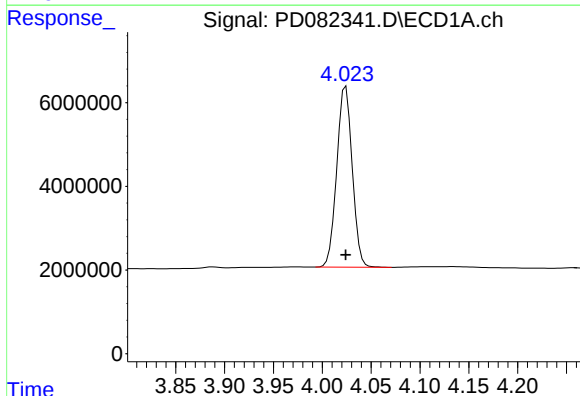


#2 alpha-BHC

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 47699469
Conc: 20.00 ng/ml

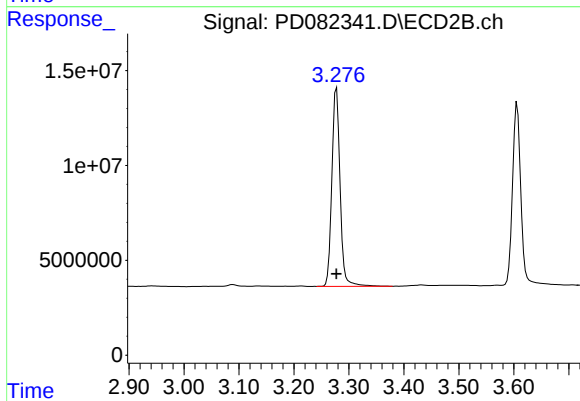

#2 alpha-BHC


R.T.: 3.277 min
Delta R.T.: 0.000 min
Response: 108232269
Conc: 20.00 ng/ml

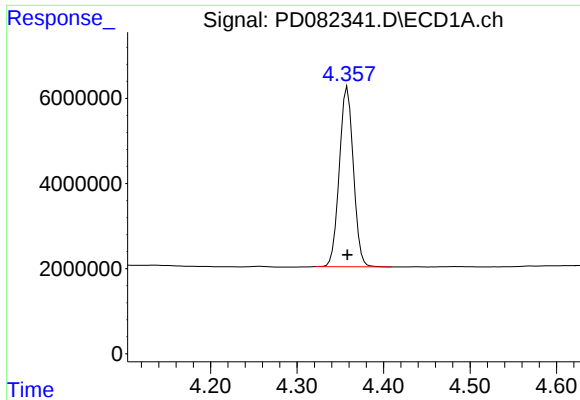

#3 gamma-BHC (Lindane)


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 47402865
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3007

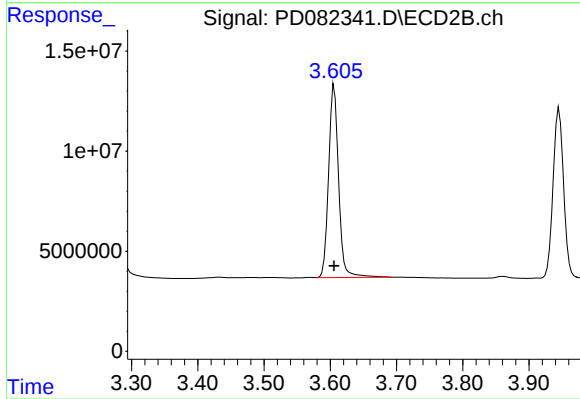


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 101123637
Conc: 20.00 ng/ml

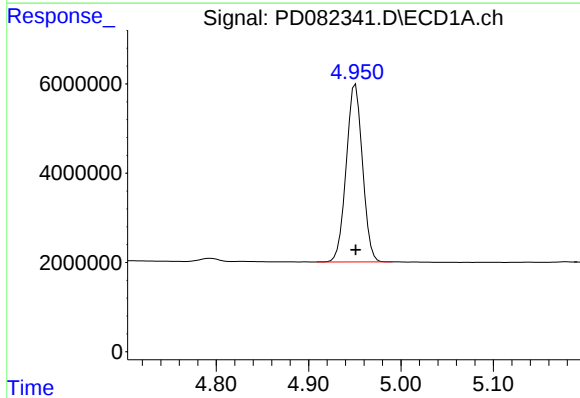


#4 Heptachlor

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 48574304
Conc: 20.00 ng/ml

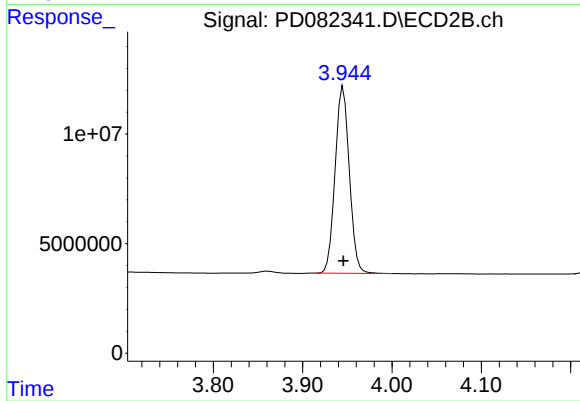

#4 Heptachlor


R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 94118037
Conc: 20.00 ng/ml

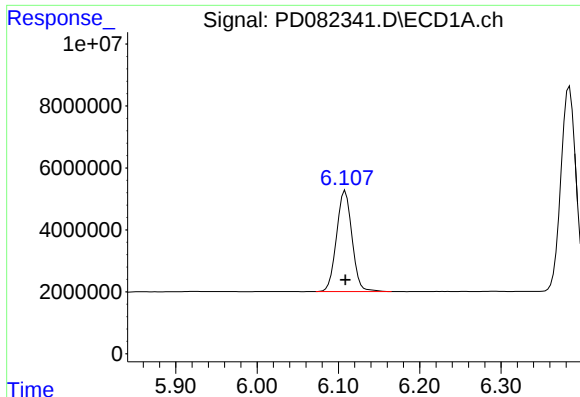

#9 Endosulfan I


R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 42983949
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3007

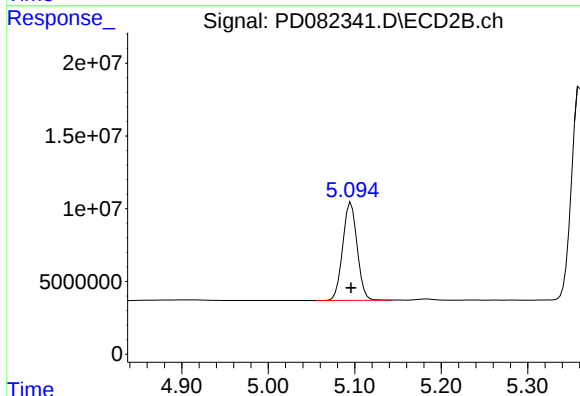


#9 Endosulfan I

R.T.: 5.096 min
Delta R.T.: 0.000 min
Response: 77484890
Conc: 20.00 ng/ml

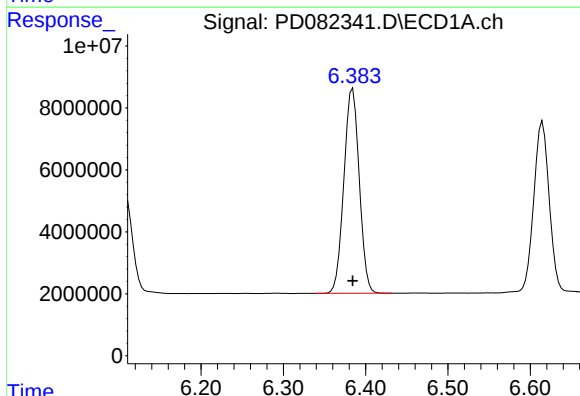


#13 Dieldrin

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 86056509
Conc: 40.00 ng/ml

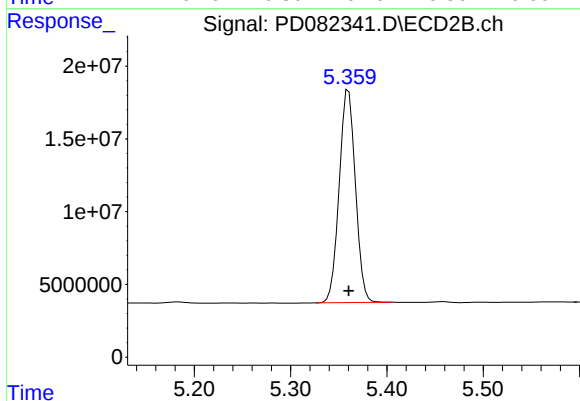

#13 Dieldrin


R.T.: 5.360 min
Delta R.T.: 0.000 min
Response: 170982133
Conc: 40.00 ng/ml

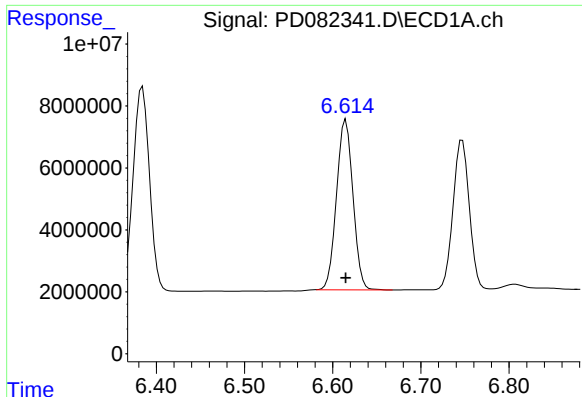

#14 Endrin


R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 71219799
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3007

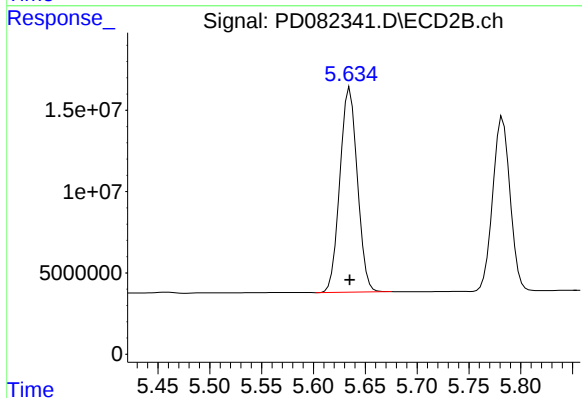


#14 Endrin

R.T.: 5.635 min
Delta R.T.: 0.000 min
Response: 147677452
Conc: 40.00 ng/ml

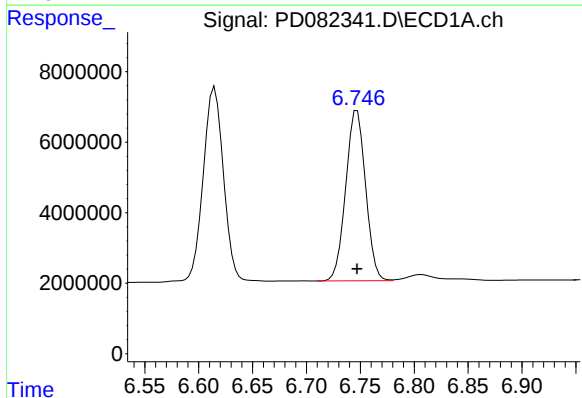


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 62056933
Conc: 40.00 ng/ml

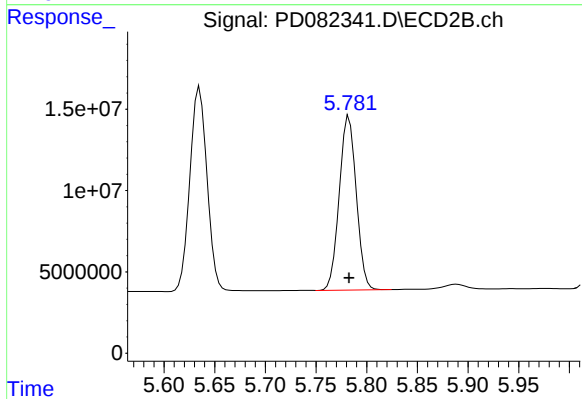

#16 4,4'-DDD


R.T.: 5.783 min
Delta R.T.: 0.000 min
Response: 124909565
Conc: 40.00 ng/ml

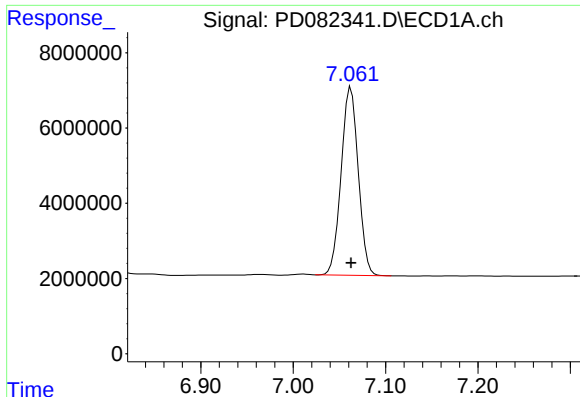

#17 4,4'-DDT


R.T.: 7.063 min
Delta R.T.: 0.000 min
Response: 64420582
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3007

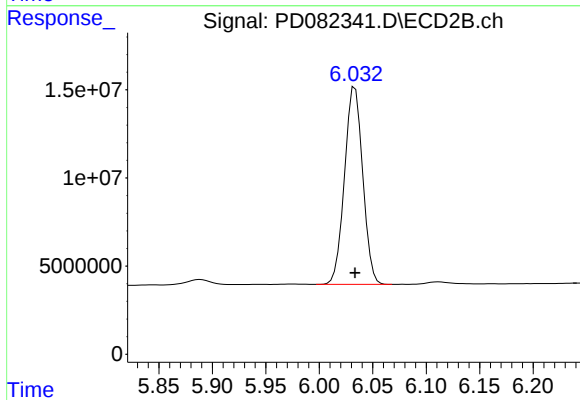


#17 4,4'-DDT

R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 133013834
Conc: 40.00 ng/ml

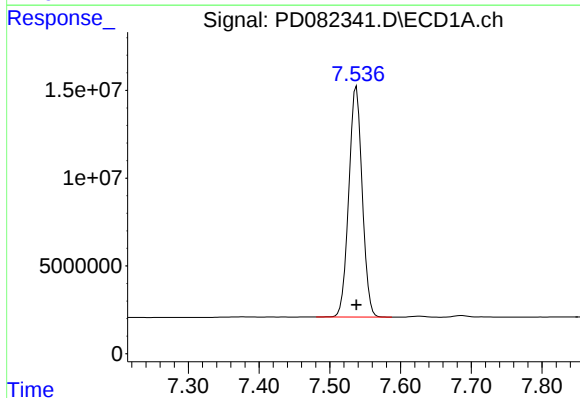


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 173182491
Conc: 200.00 ng/ml

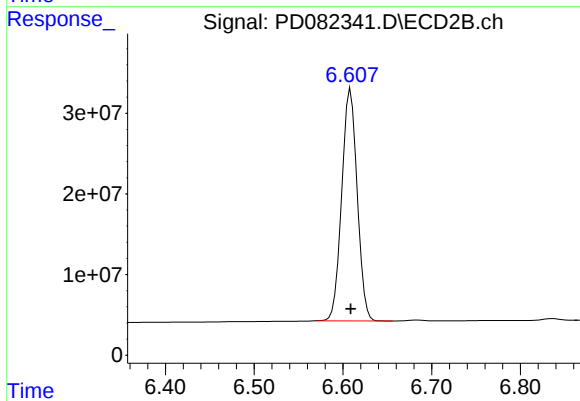

#20 Methoxychlor


R.T.: 6.609 min
Delta R.T.: 0.000 min
Response: 348245944
Conc: 200.00 ng/ml

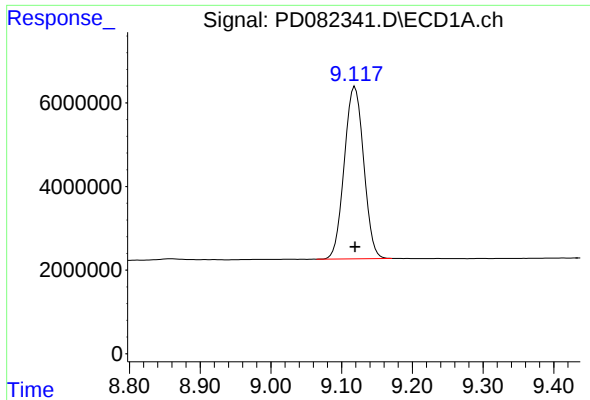

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 78553556
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3007

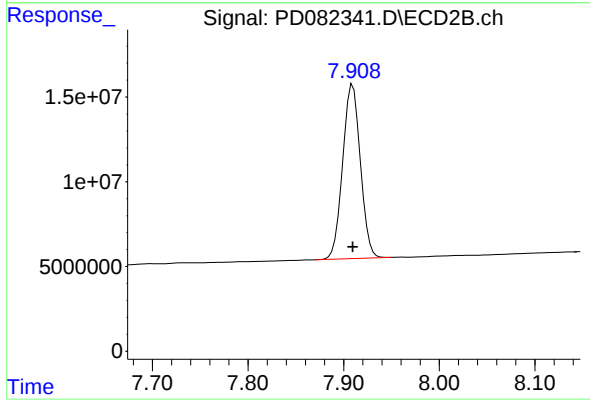

#27 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.000 min
Response: 132848938
Conc: 40.00 ng/ml