

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
 Data File : PD082343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 21:03
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4009

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:55:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 01:51:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.777	60848650	135.2E6	41.591	38.803
27)	SA Decachlor...	9.119	7.910	146.9E6	255.5E6	74.792	76.942
Target Compounds							
2)	A alpha-BHC	4.023	3.277	107.7E6	220.8E6	45.151	40.807
3)	MA gamma-BHC...	4.357	3.606	102.9E6	202.4E6	43.405	40.035
4)	MA Heptachlor	4.950	3.945	102.3E6	188.2E6	42.127	39.990
9)	A Endosulfan I	6.108	5.096	83685851	154.2E6	38.938	39.802
13)	MA Dieldrin	6.384	5.360	177.7E6	344.6E6	82.594	80.607
14)	MA Endrin	6.614	5.635	147.8E6	295.9E6	83.032	80.144
16)	A 4,4'-DDD	6.747	5.782	128.2E6	252.8E6	82.613	80.966
17)	MA 4,4'-DDT	7.062	6.033	132.4E6	274.8E6	82.238	82.653
20)	A Methoxychlor	7.537	6.608	337.3E6	646.1E6	389.493	371.084

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 21:03
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:55:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 01:51:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

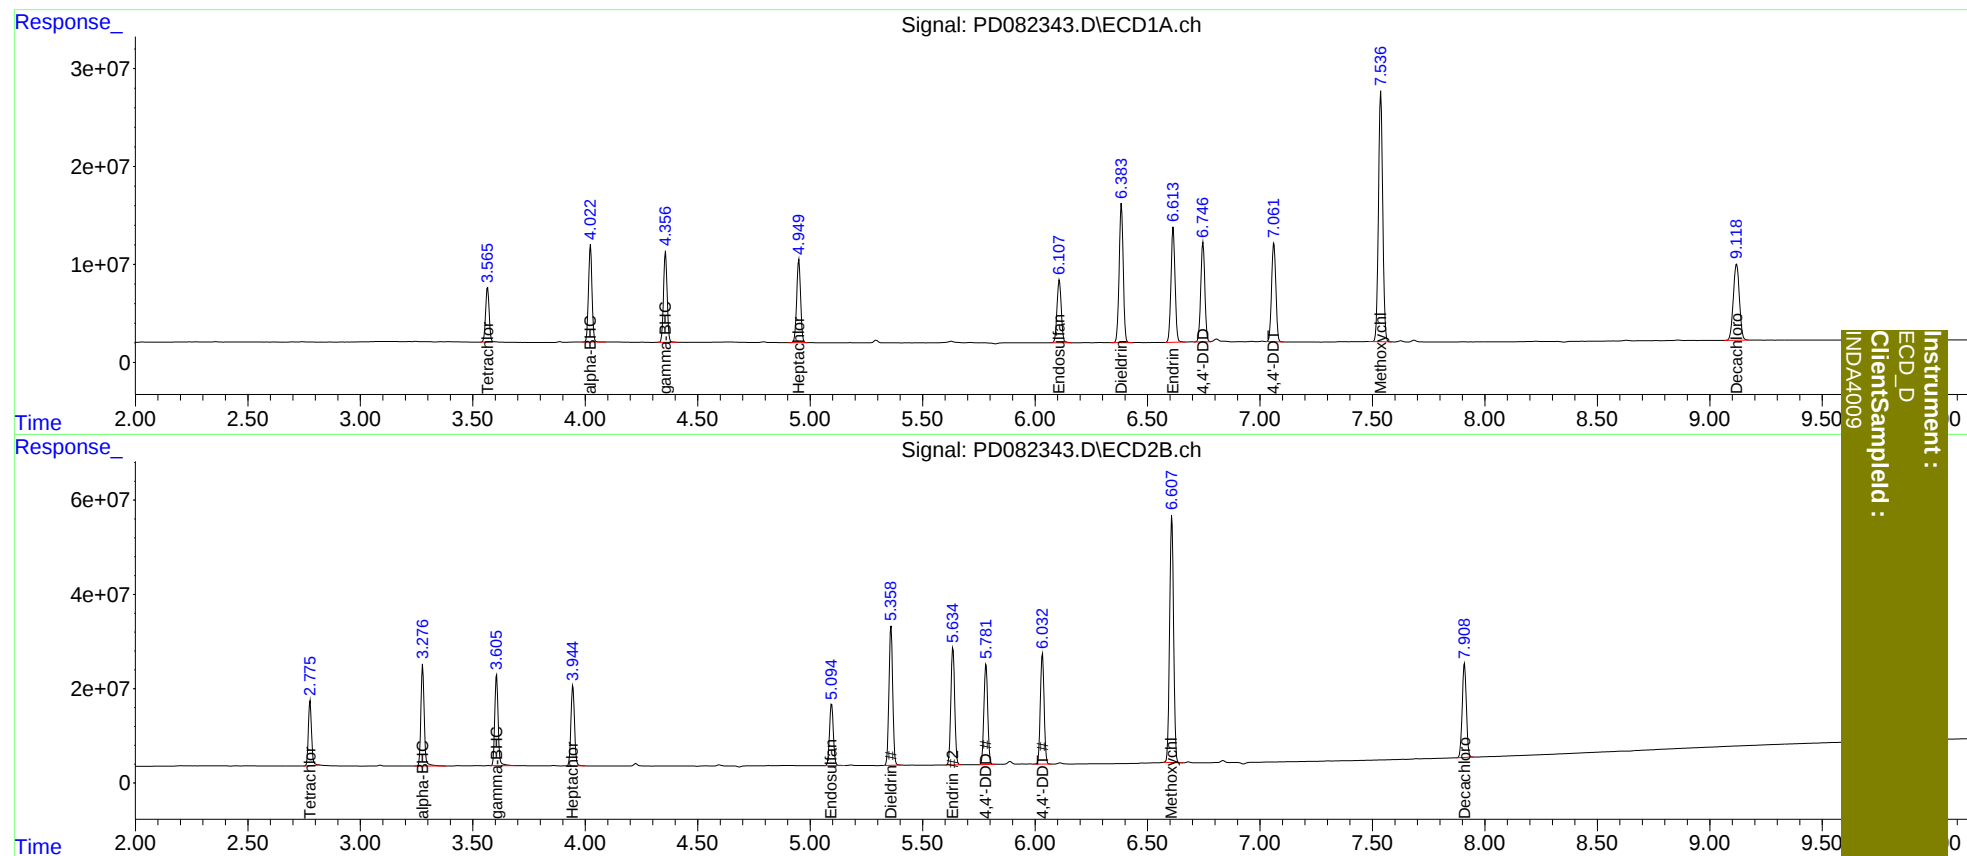


Instrument :
ECD_D
ClientSampled :
INDA4009

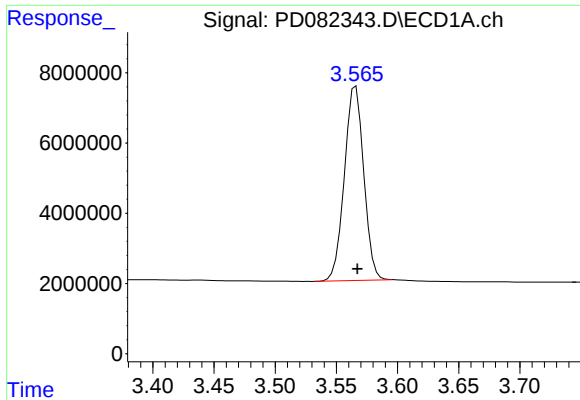

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: -0.001 min
Response: 60848650
Conc: 41.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4009

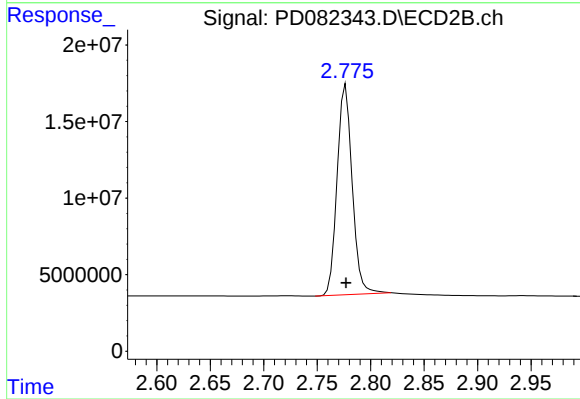


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 135235790
Conc: 38.80 ng/ml

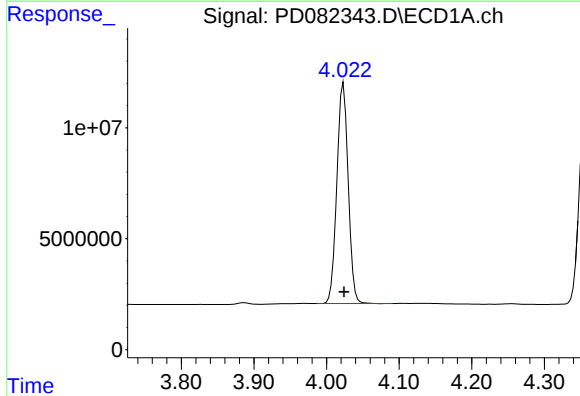


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 107683922
Conc: 45.15 ng/ml

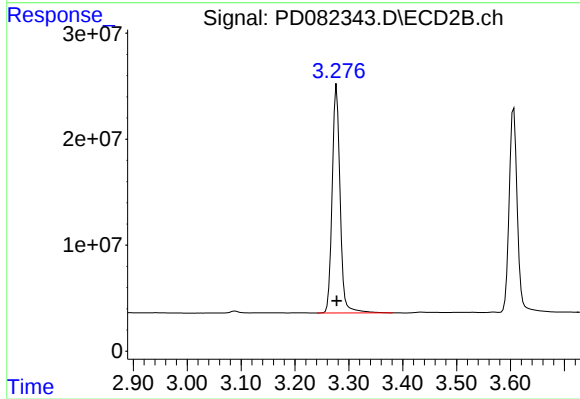

#2 alpha-BHC


R.T.: 3.277 min
Delta R.T.: 0.000 min
Response: 220831102
Conc: 40.81 ng/ml

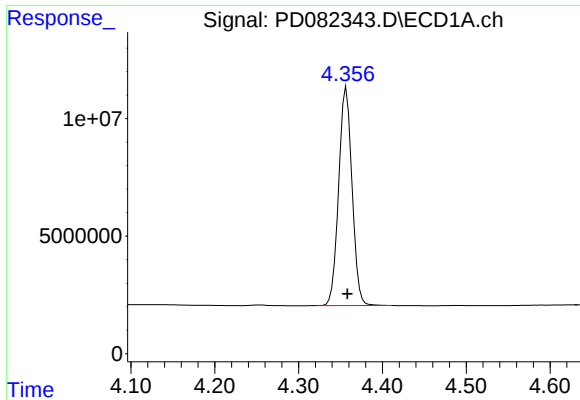

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: -0.001 min
Response: 102876581
Conc: 43.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4009

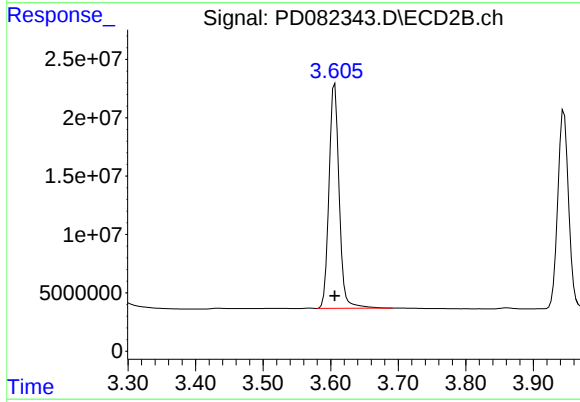


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 202425023
Conc: 40.04 ng/ml

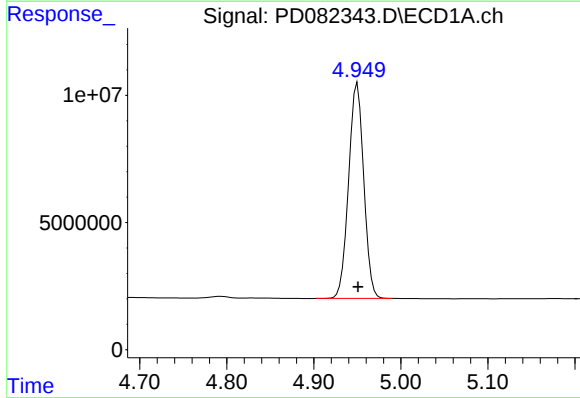


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 102313580
Conc: 42.13 ng/ml

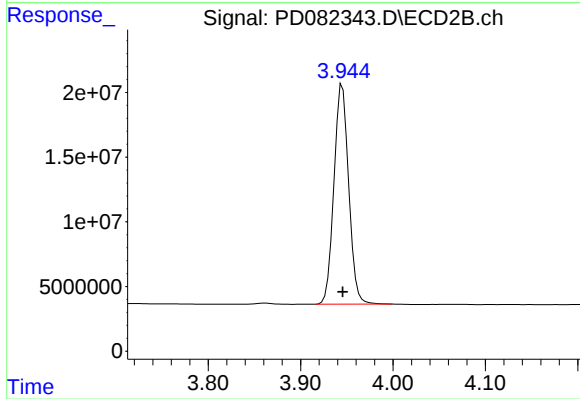

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 188188871
Conc: 39.99 ng/ml

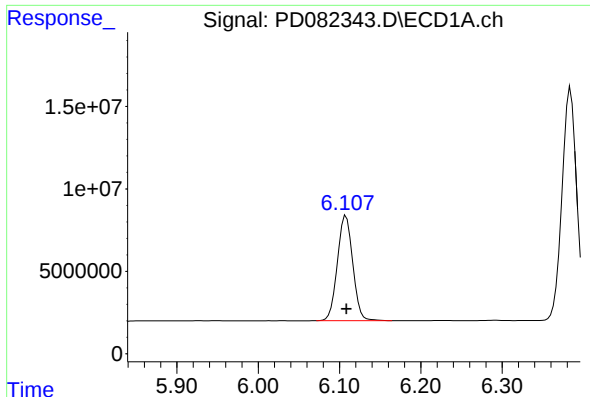

#9 Endosulfan I


R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 83685851
Conc: 38.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4009

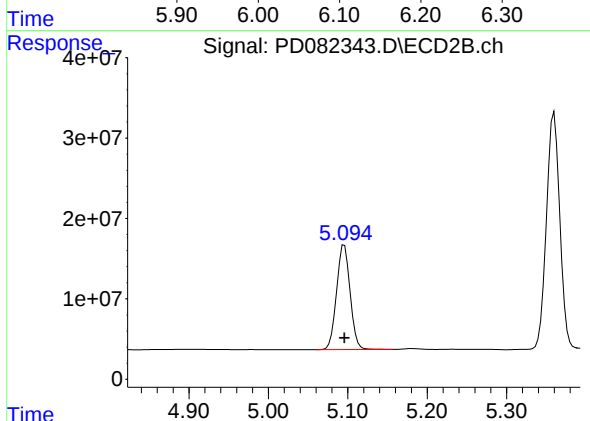


#9 Endosulfan I

R.T.: 5.096 min
Delta R.T.: 0.000 min
Response: 154203816
Conc: 39.80 ng/ml

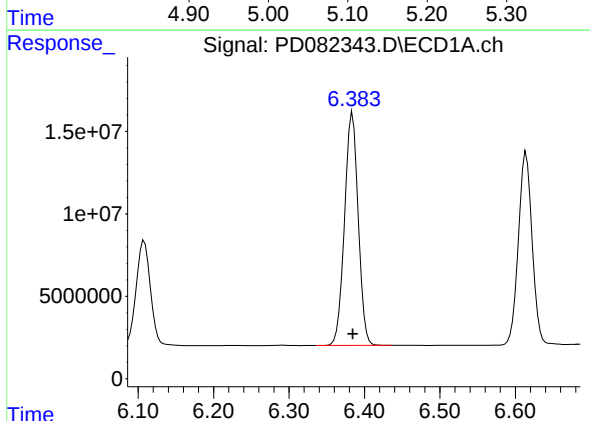


#13 Dieldrin

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 177693654
Conc: 82.59 ng/ml

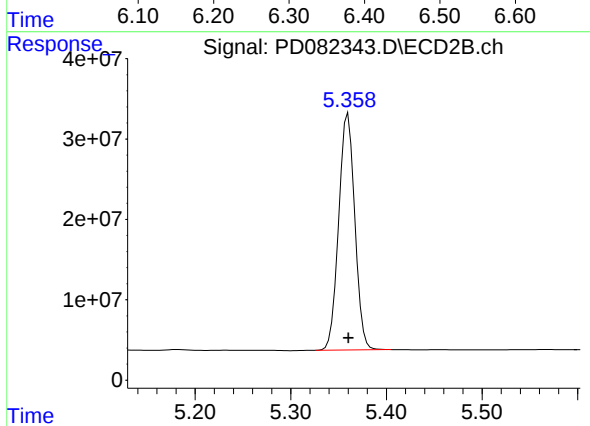

#13 Dieldrin


R.T.: 5.360 min
Delta R.T.: 0.000 min
Response: 344559800
Conc: 80.61 ng/ml

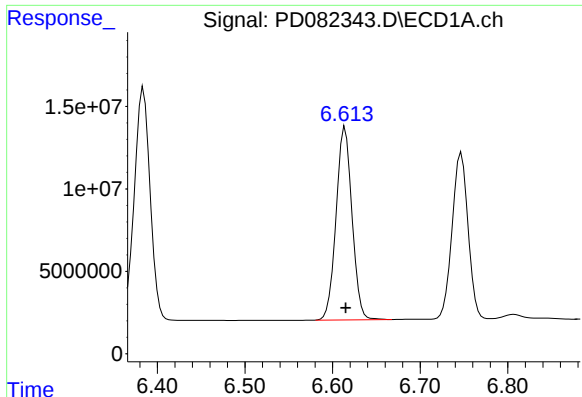

#14 Endrin


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 147838508
Conc: 83.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4009

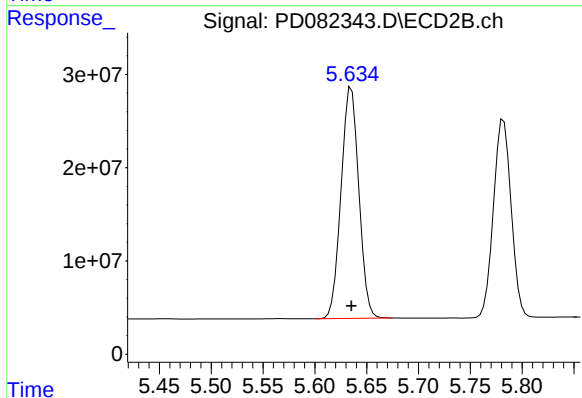


#14 Endrin

R.T.: 5.635 min
Delta R.T.: 0.000 min
Response: 295884805
Conc: 80.14 ng/ml

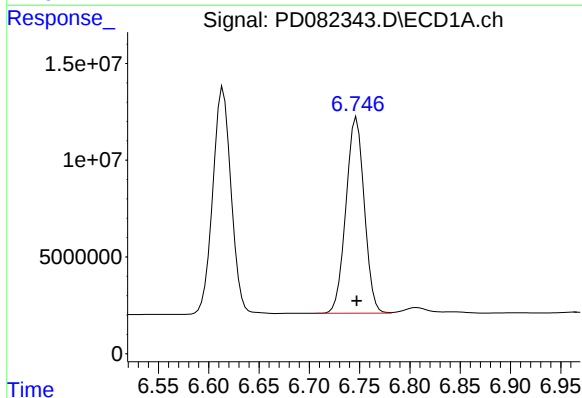


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 128167779
Conc: 82.61 ng/ml

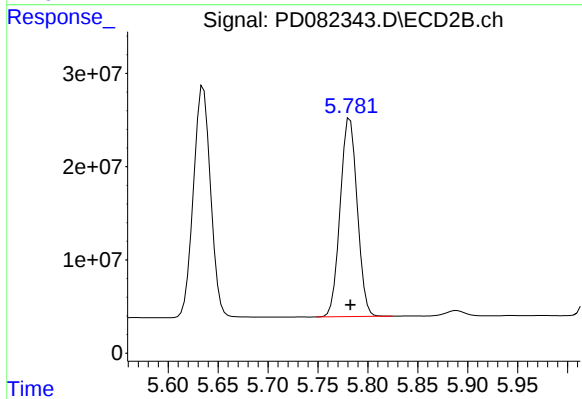

#16 4,4'-DDD


R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 252835863
Conc: 80.97 ng/ml

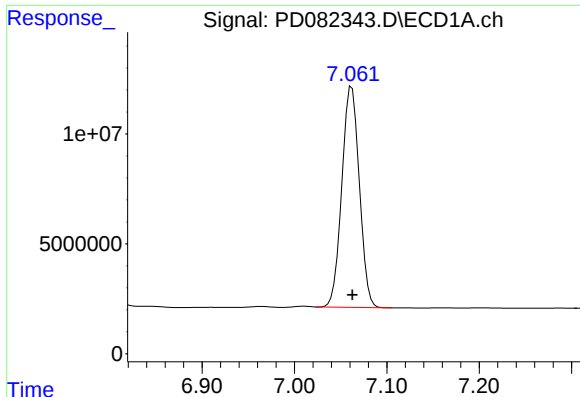

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 132446291
Conc: 82.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4009

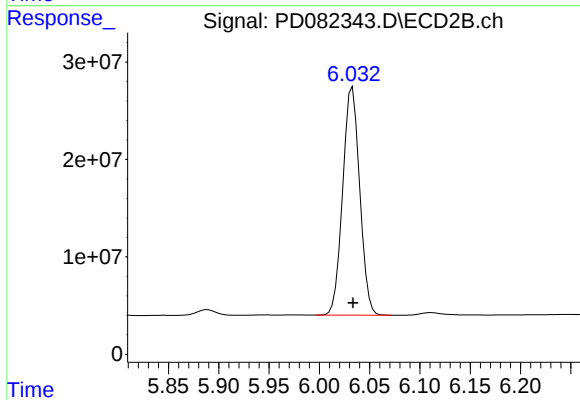


#17 4,4'-DDT

R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 274848168
Conc: 82.65 ng/ml

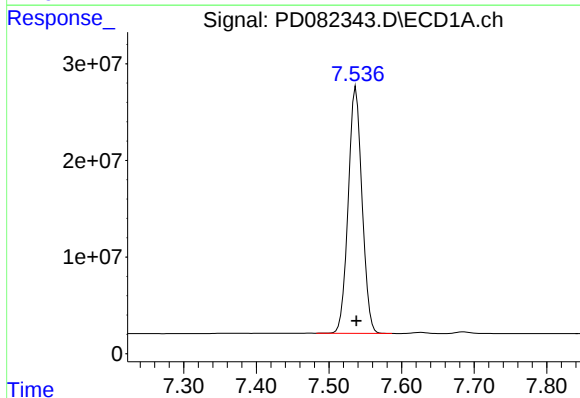


#20 Methoxychlor

R.T.: 7.537 min
Delta R.T.: 0.000 min
Response: 337266716
Conc: 389.49 ng/ml

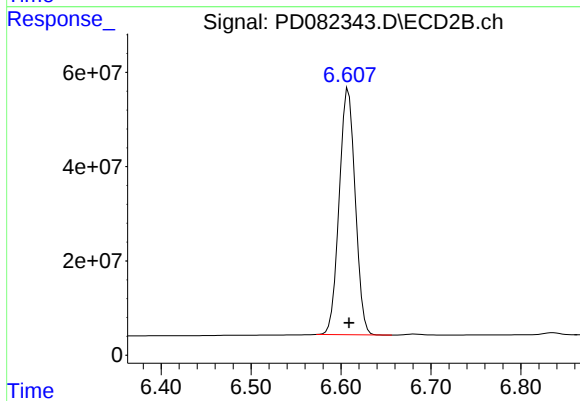

#20 Methoxychlor


R.T.: 6.608 min
Delta R.T.: 0.000 min
Response: 646141722
Conc: 371.08 ng/ml

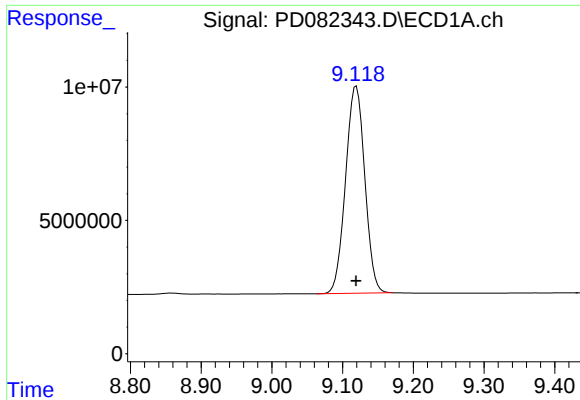

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 146880293
Conc: 74.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4009

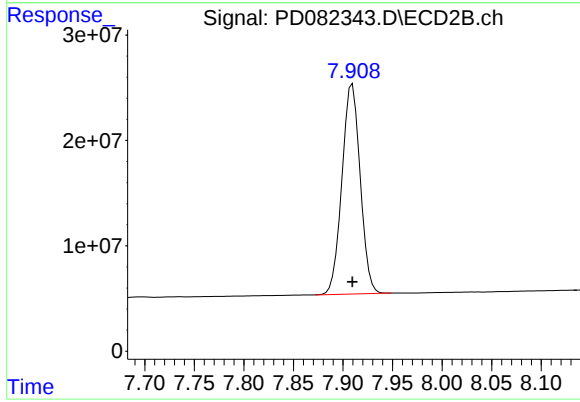

#27 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.000 min
Response: 255542193
Conc: 76.94 ng/ml