

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
 Data File : PD082345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 21:30
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5011

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:55:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 01:51:56 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.777	122.6E6	269.7E6	83.782	77.385
27)	SA Decachlor...	9.119	7.910	286.5E6	502.9E6	145.902	151.407
Target Compounds							
2)	A alpha-BHC	4.023	3.278	232.1E6	455.8E6	97.314	84.227
3)	MA gamma-BHC...	4.357	3.606	216.3E6	413.4E6	91.256	81.759
4)	MA Heptachlor	4.950	3.946	209.5E6	383.4E6	86.255	81.476
9)	A Endosulfan I	6.107	5.096	166.7E6	312.3E6	77.547	80.618
13)	MA Dieldrin	6.383	5.360	367.8E6	697.5E6	170.967	163.178
14)	MA Endrin	6.614	5.635	304.6E6	594.6E6	171.063	161.045
16)	A 4,4'-DDD	6.747	5.782	265.9E6	507.2E6	171.385	162.426
17)	MA 4,4'-DDT	7.062	6.033	279.2E6	552.1E6	173.341	166.025
20)	A Methoxychlor	7.538	6.608	663.6E6	1196.2E6	766.382	687.011


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 21:30
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:55:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 01:51:56 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

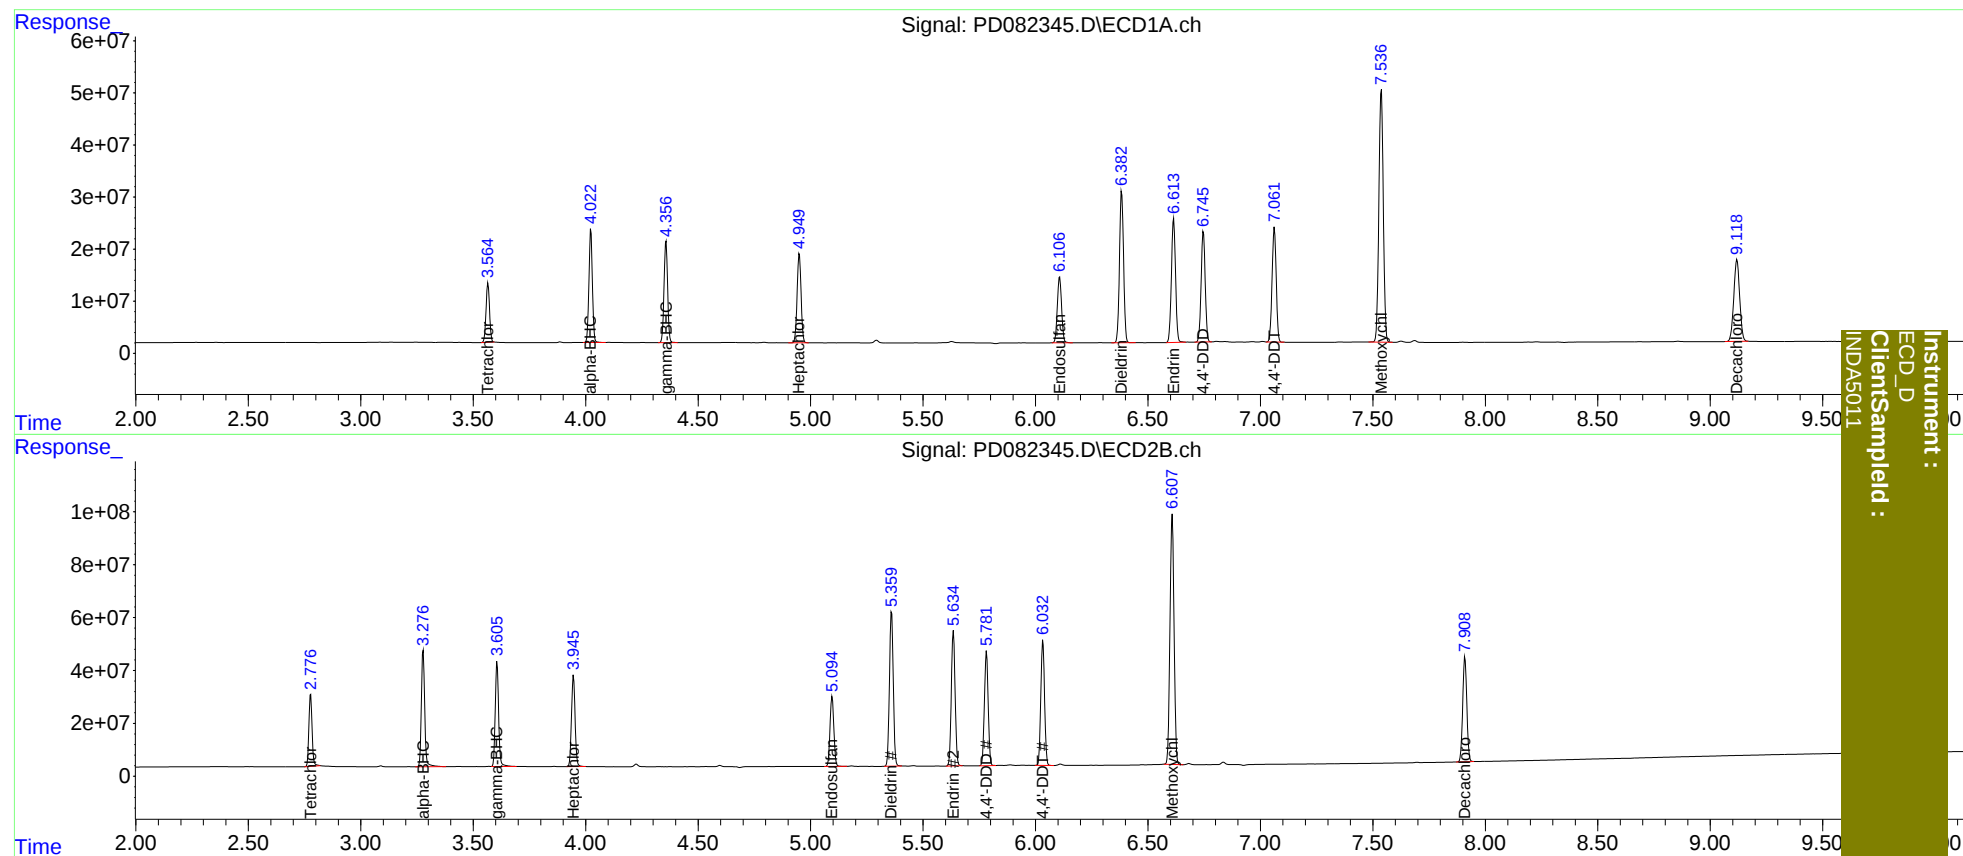


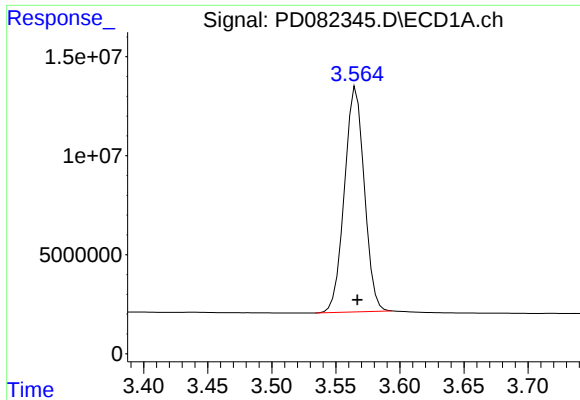

#1 Tetrachloro-m-xylene


R.T.: 3.566 min
Delta R.T.: -0.001 min
Response: 122574990
Conc: 83.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5011

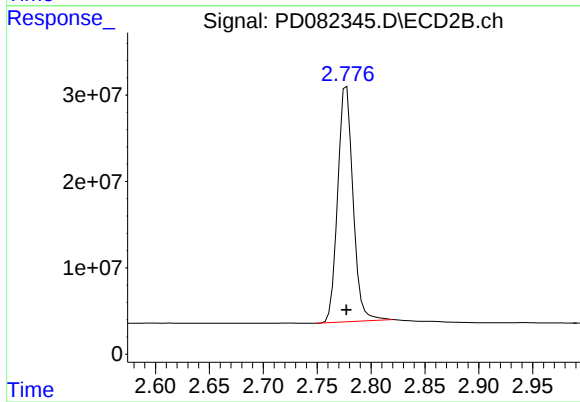


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 269701634
Conc: 77.39 ng/ml

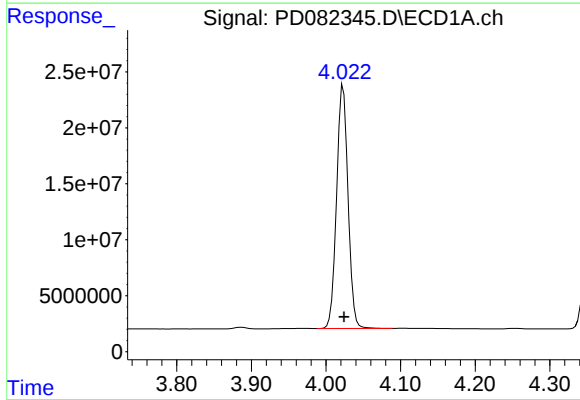


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 232090716
Conc: 97.31 ng/ml

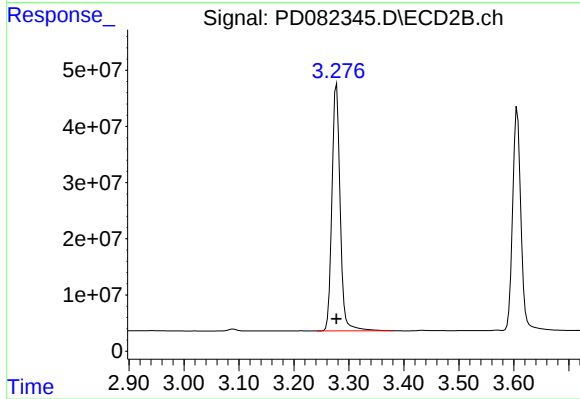

#2 alpha-BHC


R.T.: 3.278 min
Delta R.T.: 0.000 min
Response: 455805458
Conc: 84.23 ng/ml

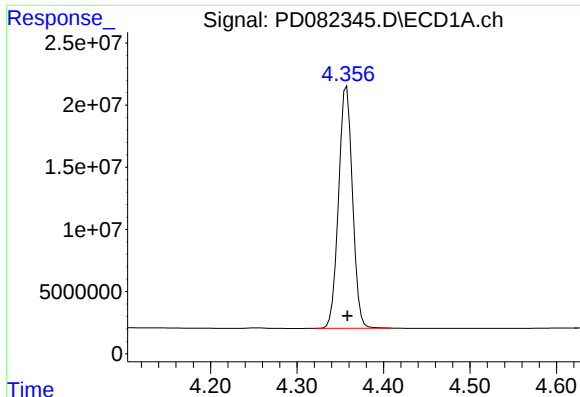

#3 gamma-BHC (Lindane)


R.T.: 4.357 min
Delta R.T.: 0.000 min
Response: 216290455
Conc: 91.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5011

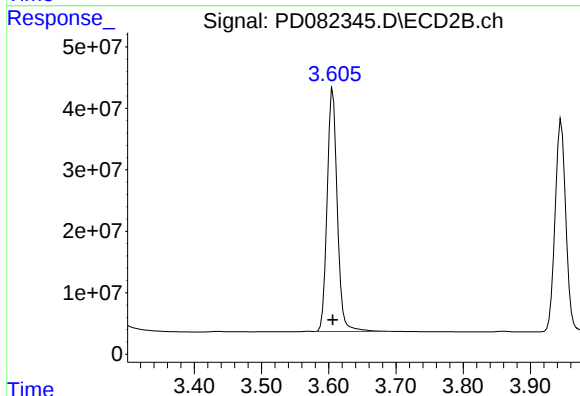


#3 gamma-BHC (Lindane)

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 413386551
Conc: 81.76 ng/ml

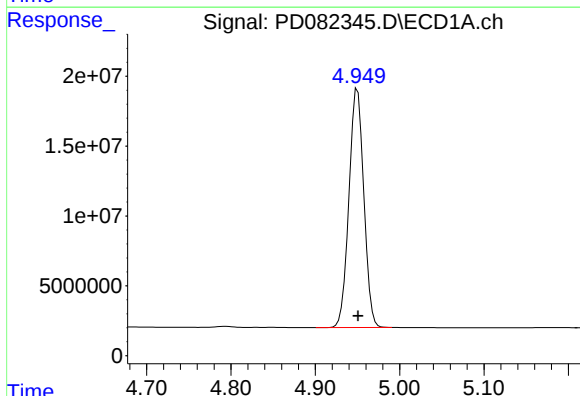


#4 Heptachlor

R.T.: 4.950 min
Delta R.T.: 0.000 min
Response: 209488490
Conc: 86.25 ng/ml

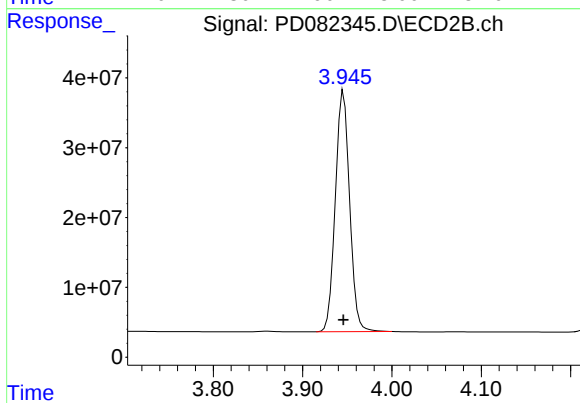

#4 Heptachlor


R.T.: 3.946 min
Delta R.T.: 0.000 min
Response: 383418666
Conc: 81.48 ng/ml

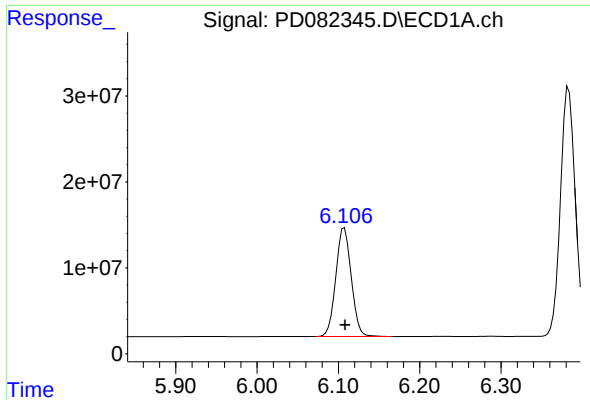

#9 Endosulfan I


R.T.: 6.107 min
Delta R.T.: -0.001 min
Response: 166663640
Conc: 77.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5011

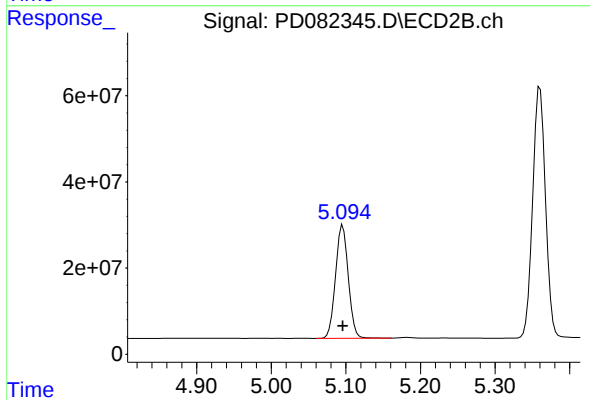


#9 Endosulfan I

R.T.: 5.096 min
Delta R.T.: 0.000 min
Response: 312333043
Conc: 80.62 ng/ml

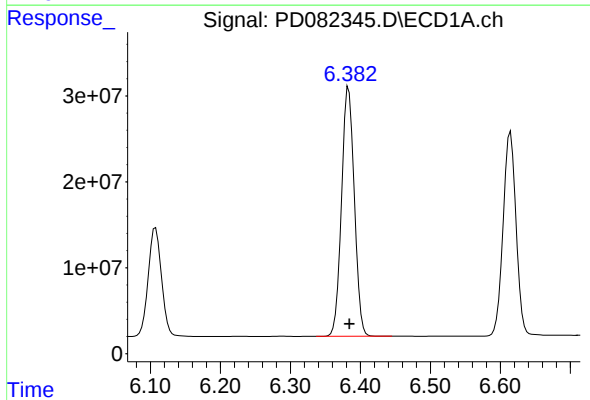


#13 Dieldrin

R.T.: 6.383 min
Delta R.T.: -0.001 min
Response: 367821626
Conc: 170.97 ng/ml

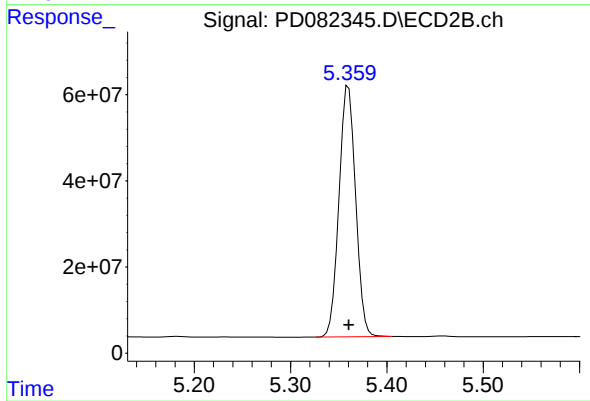

#13 Dieldrin


R.T.: 5.360 min
Delta R.T.: 0.000 min
Response: 697512742
Conc: 163.18 ng/ml

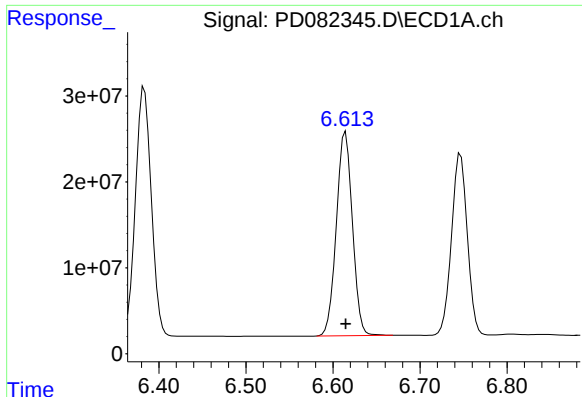

#14 Endrin


R.T.: 6.614 min
Delta R.T.: 0.000 min
Response: 304576716
Conc: 171.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5011

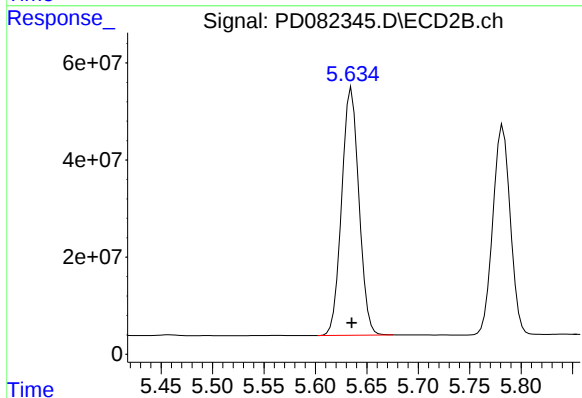


#14 Endrin

R.T.: 5.635 min
Delta R.T.: 0.000 min
Response: 594569344
Conc: 161.05 ng/ml

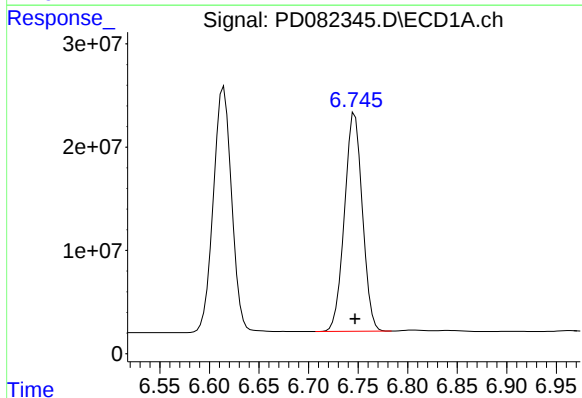


#16 4,4'-DDD

R.T.: 6.747 min
Delta R.T.: 0.000 min
Response: 265890247
Conc: 171.38 ng/ml

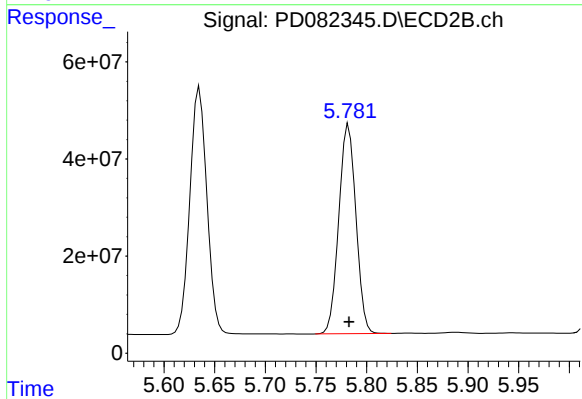

#16 4,4'-DDD


R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 507213956
Conc: 162.43 ng/ml

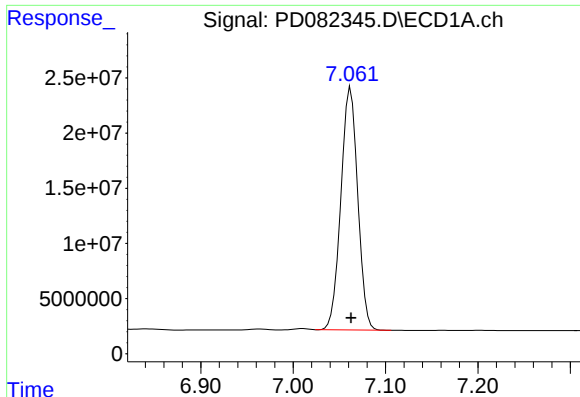

#17 4,4'-DDT


R.T.: 7.062 min
Delta R.T.: 0.000 min
Response: 279168905
Conc: 173.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5011

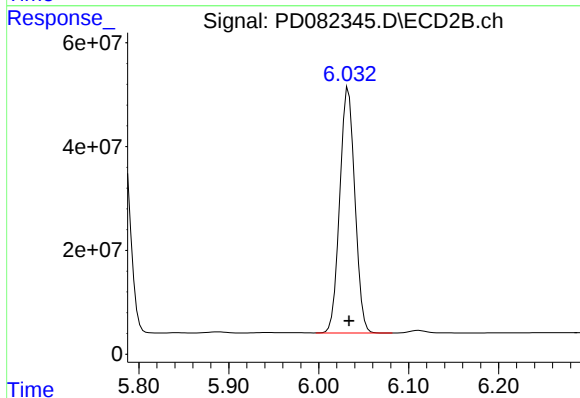


#17 4,4'-DDT

R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 552089025
Conc: 166.02 ng/ml

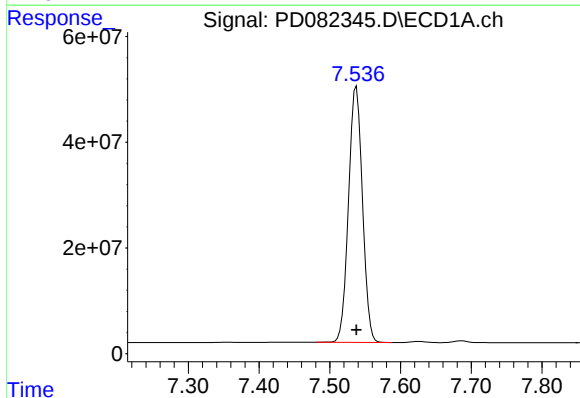


#20 Methoxychlor

R.T.: 7.538 min
Delta R.T.: 0.000 min
Response: 663619437
Conc: 766.38 ng/ml

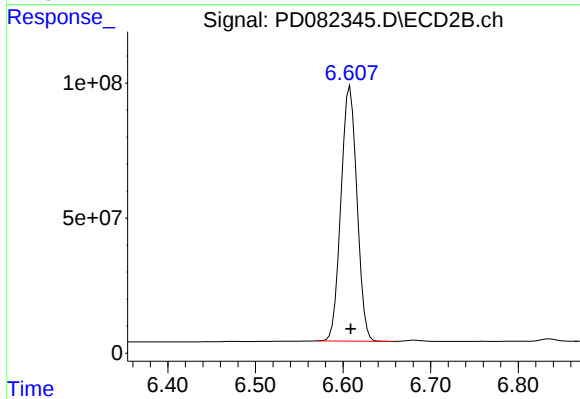

#20 Methoxychlor


R.T.: 6.608 min
Delta R.T.: 0.000 min
Response: 1196244216
Conc: 687.01 ng/ml

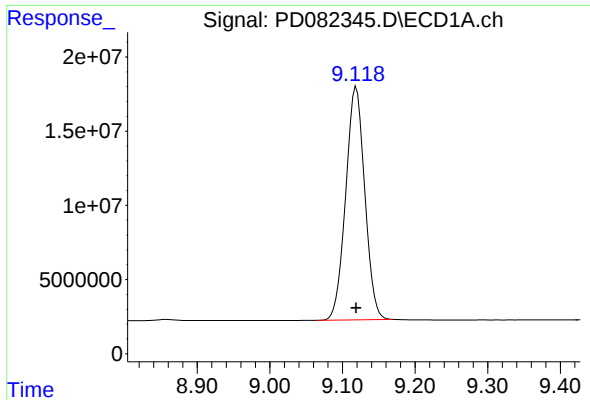

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 286528639
Conc: 145.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5011

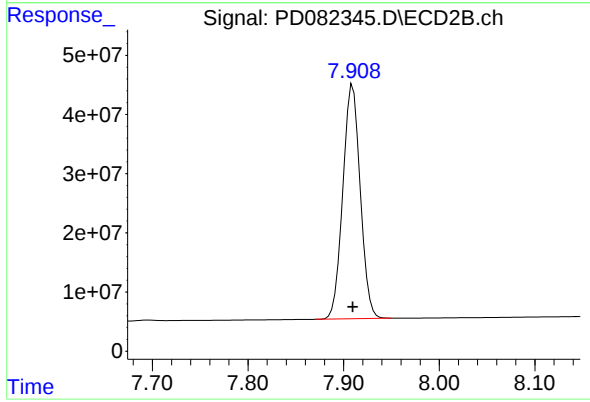

#27 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.000 min
Response: 502856751
Conc: 151.41 ng/ml