

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
 Data File : PD082330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 18:10
 Operator : AR\AJ
 Sample : RESC027
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC028

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 03:42:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 02:08:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.777	29018204	65302281	19.136	18.941
27)	SA Decachlor...	9.118	7.909	77481810	124.9E6	39.622	38.397
Target Compounds							
2)	A alpha-BHC	4.023	3.277	23921675	50077651	9.312	9.326
3)	MA gamma-BHC...	4.357	3.606	23468813	46590028	9.440	9.292
4)	MA Heptachlor	4.950	3.946	24000081	43946497	9.502	9.391
5)	MB Aldrin	5.294	4.225	22551216	43542427	9.692	9.471
6)	B beta-BHC	4.553	3.902	10186900	19609942	9.716	9.433
7)	B delta-BHC	4.802	4.132	22586816	43901662	9.355	8.995
8)	B Heptachlo...	5.721	4.726	21212656	38694038	9.773	9.142
9)	A Endosulfan I	6.108	5.096	21096650	36319824	9.764	9.458
10)	B trans-Chl...	5.977	4.976	19953104	36373612	9.717	9.035
11)	B cis-Chlor...	6.057	5.040	20538399	37194763	9.715	8.999
12)	B 4,4'-DDE	6.228	5.229	39009951	69809433	18.953	18.018
13)	MA Dieldrin	6.384	5.360	41774632	78565838	18.961	18.646
14)	MA Endrin	6.615	5.635	35319570	67874569	19.265	18.711
15)	B Endosulfa...	6.834	5.929	37979728	63706142	19.997	18.405
16)	A 4,4'-DDD	6.747	5.782	30418129	59817413	19.306	19.422
17)	MA 4,4'-DDT	7.062	6.033	32562645	61254019	19.908	18.661
18)	B Endrin al...	6.964	6.108	25997325	48095758	19.165	18.182
19)	B Endosulfa...	7.199	6.330	33833626	62273561	20.053	18.642
20)	A Methoxychlor	7.537	6.608	91137688	174.0E6	103.456	103.905
21)	B Endrin ke...	7.685	6.836	36345312	71677847	20.232	19.062

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 18:10
Operator : AR\AJ
Sample : RESC027
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 03:42:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 02:08:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

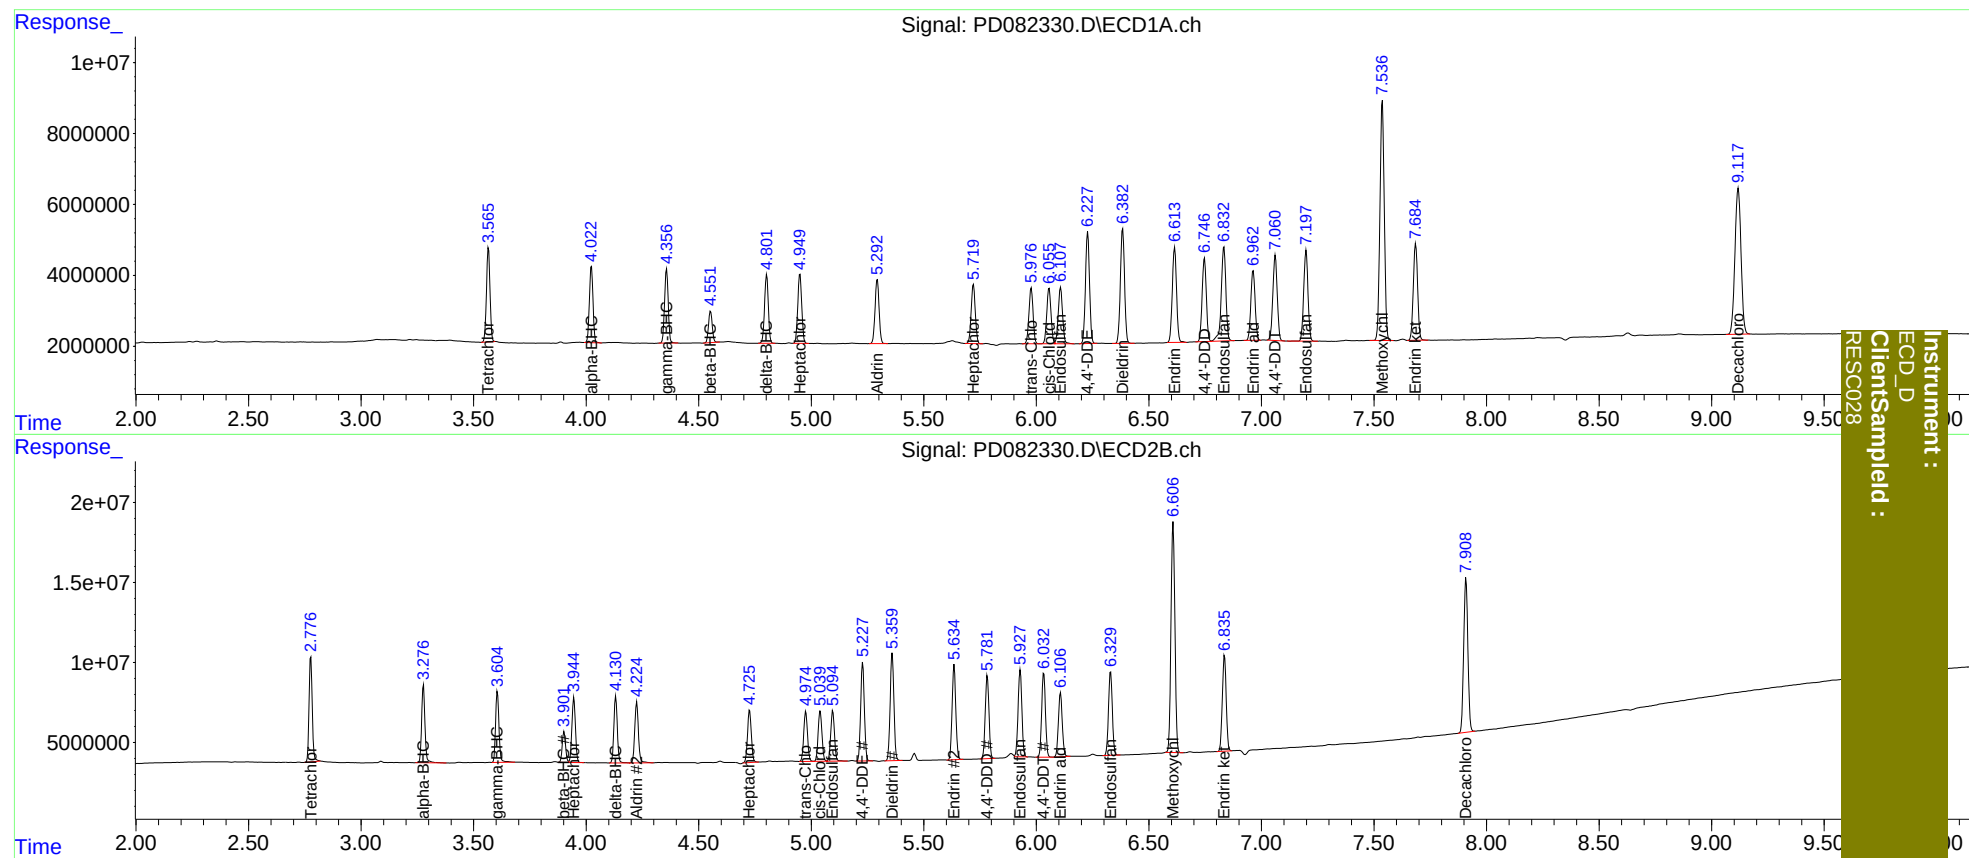

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082330.D
Acq On : 09 Apr 2024 18:10
Operator : AR\AJ
Sample : RESC027
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC028

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Title : GC Extractables
Last Update : Wed Apr 10 02:08:54 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.566	4.023	100.00%
4.023	4.357	100.00%
4.357	4.553	100.00%
4.553	4.802	100.00%
4.802	4.950	100.00%
4.950	5.294	100.00%
5.294	5.721	100.00%
5.721	5.977	100.00%
5.977	6.057	100.00%
6.057	6.108	96.69%
6.108	6.228	100.00%
6.228	6.384	100.00%
6.384	6.615	100.00%
6.615	6.747	100.00%
6.747	6.834	99.47%
6.834	6.964	100.00%
6.964	7.062	100.00%
7.062	7.199	100.00%
7.199	7.537	100.00%
7.537	7.685	100.00%
7.685	9.118	100.00%

Signal #2


2.777	3.277	100.00%
3.277	3.606	100.00%
3.606	3.902	100.00%
3.902	3.946	98.70%
3.946	4.132	100.00%
4.132	4.225	100.00%
4.225	4.726	100.00%
4.726	4.976	100.00%
4.976	5.040	100.00%
5.040	5.096	100.00%
5.096	5.229	100.00%
5.229	5.360	100.00%
5.360	5.635	100.00%
5.635	5.782	100.00%
5.782	5.929	100.00%
5.929	6.033	100.00%
6.033	6.108	100.00%
6.108	6.330	100.00%
6.330	6.608	100.00%
6.608	6.836	100.00%
6.836	7.909	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 18:10
Operator : AR\AJ
Sample : RESC027
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC028

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 03:42:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 02:08:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

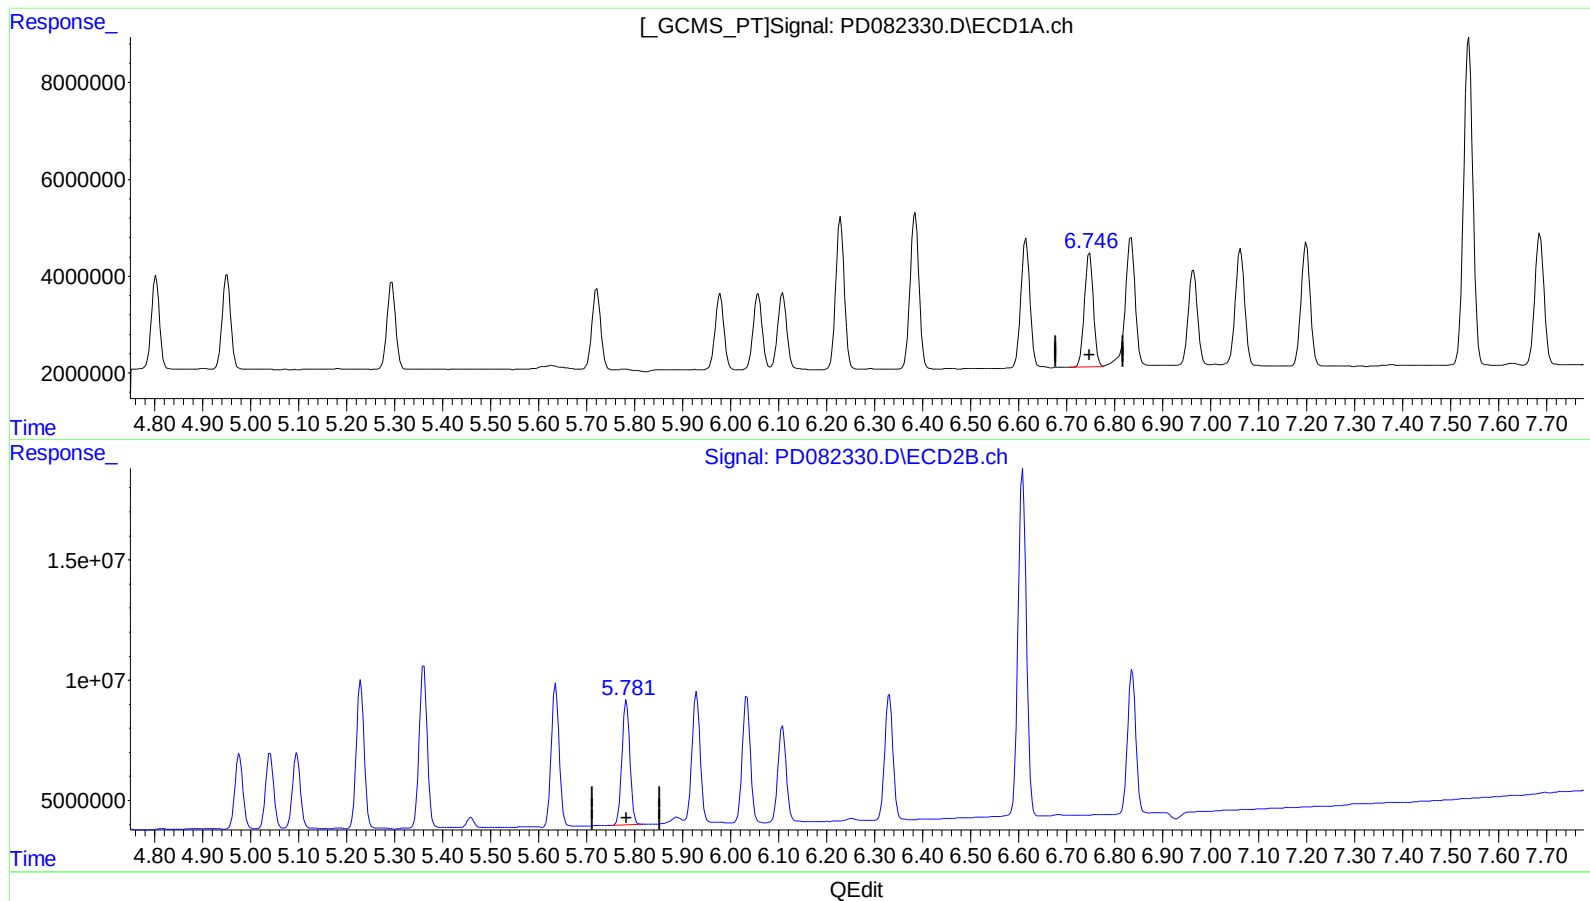

(16) 4,4'-DDD (A)
6.747min 19.306 ng/ml
response 30418129


(16) 4,4'-DDD #2 (A)
5.782min 19.422 ng/ml
response 59817413

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041024\
Data File : PD082330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 18:10
Operator : AR\AJ
Sample : RESC027
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC028

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 03:42:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 02:08:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

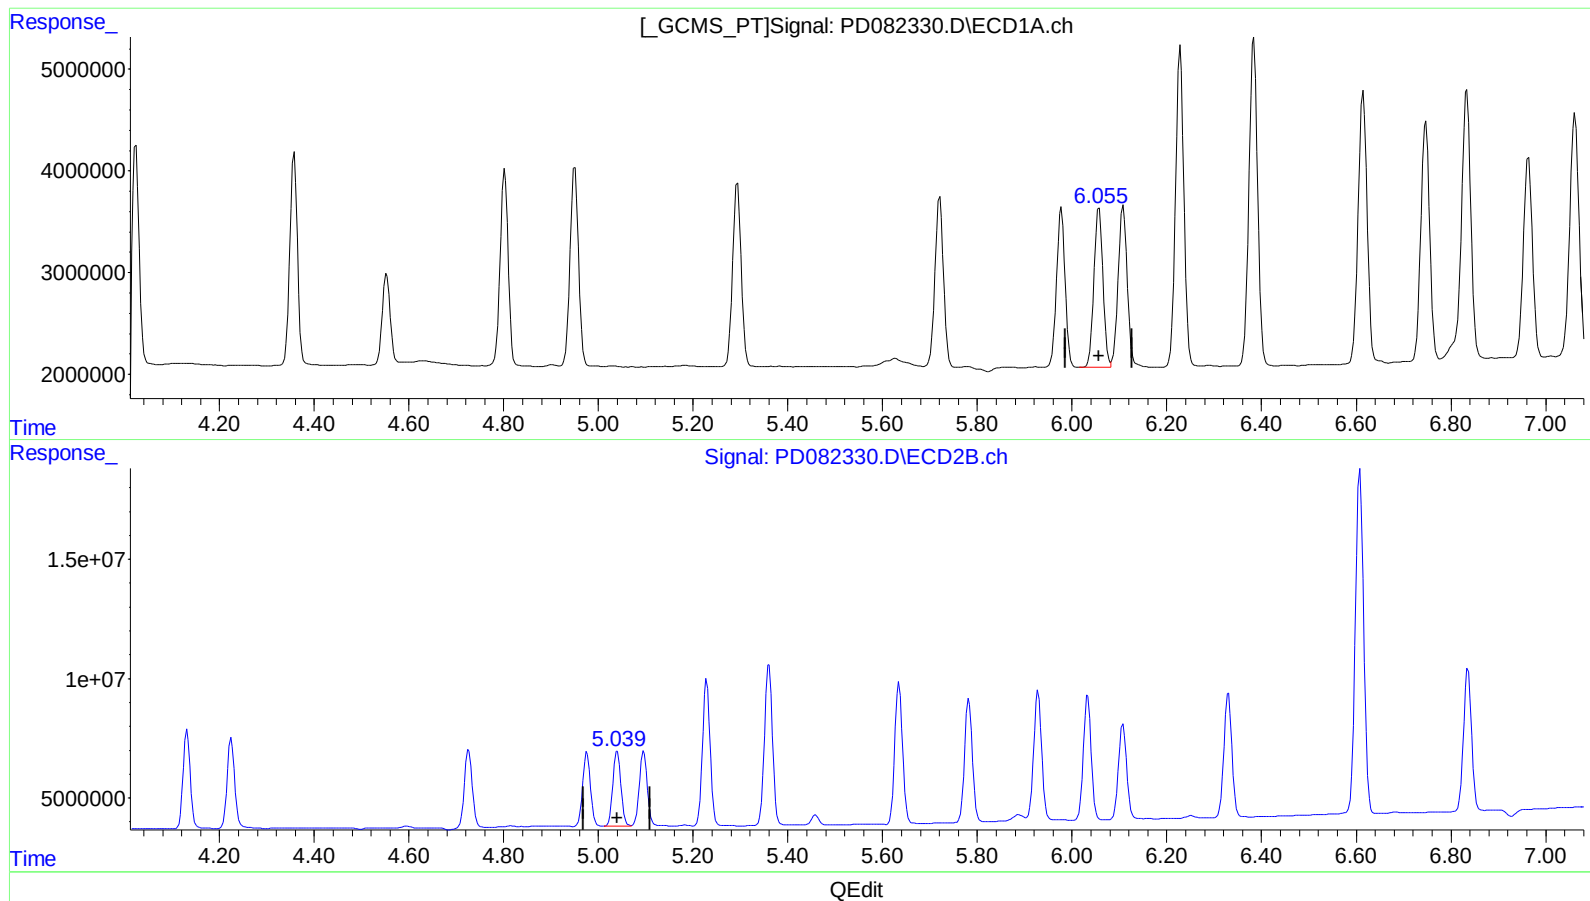

(11) cis-Chlordane (B)

6.057min 9.715 ng/ml

response 20538399

(11) cis-Chlordane #2 (B)

5.040min 8.999 ng/ml

response 37194763