

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041025\
 Data File : PD088076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2025 21:49
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4016

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 13:08:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041025CLP-.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 11 12:59:56 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	2.882	71694919	531.8E6	38.528	38.619
2)	SA Decachlor...	9.073	8.076	223.7E6	1269.3E6	77.185	77.039
Target Compounds							
2)	A alpha-BHC	4.000	3.395	157.9E6	854.2E6	38.498	38.639
3)	MA gamma-BHC...	4.331	3.732	149.9E6	782.3E6	38.480	38.639
4)	MA Heptachlor	4.931	4.085	146.4E6	792.8E6	38.539	38.688
9)	A Endosulfan I	6.075	5.250	119.2E6	655.6E6	38.540	38.722
13)	MA Dieldrin	6.348	5.516	269.0E6	1407.7E6	77.339	77.645
14)	MA Endrin	6.575	5.792	217.5E6	1243.5E6	77.152	77.588
16)	A 4,4'-DDD	6.705	5.933	183.8E6	1136.7E6	77.147	77.402
17)	MA 4,4'-DDT	7.021	6.187	194.8E6	1202.0E6	77.138	77.585
20)	A Methoxychlor	7.493	6.758	523.2E6	2554.6E6	386.736	389.636

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041025\
Data File : PD088076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2025 21:49
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 13:08:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041025CLP-.M
Quant Title : GC Extractables
QLast Update : Fri Apr 11 12:59:56 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

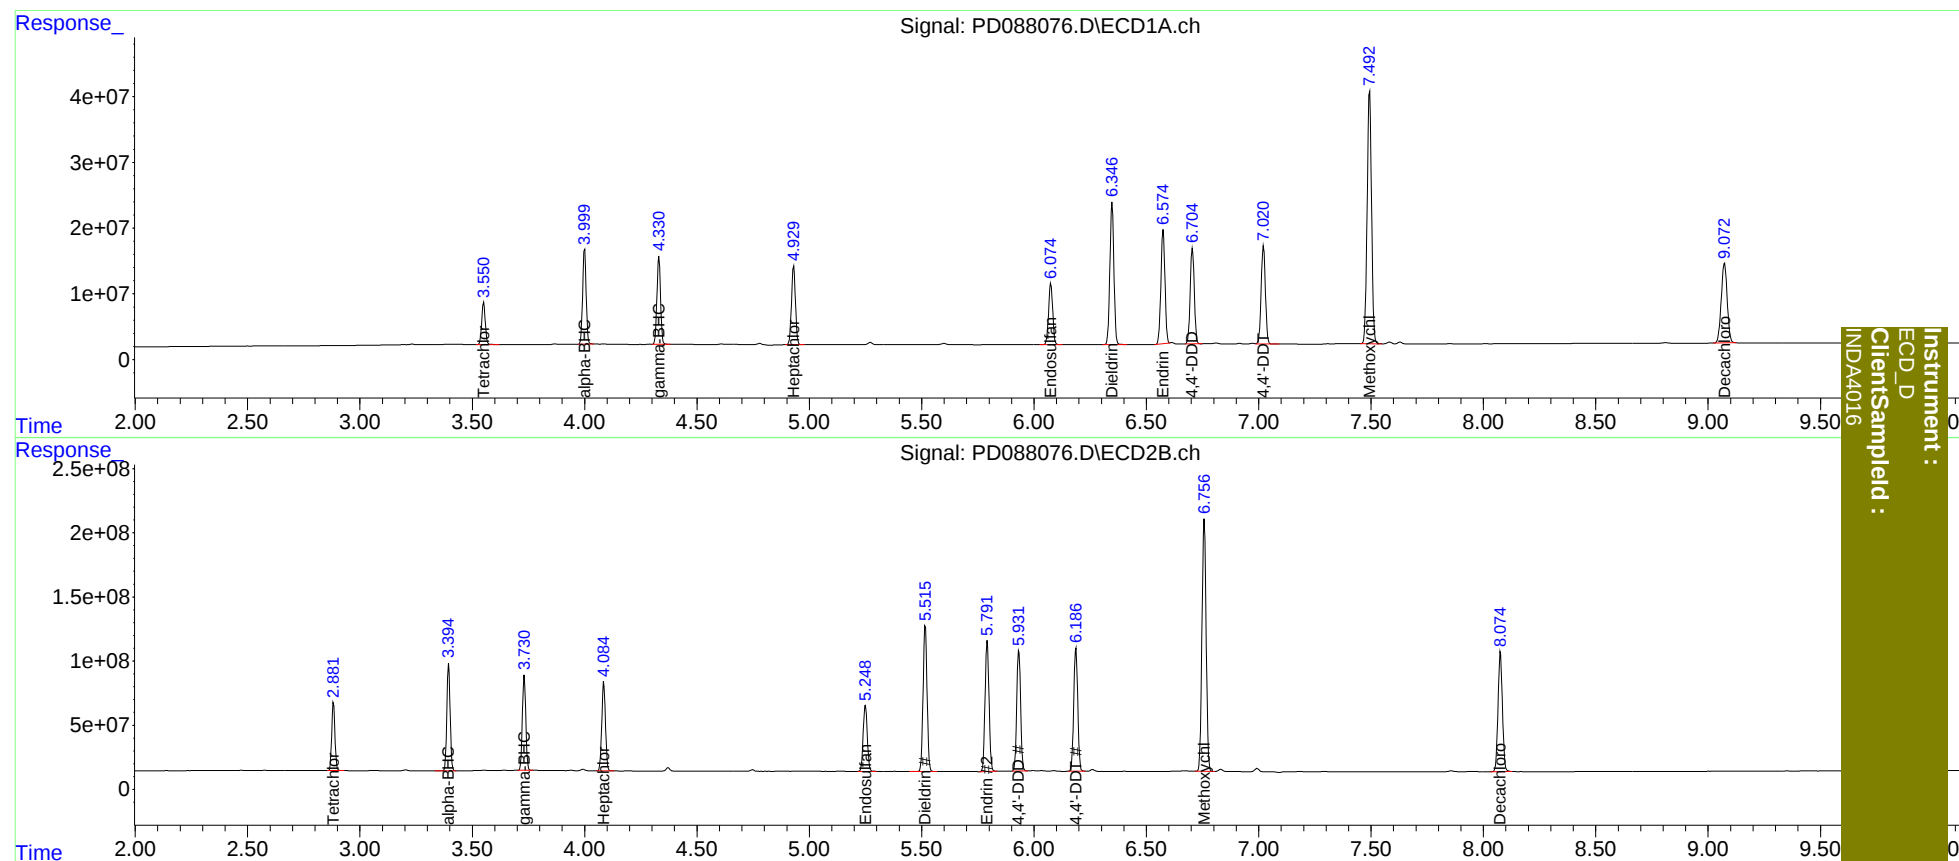

Instrument :
ECD_D
ClientSampled :
INDA4016