

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
 Data File : PD052862.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 17:20
 Operator : AJ\SJ
 Sample : PIBLK37
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:03:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.218	4.041	27608582	570.1E6	18.133	18.016
27) SA Decachlor...	7.813	9.158	52031553	523.8E6	36.902	36.326
Target Compounds						
6) B beta-BHC	0.000	4.925f	0 43605448	N.D.	2.230	
8) B Heptachlo...	0.000	5.921	0 44430711	N.D.	1.254	
9) A Endosulfan I	0.000	6.294	0 18594643	N.D.	0.568	
11) B cis-Chlor...	0.000	6.294f	0 18594643	N.D.	0.541	
14) MA Endrin	0.000	6.761	0 47146983	N.D.	1.865	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
Data File : PD052862.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 17:20
Operator : AJ\SJ
Sample : PIBLK37
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:03:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

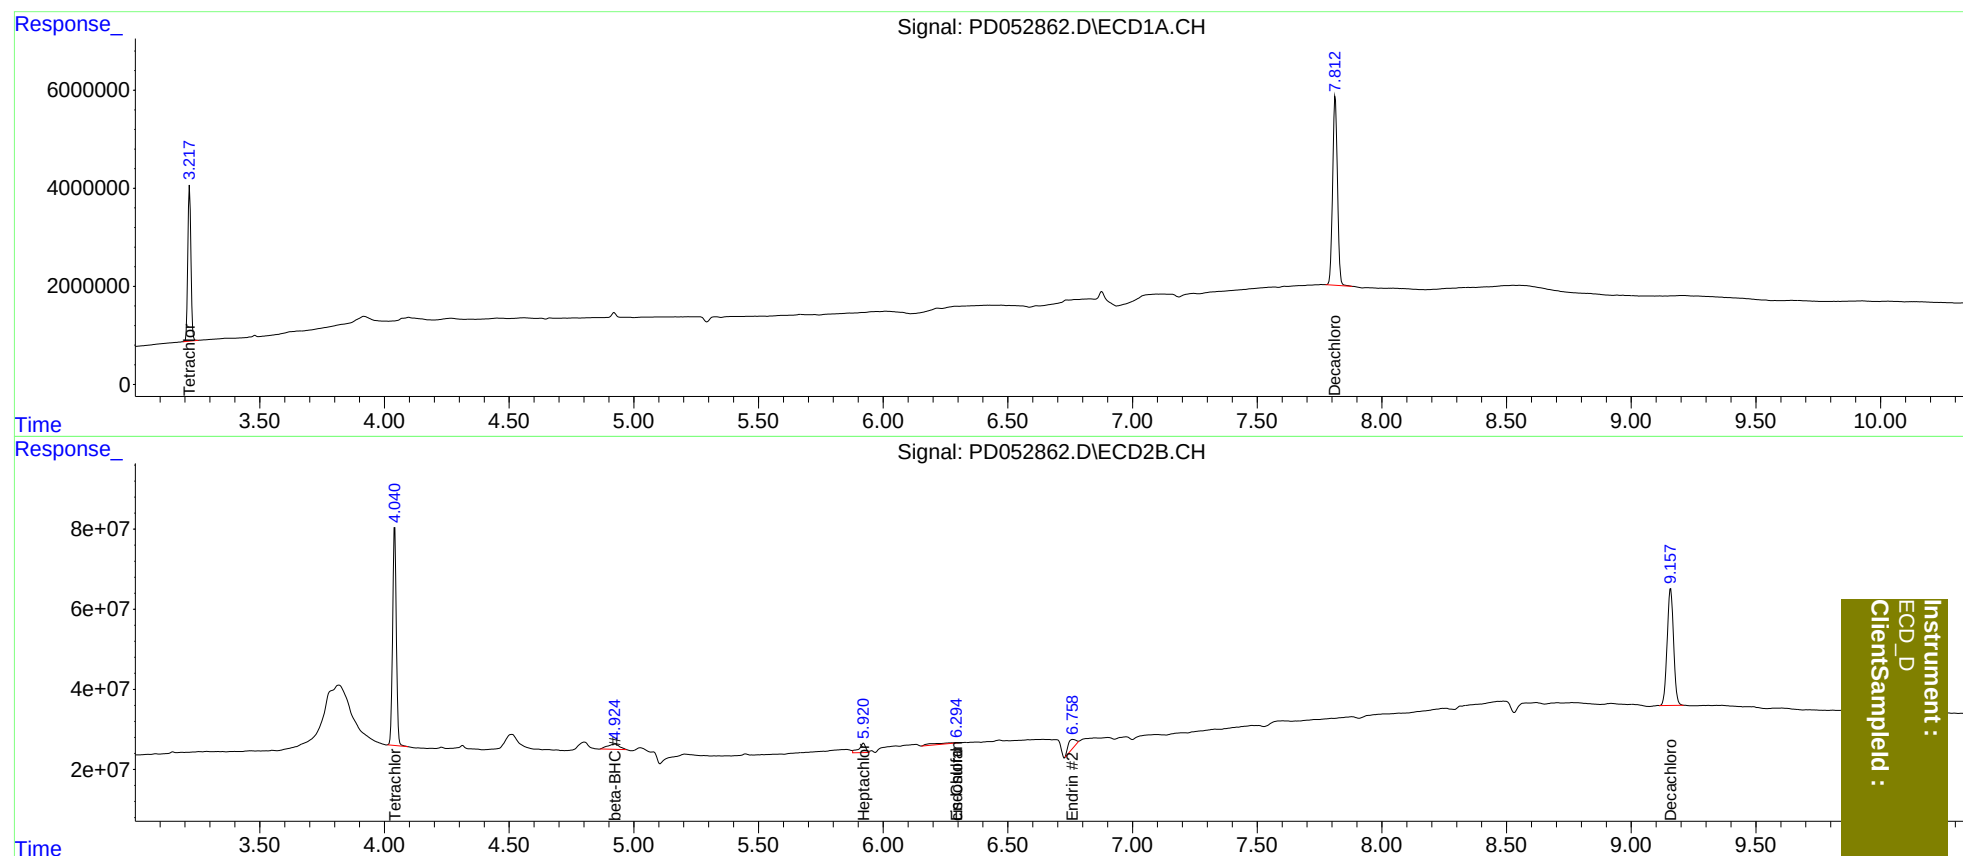


Instrument :
ECD_D
ClientSampleId :

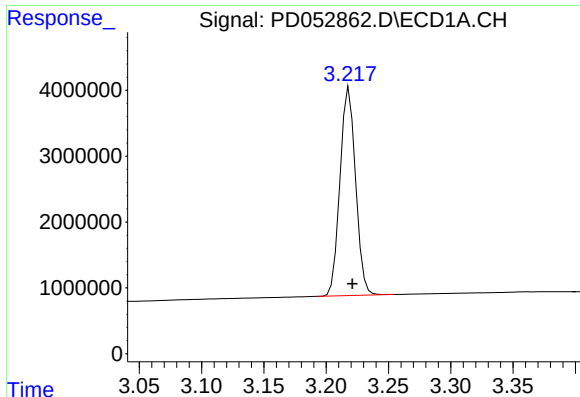

#1 Tetrachloro-m-xylene


R.T.: 3.218 min
Delta R.T.: -0.003 min
Response: 27608582
Conc: 18.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

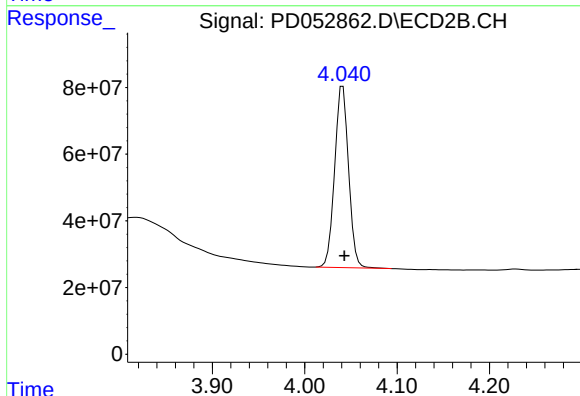


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 570132846
Conc: 18.02 ng/ml

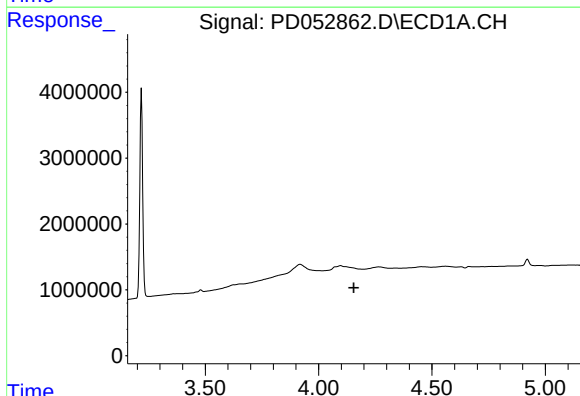


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

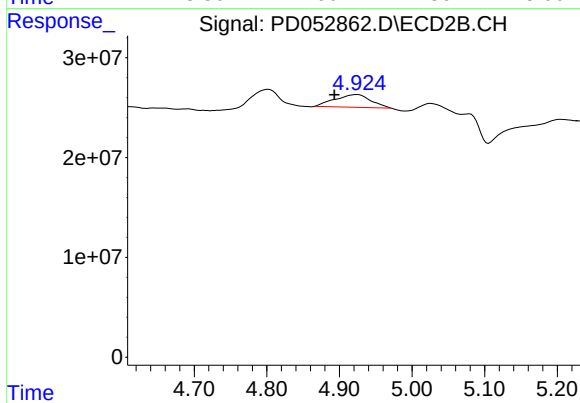

#6 beta-BHC


R.T.: 4.925 min
Delta R.T.: 0.032 min
Response: 43605448
Conc: 2.23 ng/ml

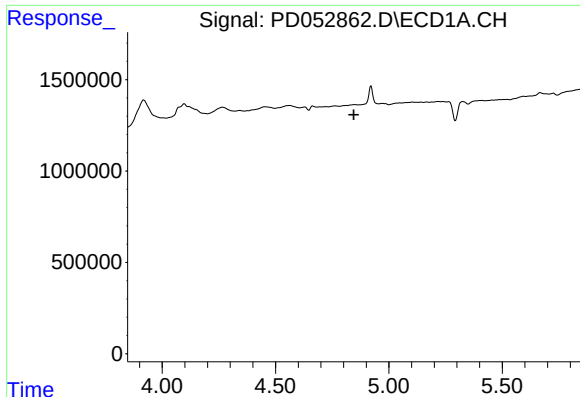

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

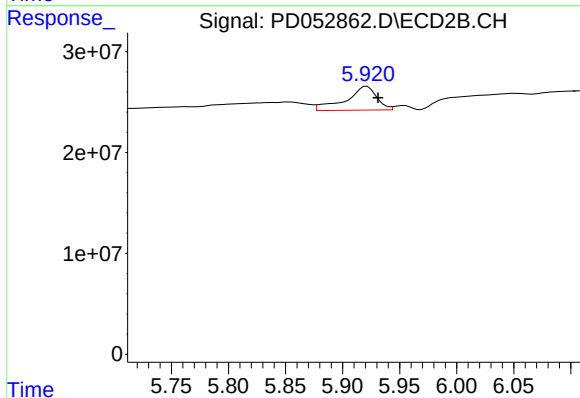


#8 Heptachlor epoxide

R.T.: 5.921 min
Delta R.T.: -0.010 min
Response: 44430711
Conc: 1.25 ng/ml

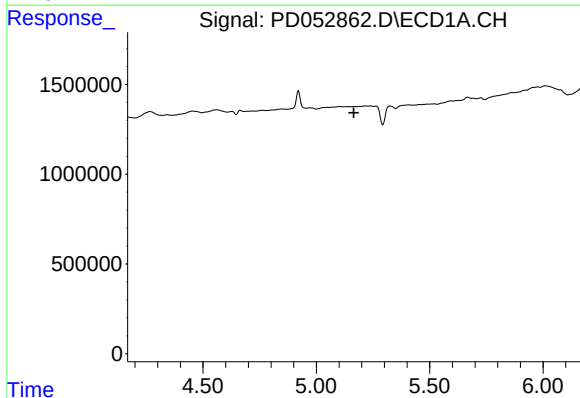


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

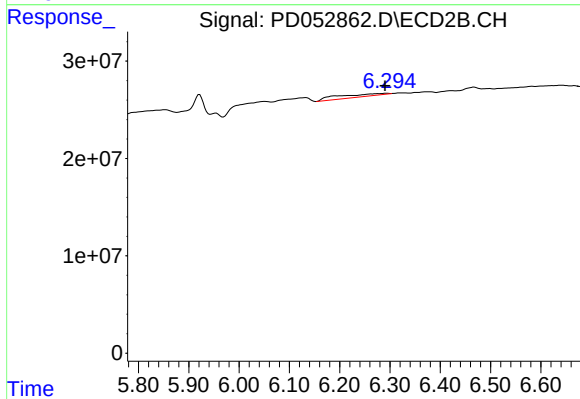

#9 Endosulfan I


R.T.: 6.294 min
Delta R.T.: 0.004 min
Response: 18594643
Conc: 0.57 ng/ml

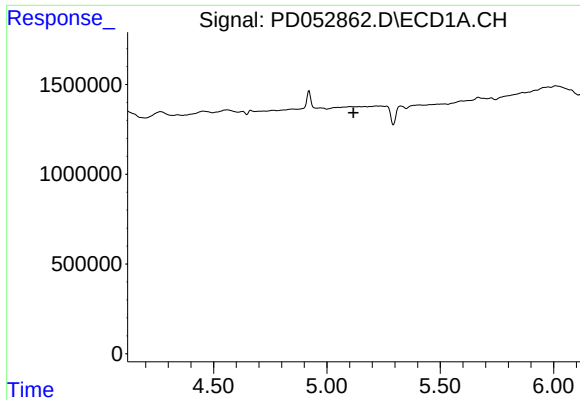

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

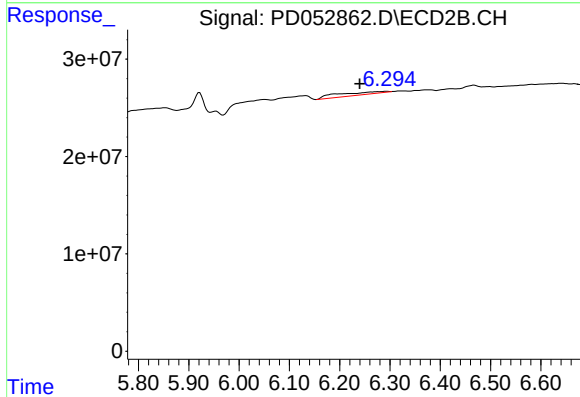


#11 cis-Chlordane

R.T.: 6.294 min
Delta R.T.: 0.054 min
Response: 18594643
Conc: 0.54 ng/ml

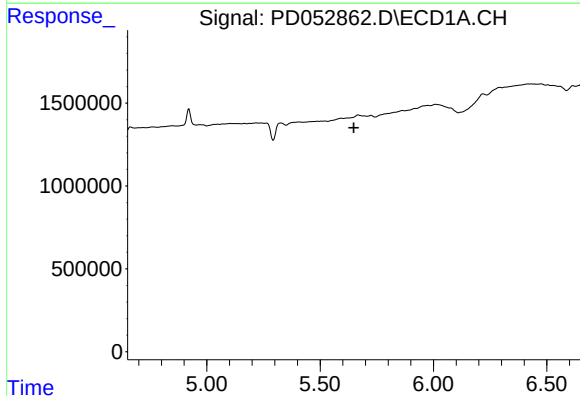


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.648 min
Response: 0
Conc: N.D.

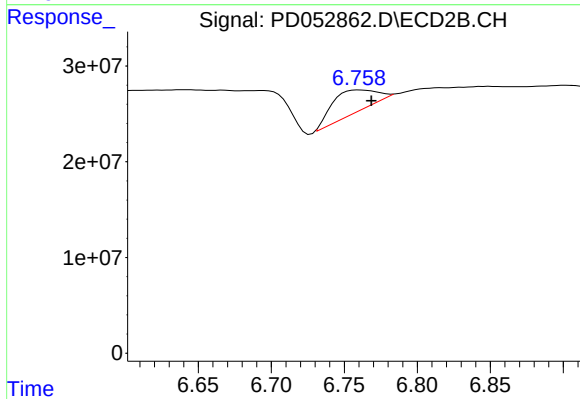

#14 Endrin


R.T.: 6.761 min
Delta R.T.: -0.008 min
Response: 47146983
Conc: 1.87 ng/ml

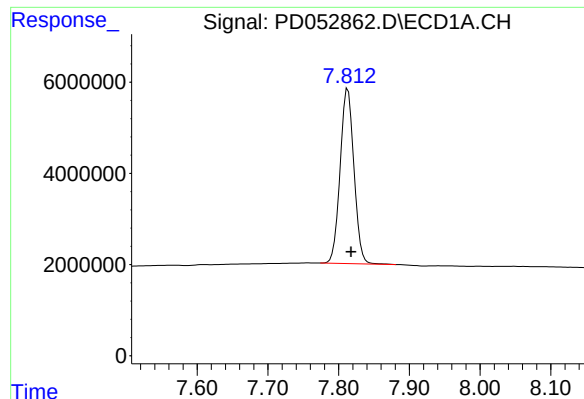

#27 Decachlorobiphenyl

R.T.: 7.813 min
Delta R.T.: -0.004 min
Response: 52031553
Conc: 36.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

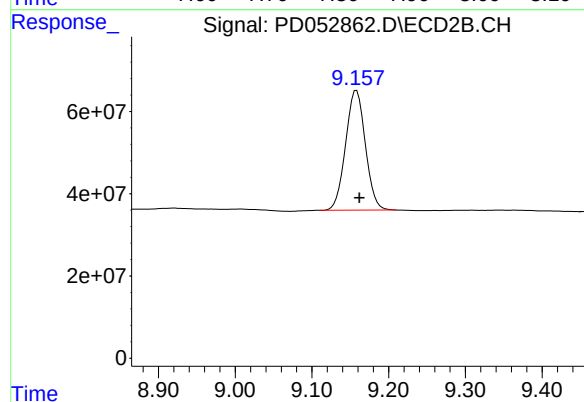

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: -0.004 min
Response: 523767506
Conc: 36.33 ng/ml