

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
 Data File : PD052877.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 20:52
 Operator : AJ\SJ
 Sample : K2304-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF891

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:07:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.219	4.041	29131115	572.0E6	19.133	18.076
27) SA Decachlor...	7.813	9.157	45317980	473.9E6	32.141	32.865
Target Compounds						
2) A alpha-BHC	0.000	4.404f	0	66127215	N.D.	1.390
6) B beta-BHC	0.000	4.934f	0	13680043	N.D.	0.700
7) B delta-BHC	0.000	5.079f	0	61011094	N.D.	1.692
8) B Heptachlo...	0.000	5.910	0	60977036	N.D.	1.721
10) B trans-Chl...	0.000	6.111f	0	4872206	N.D.	0.136


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
Data File : PD052877.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 20:52
Operator : AJ\SJ
Sample : K2304-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:07:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

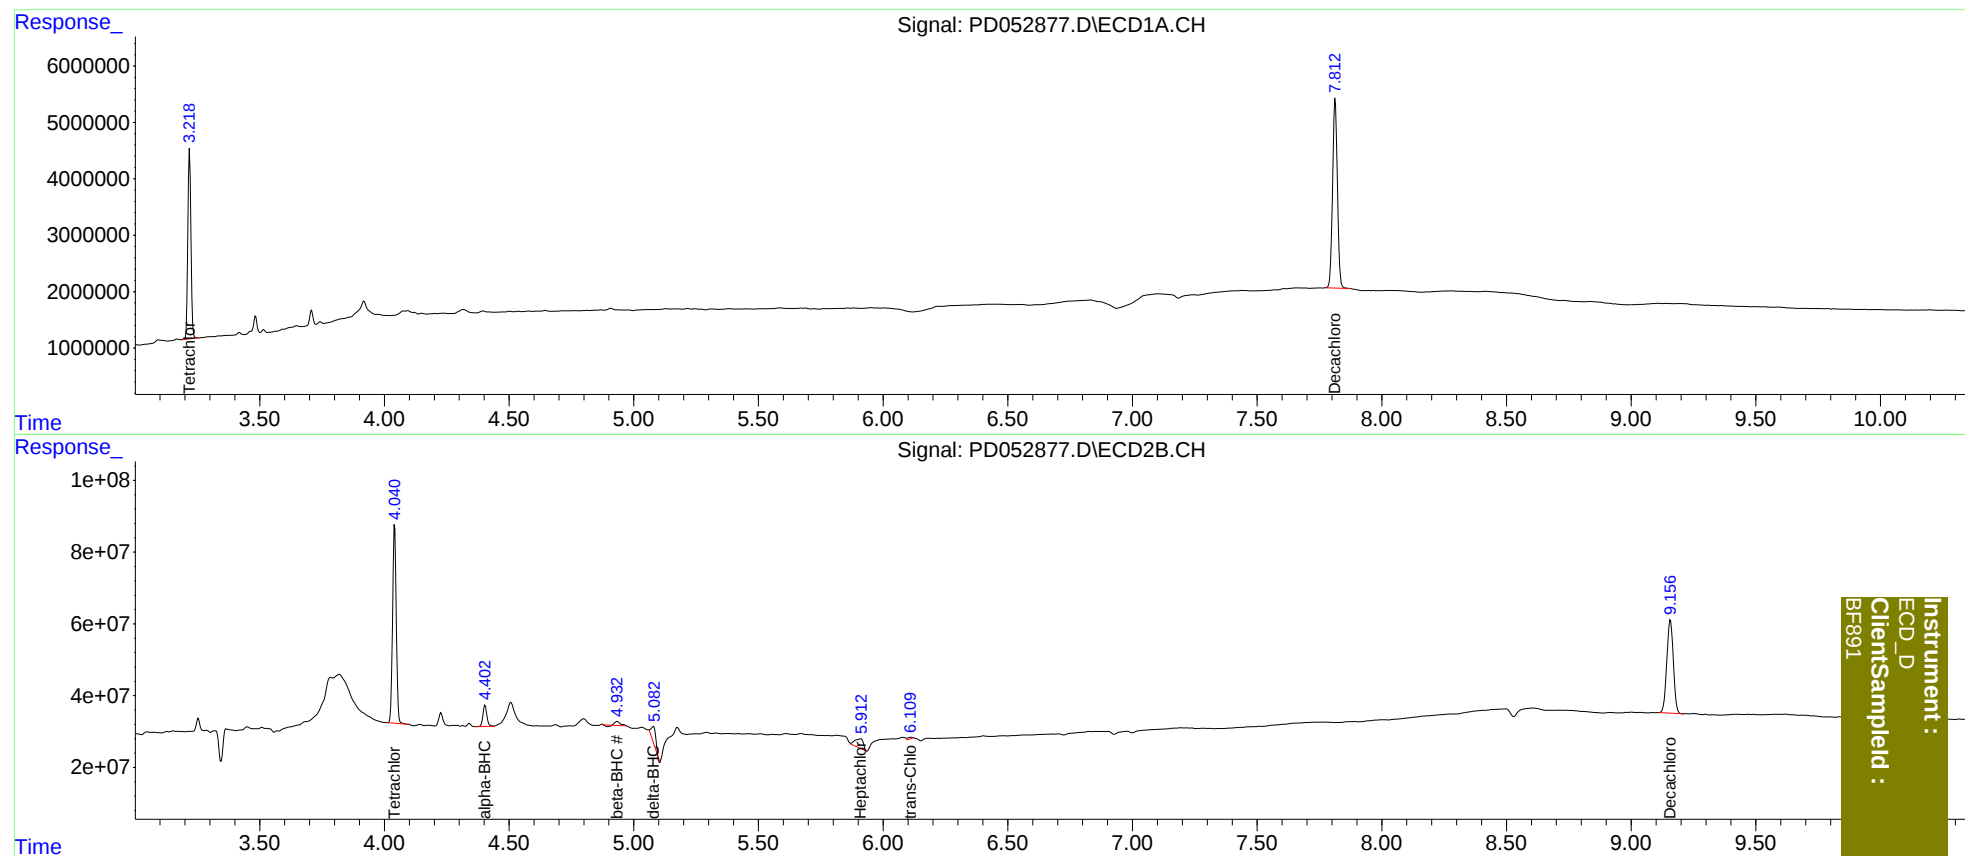


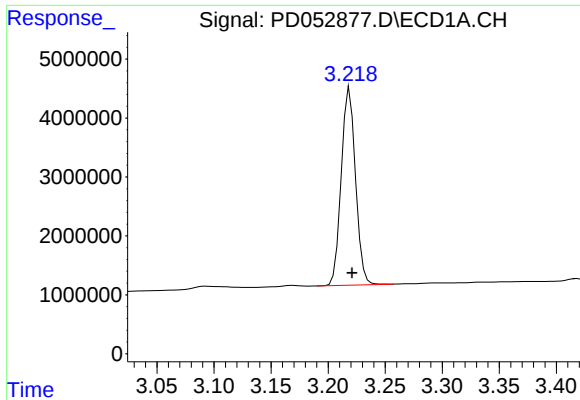

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: -0.002 min
Response: 29131115
Conc: 19.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF891

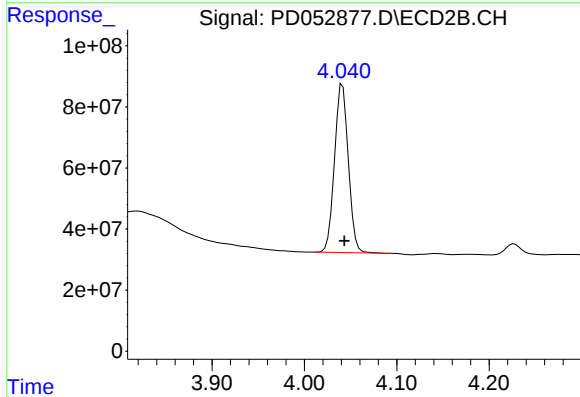


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 572013537
Conc: 18.08 ng/ml

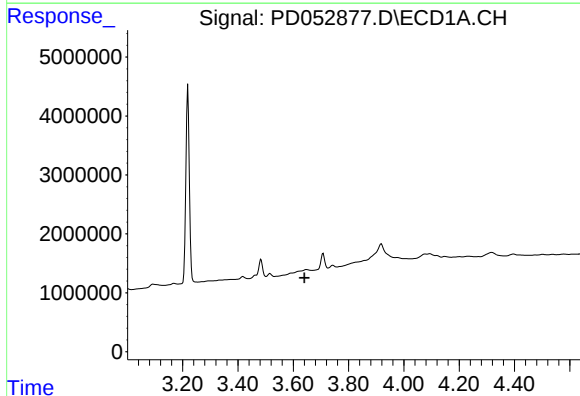


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.640 min
Response: 0
Conc: N.D.

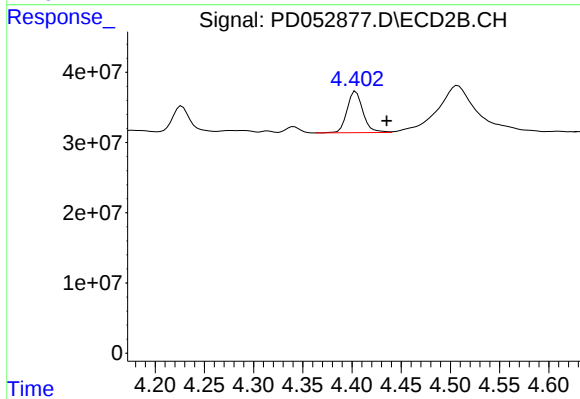

#2 alpha-BHC


R.T.: 4.404 min
Delta R.T.: -0.031 min
Response: 66127215
Conc: 1.39 ng/ml

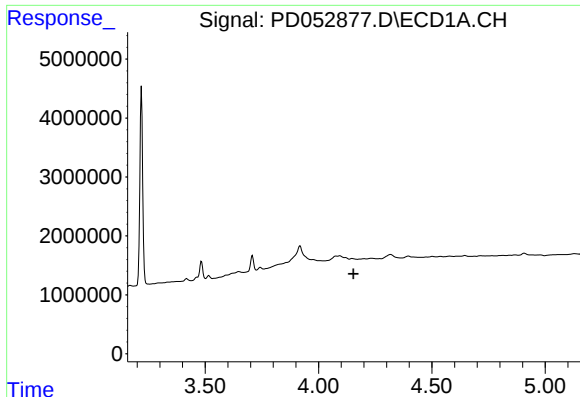

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF891

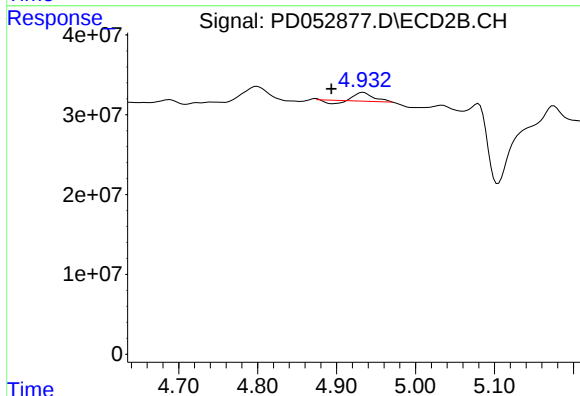


#6 beta-BHC

R.T.: 4.934 min
Delta R.T.: 0.040 min
Response: 13680043
Conc: 0.70 ng/ml

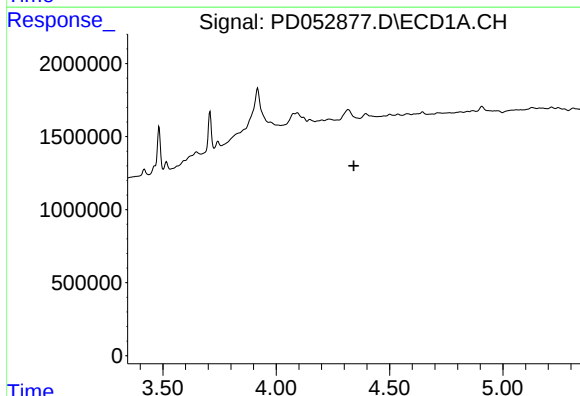


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.343 min
Response: 0
Conc: N.D.

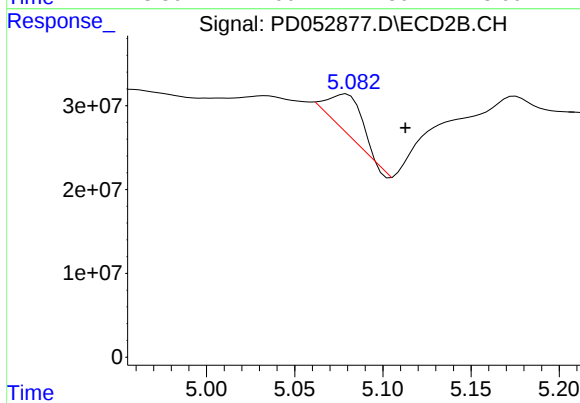

#7 delta-BHC


R.T.: 5.079 min
Delta R.T.: -0.034 min
Response: 61011094
Conc: 1.69 ng/ml

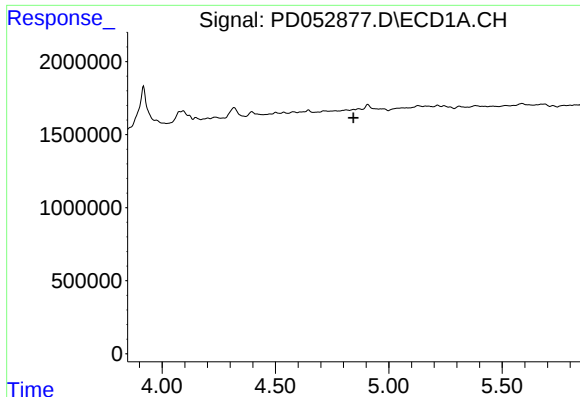

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF891

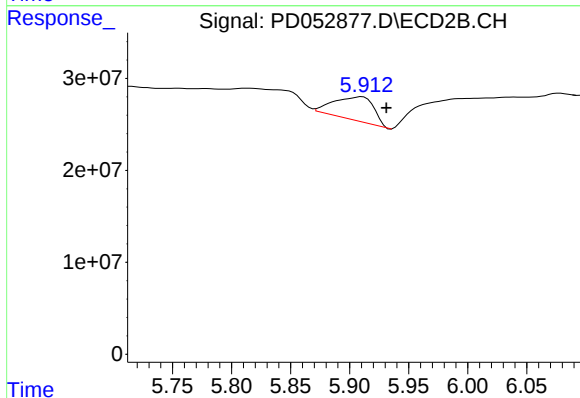


#8 Heptachlor epoxide

R.T.: 5.910 min
Delta R.T.: -0.021 min
Response: 60977036
Conc: 1.72 ng/ml

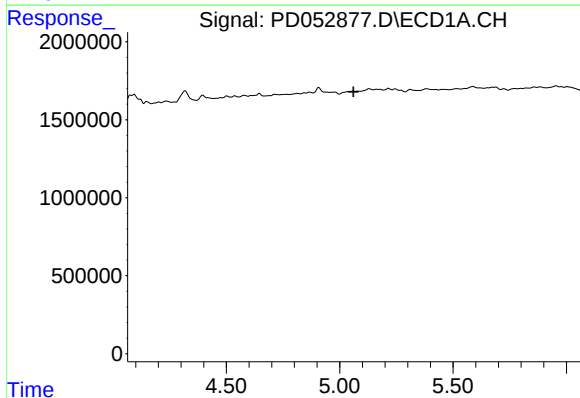


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.061 min
Response: 0
Conc: N.D.

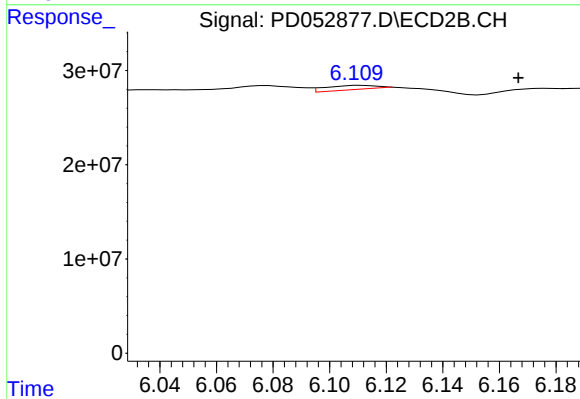

#10 trans-Chlordane


R.T.: 6.111 min
Delta R.T.: -0.055 min
Response: 4872206
Conc: 0.14 ng/ml

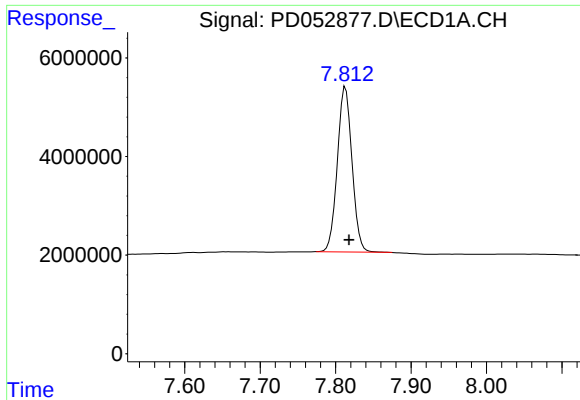

#27 Decachlorobiphenyl

R.T.: 7.813 min
Delta R.T.: -0.004 min
Response: 45317980
Conc: 32.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF891

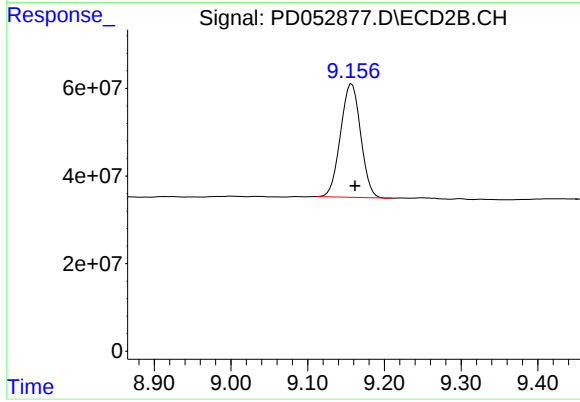

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: -0.004 min
Response: 473872195
Conc: 32.87 ng/ml