

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
 Data File : PD052881.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 21:49
 Operator : AJ\SJ
 Sample : K2273-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFC53

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:07:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.041	18540940	397.5E6	12.178	12.560
27)	SA Decachlor...	7.812	9.160	29399687	309.6E6	20.851	21.469
Target Compounds							
6)	B beta-BHC	0.000	4.932f	0 28701927	N.D.	1.468	
7)	B delta-BHC	0.000	5.080f	0 55061914	N.D.	1.527	
8)	B Heptachlo...	0.000	5.914	0 39136186	N.D.	1.105	
9)	A Endosulfan I	0.000	6.263	0 11020888	N.D.	0.336	
10)	B trans-Chl...	0.000	6.198	0 26297743	N.D.	0.732	
11)	B cis-Chlor...	0.000	6.263	0 11020888	N.D.	0.320	
15)	B Endosulfa...	0.000	6.974	0 37568978	N.D.	1.427	
16)	A 4,4'-DDD	0.000	6.867	0 91370892	N.D.	3.661	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
Data File : PD052881.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 21:49
Operator : AJ\SJ
Sample : K2273-05
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:07:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

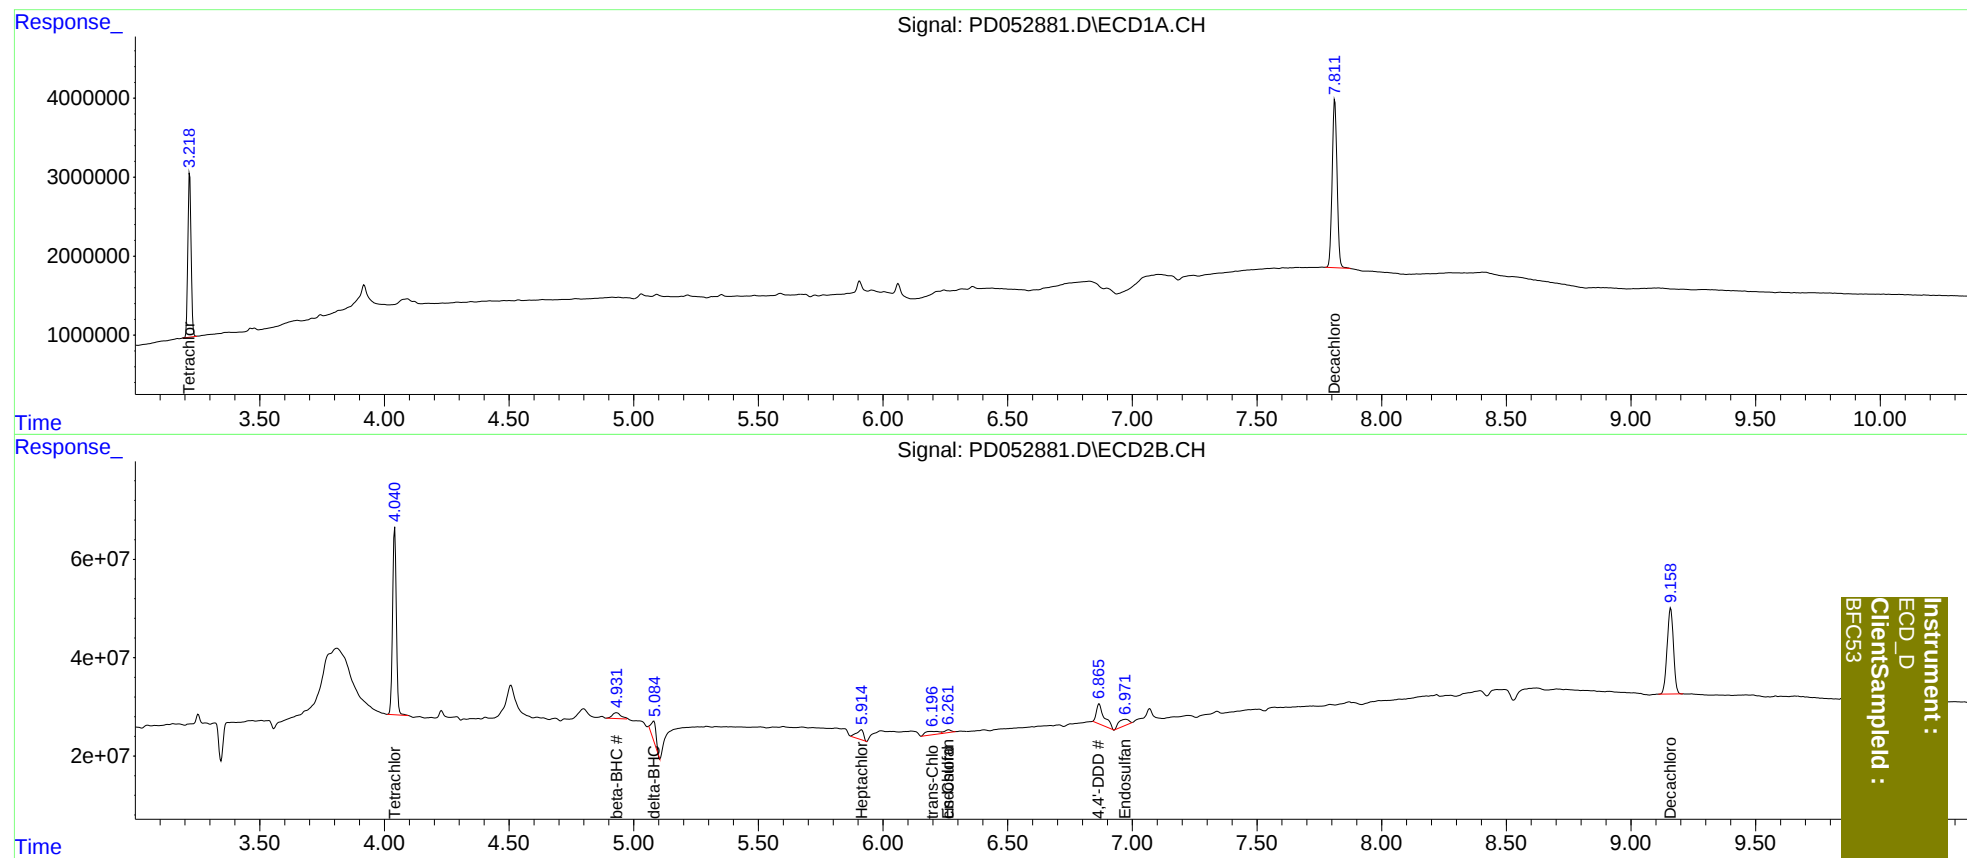


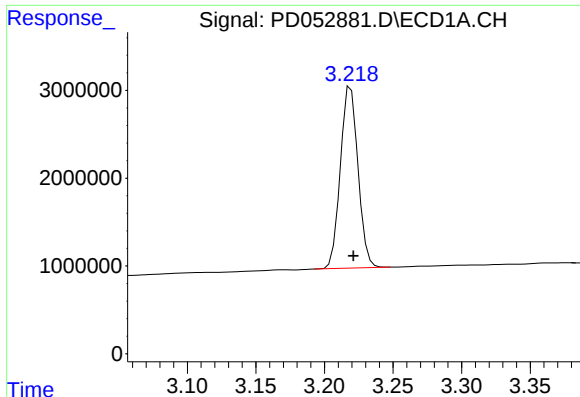

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: -0.002 min
Response: 18540940
Conc: 12.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
BFC53

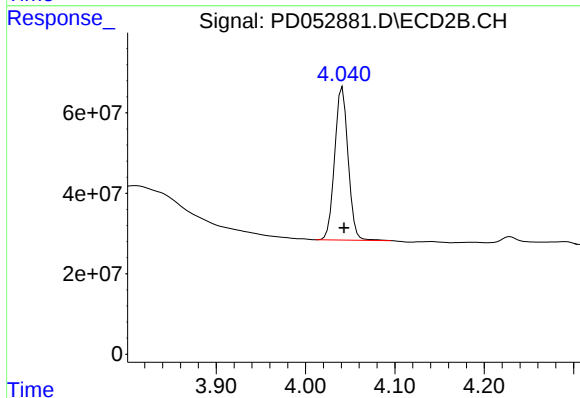


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 397464969
Conc: 12.56 ng/ml

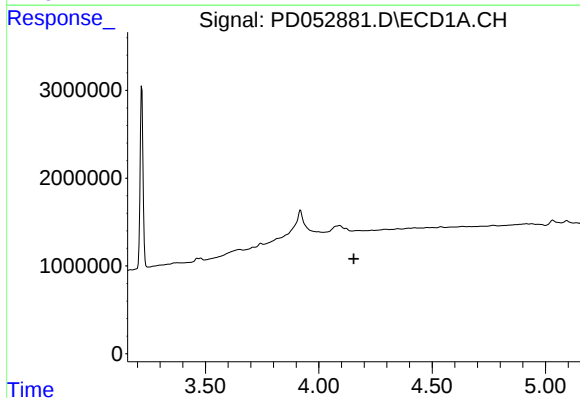


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

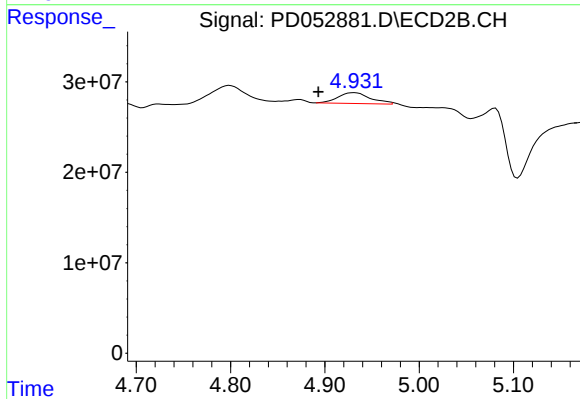

#6 beta-BHC


R.T.: 4.932 min
Delta R.T.: 0.038 min
Response: 28701927
Conc: 1.47 ng/ml

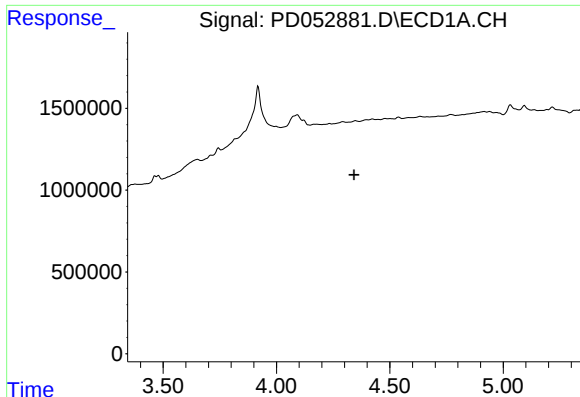

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC53

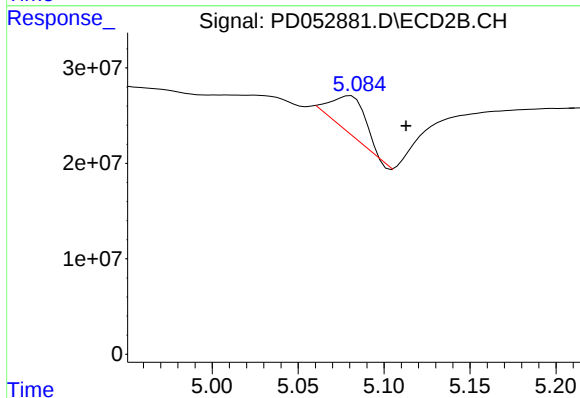


#7 delta-BHC

R.T.: 5.080 min
Delta R.T.: -0.032 min
Response: 55061914
Conc: 1.53 ng/ml

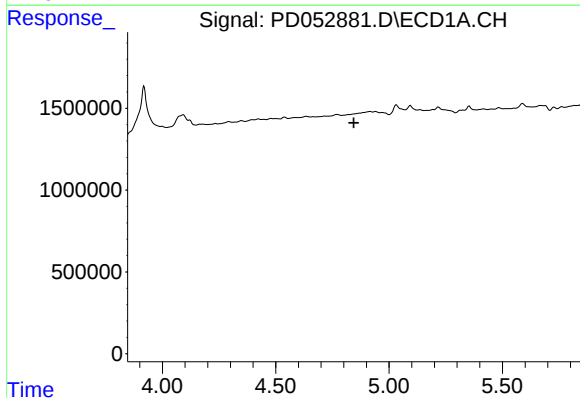


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.845 min
Response: 0
Conc: N.D.

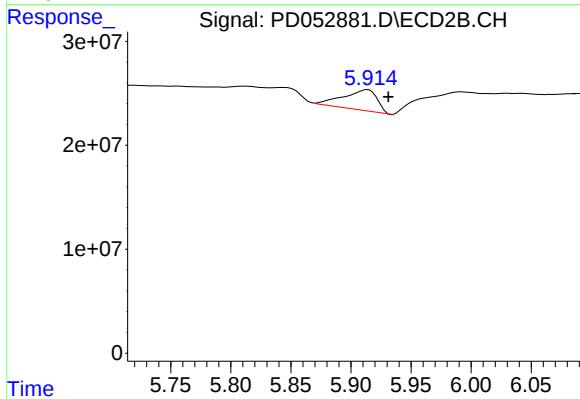

#8 Heptachlor epoxide


R.T.: 5.914 min
Delta R.T.: -0.017 min
Response: 39136186
Conc: 1.10 ng/ml

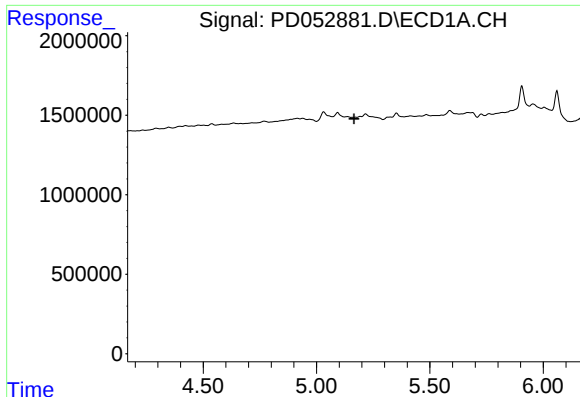

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC53

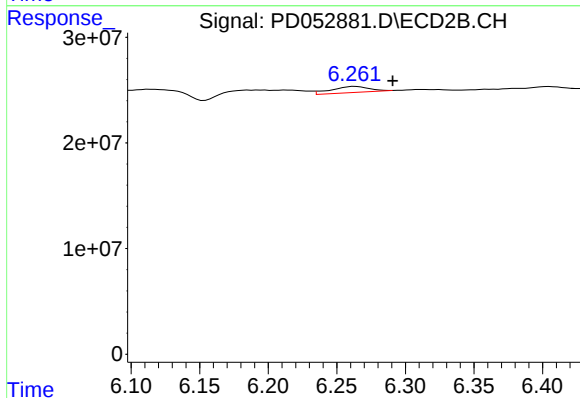


#9 Endosulfan I

R.T.: 6.263 min
Delta R.T.: -0.027 min
Response: 11020888
Conc: 0.34 ng/ml

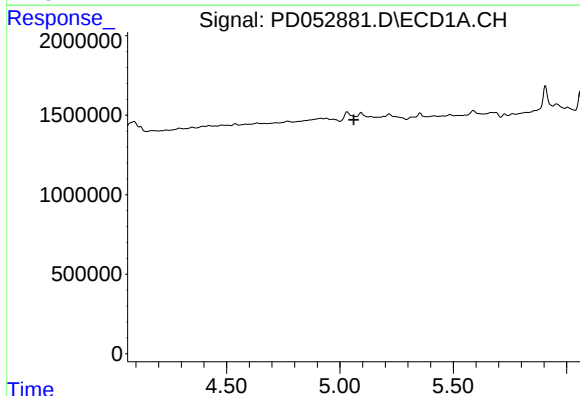


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.061 min
Response: 0
Conc: N.D.

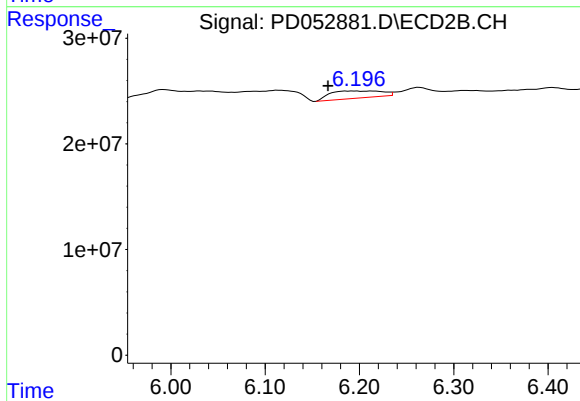

#10 trans-Chlordane


R.T.: 6.198 min
Delta R.T.: 0.031 min
Response: 26297743
Conc: 0.73 ng/ml

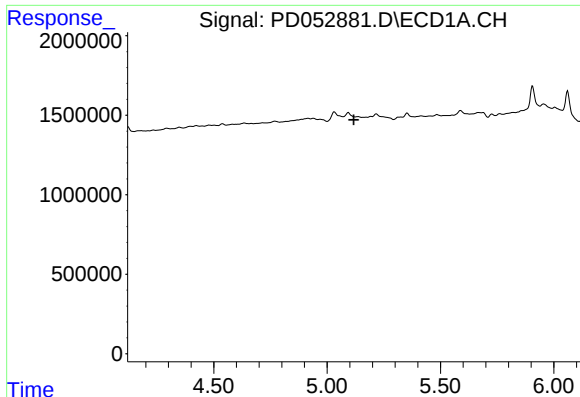

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC53

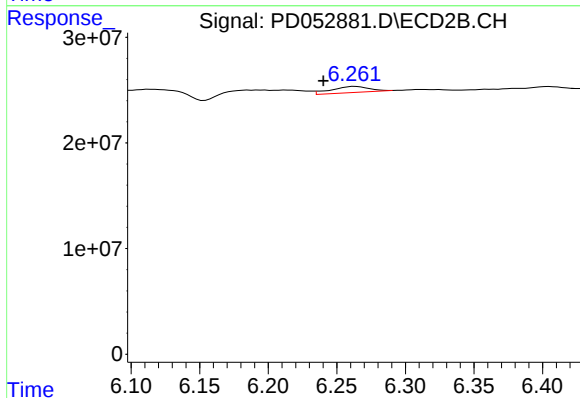


#11 cis-Chlordane

R.T.: 6.263 min
Delta R.T.: 0.023 min
Response: 11020888
Conc: 0.32 ng/ml

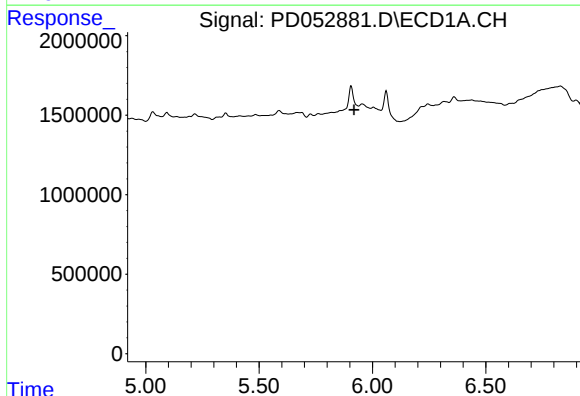


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

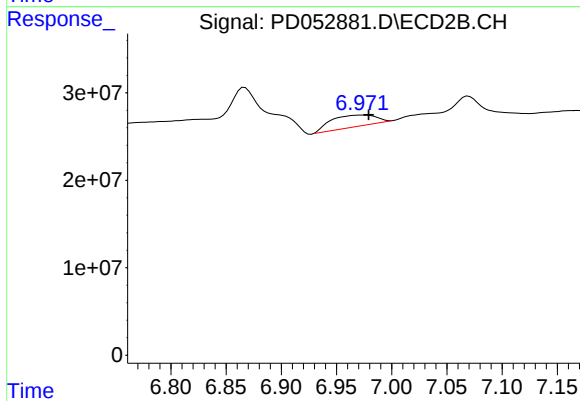

#15 Endosulfan II


R.T.: 6.974 min
Delta R.T.: -0.005 min
Response: 37568978
Conc: 1.43 ng/ml

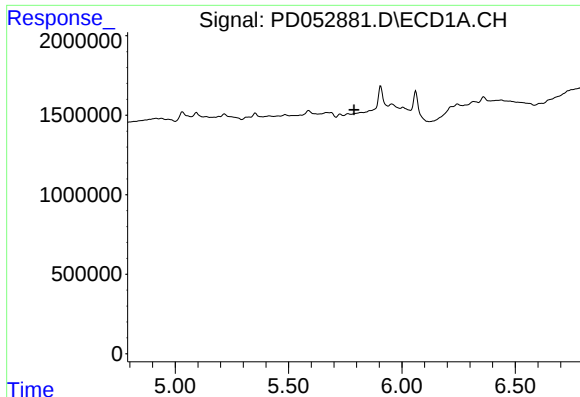

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.789 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BFC53

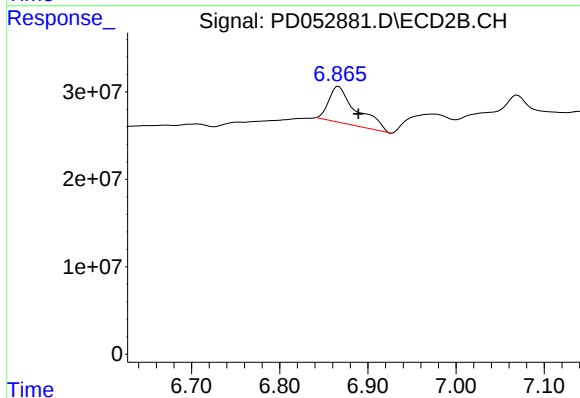


#16 4,4'-DDD

R.T.: 6.867 min
Delta R.T.: -0.022 min
Response: 91370892
Conc: 3.66 ng/ml

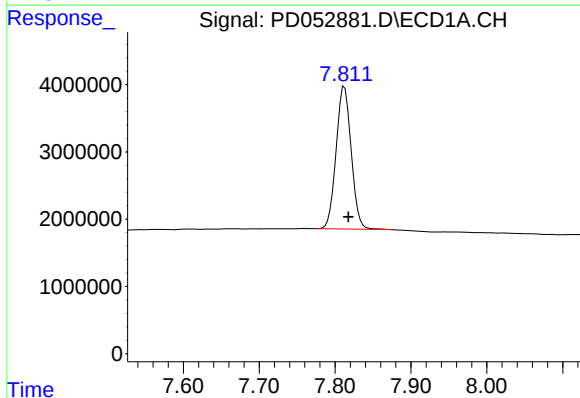

#27 Decachlorobiphenyl

R.T.: 7.812 min
Delta R.T.: -0.005 min
Response: 29399687
Conc: 20.85 ng/ml

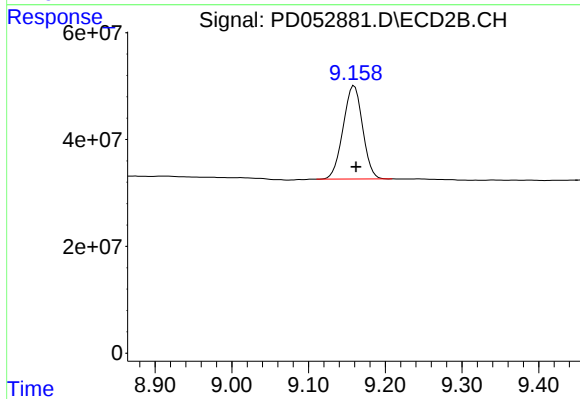

#27 Decachlorobiphenyl

R.T.: 9.160 min
Delta R.T.: -0.002 min
Response: 309551218
Conc: 21.47 ng/ml