

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
 Data File : PD052885.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 22:46
 Operator : AJ\SJ
 Sample : K2303-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:08:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.041	16671367	350.1E6	10.950	11.064
27)	SA Decachlor...	7.812	9.157	28576782	306.7E6	20.268	21.268
Target Compounds							
6)	B beta-BHC	0.000	4.934f	0	21792925	N.D.	1.114
20)	A Methoxychlor	6.561	7.646	3892318	41824773	3.932	4.405


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
Data File : PD052885.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 22:46
Operator : AJ\SJ
Sample : K2303-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:08:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

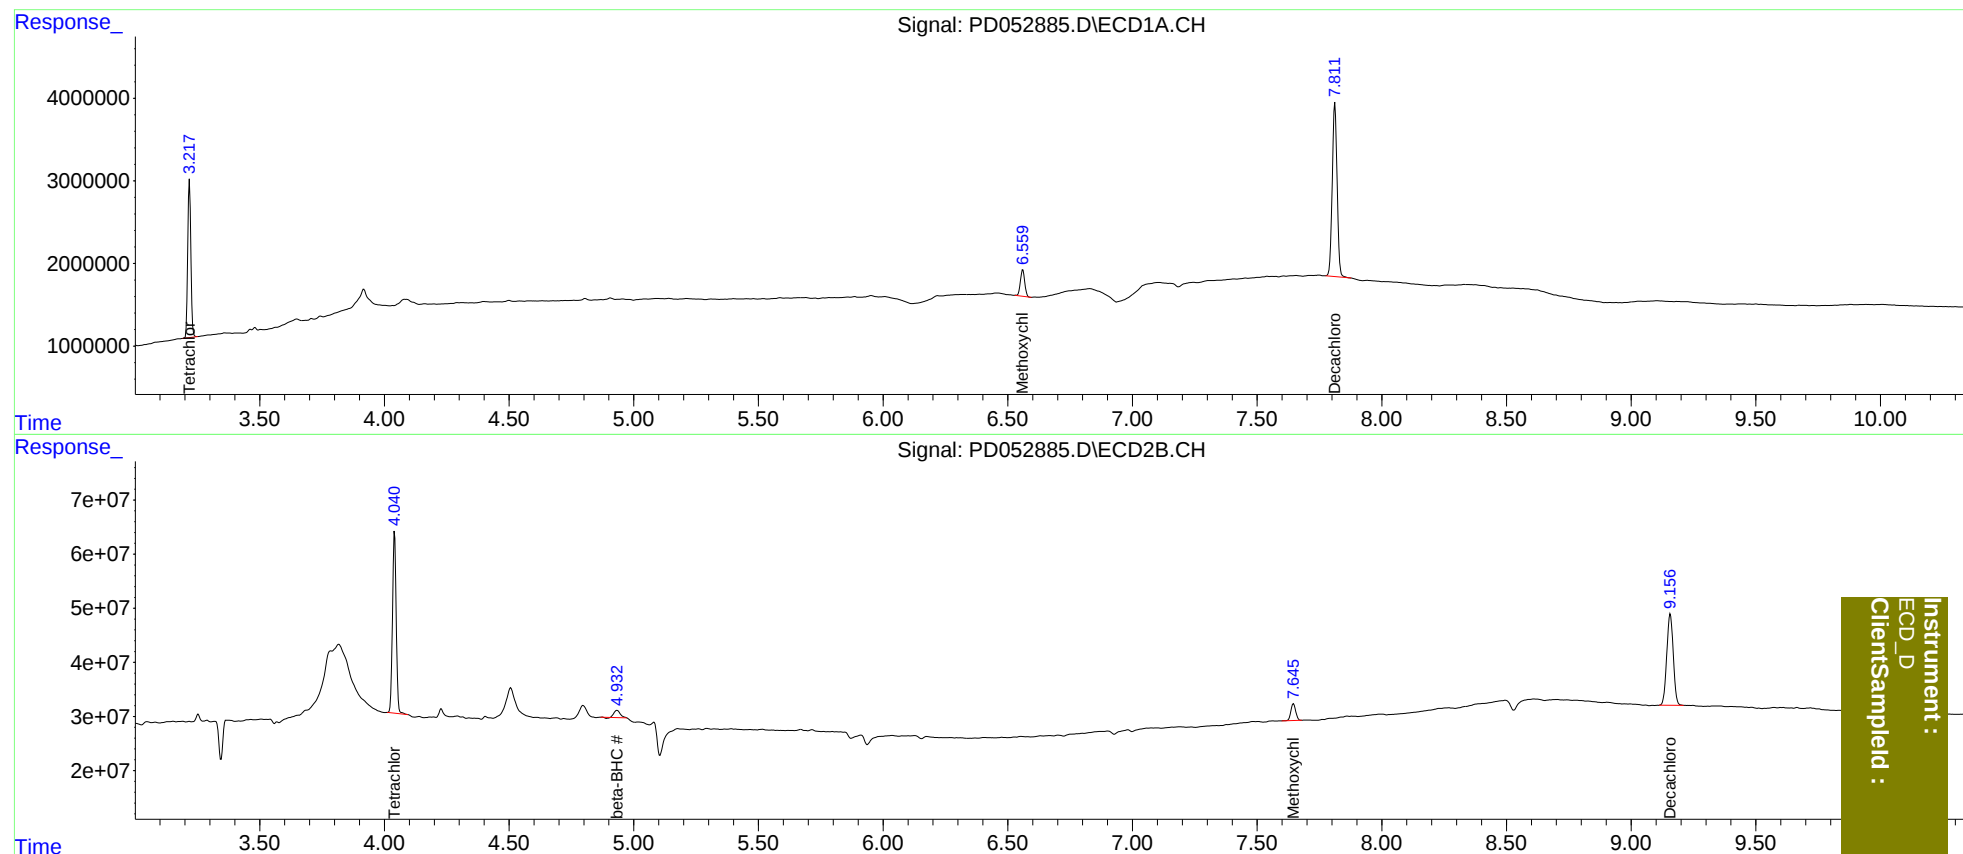


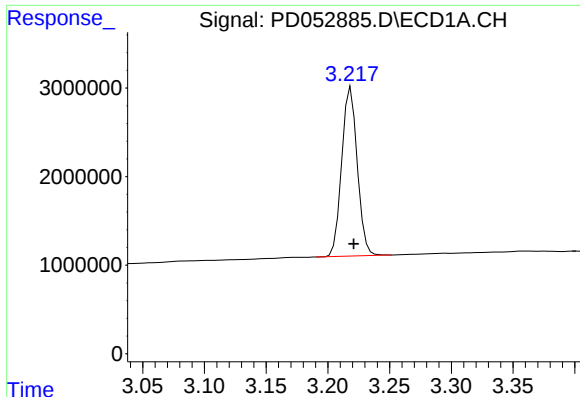

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: -0.002 min
Response: 16671367
Conc: 10.95 ng/ml

Instrument :
ECD_D
ClientSampleId :

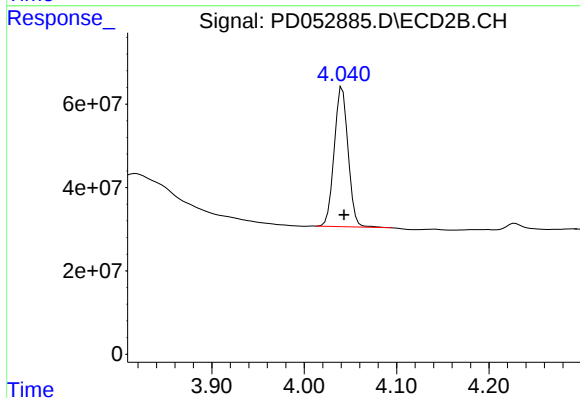


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 350130157
Conc: 11.06 ng/ml

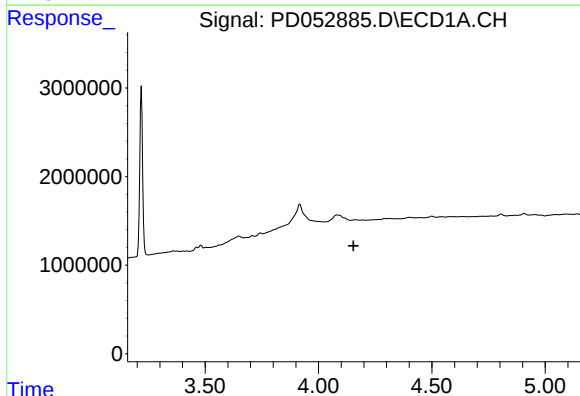


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

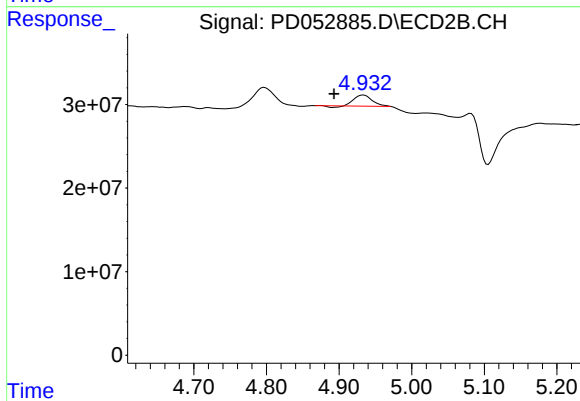

#6 beta-BHC


R.T.: 4.934 min
Delta R.T.: 0.040 min
Response: 21792925
Conc: 1.11 ng/ml

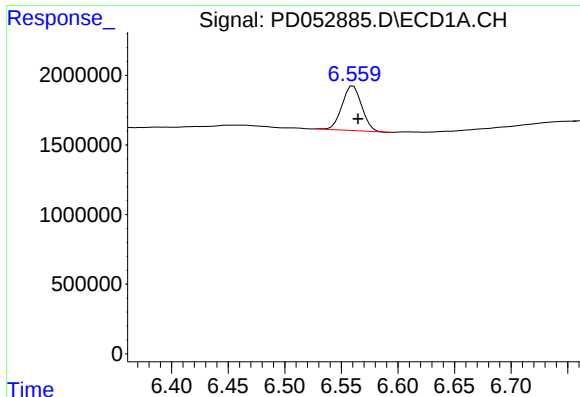

#20 Methoxychlor


R.T.: 6.561 min
Delta R.T.: -0.004 min
Response: 3892318
Conc: 3.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

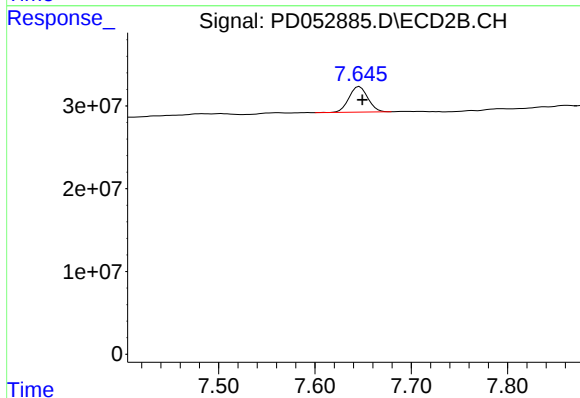


#20 Methoxychlor

R.T.: 7.646 min
Delta R.T.: -0.003 min
Response: 41824773
Conc: 4.40 ng/ml

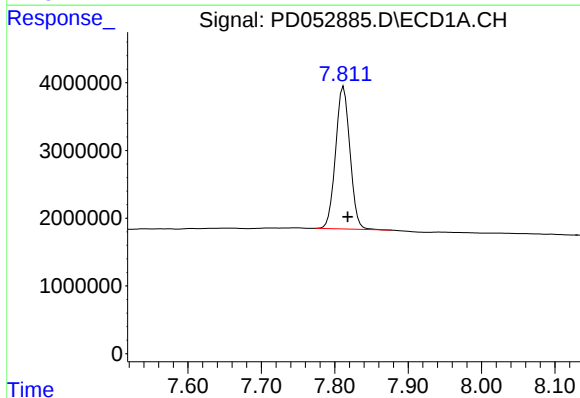

#27 Decachlorobiphenyl

R.T.: 7.812 min
Delta R.T.: -0.005 min
Response: 28576782
Conc: 20.27 ng/ml

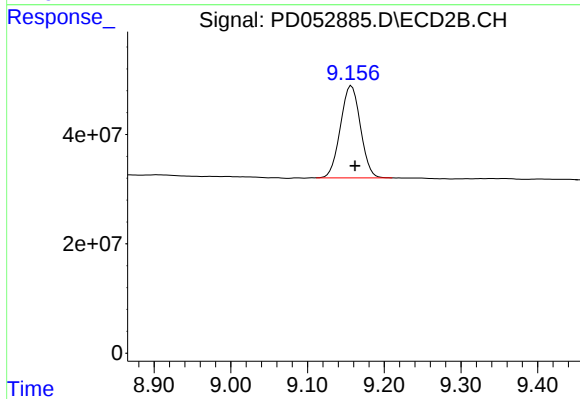

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: -0.005 min
Response: 306659196
Conc: 21.27 ng/ml