

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
 Data File : PD052890.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 23:57
 Operator : AJ\SJ
 Sample : K2303-14
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF882

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:09:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.041	13881488	298.1E6	9.117	9.420
27)	SA Decachlor...	7.813	9.158	23536507	258.2E6	16.693	17.909
Target Compounds							
2)	A alpha-BHC	0.000	4.405f	0 12515137	N.D.	0.263	
4)	MA Heptachlor	0.000	5.255	0 17290460	N.D.	0.396	
6)	B beta-BHC	0.000	4.935f	0 19853868	N.D.	1.015	
8)	B Heptachlo...	0.000	5.914	0 58186168	N.D.	1.643	
9)	A Endosulfan I	5.112f	6.238f	10116354 93107782	4.947	2.843	#
10)	B trans-Chl...	5.059	6.163	3936475 70778699	1.789	1.971	
11)	B cis-Chlor...	5.112	6.238	10116354 93107782	4.692	2.707	#
15)	B Endosulfa...	0.000	6.984	0 23226902	N.D.	0.882	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041119\
Data File : PD052890.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 23:57
Operator : AJ\SJ
Sample : K2303-14
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:09:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

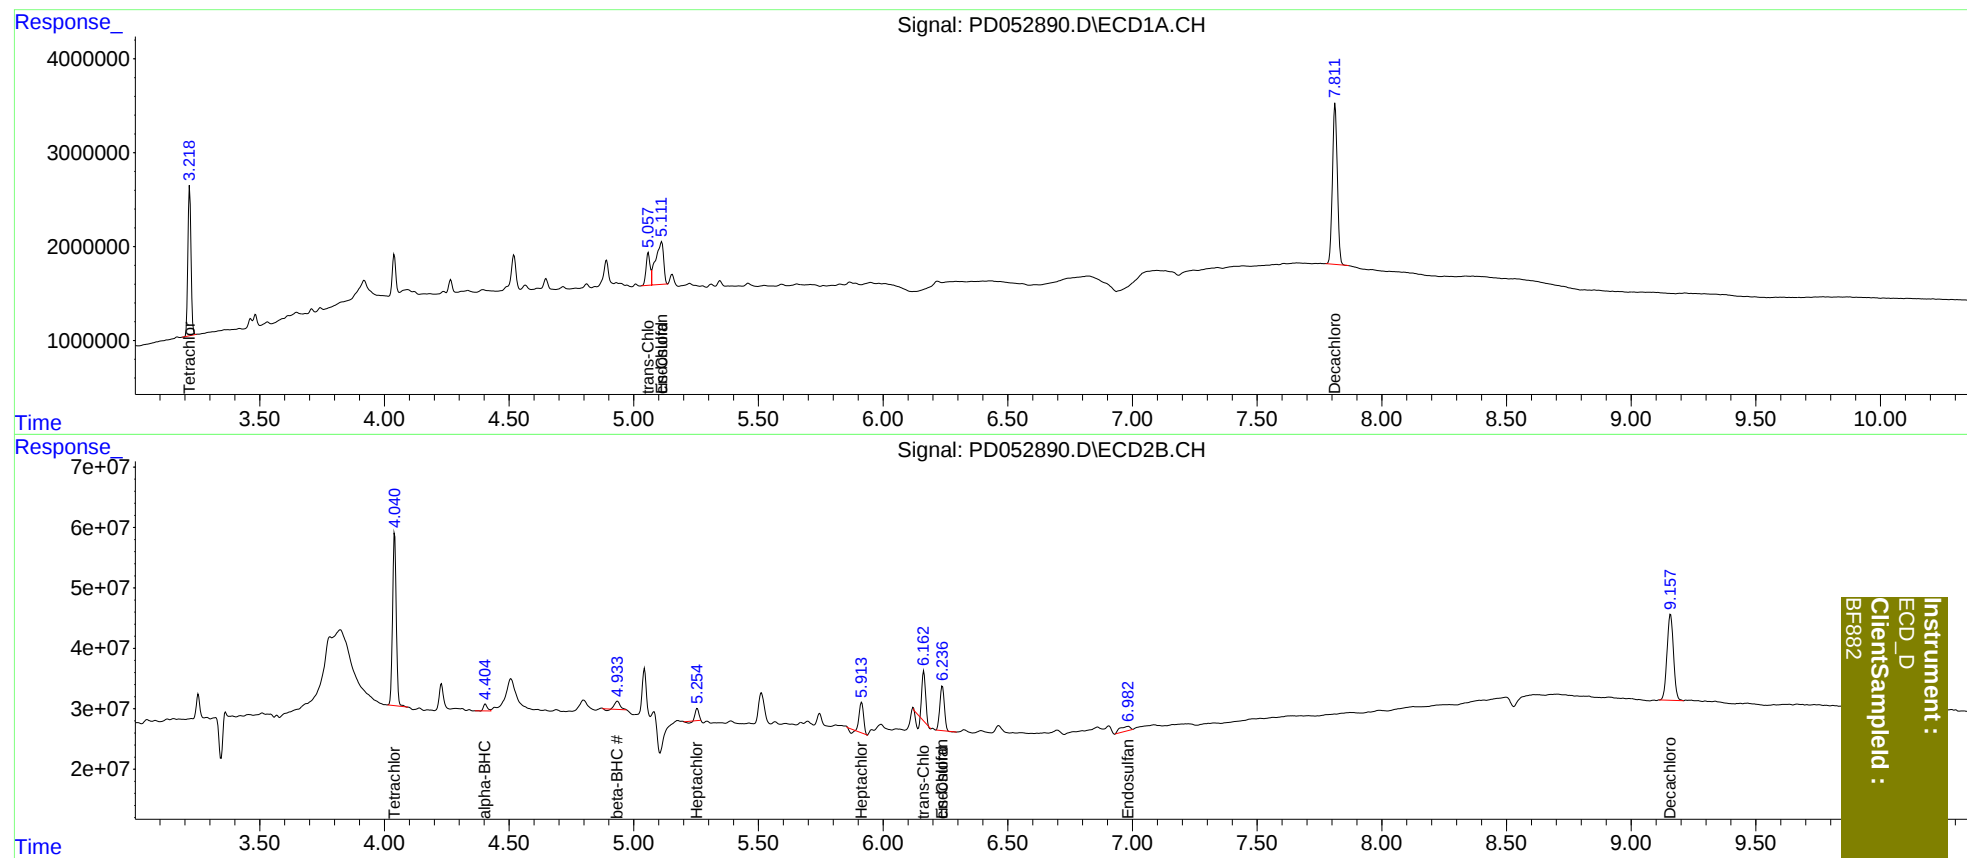


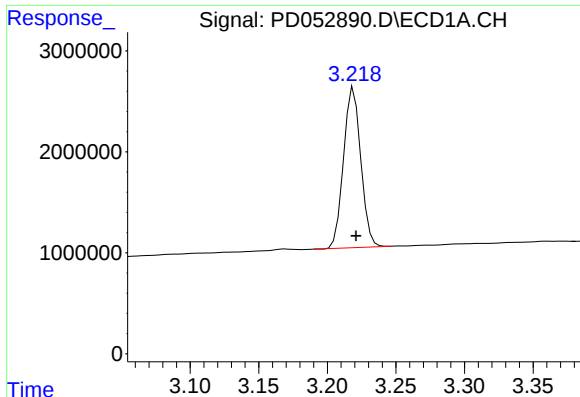

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: -0.002 min
Response: 13881488
Conc: 9.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF882

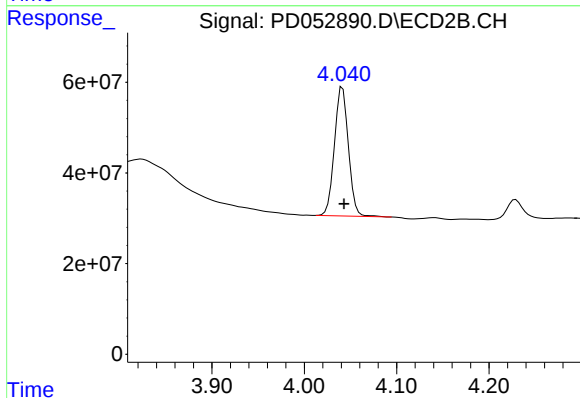


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 298097862
Conc: 9.42 ng/ml

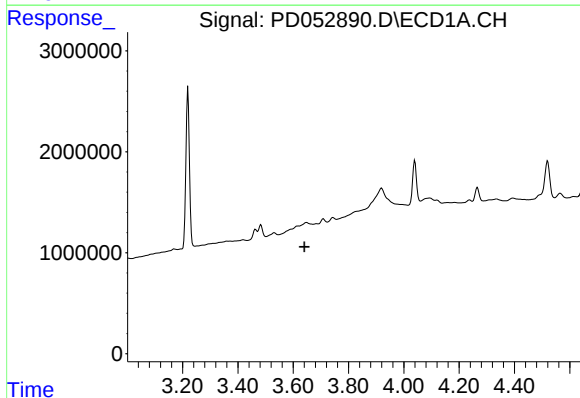


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.640 min
Response: 0
Conc: N.D.

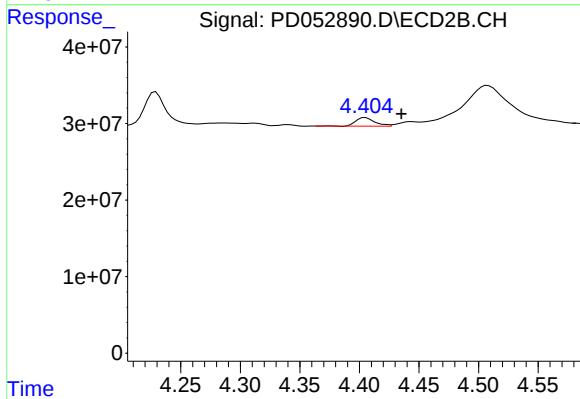

#2 alpha-BHC


R.T.: 4.405 min
Delta R.T.: -0.030 min
Response: 12515137
Conc: 0.26 ng/ml

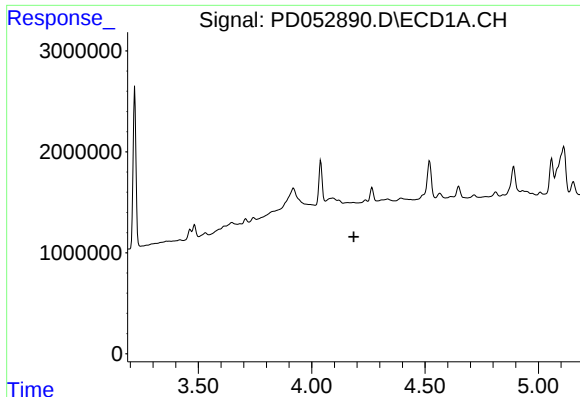

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.185 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF882

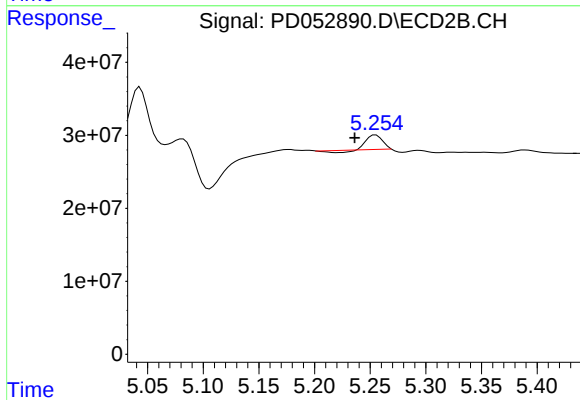


#4 Heptachlor

R.T.: 5.255 min
Delta R.T.: 0.019 min
Response: 17290460
Conc: 0.40 ng/ml

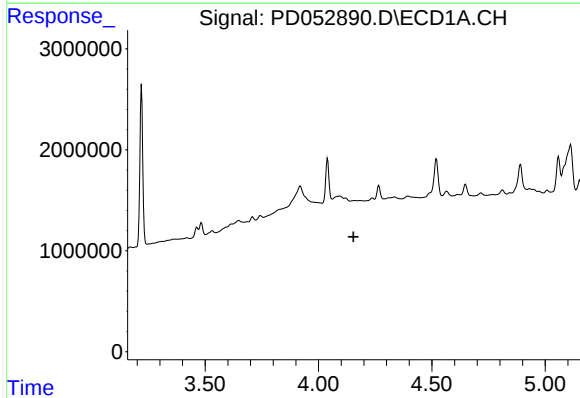


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.155 min
Response: 0
Conc: N.D.

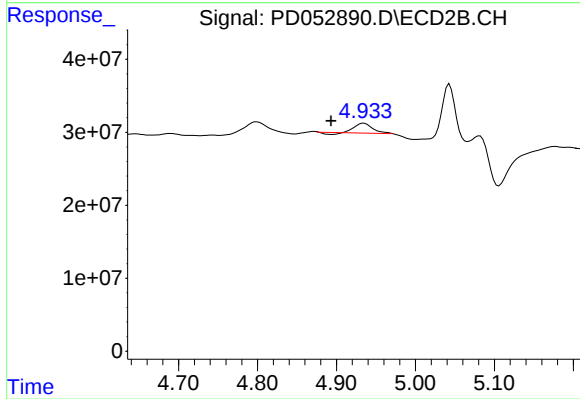

#6 beta-BHC


R.T.: 4.935 min
Delta R.T.: 0.041 min
Response: 19853868
Conc: 1.02 ng/ml

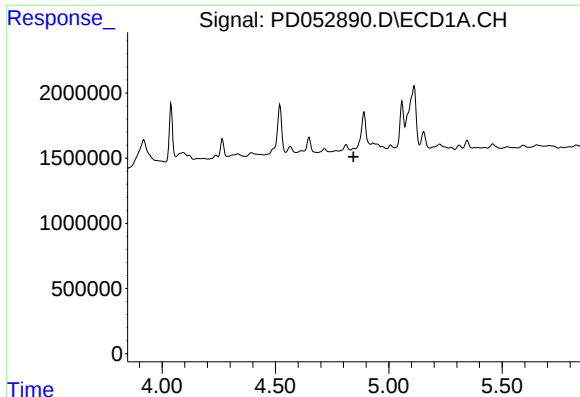

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.845 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF882

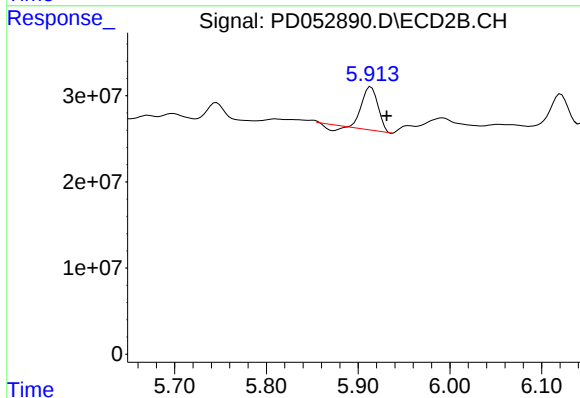


#8 Heptachlor epoxide

R.T.: 5.914 min
Delta R.T.: -0.017 min
Response: 58186168
Conc: 1.64 ng/ml

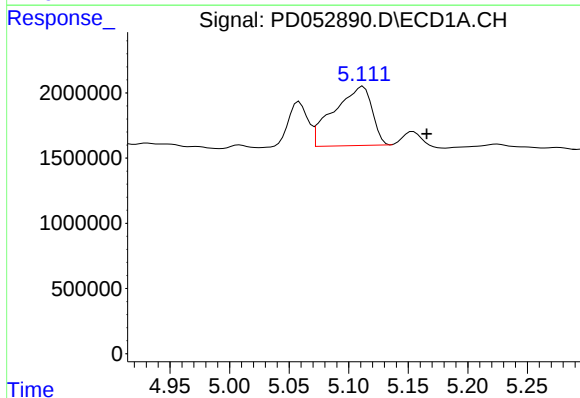


#9 Endosulfan I

R.T.: 5.112 min
Delta R.T.: -0.053 min
Response: 10116354
Conc: 4.95 ng/ml

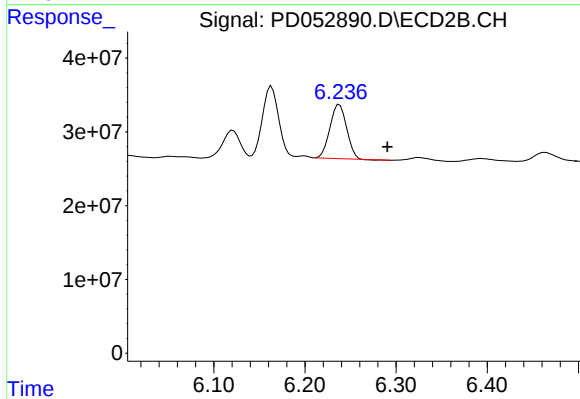

#9 Endosulfan I


R.T.: 6.238 min
Delta R.T.: -0.053 min
Response: 93107782
Conc: 2.84 ng/ml

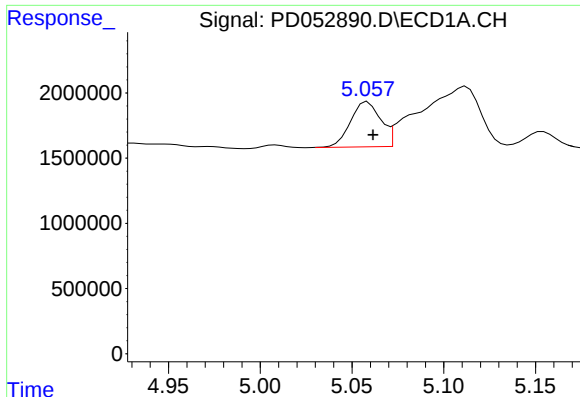

#10 trans-Chlordane


R.T.: 5.059 min
Delta R.T.: -0.003 min
Response: 3936475
Conc: 1.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF882

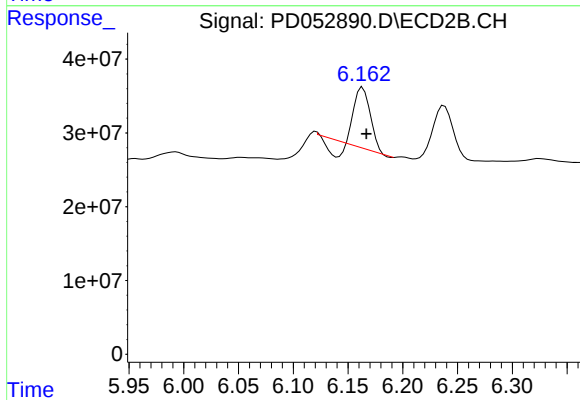


#10 trans-Chlordane

R.T.: 6.163 min
Delta R.T.: -0.003 min
Response: 70778699
Conc: 1.97 ng/ml

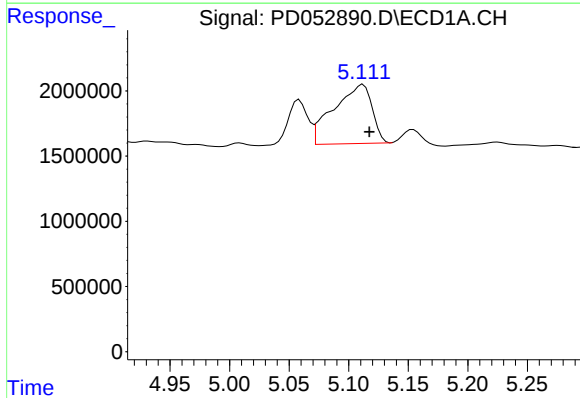


#11 cis-Chlordane

R.T.: 5.112 min
Delta R.T.: -0.005 min
Response: 10116354
Conc: 4.69 ng/ml

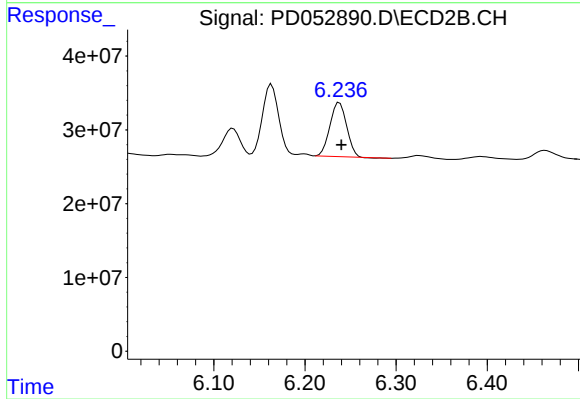

#11 cis-Chlordane


R.T.: 6.238 min
Delta R.T.: -0.002 min
Response: 93107782
Conc: 2.71 ng/ml

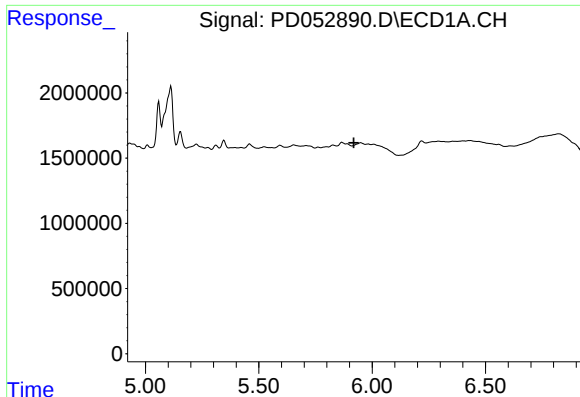

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.919 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF882

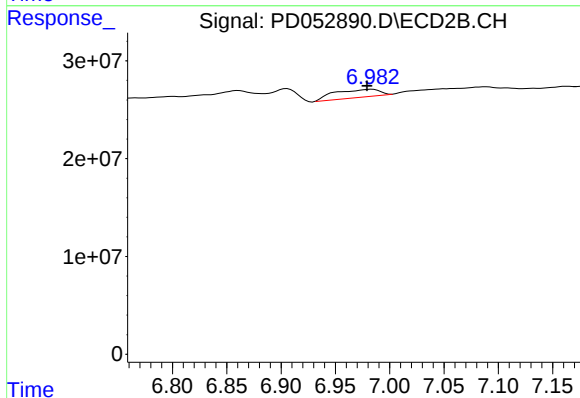


#15 Endosulfan II

R.T.: 6.984 min
Delta R.T.: 0.004 min
Response: 23226902
Conc: 0.88 ng/ml

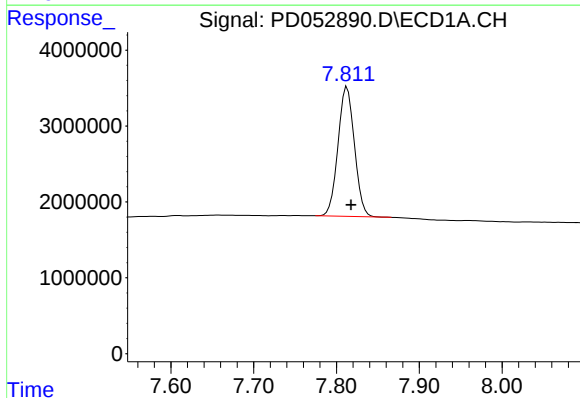

#27 Decachlorobiphenyl

R.T.: 7.813 min
Delta R.T.: -0.005 min
Response: 23536507
Conc: 16.69 ng/ml

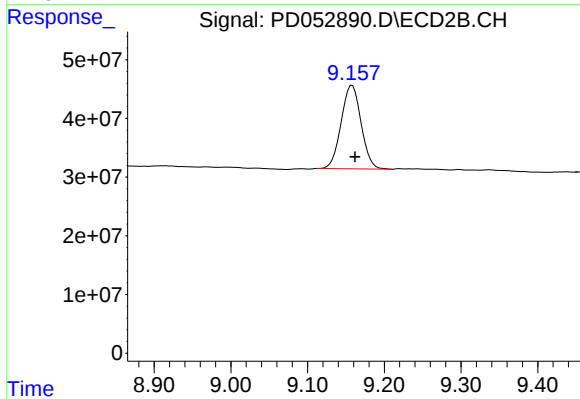

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: -0.004 min
Response: 258230098
Conc: 17.91 ng/ml