

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041123\
 Data File : PD074660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2023 13:45
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 22:18:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:23:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.556	2.771	48371309	25952251	20.737	21.325
28)	SA Decachlor...	9.105	7.926	65114261	29807994	24.346	24.295
Target Compounds							
4)	MA Heptachlor	4.927	0.000	853171	0	0.249	N.D. #
5)	MB Aldrin	0.000	4.237	0	1128387	N.D.	0.669 #
6)	B beta-BHC	0.000	3.910	0	275512	N.D.	0.365 #
7)	B delta-BHC	4.784	0.000	6884722	0	2.509	N.D. #
8)	B Heptachlo...	5.705	0.000	2035704	0	0.724	N.D. #
15)	B Endosulfa...	6.801f	0.000	216936	0	0.084	N.D. #
21)	B Endrin ke...	7.692f	0.000	2987364	0	1.073	N.D. #
22)	Mirex	8.173f	0.000	170983	0	0.081	N.D. #
24)	Chlordane-2	0.000	4.328f	0	397017	N.D.	6.812 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041123\
Data File : PD074660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2023 13:45
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 22:18:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:23:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

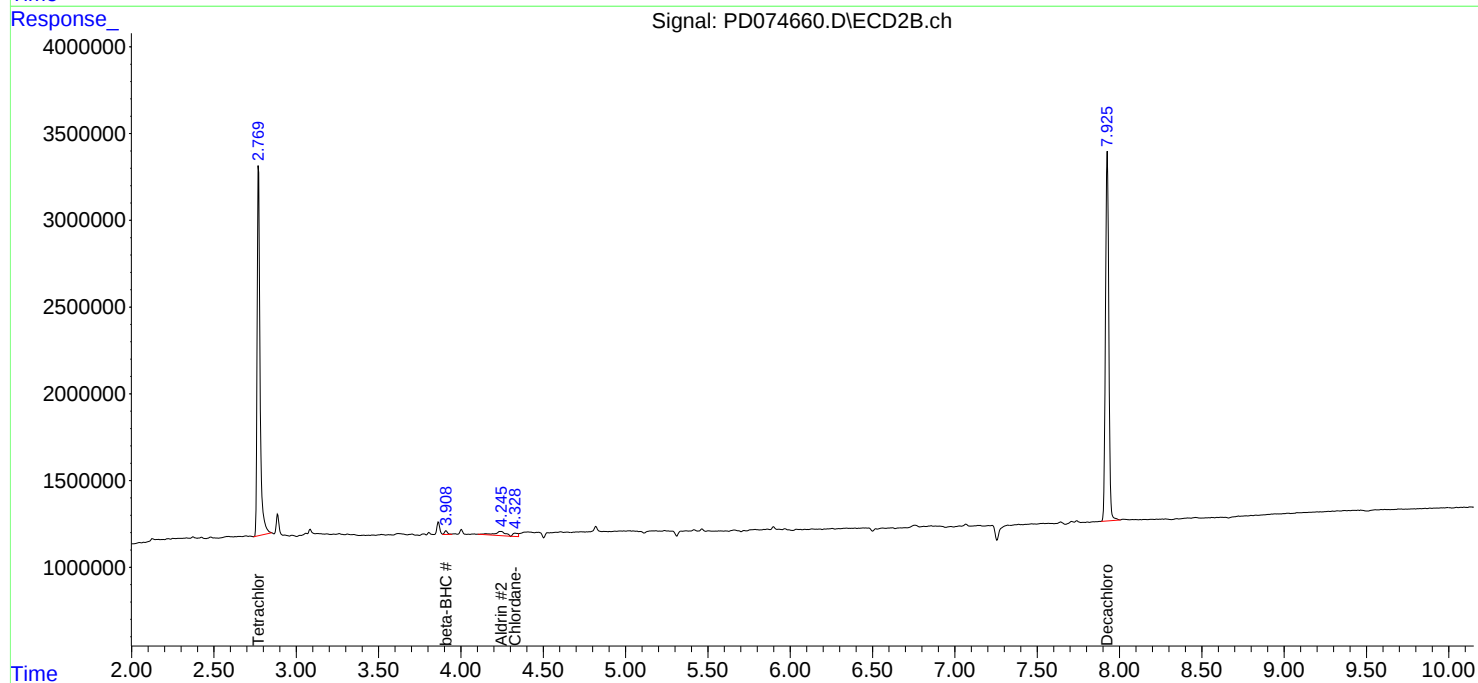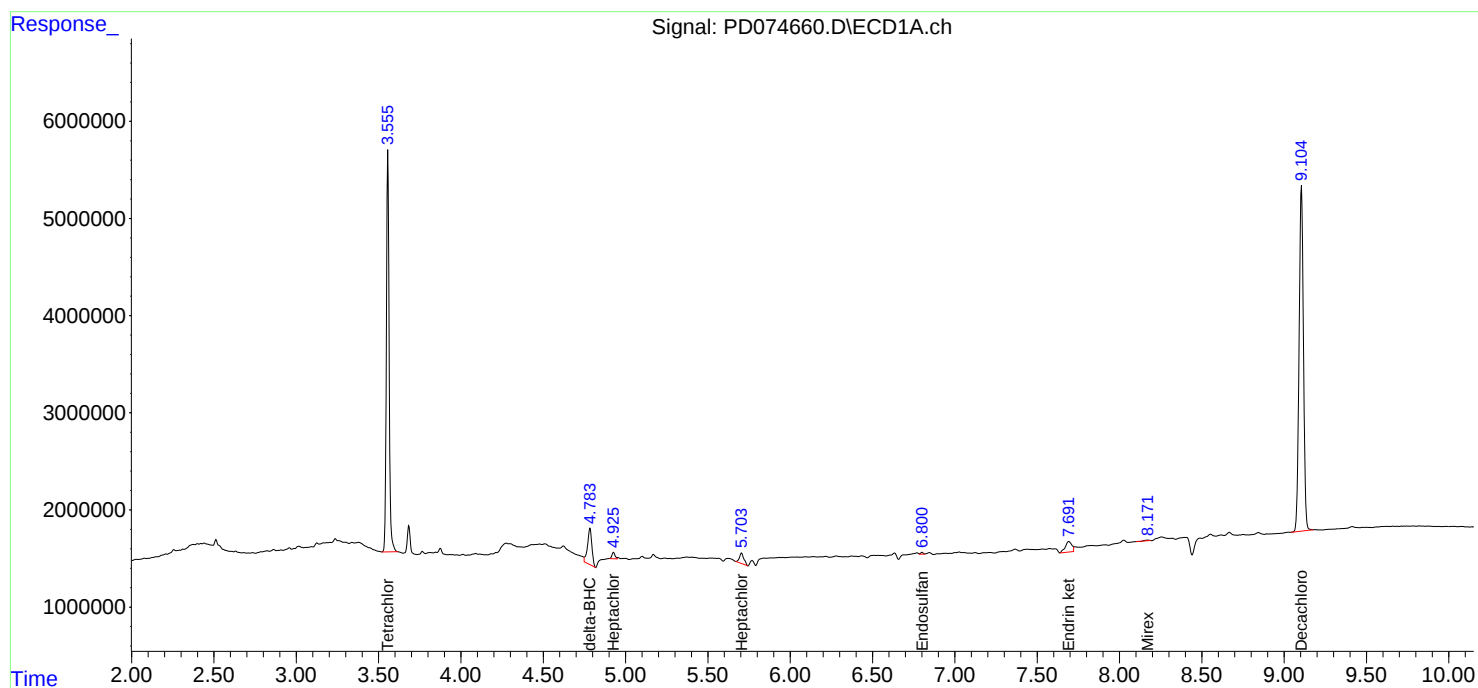


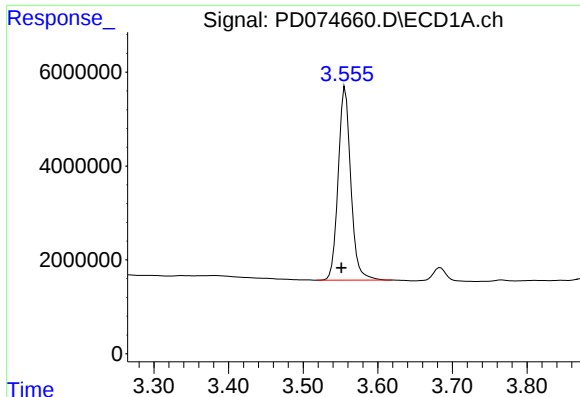

#1 Tetrachloro-m-xylene


R.T.: 3.556 min
Delta R.T.: 0.005 min
Response: 48371309
Conc: 20.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

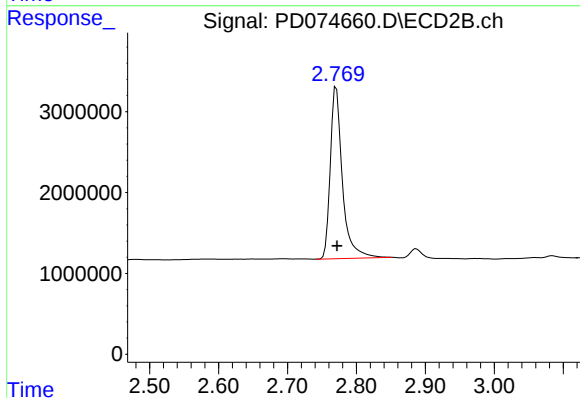


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 25952251
Conc: 21.32 ng/ml

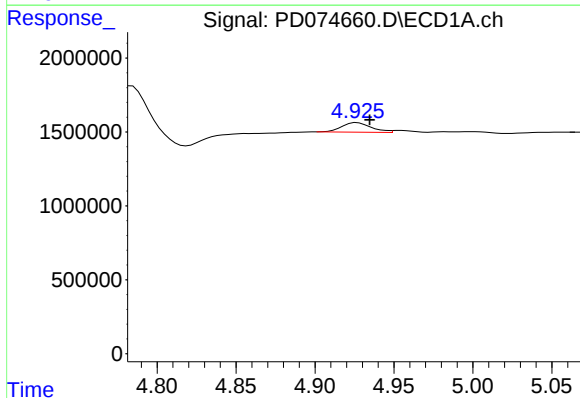


#4 Heptachlor

R.T.: 4.927 min
Delta R.T.: -0.008 min
Response: 853171
Conc: 0.25 ng/ml

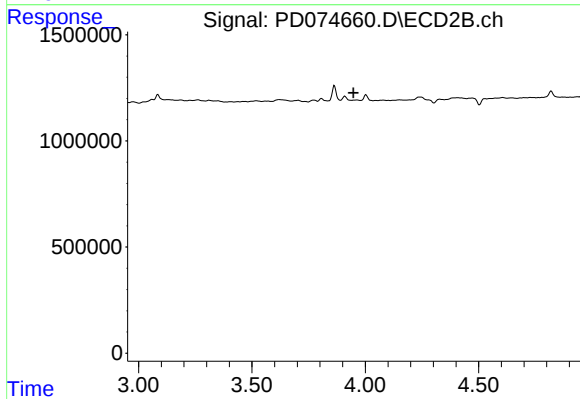

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.948 min
Response: 0
Conc: N.D.

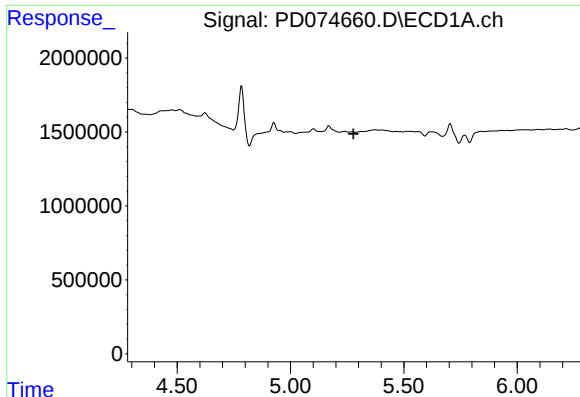

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

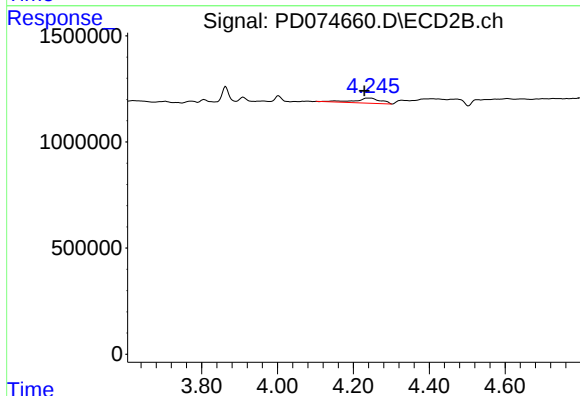


#5 Aldrin

R.T.: 4.237 min
Delta R.T.: 0.008 min
Response: 1128387
Conc: 0.67 ng/ml

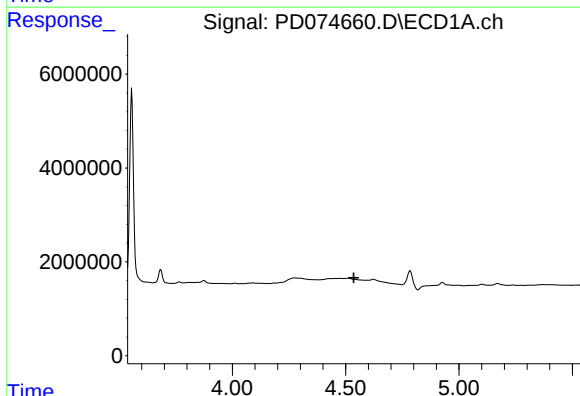


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.536 min
Response: 0
Conc: N.D.

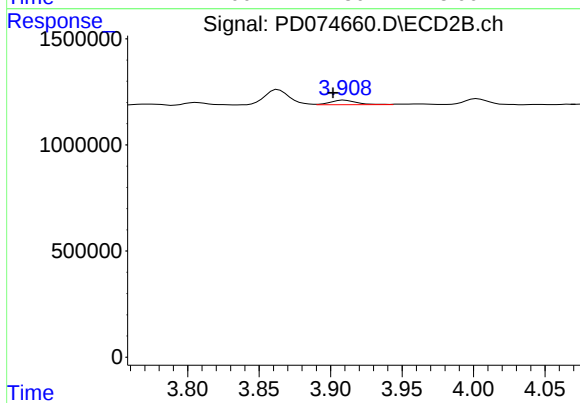

#6 beta-BHC


R.T.: 3.910 min
Delta R.T.: 0.008 min
Response: 275512
Conc: 0.36 ng/ml

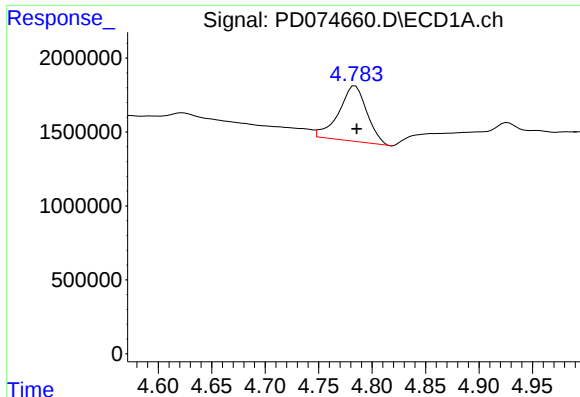

#7 delta-BHC


R.T.: 4.784 min
Delta R.T.: -0.001 min
Response: 6884722
Conc: 2.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

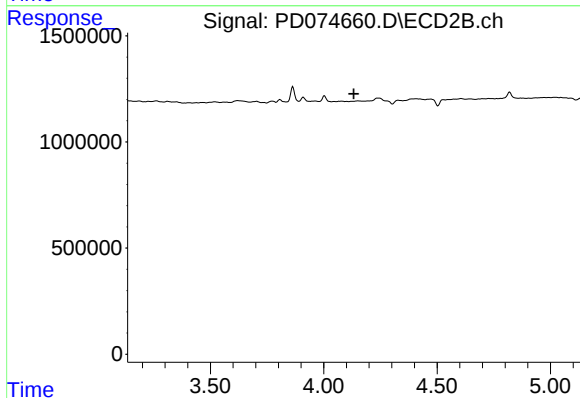


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

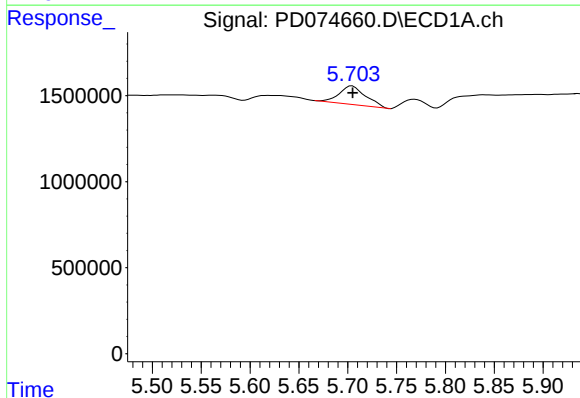


#8 Heptachlor epoxide

R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 2035704
Conc: 0.72 ng/ml

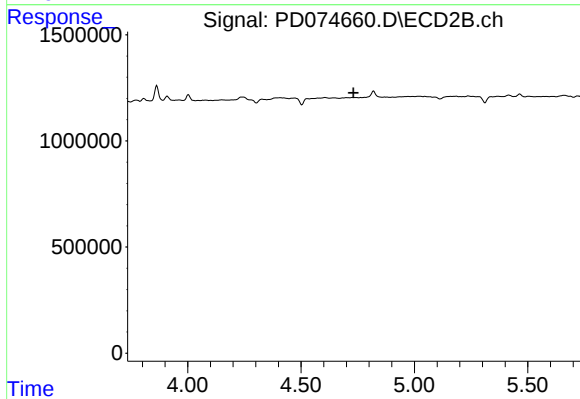

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.732 min
Response: 0
Conc: N.D.

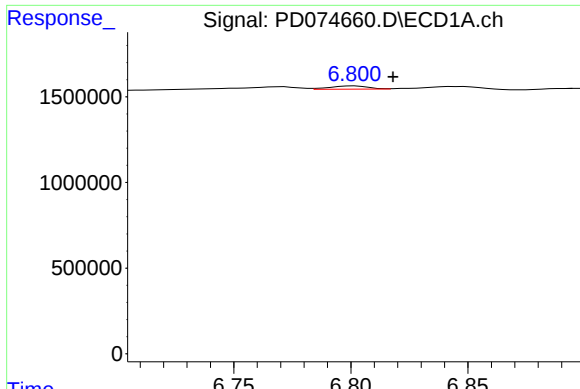

#15 Endosulfan II


R.T.: 6.801 min
Delta R.T.: -0.016 min
Response: 216936
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

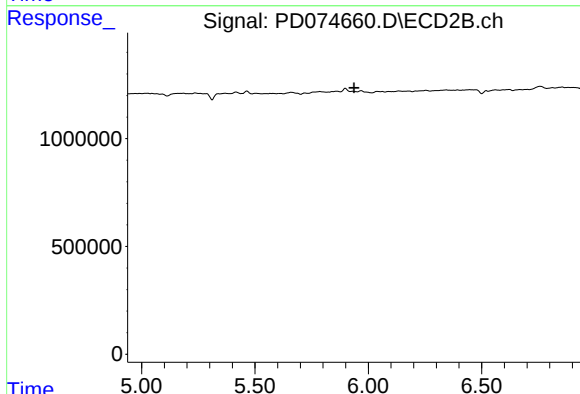


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.937 min
Response: 0
Conc: N.D.

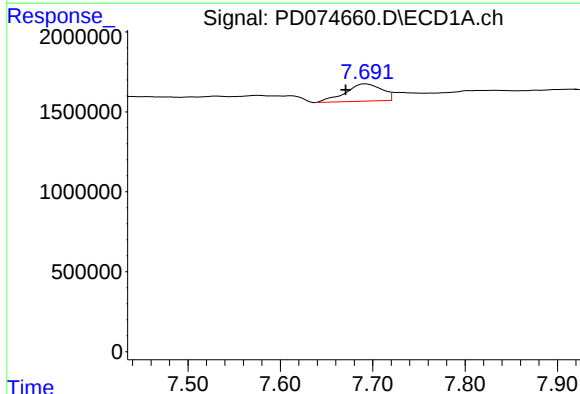


#21 Endrin ketone

R.T.: 7.692 min
Delta R.T.: 0.022 min
Response: 2987364
Conc: 1.07 ng/ml

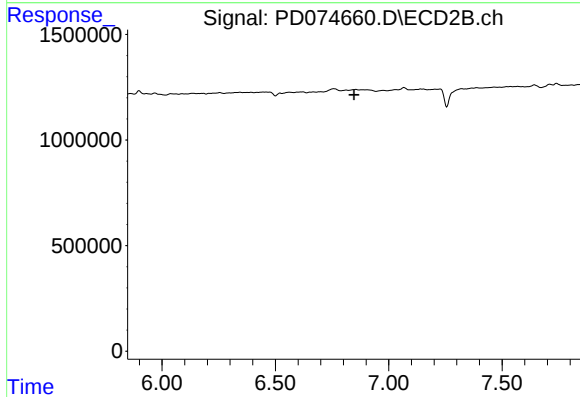

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

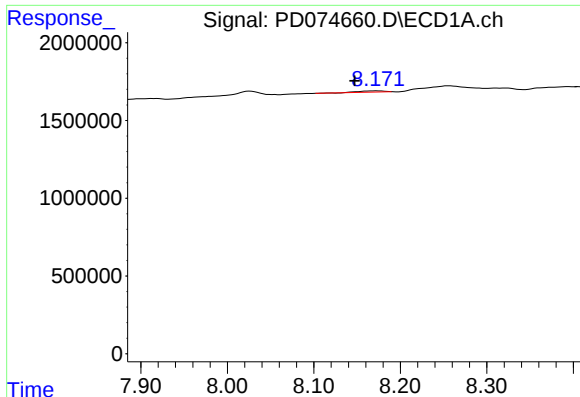

#22 Mirex


R.T.: 8.173 min
Delta R.T.: 0.026 min
Response: 170983
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

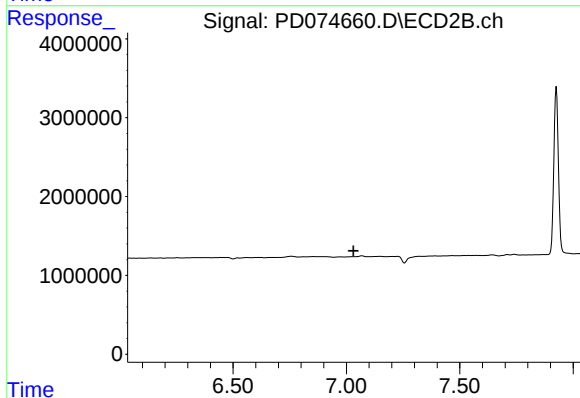


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.032 min
Response: 0
Conc: N.D.

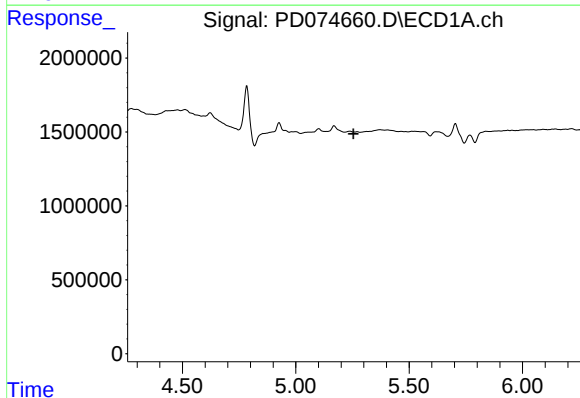


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.255 min
Response: 0
Conc: N.D.

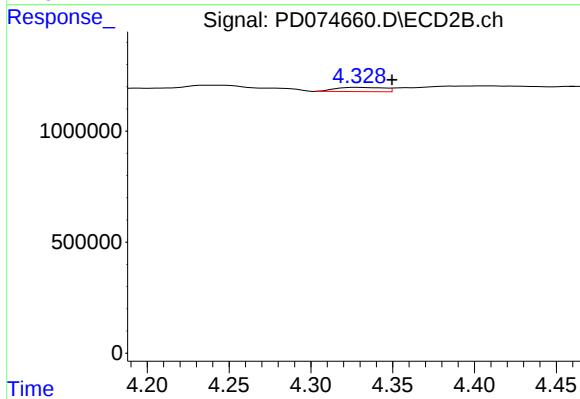

#24 Chlordane-2


R.T.: 4.328 min
Delta R.T.: -0.021 min
Response: 397017
Conc: 6.81 ng/ml

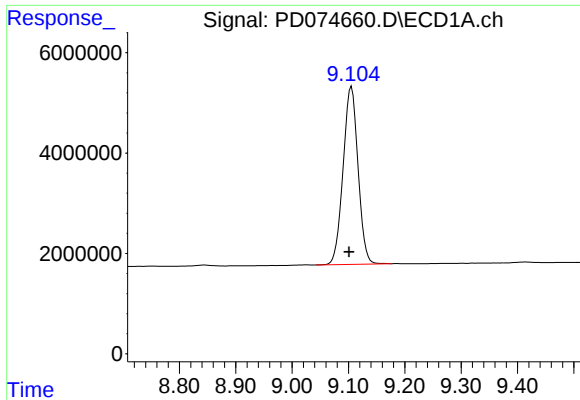

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.004 min
Response: 65114261
Conc: 24.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

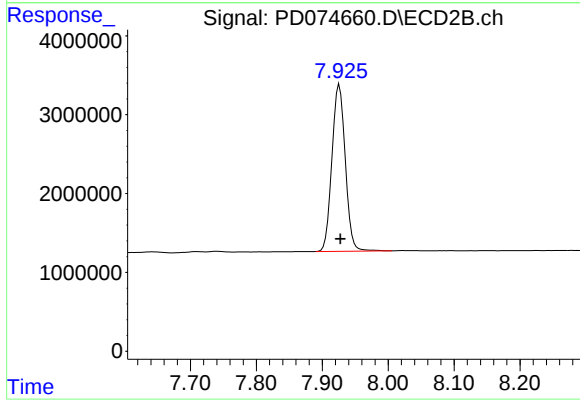

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.001 min
Response: 29807994
Conc: 24.29 ng/ml