

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041123\
 Data File : PD074650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2023 09:48
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 22:12:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 15 12:23:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.557	2.770	97118606	64310767	41.635	52.844 #
28) SA Decachlor...	9.105	7.926	120.6E6	56876750	45.075	46.357
Target Compounds						
23) Chlordane-1	4.725	3.773	54057018	22606129	453.350	448.601
24) Chlordane-2	5.256	4.350	58138950	26921372	433.905	461.922
25) Chlordane-3	5.968	4.982	220.6E6	76976150	445.846	458.583
26) Chlordane-4	6.051	5.046	276.1E6	73174804	459.546	453.561
27) Chlordane-5	6.901	5.943	50522152	27698377	490.303m	458.864



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041123\
Data File : PD074650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2023 09:48
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 22:12:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031423.M
Quant Title : GC Extractables
QLast Update : Wed Mar 15 12:23:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

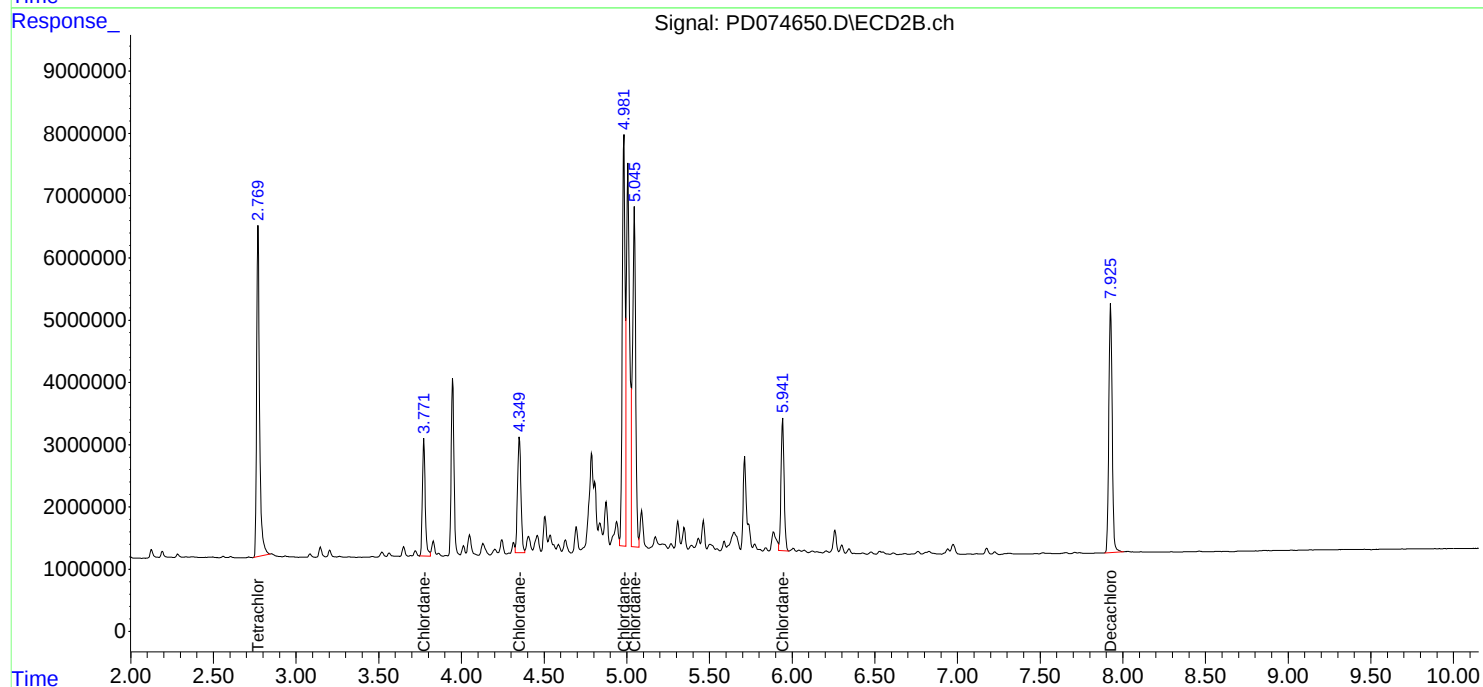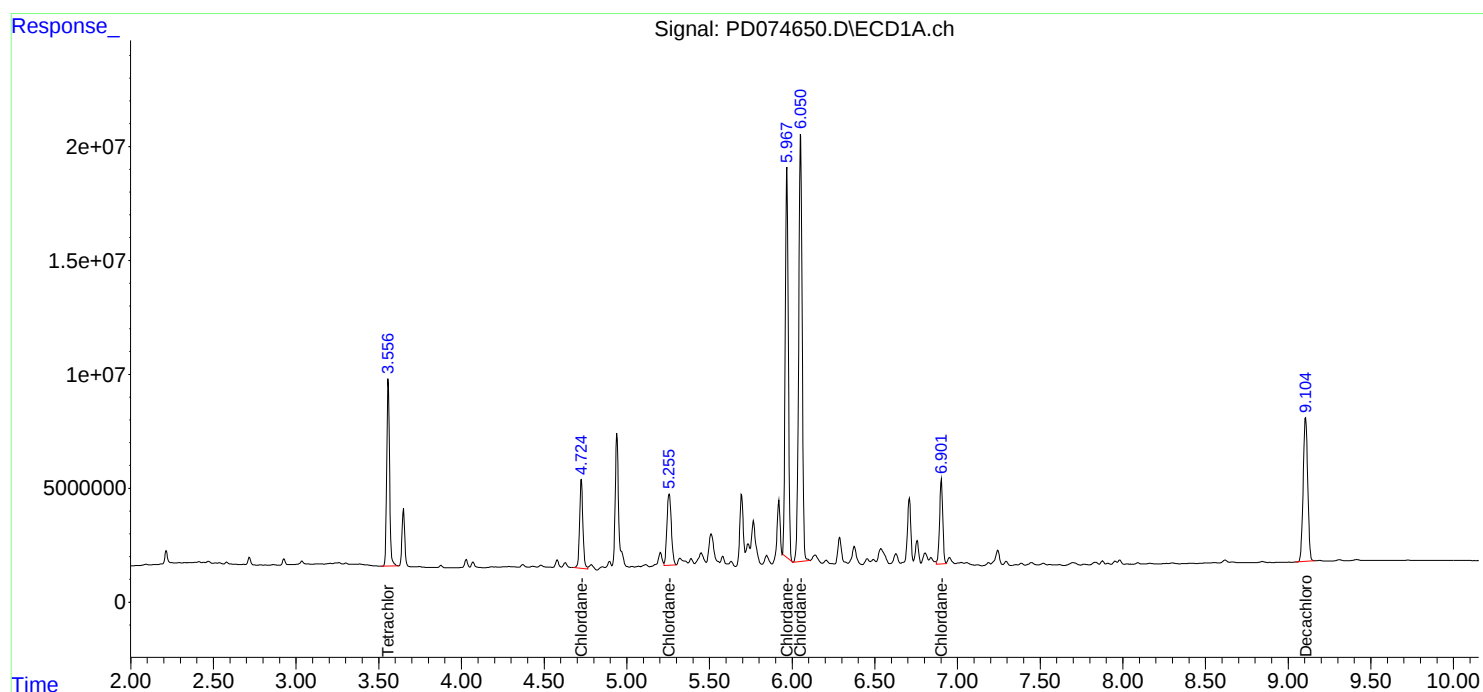


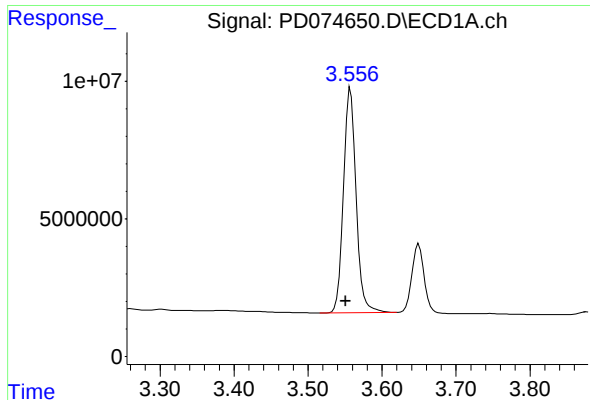

#1 Tetrachloro-m-xylene


R.T.: 3.557 min
Delta R.T.: 0.006 min
Response: 97118606
Conc: 41.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

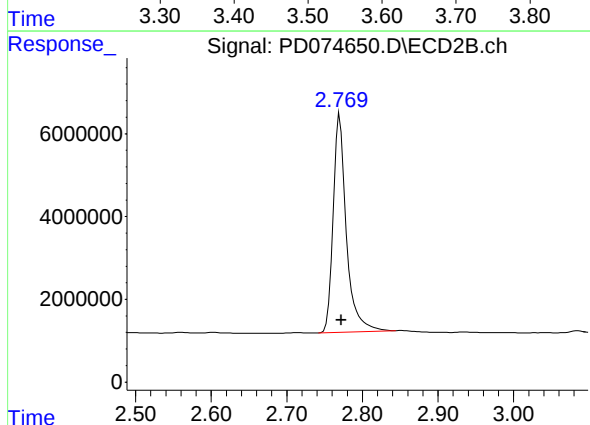


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 64310767
Conc: 52.84 ng/ml

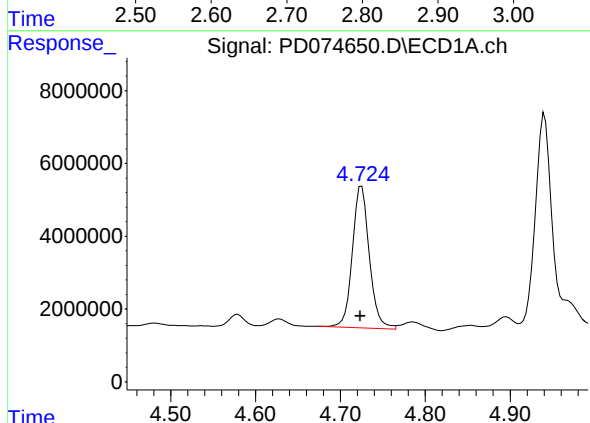


#23 Chlordane-1

R.T.: 4.725 min
Delta R.T.: 0.001 min
Response: 54057018
Conc: 453.35 ng/ml

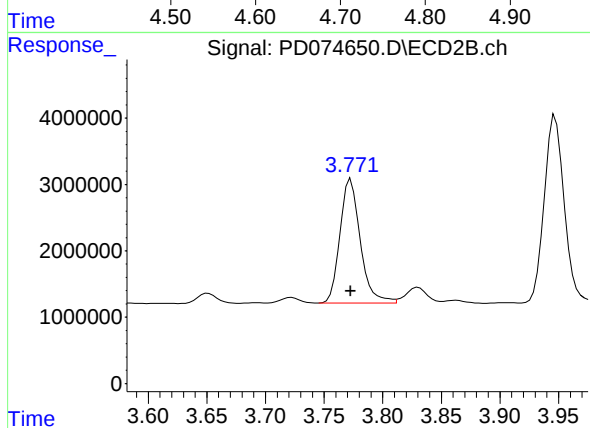

#23 Chlordane-1


R.T.: 3.773 min
Delta R.T.: 0.000 min
Response: 22606129
Conc: 448.60 ng/ml

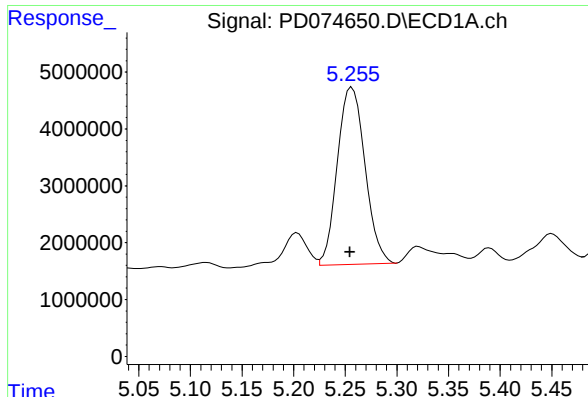

#24 Chlordane-2


R.T.: 5.256 min
Delta R.T.: 0.002 min
Response: 58138950
Conc: 433.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

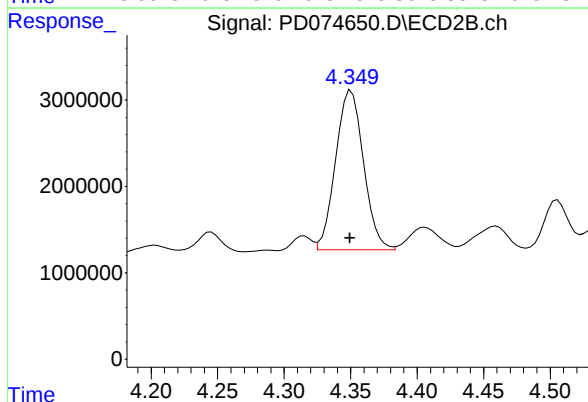


#24 Chlordane-2

R.T.: 4.350 min
Delta R.T.: 0.000 min
Response: 26921372
Conc: 461.92 ng/ml

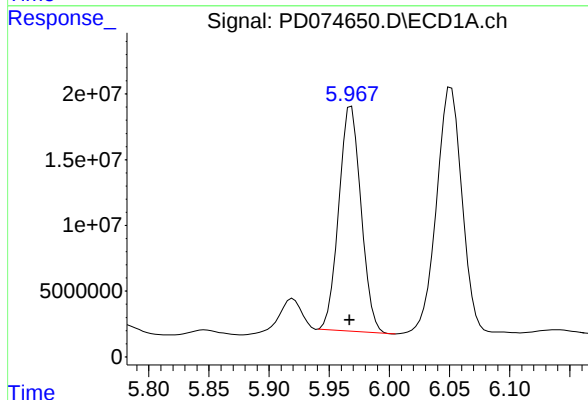


#25 Chlordane-3

R.T.: 5.968 min
Delta R.T.: 0.001 min
Response: 220557081
Conc: 445.85 ng/ml

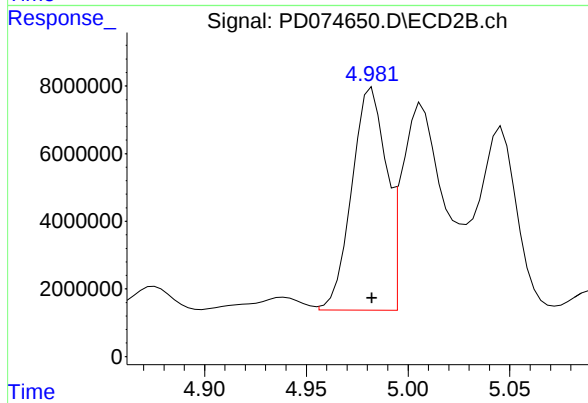

#25 Chlordane-3


R.T.: 4.982 min
Delta R.T.: 0.000 min
Response: 76976150
Conc: 458.58 ng/ml

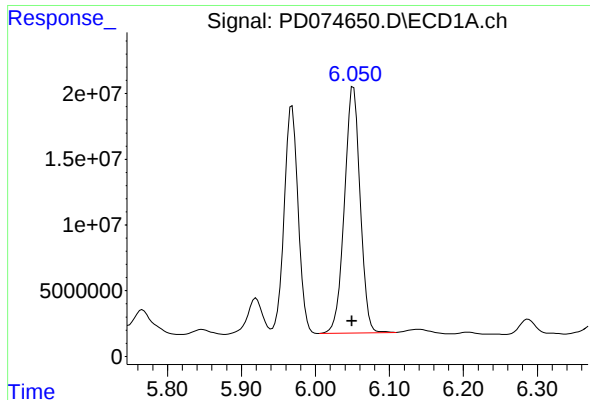

#26 Chlordane-4


R.T.: 6.051 min
Delta R.T.: 0.002 min
Response: 276065863
Conc: 459.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

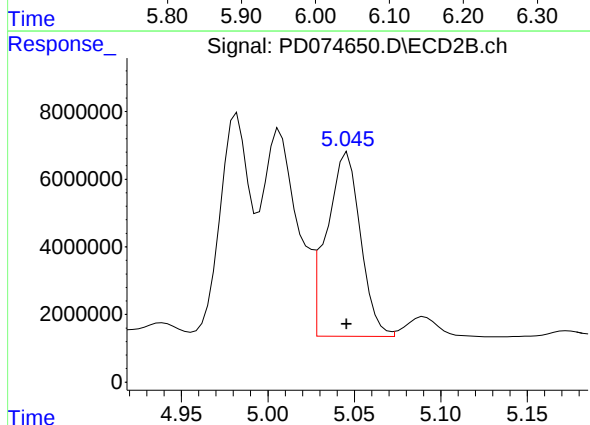


#26 Chlordane-4

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 73174804
Conc: 453.56 ng/ml

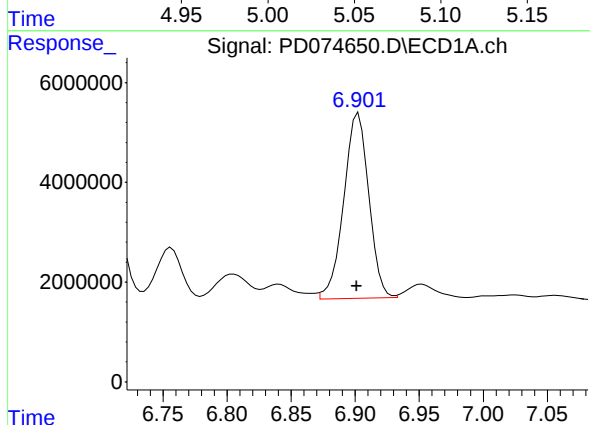


#27 Chlordane-5

R.T.: 6.901 min
Delta R.T.: 0.000 min
Response: 50522152
Conc: 490.30 ng/ml m

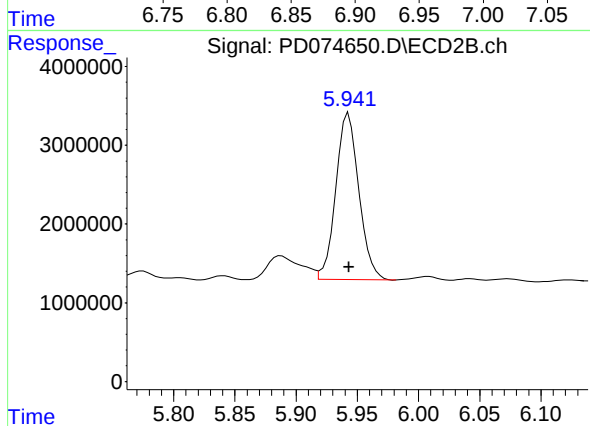

#27 Chlordane-5


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 27698377
Conc: 458.86 ng/ml

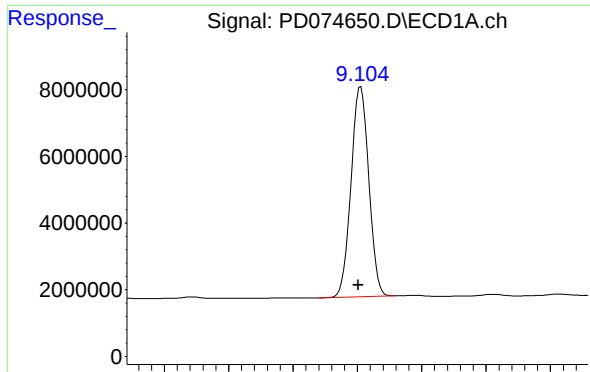

#28 Decachlorobiphenyl

R.T.: 9.105 min
Delta R.T.: 0.004 min
Response: 120556383
Conc: 45.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

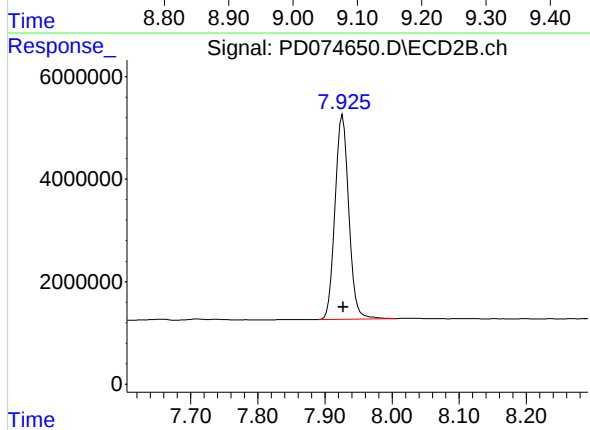

#28 Decachlorobiphenyl

R.T.: 7.926 min
Delta R.T.: -0.001 min
Response: 56876750
Conc: 46.36 ng/ml