

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041124\
 Data File : PD082376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2024 09:59
 Operator : AR\AJ
 Sample : P1979-03MSD 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0M17MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 20:53:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 06:17:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.777	30145311	59521514	19.663	17.151
27)	SA Decachlor...	9.119	7.909	35593503	57053930	18.400	17.345
Target Compounds							
2)	A alpha-BHC	4.024	3.278	113.9E6	229.2E6	42.969	41.803
3)	MA gamma-BHC...	4.358	3.606	113.2E6	216.3E6	44.448	43.217
4)	MA Heptachlor	4.950	3.946	107.1E6	204.2E6	40.305	42.269
5)	MB Aldrin	5.293	4.225	99725335	192.1E6	40.379	41.379
6)	B beta-BHC	4.553	3.902	46262799	88700865	42.791	41.842
7)	B delta-BHC	4.802	4.132	66398891	128.8E6	25.808	25.479
8)	B Heptachlo...	5.721	4.726	102.6E6	194.8E6	45.251	44.804
9)	A Endosulfan I	6.108	5.096	93336440	175.4E6	44.043	45.608
10)	B trans-Chl...	5.977	4.976	96235728	191.3E6	44.744	46.338
11)	B cis-Chlor...	6.057	5.040	100.4E6	194.2E6	45.638	46.906
12)	B 4,4'-DDE	6.228	5.229	194.6E6	365.3E6	90.680	91.993
13)	MA Dieldrin	6.384	5.360	204.4E6	393.3E6	90.158	90.544
14)	MA Endrin	6.615	5.635	172.8E6	349.3E6	93.549	93.934
15)	B Endosulfa...	6.833	5.928	172.3E6	327.7E6	90.885	91.691
16)	A 4,4'-DDD	6.747	5.782	147.3E6	296.9E6	91.995	93.605
17)	MA 4,4'-DDT	7.062	6.033	157.3E6	308.3E6	95.001	91.025
18)	B Endrin al...	6.964	6.108	123.0E6	237.1E6	88.493	87.263
19)	B Endosulfa...	7.198	6.330	145.4E6	287.8E6	85.506	84.542
20)	A Methoxychlor	7.537	6.608	382.7E6	701.5E6	447.206	422.820
21)	B Endrin ke...	7.686	6.835	171.3E6	360.6E6	95.864	95.002

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041124\
Data File : PD082376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2024 09:59
Operator : AR\AJ
Sample : P1979-03MSD 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 20:53:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 06:17:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

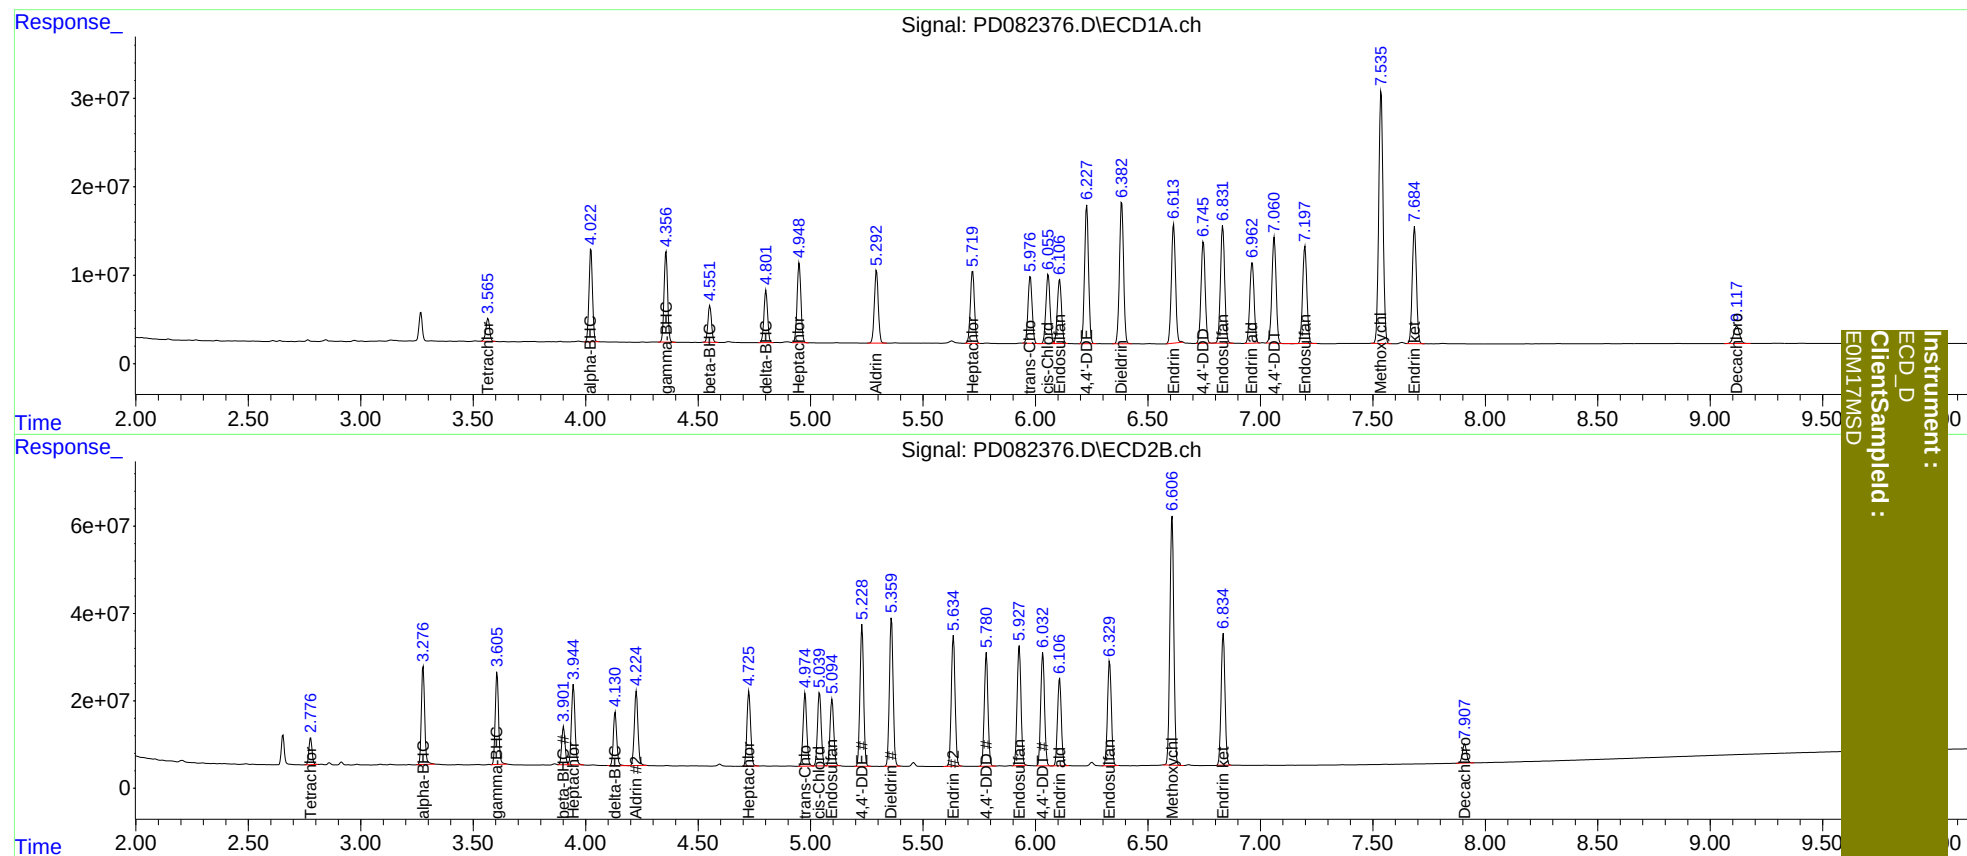

Instrument :
ECD_D
ClientSampled :
EOM17MSD