

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041124\
 Data File : PD082350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Apr 2024 22:36
 Operator : AR\AJ
 Sample : RESC028
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC029

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 06:31:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 10 06:17:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.566	2.777	29997425	65893923	19.566	18.987
2)	SA Decachlor...	9.119	7.909	76321366	129.1E6	39.454	39.241
Target Compounds							
2)	A alpha-BHC	4.023	3.277	24856509	50565617	9.374	9.223
3)	MA gamma-BHC...	4.357	3.606	24300566	47090103	9.540	9.408
4)	MA Heptachlor	4.950	3.946	24741904	46226245	9.308	9.568
5)	MB Aldrin	5.293	4.225	22928973	44392818	9.284	9.562
6)	B beta-BHC	4.553	3.902	10662170	20546169	9.862	9.692
7)	B delta-BHC	4.802	4.132	23298109	46016148	9.056	9.102
8)	B Heptachlo...	5.721	4.726	20790187	41216376	9.168	9.479
9)	A Endosulfan I	6.108	5.095	20645596	37674501	9.742	9.798
10)	B trans-Chl...	5.977	4.976	19922303	38599861	9.263	9.352
11)	B cis-Chlor...	6.057	5.040	20485625	39304379	9.309	9.491
12)	B 4,4'-DDE	6.228	5.229	39766974	73982749	18.534	18.631
13)	MA Dieldrin	6.384	5.360	42743914	83861443	18.849	19.305
14)	MA Endrin	6.615	5.635	35297377	72132348	19.111	19.397
15)	B Endosulfa...	6.833	5.928	37240967	68825194	19.639	19.258
16)	A 4,4'-DDD	6.746	5.782	30616130	63470963	19.115	20.014
17)	MA 4,4'-DDT	7.062	6.033	32172788	65233079	19.426	19.258
18)	B Endrin al...	6.964	6.108	27261588	53581799	19.609	19.718
19)	B Endosulfa...	7.199	6.330	33291889	66216606	19.574	19.453
20)	A Methoxychlor	7.538	6.608	90994366	179.0E6	106.337	107.877
21)	B Endrin ke...	7.685	6.835	36984467	75746091	20.703	19.954

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041124\
Data File : PD082350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 22:36
Operator : AR\AJ
Sample : RESC028
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 06:31:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 06:17:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

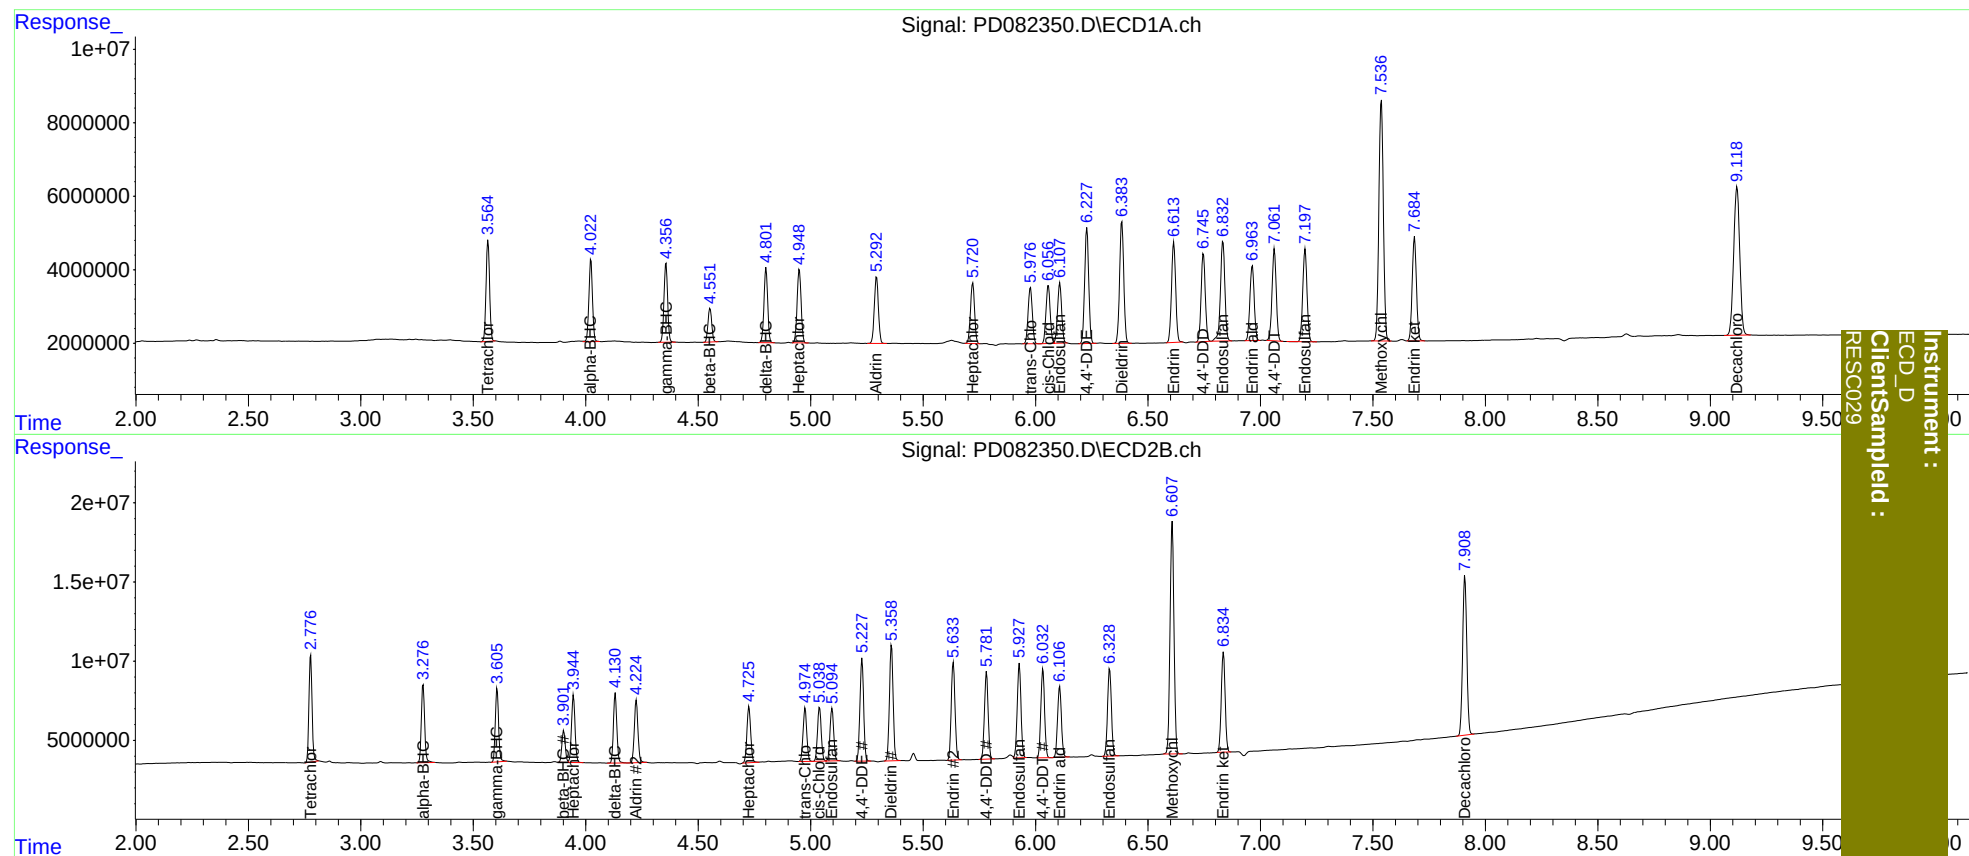

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041124\
Data File : PD082350.D
Acq On : 09 Apr 2024 22:36
Operator : AR\AJ
Sample : RESC028
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC029

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
Title : GC Extractables
Last Update : Wed Apr 10 06:17:48 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.566	4.023	100.00%
4.023	4.357	100.00%
4.357	4.553	100.00%
4.553	4.802	100.00%
4.802	4.950	100.00%
4.950	5.293	100.00%
5.293	5.721	100.00%
5.721	5.977	100.00%
5.977	6.057	100.00%
6.057	6.108	96.69%
6.108	6.228	100.00%
6.228	6.384	100.00%
6.384	6.615	100.00%
6.615	6.746	100.00%
6.746	6.833	100.00%
6.833	6.964	100.00%
6.964	7.062	100.00%
7.062	7.199	100.00%
7.199	7.538	100.00%
7.538	7.685	100.00%
7.685	9.119	100.00%

Signal #2


2.777	3.277	100.00%
3.277	3.606	100.00%
3.606	3.902	100.00%
3.902	3.946	98.23%
3.946	4.132	100.00%
4.132	4.225	100.00%
4.225	4.726	100.00%
4.726	4.976	100.00%
4.976	5.040	100.00%
5.040	5.095	100.00%
5.095	5.229	100.00%
5.229	5.360	100.00%
5.360	5.635	100.00%
5.635	5.782	100.00%
5.782	5.928	100.00%
5.928	6.033	100.00%
6.033	6.108	100.00%
6.108	6.330	100.00%
6.330	6.608	100.00%
6.608	6.835	100.00%
6.835	7.909	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041124\
Data File : PD082350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Apr 2024 22:36
Operator : AR\AJ
Sample : RESC028
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC029

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 06:31:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041124CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Apr 10 06:17:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

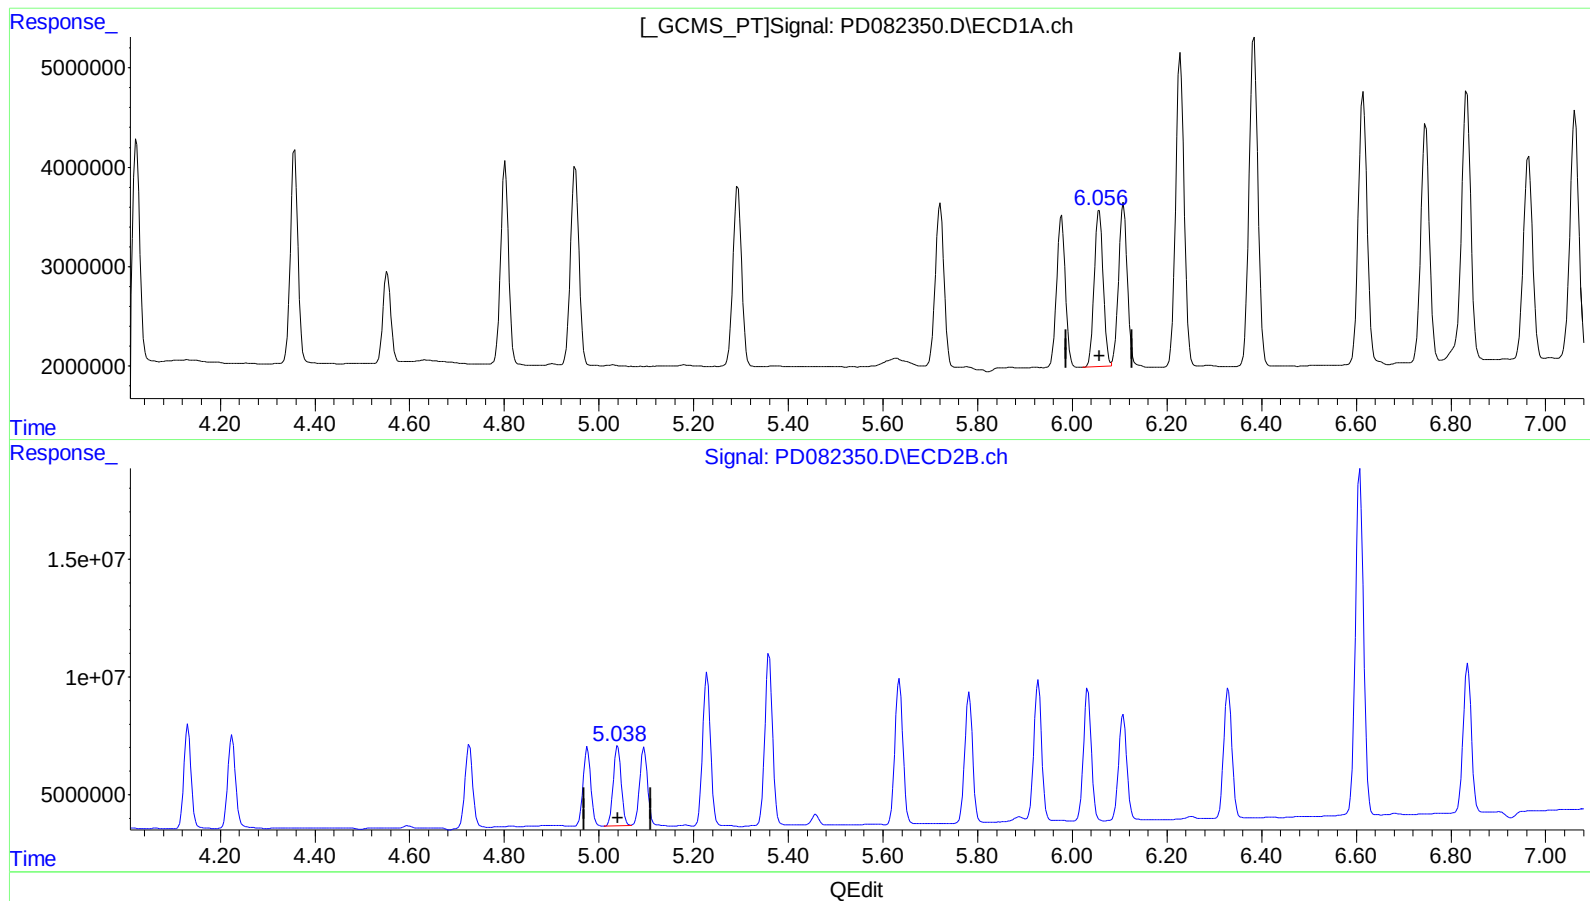

(11) cis-Chlordane (B)

6.057min 9.309 ng/ml

response 20485625

(11) cis-Chlordane #2 (B)

5.040min 9.491 ng/ml

response 39304379