

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD041124\  
 Data File : PD082375.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 10 Apr 2024 09:46  
 Operator : AR\AJ  
 Sample : P1979-02MS 10X  
 Misc :  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 E0M17MS

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 10 20:53:17 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD041124CLP-TCLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Apr 10 06:17:48 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|---------|
| -----                       |                 |       |       |          |          |         |         |
| System Monitoring Compounds |                 |       |       |          |          |         |         |
| 1)                          | SA Tetrachlo... | 3.566 | 2.778 | 30043690 | 59324160 | 19.596  | 17.094  |
| 2)                          | SA Decachlor... | 9.119 | 7.909 | 35341647 | 56259642 | 18.270  | 17.104  |
| Target Compounds            |                 |       |       |          |          |         |         |
| 2)                          | A alpha-BHC     | 4.024 | 3.278 | 113.7E6  | 228.0E6  | 42.895  | 41.596  |
| 3)                          | MA gamma-BHC... | 4.358 | 3.606 | 112.7E6  | 215.2E6  | 44.243  | 43.002  |
| 4)                          | MA Heptachlor   | 4.950 | 3.946 | 108.6E6  | 202.5E6  | 40.850  | 41.903  |
| 5)                          | MB Aldrin       | 5.294 | 4.225 | 100.4E6  | 190.9E6  | 40.667  | 41.119  |
| 6)                          | B beta-BHC      | 4.553 | 3.902 | 46056369 | 87732931 | 42.600  | 41.385  |
| 7)                          | B delta-BHC     | 4.802 | 4.132 | 66704324 | 127.5E6  | 25.927  | 25.226  |
| 8)                          | B Heptachlo...  | 5.721 | 4.726 | 104.1E6  | 193.3E6  | 45.886  | 44.466  |
| 9)                          | A Endosulfan I  | 6.108 | 5.096 | 95666284 | 174.0E6  | 45.142  | 45.264  |
| 10)                         | B trans-Chl...  | 5.977 | 4.976 | 98870005 | 189.5E6  | 45.969  | 45.922  |
| 11)                         | B cis-Chlor...  | 6.057 | 5.040 | 103.0E6  | 192.8E6  | 46.817  | 46.563  |
| 12)                         | B 4,4'-DDE      | 6.228 | 5.228 | 197.7E6  | 368.5E6  | 92.124  | 92.811  |
| 13)                         | MA Dieldrin     | 6.384 | 5.360 | 206.7E6  | 395.6E6  | 91.164  | 91.073  |
| 14)                         | MA Endrin       | 6.615 | 5.635 | 173.5E6  | 350.8E6  | 93.948  | 94.339  |
| 15)                         | B Endosulfa...  | 6.833 | 5.928 | 172.6E6  | 330.8E6  | 91.009  | 92.558  |
| 16)                         | A 4,4'-DDD      | 6.747 | 5.782 | 148.4E6  | 299.0E6  | 92.652  | 94.293  |
| 17)                         | MA 4,4'-DDT     | 7.062 | 6.032 | 158.9E6  | 310.9E6  | 95.925  | 91.782  |
| 18)                         | B Endrin al...  | 6.963 | 6.107 | 123.6E6  | 240.0E6  | 88.914  | 88.322  |
| 19)                         | B Endosulfa...  | 7.198 | 6.329 | 147.7E6  | 290.9E6  | 86.827  | 85.453  |
| 20)                         | A Methoxychlor  | 7.538 | 6.607 | 389.4E6  | 695.2E6  | 455.068 | 419.021 |
| 21)                         | B Endrin ke...  | 7.686 | 6.835 | 174.1E6  | 357.8E6  | 97.482  | 94.261  |
| -----                       |                 |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD041124\  
Data File : PD082375.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 10 Apr 2024 09:46  
Operator : AR\AJ  
Sample : P1979-02MS 10X  
Misc :  
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 10 20:53:17 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD041124CLP-TCLP.M  
Quant Title : GC Extractables  
QLast Update : Wed Apr 10 06:17:48 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

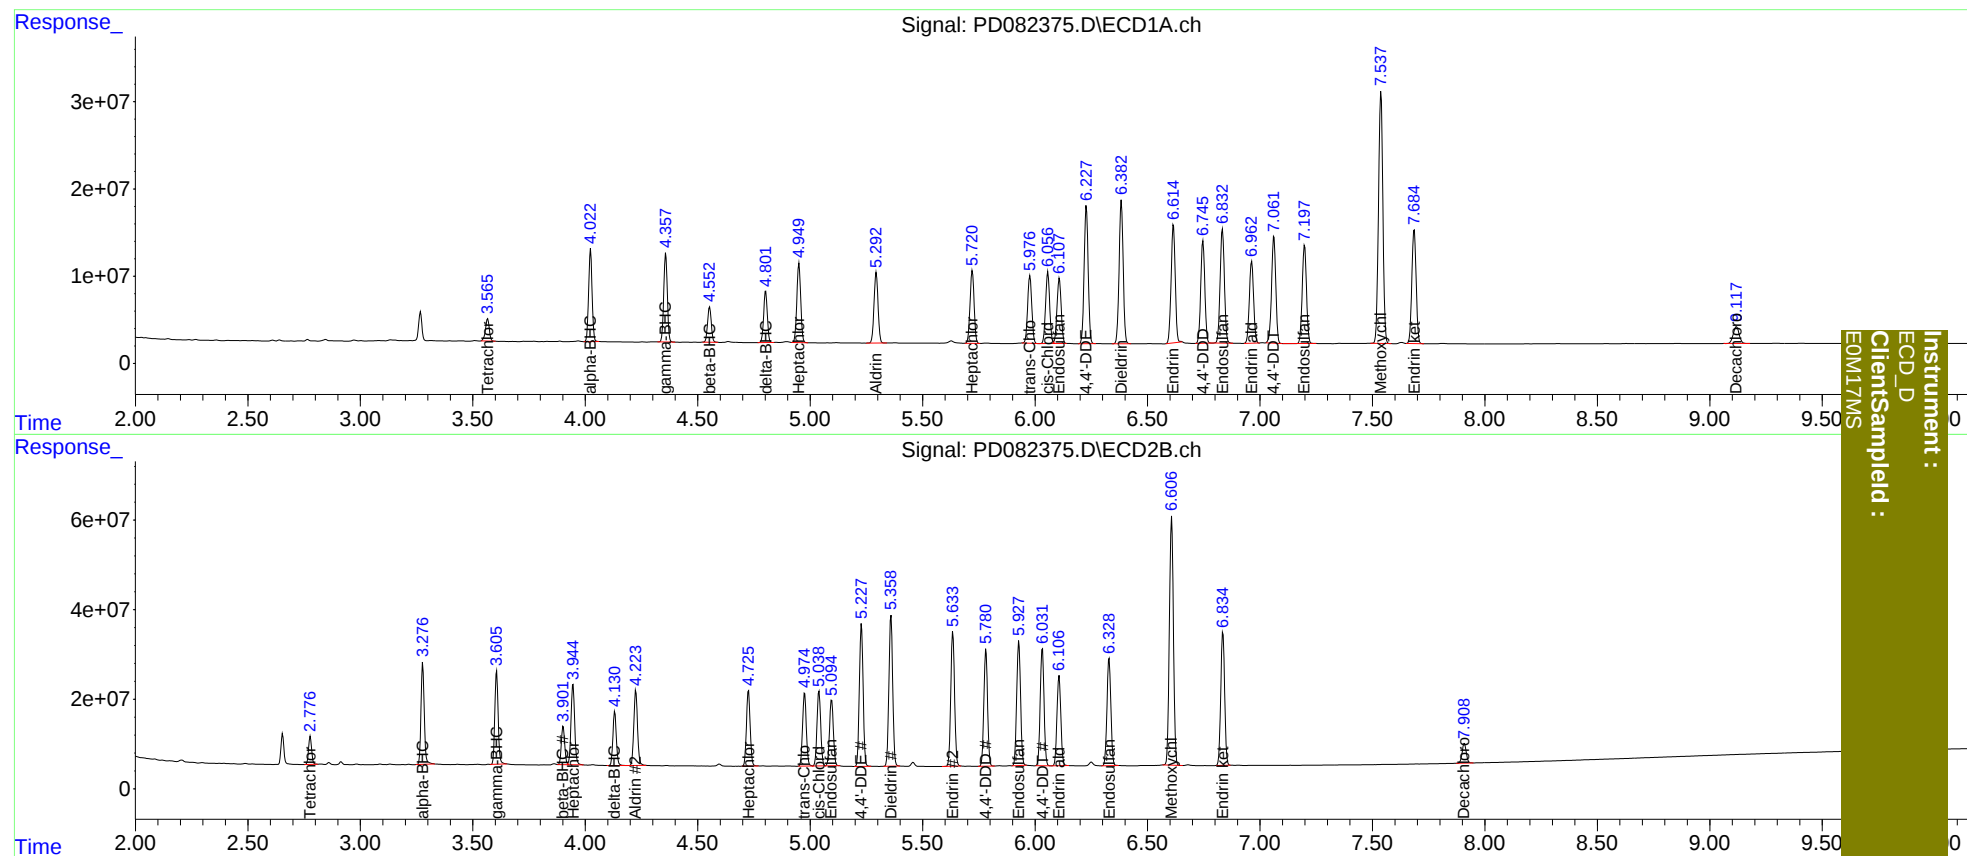

Instrument :  
ECD\_D  
ClientSampled :  
EOM17MS