

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041219\
 Data File : PD052903.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 10:04
 Operator : AJ\SJ
 Sample : PIBLK39
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 23:33:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.040	30188294	668.1E6	19.828	21.112
27)	SA Decachlor...	7.814	9.157	56723395	620.6E6	40.230	43.043
Target Compounds							
8)	B Heptachlo...	0.000	5.922	0	175.4E6	N.D.	4.952
14)	MA Endrin	0.000	6.761	0	82003475	N.D.	3.244
20)	A Methoxychlor	0.000	7.584f	0	35977098	N.D.	3.789

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041219\
Data File : PD052903.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 10:04
Operator : AJ\SJ
Sample : PIBLK39
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 23:33:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

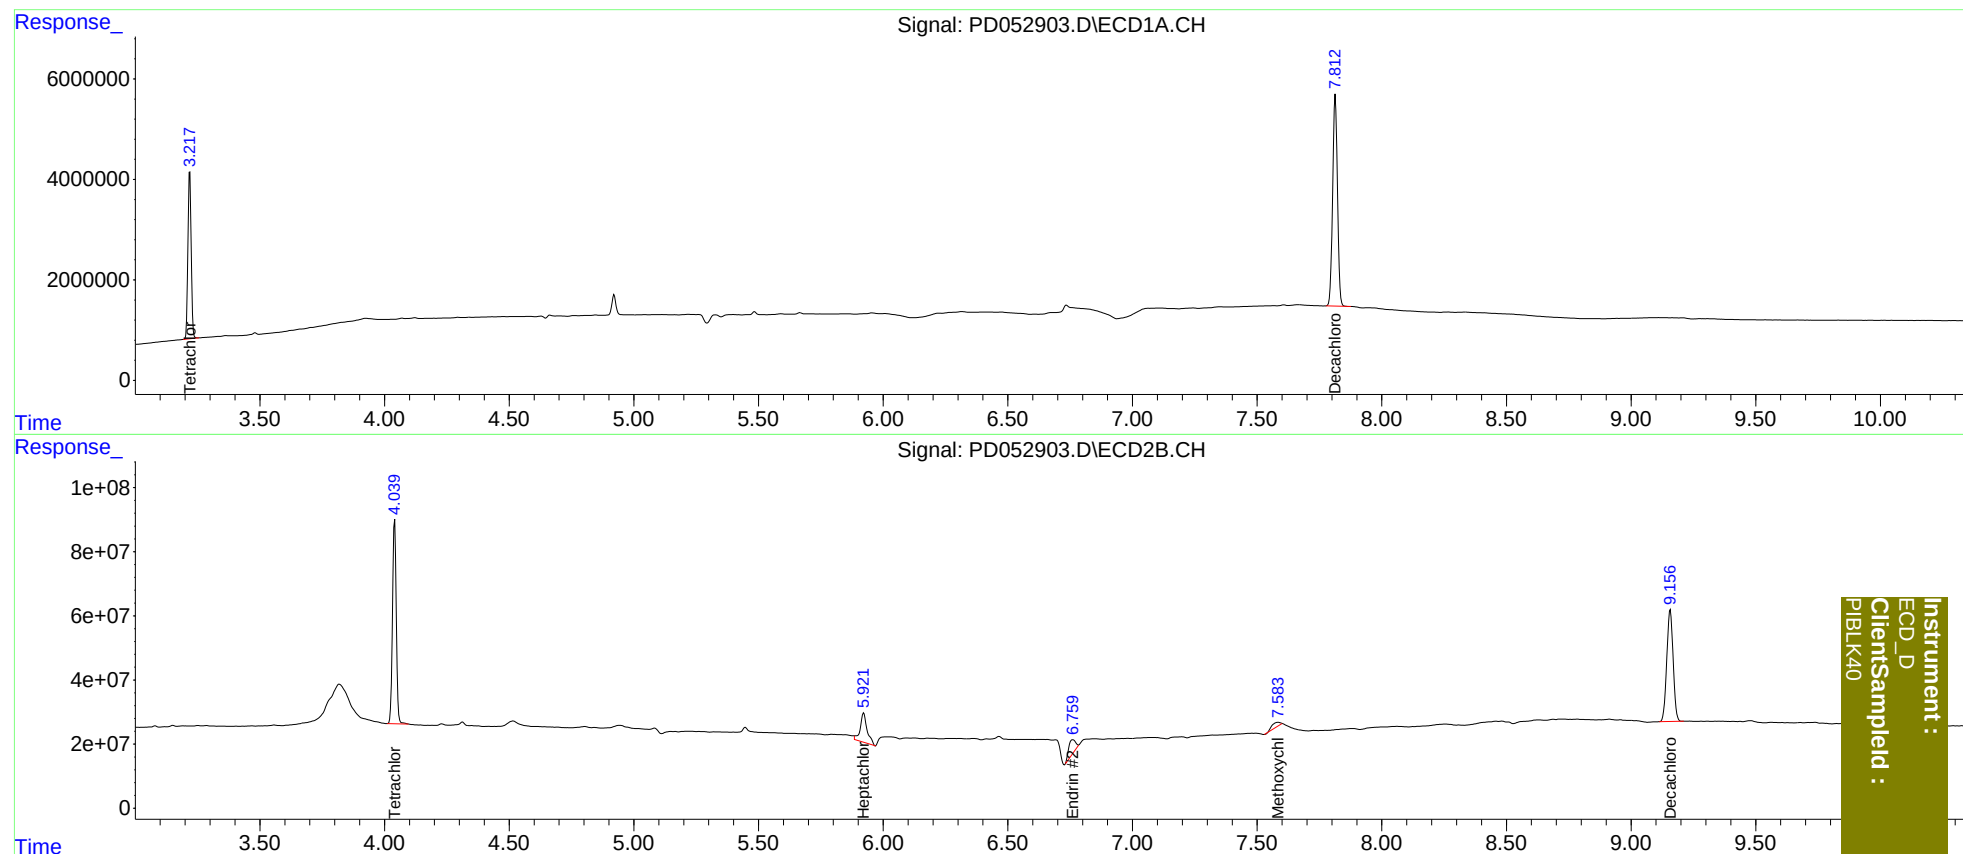


Instrument :
ECD_D
ClientSampleId :
PIBLK40

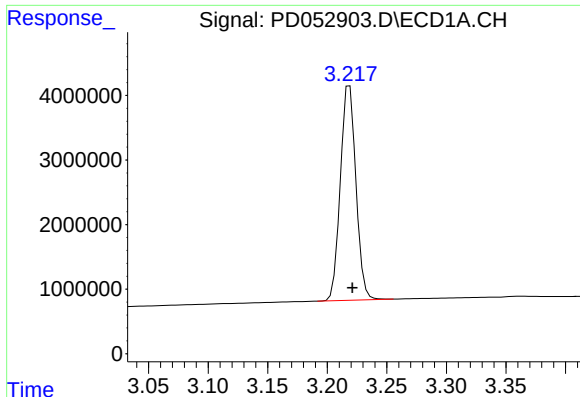

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: -0.002 min
Response: 30188294
Conc: 19.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK40

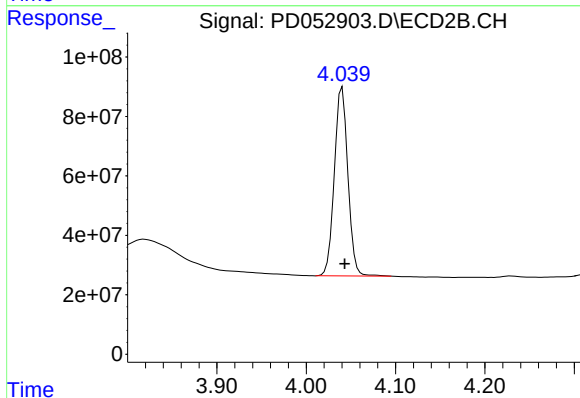


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: -0.003 min
Response: 668103406
Conc: 21.11 ng/ml

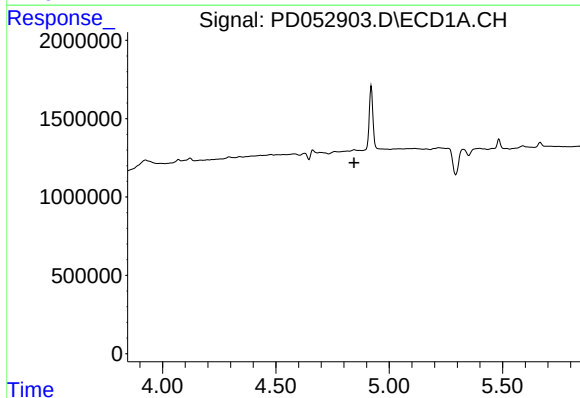


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.845 min
Response: 0
Conc: N.D.

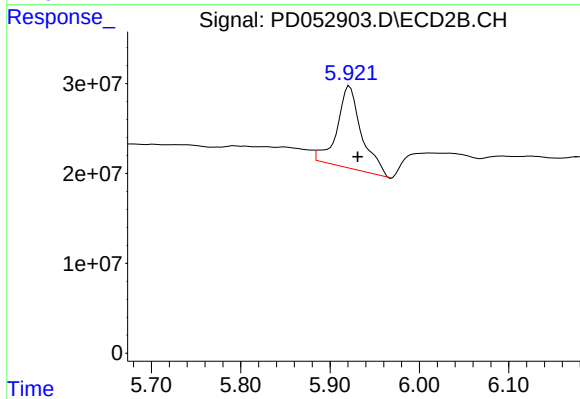

#8 Heptachlor epoxide


R.T.: 5.922 min
Delta R.T.: -0.009 min
Response: 175397660
Conc: 4.95 ng/ml

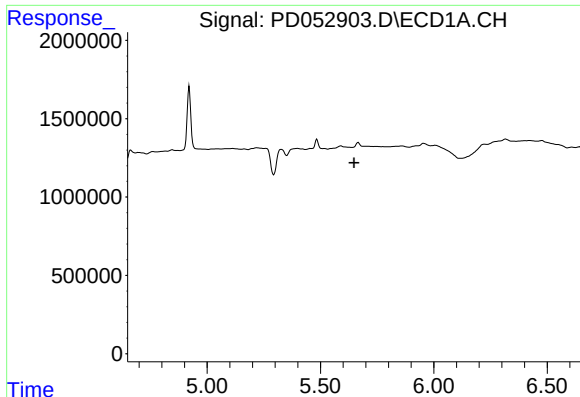

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK40

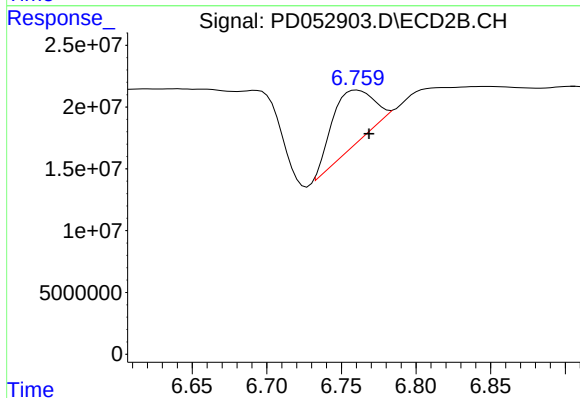


#14 Endrin

R.T.: 6.761 min
Delta R.T.: -0.008 min
Response: 82003475
Conc: 3.24 ng/ml

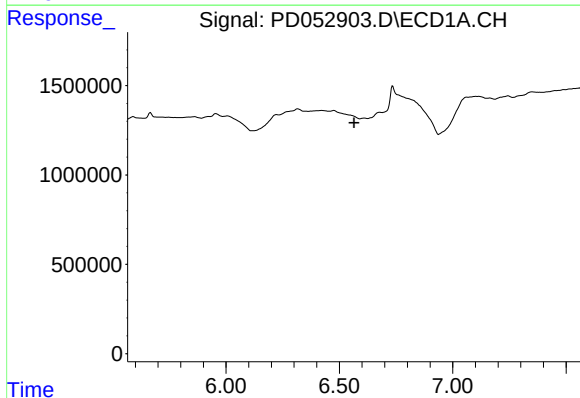


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.565 min
Response: 0
Conc: N.D.

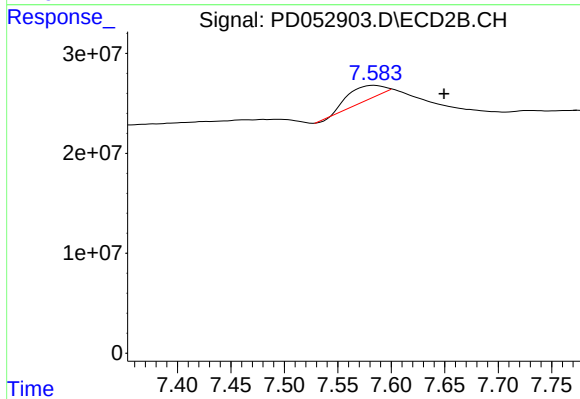

#20 Methoxychlor


R.T.: 7.584 min
Delta R.T.: -0.065 min
Response: 35977098
Conc: 3.79 ng/ml

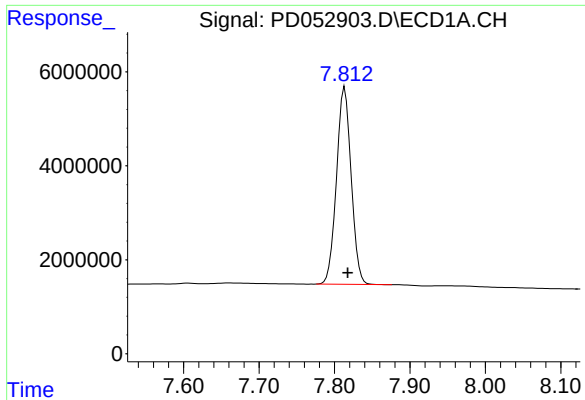

#27 Decachlorobiphenyl

R.T.: 7.814 min
Delta R.T.: -0.004 min
Response: 56723395
Conc: 40.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK40

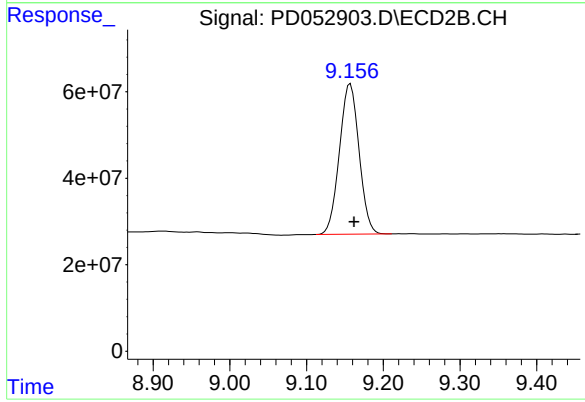

#27 Decachlorobiphenyl

R.T.: 9.157 min
Delta R.T.: -0.005 min
Response: 620620736
Conc: 43.04 ng/ml