

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041219\
 Data File : PD052905.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 10:33
 Operator : AJ\SJ
 Sample : K2303-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BF887

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 23:33:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.220	4.041	9162229	210.6E6	6.018	6.656
27)	SA Decachlor...	7.813	9.158	14484790	159.9E6	10.273	11.089
Target Compounds							
7)	B delta-BHC	0.000	5.083f	0	46850373	N.D.	1.300
14)	MA Endrin	0.000	6.764	0	21845397	N.D.	0.864
20)	A Methoxychlor	0.000	7.593f	0	9539086	N.D.	1.005

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041219\
Data File : PD052905.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 10:33
Operator : AJ\SJ
Sample : K2303-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 23:33:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

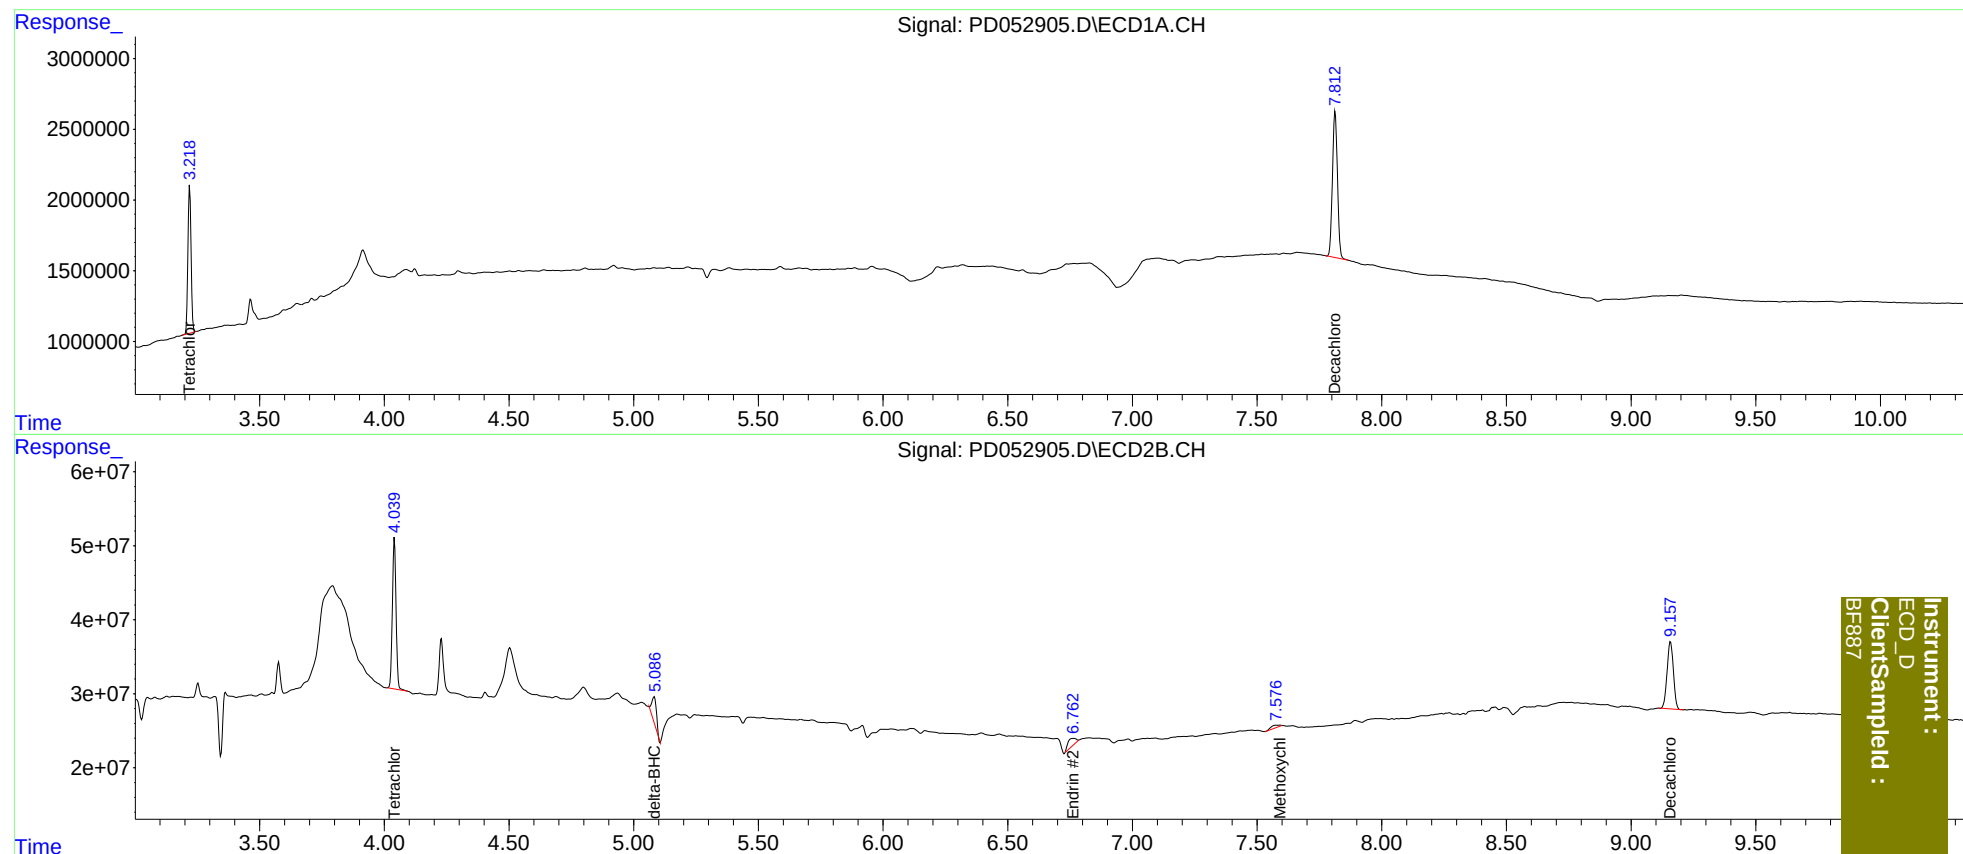


Instrument :
ECD_D
ClientSampled :
BF887

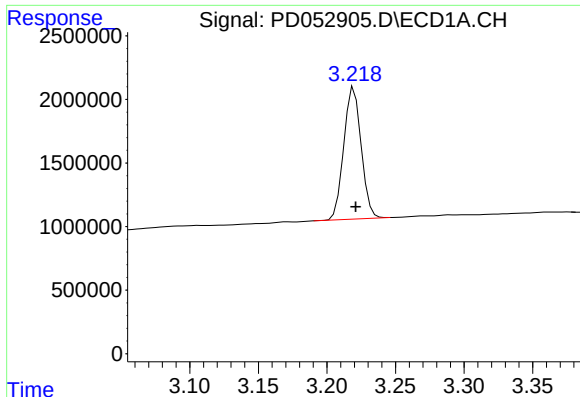

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: -0.001 min
Response: 9162229
Conc: 6.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF887

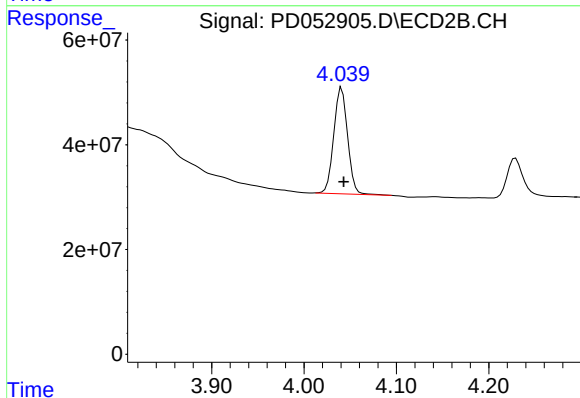


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 210640882
Conc: 6.66 ng/ml

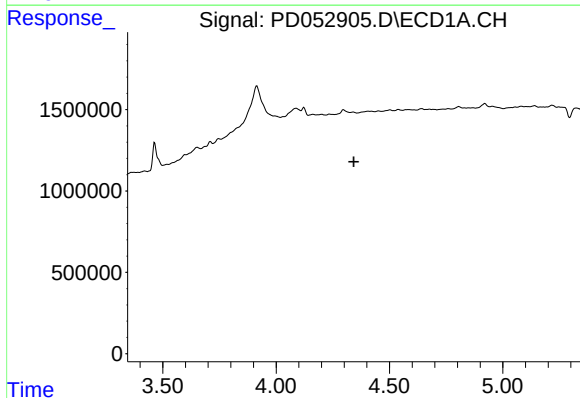


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.343 min
Response: 0
Conc: N.D.

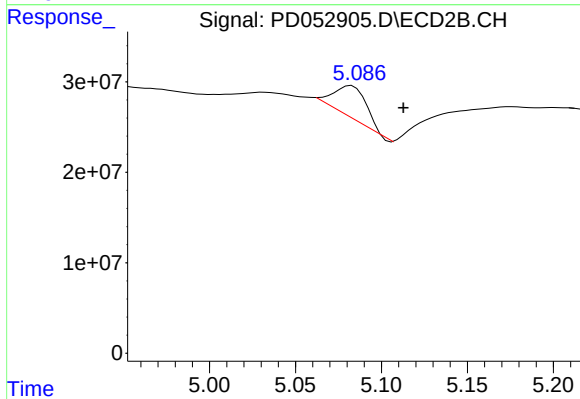

#7 delta-BHC


R.T.: 5.083 min
Delta R.T.: -0.030 min
Response: 46850373
Conc: 1.30 ng/ml

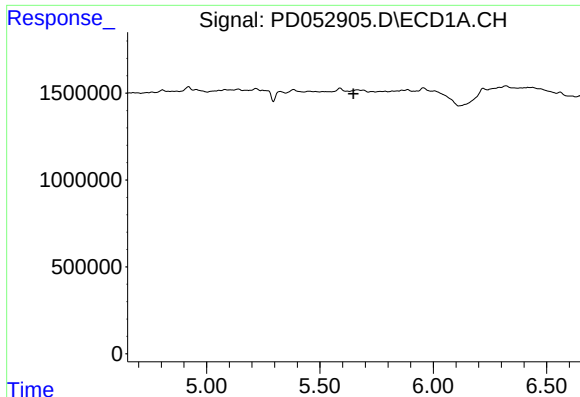

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
BF887

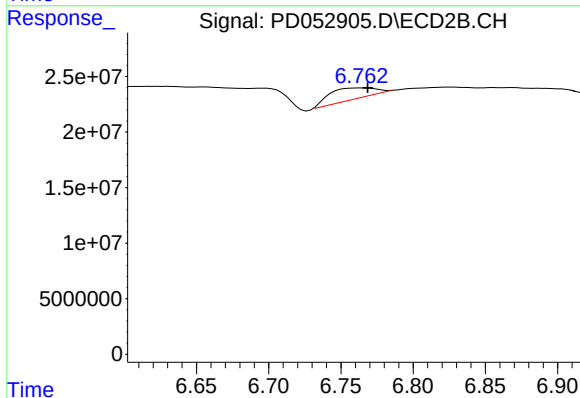


#14 Endrin

R.T.: 6.764 min
Delta R.T.: -0.005 min
Response: 21845397
Conc: 0.86 ng/ml

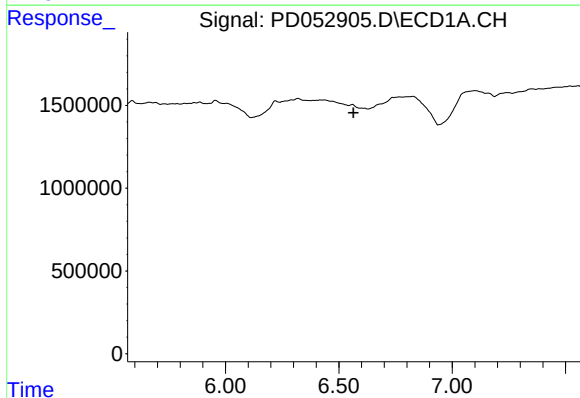


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.565 min
Response: 0
Conc: N.D.

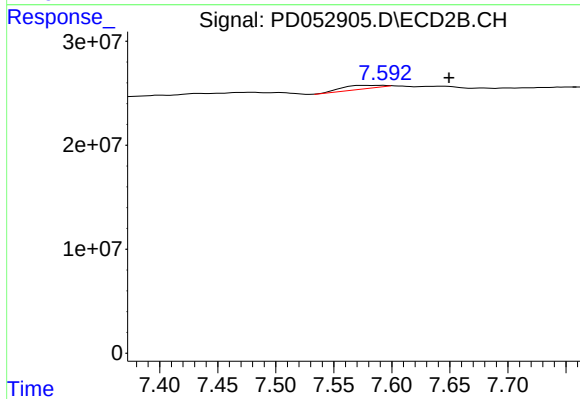

#20 Methoxychlor


R.T.: 7.593 min
Delta R.T.: -0.056 min
Response: 9539086
Conc: 1.00 ng/ml

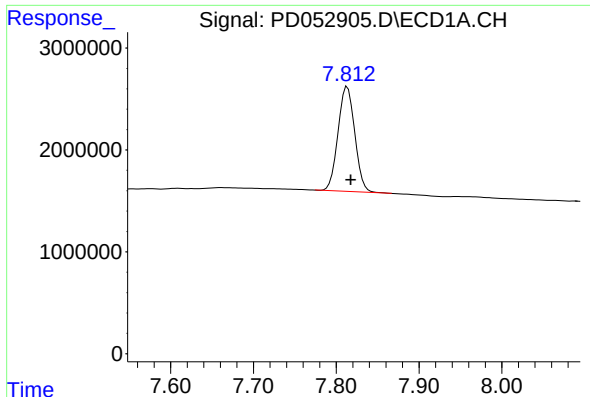

#27 Decachlorobiphenyl

R.T.: 7.813 min
Delta R.T.: -0.004 min
Response: 14484790
Conc: 10.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
BF887

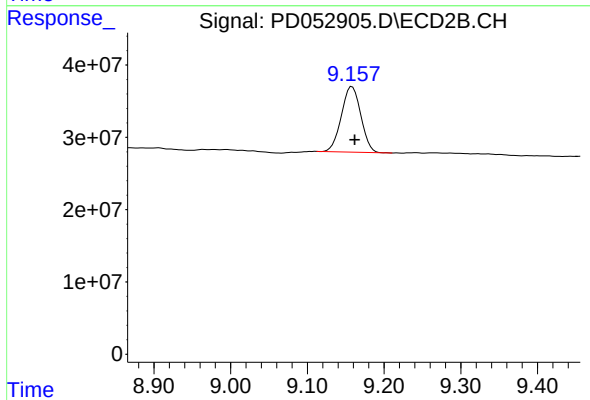

#27 Decachlorobiphenyl

R.T.: 9.158 min
Delta R.T.: -0.004 min
Response: 159891452
Conc: 11.09 ng/ml