

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041221\
 Data File : PD062111.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 12:19
 Operator : AR\AJ
 Sample : M1881-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQG8

Manual Integrations
 APPROVED

Ankita
 4/13/2021 1:22:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:17:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 05:02:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	10095747	107.2E6	10.314	10.741
27)	SA Decachlor...	8.257	9.039	35562538	144.6E6	26.521	15.706m#
Target Compounds							
3)	MA gamma-BHC...	4.215	4.633	9058929	52659176	6.506	3.540m#
10)	B trans-Chl...	5.429	6.073	967659	401.1E6	0.705m	28.964 #
11)	B cis-Chlor...	5.500	6.151	2739778	15499296	2.030	1.202m#
15)	B Endosulfa...	6.323	6.887	3251220	30999777	2.903m	3.055
16)	A 4,4'-DDD	6.176	6.801	5171956	85665862	4.738m	8.167 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041221\
Data File : PD062111.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 12:19
Operator : AR\AJ
Sample : M1881-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:17:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 05:02:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

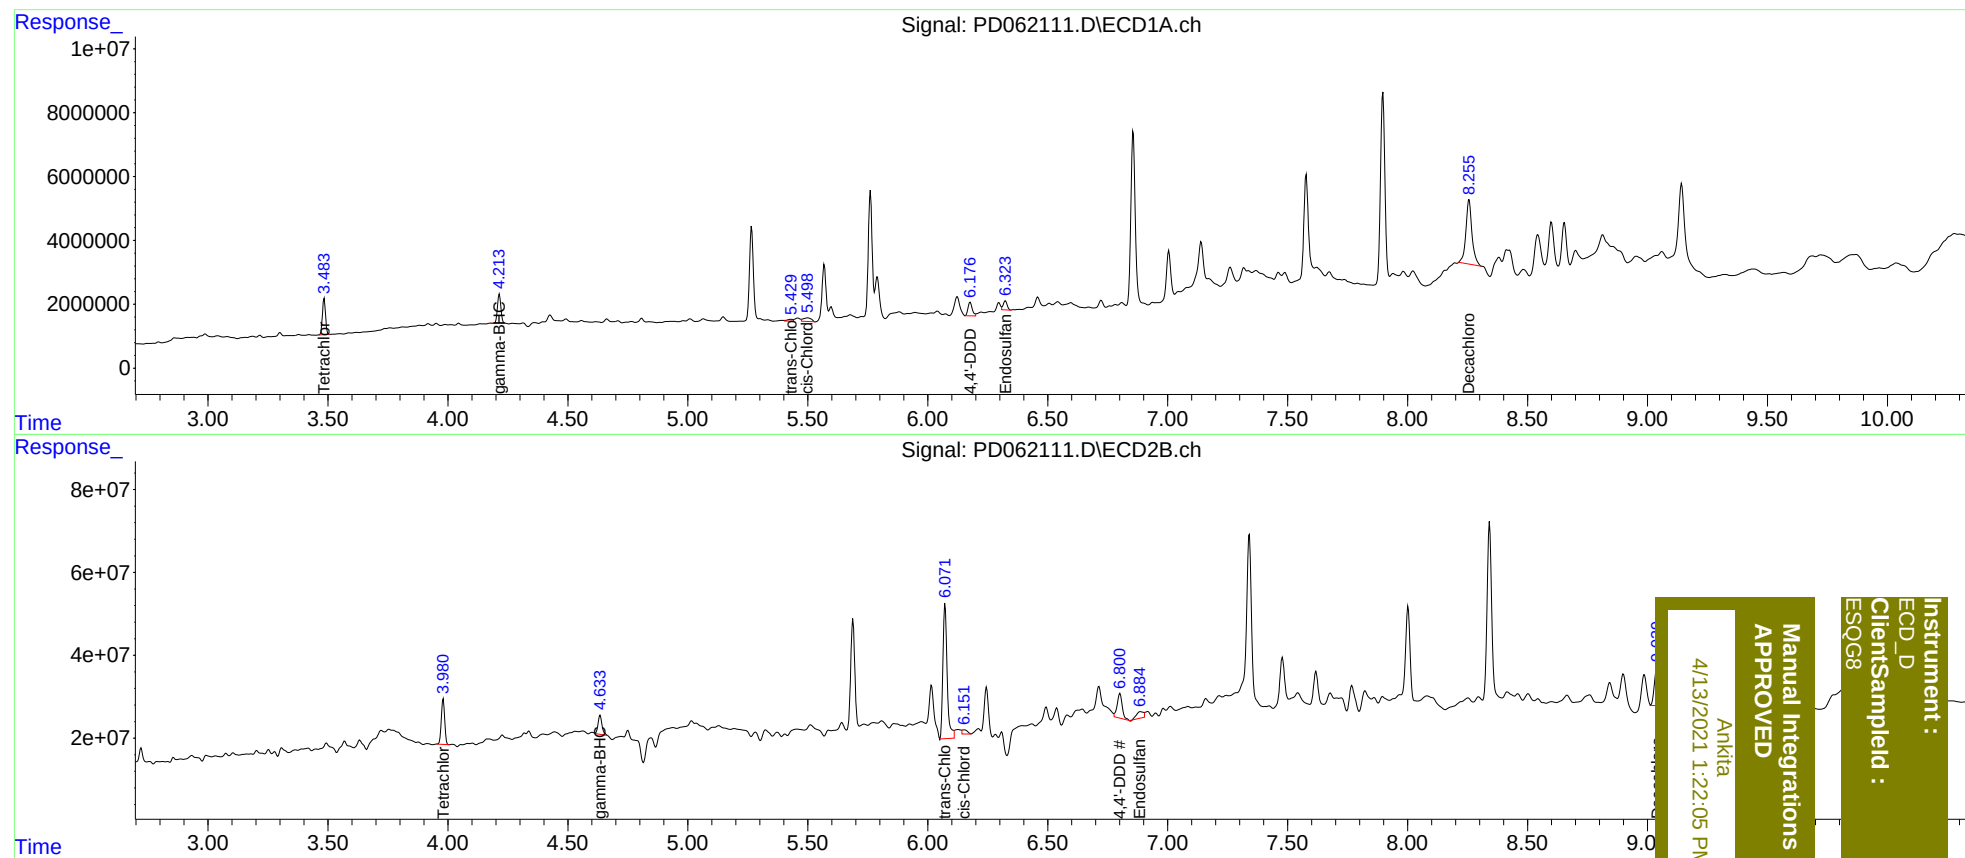

4/13/2021 1:22:05 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSample :
ESQ68