

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041221\
 Data File : PD062112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2021 12:47
 Operator : AR\AJ
 Sample : M1881-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQG9

Manual Integrations
 APPROVED

Ankita
 4/13/2021 1:22:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 01:18:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 03 05:02:01 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.485	3.981	10116857	99398559	10.336	9.960
2)	SA Decachlor...	8.256	9.040	34127117	182.4E6	25.451	19.810m
Target Compounds							
3)	MA gamma-BHC...	4.215	4.634	9606111	59783424	6.899	4.019m#
11)	B cis-Chlor...	5.506	6.156	1681685	16325201	1.246	1.266m
15)	B Endosulfa...	6.323	6.884	4693723	20607465	4.191m	2.031 #
16)	A 4,4'-DDD	6.176	6.802	3480723	73680036	3.189m	7.024 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041221\
Data File : PD062112.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2021 12:47
Operator : AR\AJ
Sample : M1881-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 01:18:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040321CLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 03 05:02:01 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

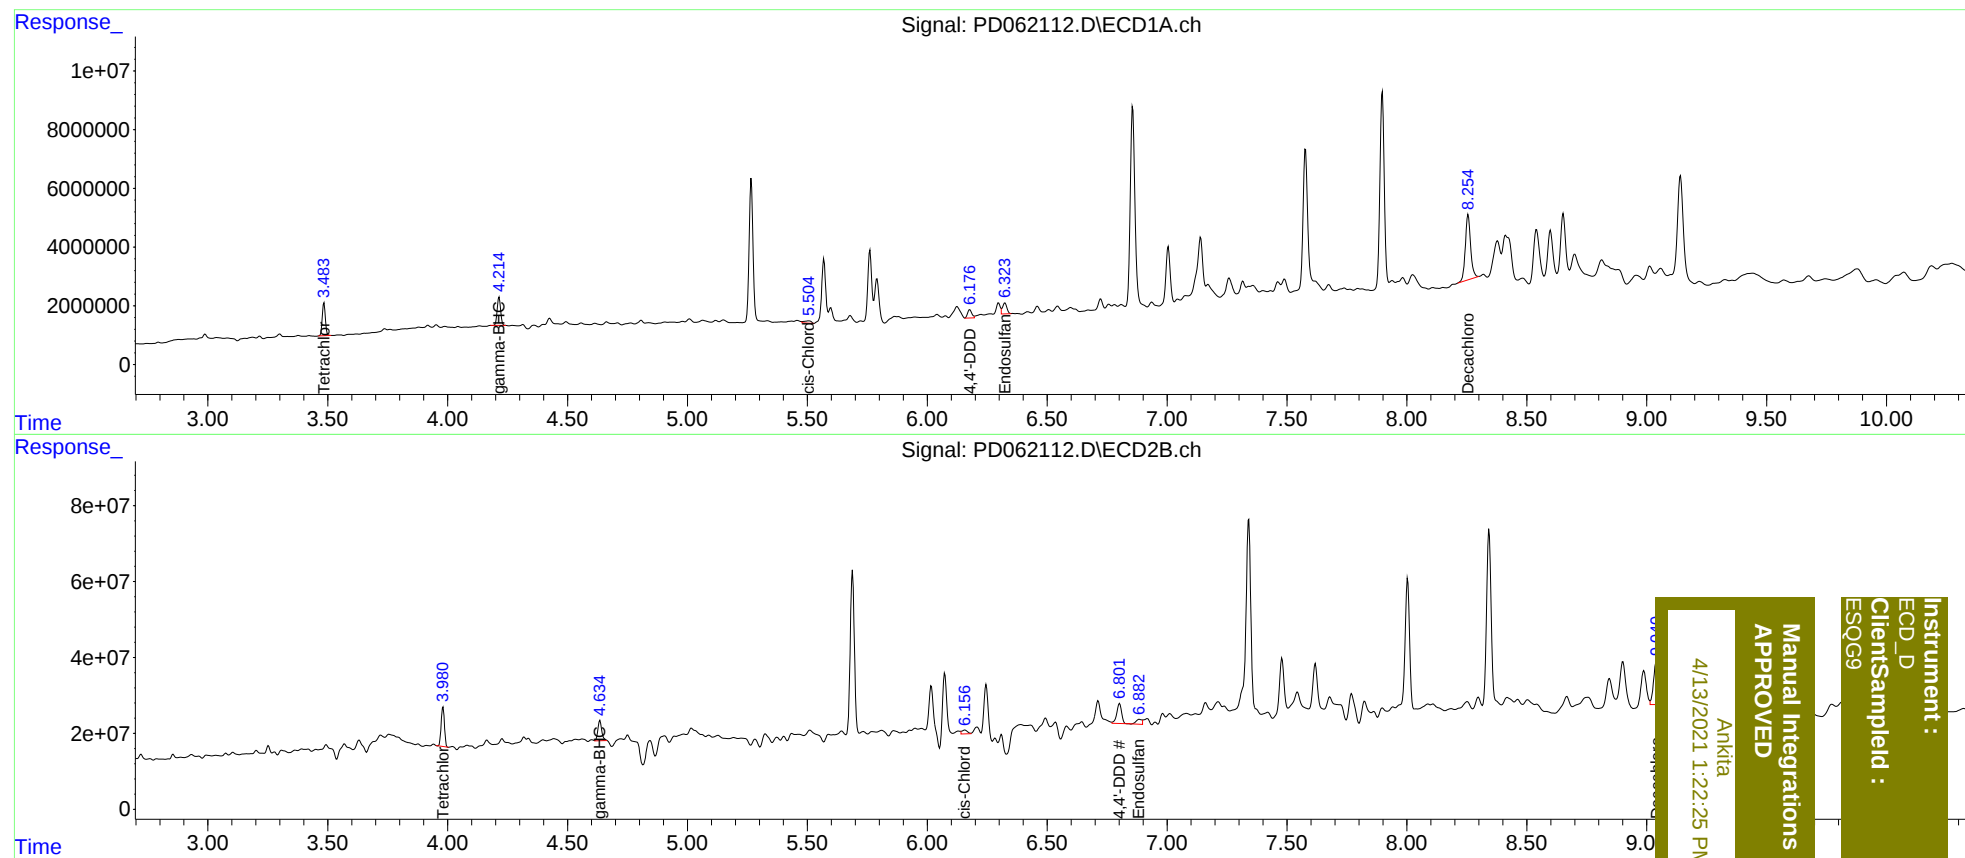

4/13/2021 1:22:25 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSample :
ESQ69