

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
 Data File : PD069070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 11:53
 Operator : AR\AJ
 Sample : PB144002BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 00:49:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.171	19564395	193.5E6	14.367	17.677
27)	SA Decachlor...	8.202	9.366	43056645	234.6E6	30.964	37.197
Target Compounds							
4)	MA Heptachlor	0.000	5.341f	0	777266	N.D.	<MDL
10)	B trans-Chl...	0.000	6.355	0	9504046	N.D.	0.799
11)	B cis-Chlor...	0.000	6.355f	0	9504046	N.D.	0.829
12)	B 4,4'-DDE	0.000	6.562	0	1638935	N.D.	0.160
13)	MA Dieldrin	0.000	6.707	0	560673	N.D.	<MDL
15)	B Endosulfa...	6.221f	0.000	2900761	0	2.000	N.D. #
18)	B Endrin al...	0.000	7.216f	0	252844	N.D.	<MDL
20)	A Methoxychlor	0.000	7.741f	0	2405220	N.D.	0.687
22)	Toxaphene-1	0.000	6.562f	0	1638935	N.D.	38.516
23)	Toxaphene-2	6.221	6.746f	2900761	1449086	270.486	14.393 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
Data File : PD069070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 11:53
Operator : AR\AJ
Sample : PB144002BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:49:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

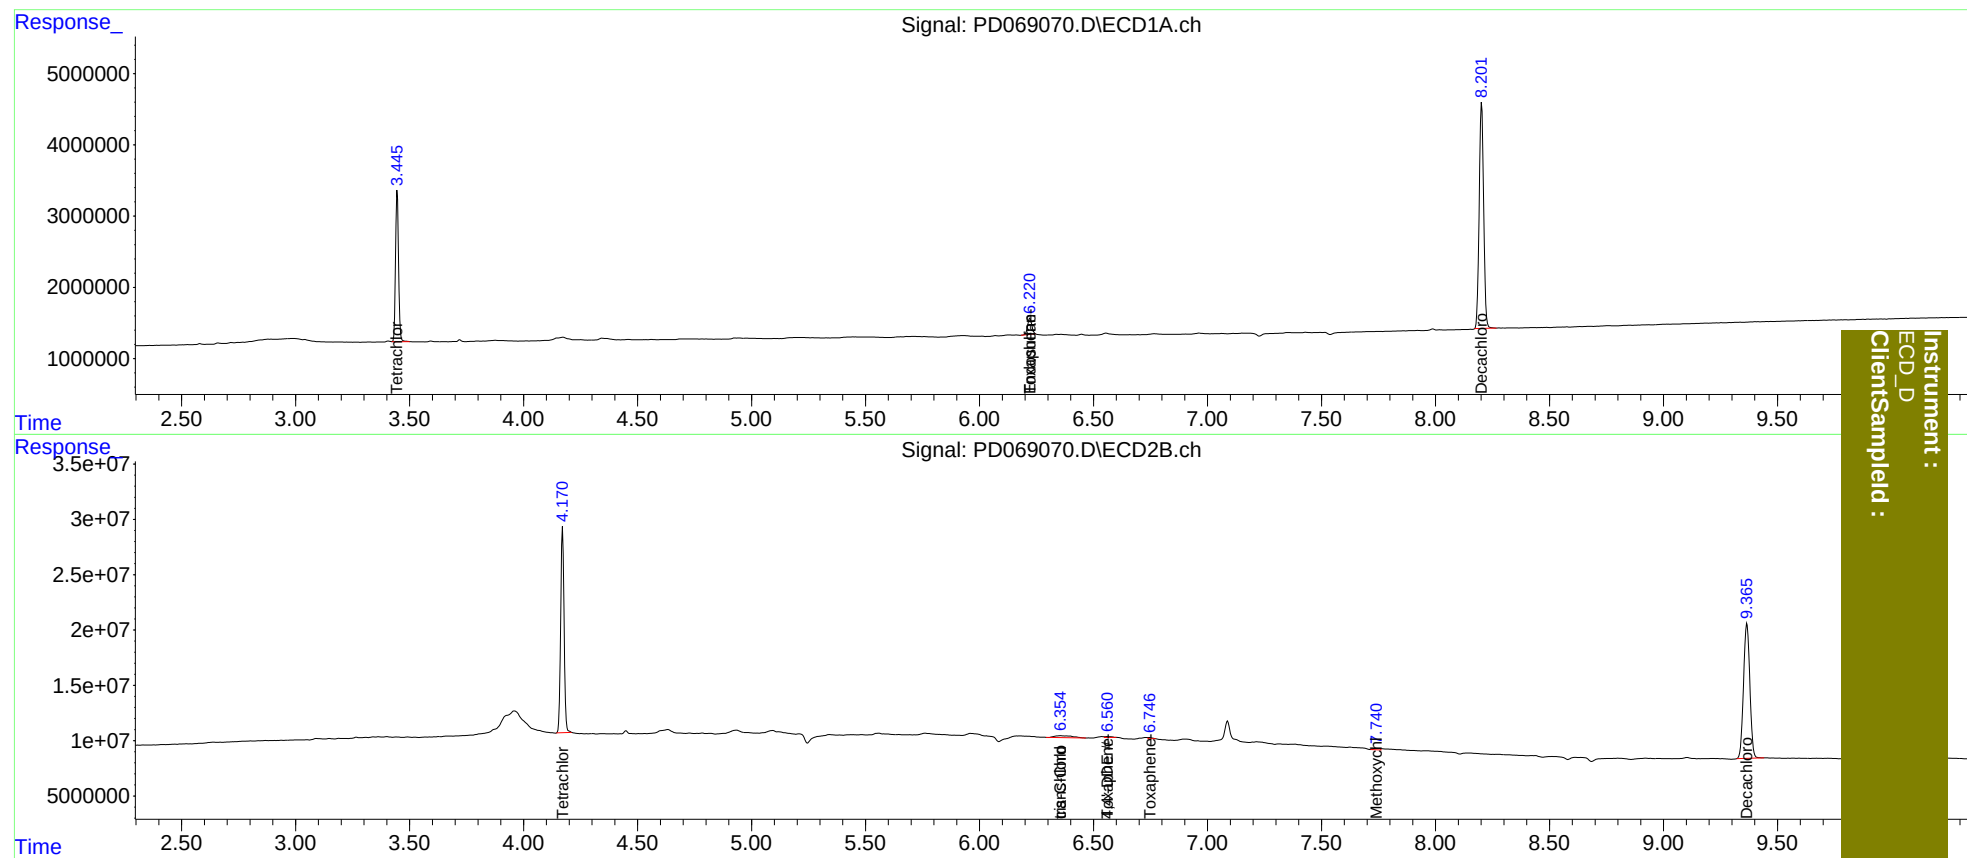


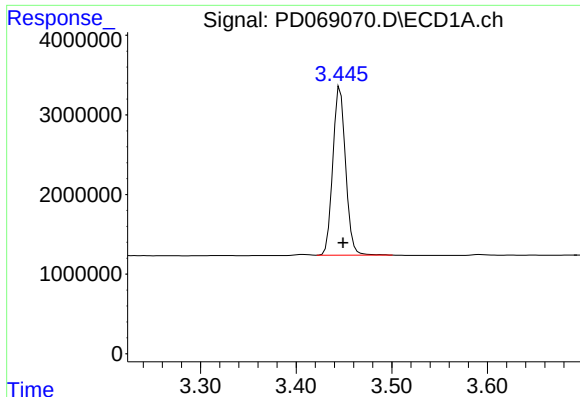

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.003 min
Response: 19564395
Conc: 14.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

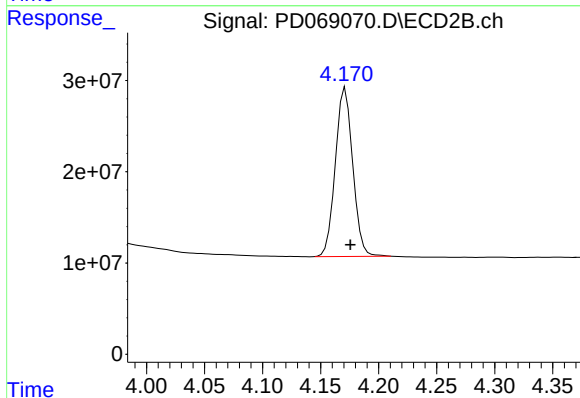


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: -0.004 min
Response: 193483911
Conc: 17.68 ng/ml

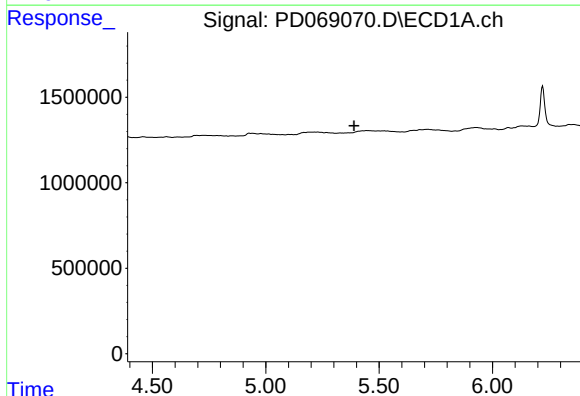


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.389 min
Response: 0
Conc: N.D.

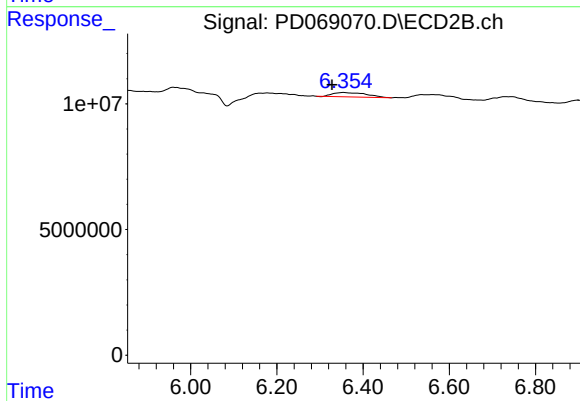

#10 trans-Chlordane


R.T.: 6.355 min
Delta R.T.: 0.027 min
Response: 9504046
Conc: 0.80 ng/ml

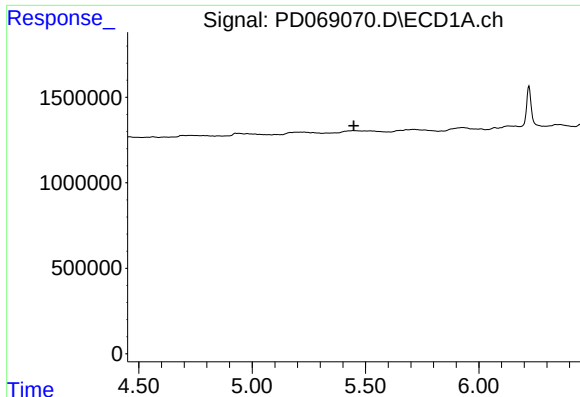

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

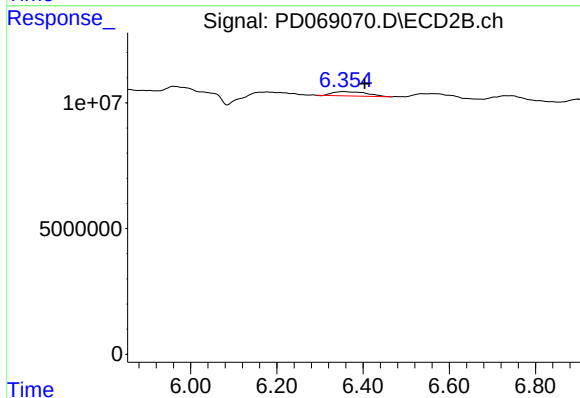


#11 cis-Chlordane

R.T.: 6.355 min
Delta R.T.: -0.049 min
Response: 9504046
Conc: 0.83 ng/ml

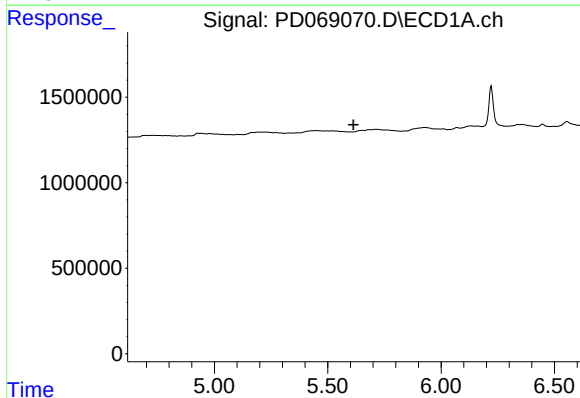


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.614 min
Response: 0
Conc: N.D.

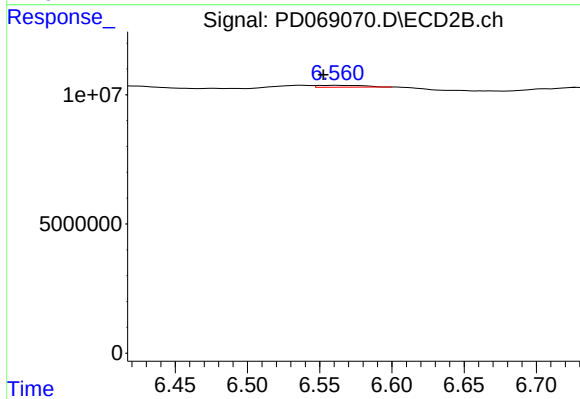

#12 4,4'-DDE


R.T.: 6.562 min
Delta R.T.: 0.009 min
Response: 1638935
Conc: 0.16 ng/ml

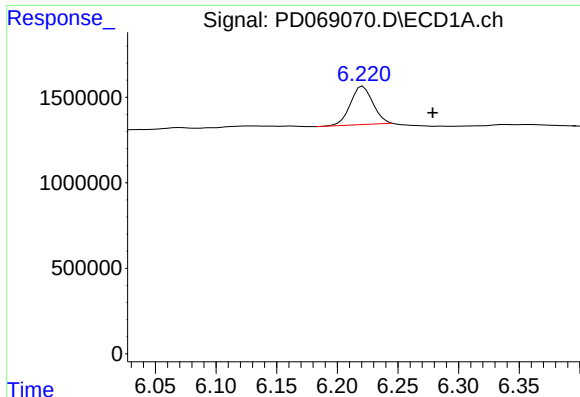

#15 Endosulfan II


R.T.: 6.221 min
Delta R.T.: -0.057 min
Response: 2900761
Conc: 2.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

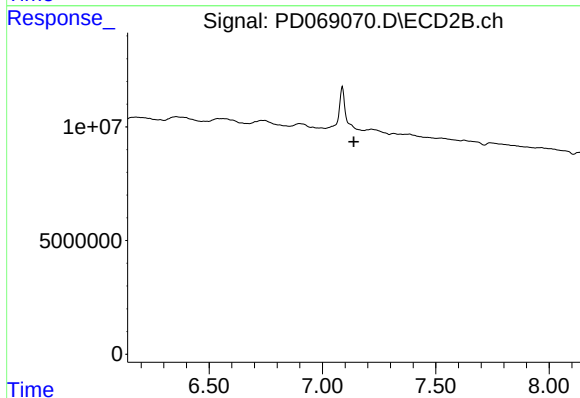


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.138 min
Response: 0
Conc: N.D.

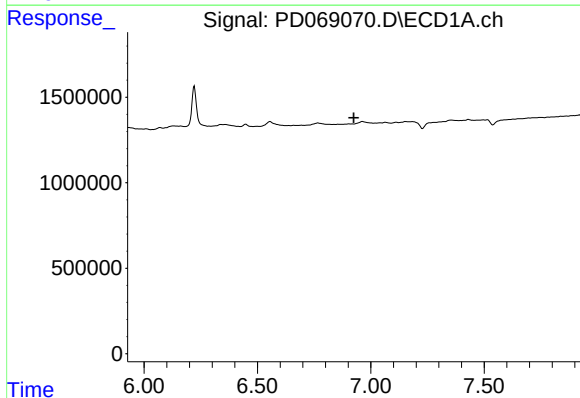


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

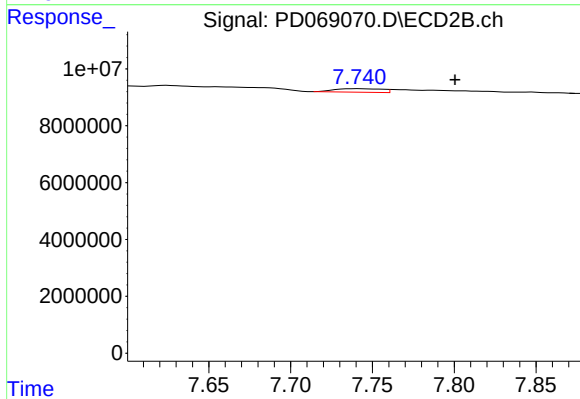

#20 Methoxychlor


R.T.: 7.741 min
Delta R.T.: -0.060 min
Response: 2405220
Conc: 0.69 ng/ml

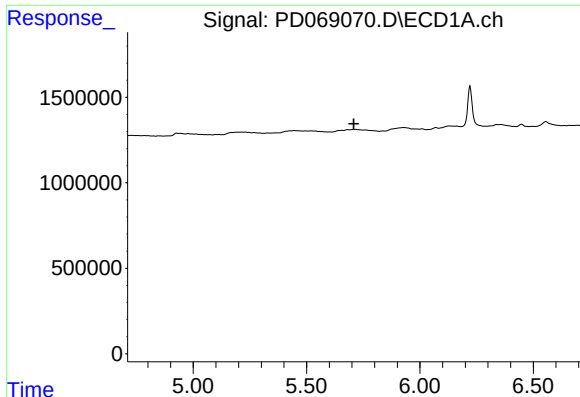

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

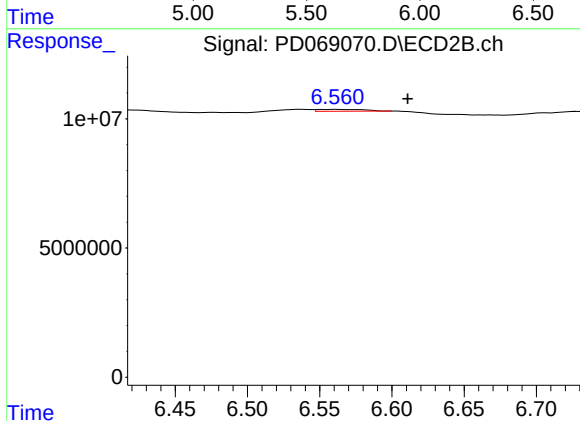


#22 Toxaphene-1

R.T.: 6.562 min
Delta R.T.: -0.049 min
Response: 1638935
Conc: 38.52 ng/ml

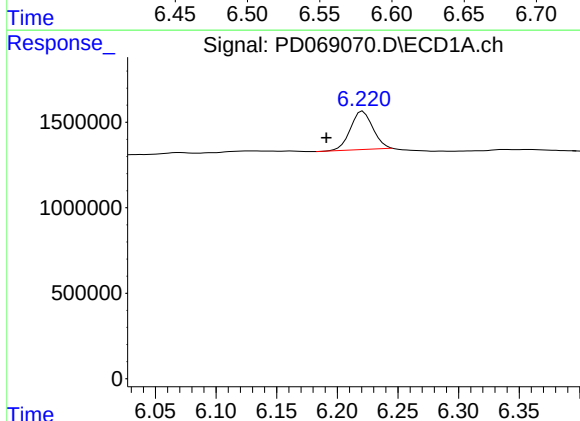


#23 Toxaphene-2

R.T.: 6.221 min
Delta R.T.: 0.030 min
Response: 2900761
Conc: 270.49 ng/ml

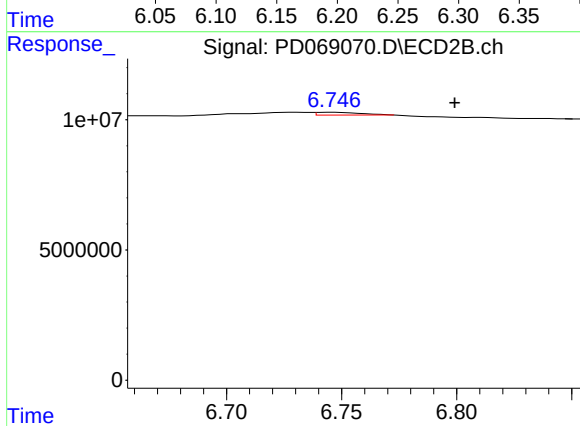

#23 Toxaphene-2


R.T.: 6.746 min
Delta R.T.: -0.053 min
Response: 1449086
Conc: 14.39 ng/ml

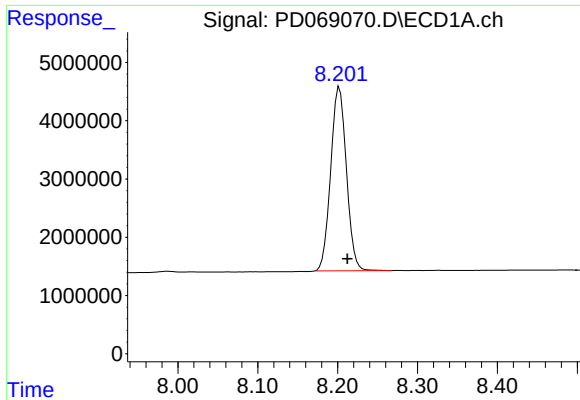

#27 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.010 min
Response: 43056645
Conc: 30.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

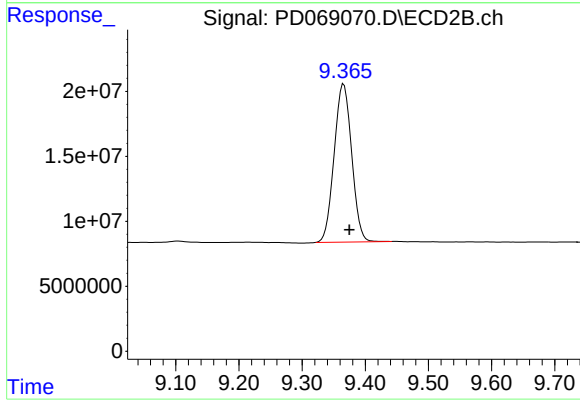

#27 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.009 min
Response: 234606192
Conc: 37.20 ng/ml