

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
 Data File : PD069076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 13:27
 Operator : AR\AJ
 Sample : I.BLK262
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 00:51:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.172	24341894	236.4E6	17.875	21.596
2)	SA Decachlor...	8.202	9.366	52221497	282.6E6	37.555	44.808
Target Compounds							
3)	MA gamma-BHC...	0.000	4.816f	0	847810	N.D.	<MDL
5)	MB Aldrin	0.000	5.752f	0	1036445	N.D.	<MDL
7)	B delta-BHC	0.000	5.221f	0	10120786	N.D.	0.715
8)	B Heptachlo...	0.000	6.104	0	2662346	N.D.	0.221
9)	A Endosulfan I	0.000	6.453	0	1031376	N.D.	<MDL
10)	B trans-Chl...	0.000	6.341	0	9575594	N.D.	0.805
11)	B cis-Chlor...	0.000	6.439f	0	823841	N.D.	<MDL
12)	B 4,4'-DDE	0.000	6.549	0	2144751	N.D.	0.210
13)	MA Dieldrin	0.000	6.719	0	511865	N.D.	<MDL
15)	B Endosulfa...	6.222f	0.000	2559954	0	1.765	N.D. #
17)	MA 4,4'-DDT	0.000	7.366	0	4693564	N.D.	0.596
20)	A Methoxychlor	0.000	7.752f	0	8348726	N.D.	2.383
22)	Toxaphene-1	0.000	6.615	0	1150885	N.D.	27.047
23)	Toxaphene-2	6.222	0.000	2559954	0	238.706	N.D. #
24)	Toxaphene-3	0.000	7.366	0	4693564	N.D.	21.143


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
Data File : PD069076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 13:27
Operator : AR\AJ
Sample : I.BLK262
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:51:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

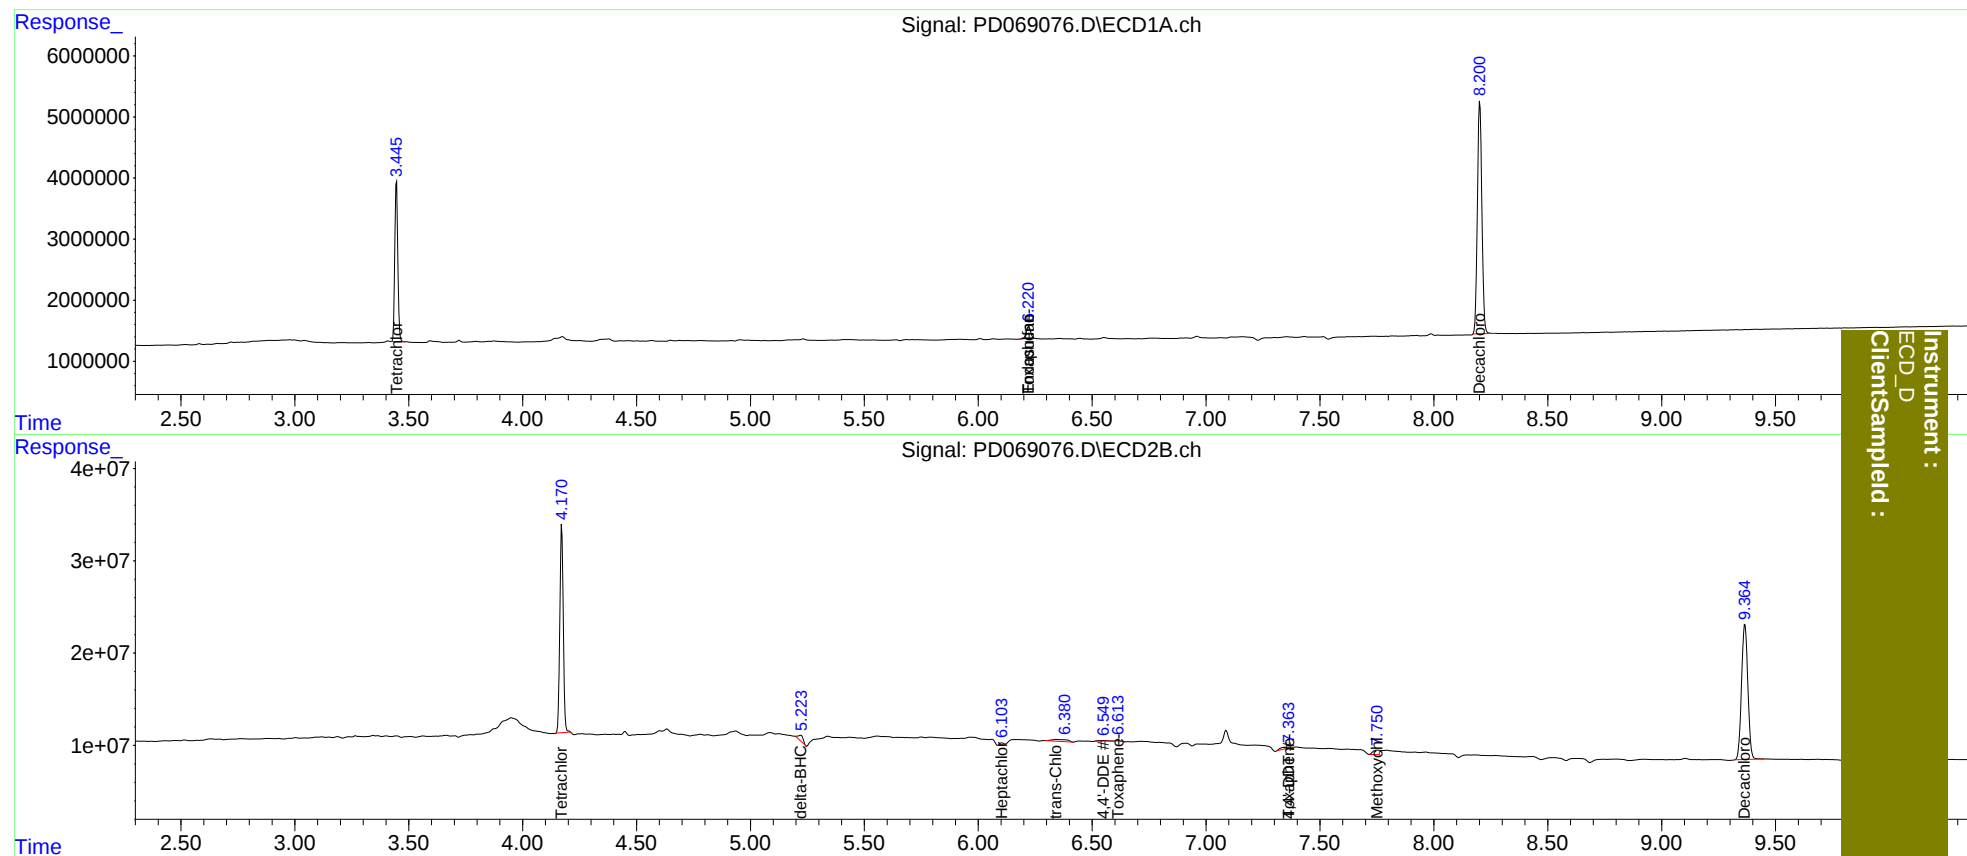


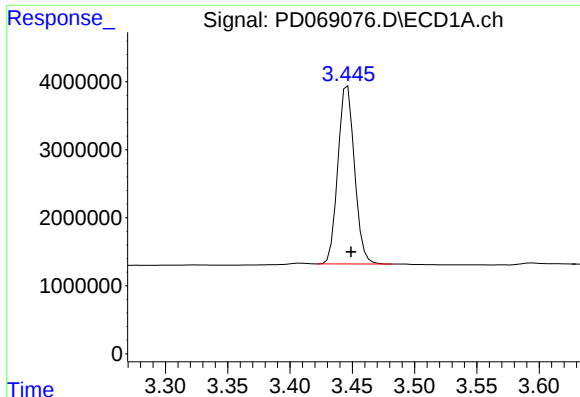

#1 Tetrachloro-m-xylene


R.T.: 3.446 min
Delta R.T.: -0.003 min
Response: 24341894
Conc: 17.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

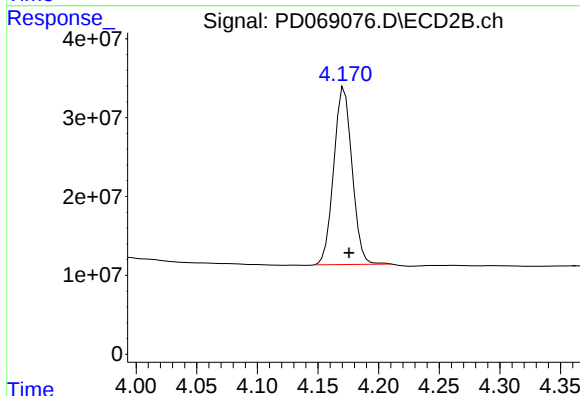


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.004 min
Response: 236376716
Conc: 21.60 ng/ml

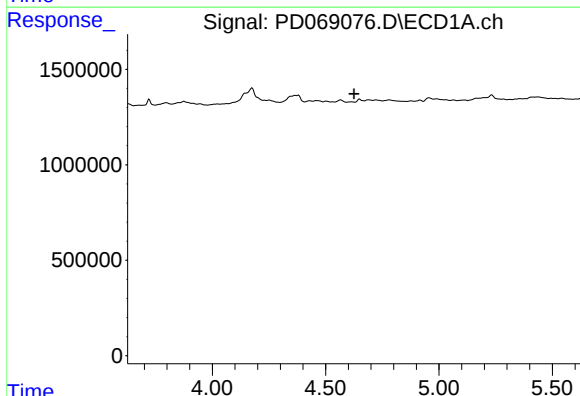


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.625 min
Response: 0
Conc: N.D.

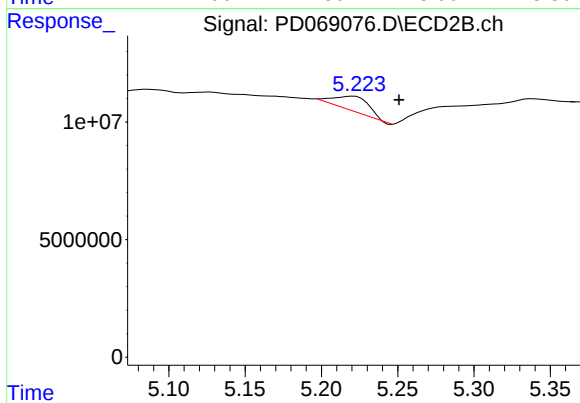

#7 delta-BHC


R.T.: 5.221 min
Delta R.T.: -0.030 min
Response: 10120786
Conc: 0.71 ng/ml

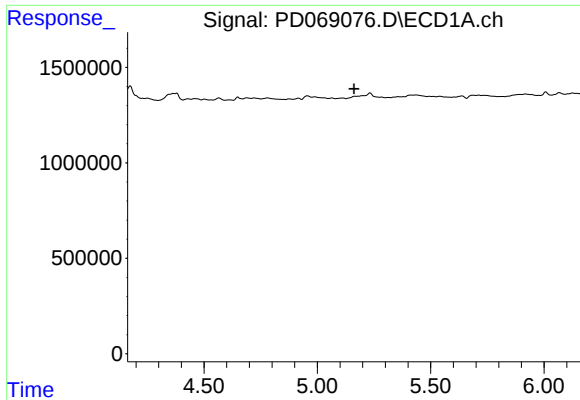

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

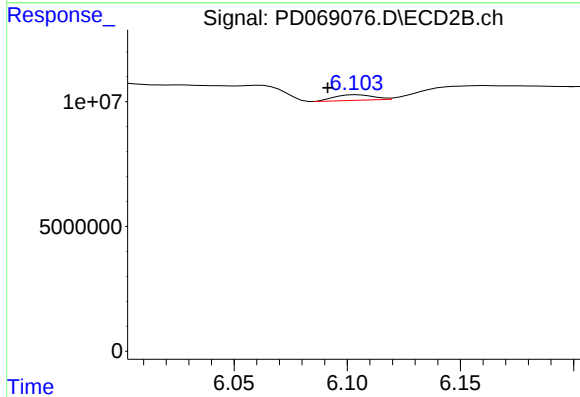


#8 Heptachlor epoxide

R.T.: 6.104 min
Delta R.T.: 0.013 min
Response: 2662346
Conc: 0.22 ng/ml

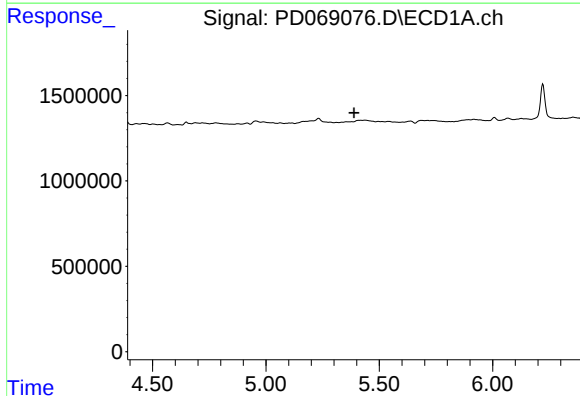


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

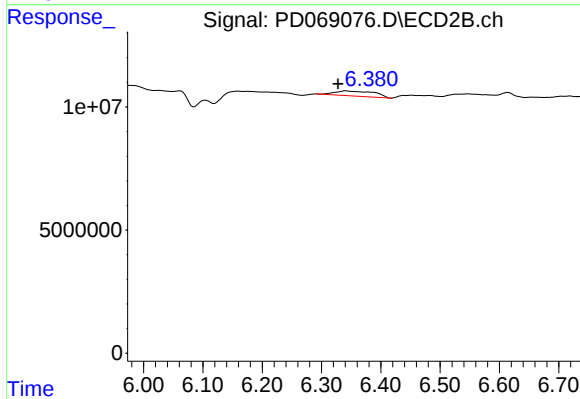

#10 trans-Chlordane


R.T.: 6.341 min
Delta R.T.: 0.013 min
Response: 9575594
Conc: 0.81 ng/ml

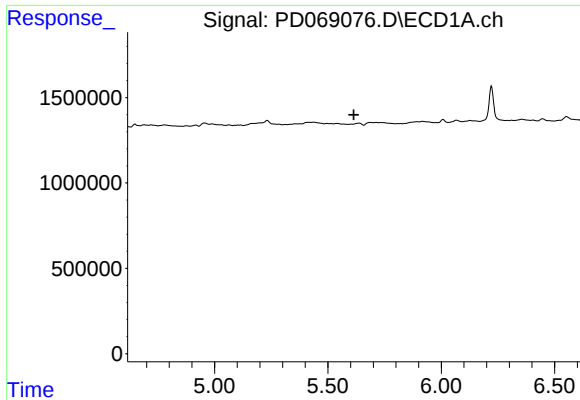

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.614 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

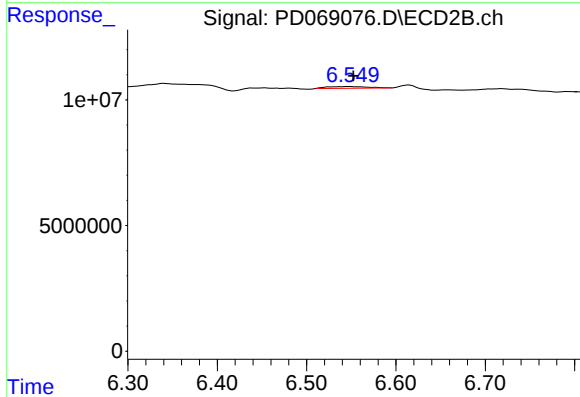


#12 4,4'-DDE

R.T.: 6.549 min
Delta R.T.: -0.003 min
Response: 2144751
Conc: 0.21 ng/ml

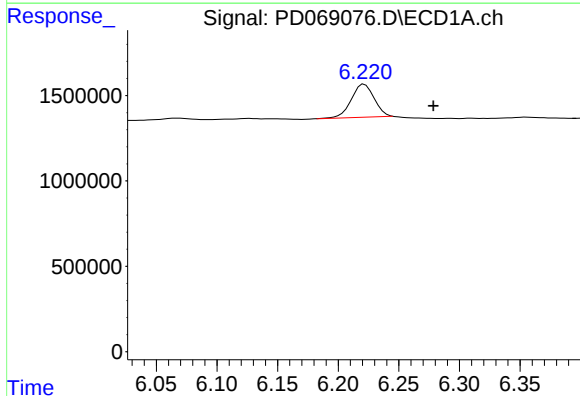


#15 Endosulfan II

R.T.: 6.222 min
Delta R.T.: -0.057 min
Response: 2559954
Conc: 1.76 ng/ml

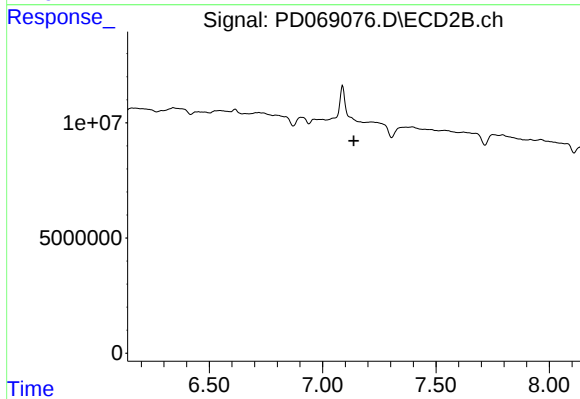

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.138 min
Response: 0
Conc: N.D.

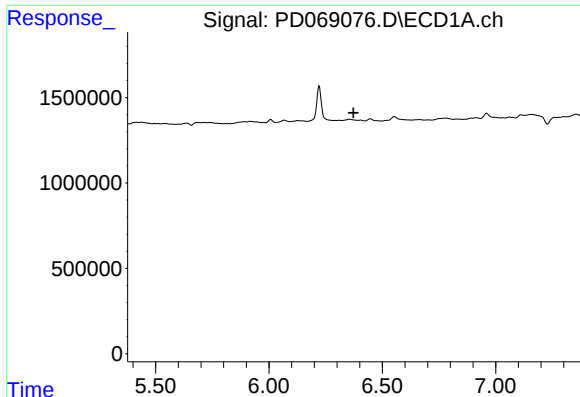

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.373 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

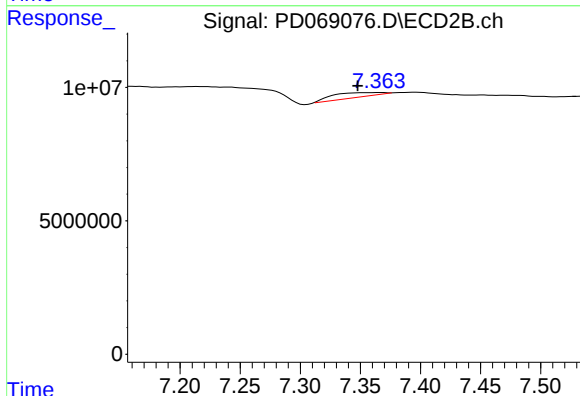


#17 4,4'-DDT

R.T.: 7.366 min
Delta R.T.: 0.019 min
Response: 4693564
Conc: 0.60 ng/ml

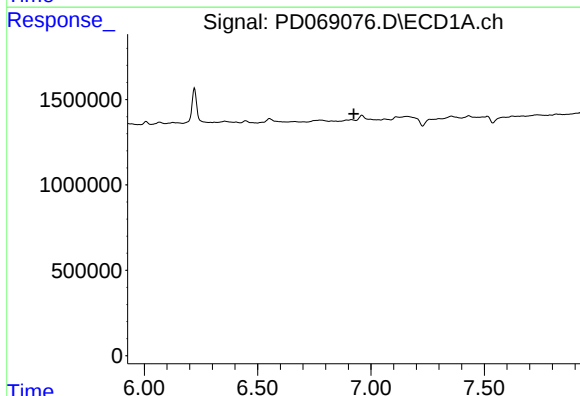


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

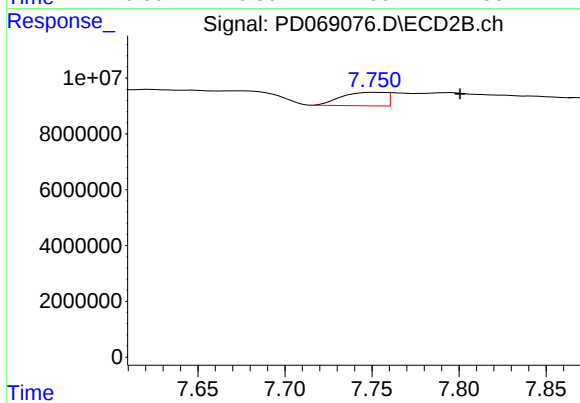

#20 Methoxychlor


R.T.: 7.752 min
Delta R.T.: -0.049 min
Response: 8348726
Conc: 2.38 ng/ml

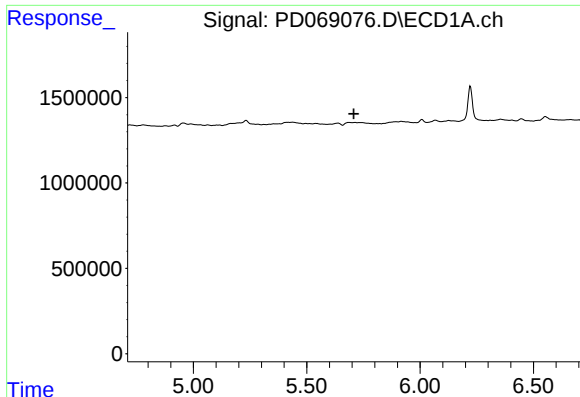

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

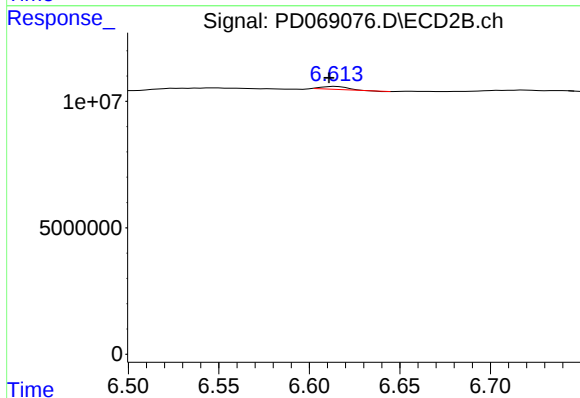


#22 Toxaphene-1

R.T.: 6.615 min
Delta R.T.: 0.004 min
Response: 1150885
Conc: 27.05 ng/ml

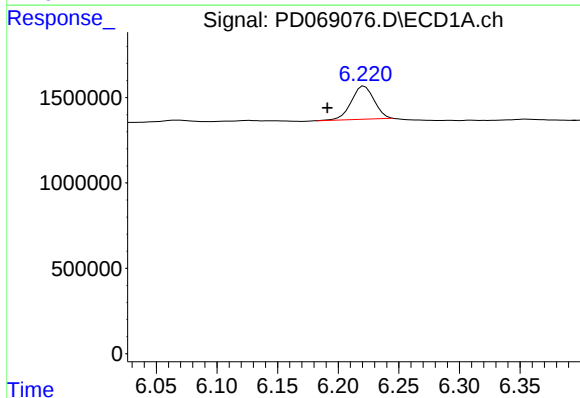


#23 Toxaphene-2

R.T.: 6.222 min
Delta R.T.: 0.031 min
Response: 2559954
Conc: 238.71 ng/ml

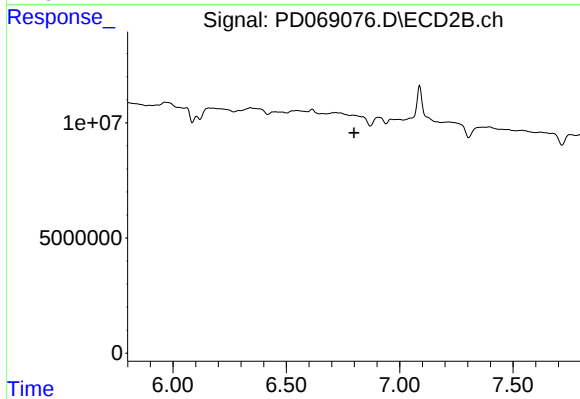

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 6.799 min
Response: 0
Conc: N.D.

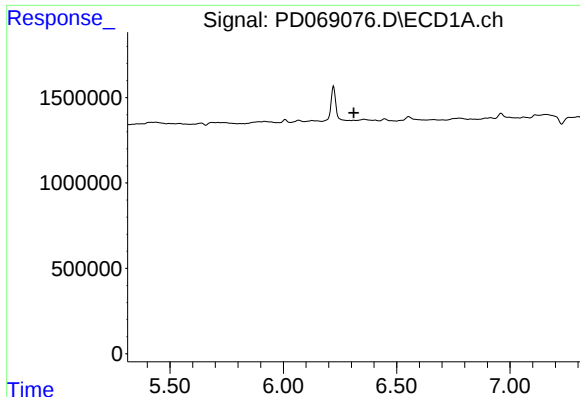

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T.: 6.311 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

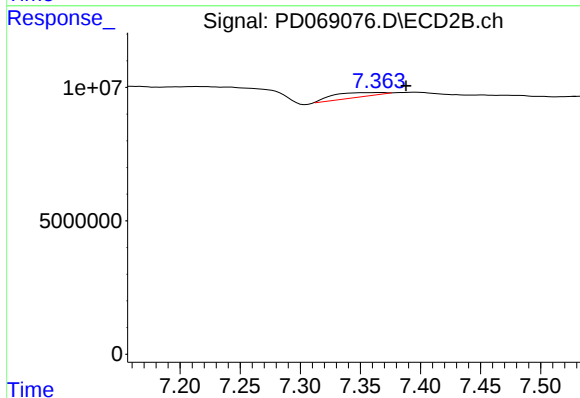


#24 Toxaphene-3

R.T.: 7.366 min
Delta R.T.: -0.022 min
Response: 4693564
Conc: 21.14 ng/ml

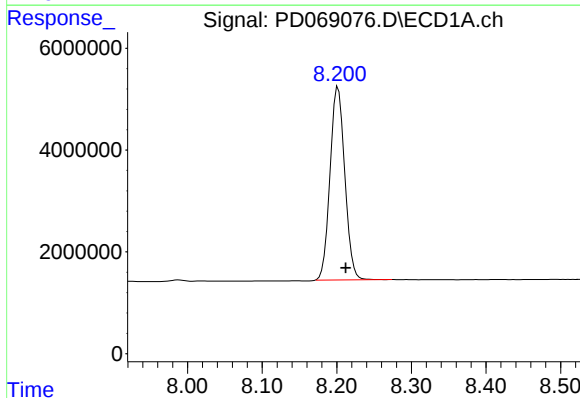

#27 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.010 min
Response: 52221497
Conc: 37.55 ng/ml

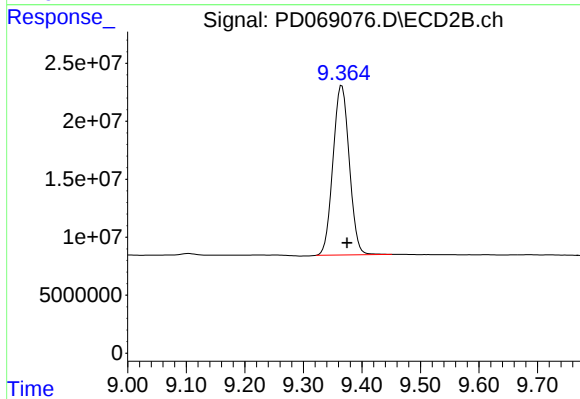

#27 Decachlorobiphenyl

R.T.: 9.366 min
Delta R.T.: -0.009 min
Response: 282612963
Conc: 44.81 ng/ml