

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
 Data File : PD069078.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 16:33
 Operator : AR\AJ
 Sample : PB144045BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 00:52:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	4.172	18329051	188.0E6	13.460	17.172 #
27)	SA Decachlor...	8.214	9.371	41672534	241.3E6	29.968	38.257 #
Target Compounds							
4)	MA Heptachlor	0.000	5.348f	0	877231	N.D.	<MDL
7)	B delta-BHC	0.000	5.227	0	2883711	N.D.	0.204
8)	B Heptachlo...	0.000	6.044f	0	374857	N.D.	<MDL
10)	B trans-Chl...	0.000	6.283f	0	1767275	N.D.	0.149
11)	B cis-Chlor...	0.000	6.375	0	3031865	N.D.	0.264
12)	B 4,4'-DDE	0.000	6.543	0	3137804	N.D.	0.307
14)	MA Endrin	6.016	6.981f	-100129	4762338	N.D.	0.563
16)	A 4,4'-DDD	0.000	7.059	0	5787320	N.D.	0.690
18)	B Endrin al...	0.000	7.255	0	3671568	N.D.	0.553
19)	B Endosulfa...	0.000	7.527f	0	2345902	N.D.	0.286
20)	A Methoxychlor	0.000	7.845f	0	2613422	N.D.	0.746
22)	Toxaphene-1	0.000	6.543f	0	3137804	N.D.	73.741
25)	Toxaphene-4	0.000	7.527f	0	2345902	N.D.	17.559
26)	Toxaphene-5	0.000	7.845f	0	2613422	N.D.	29.826


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
Data File : PD069078.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 16:33
Operator : AR\AJ
Sample : PB144045BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:52:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

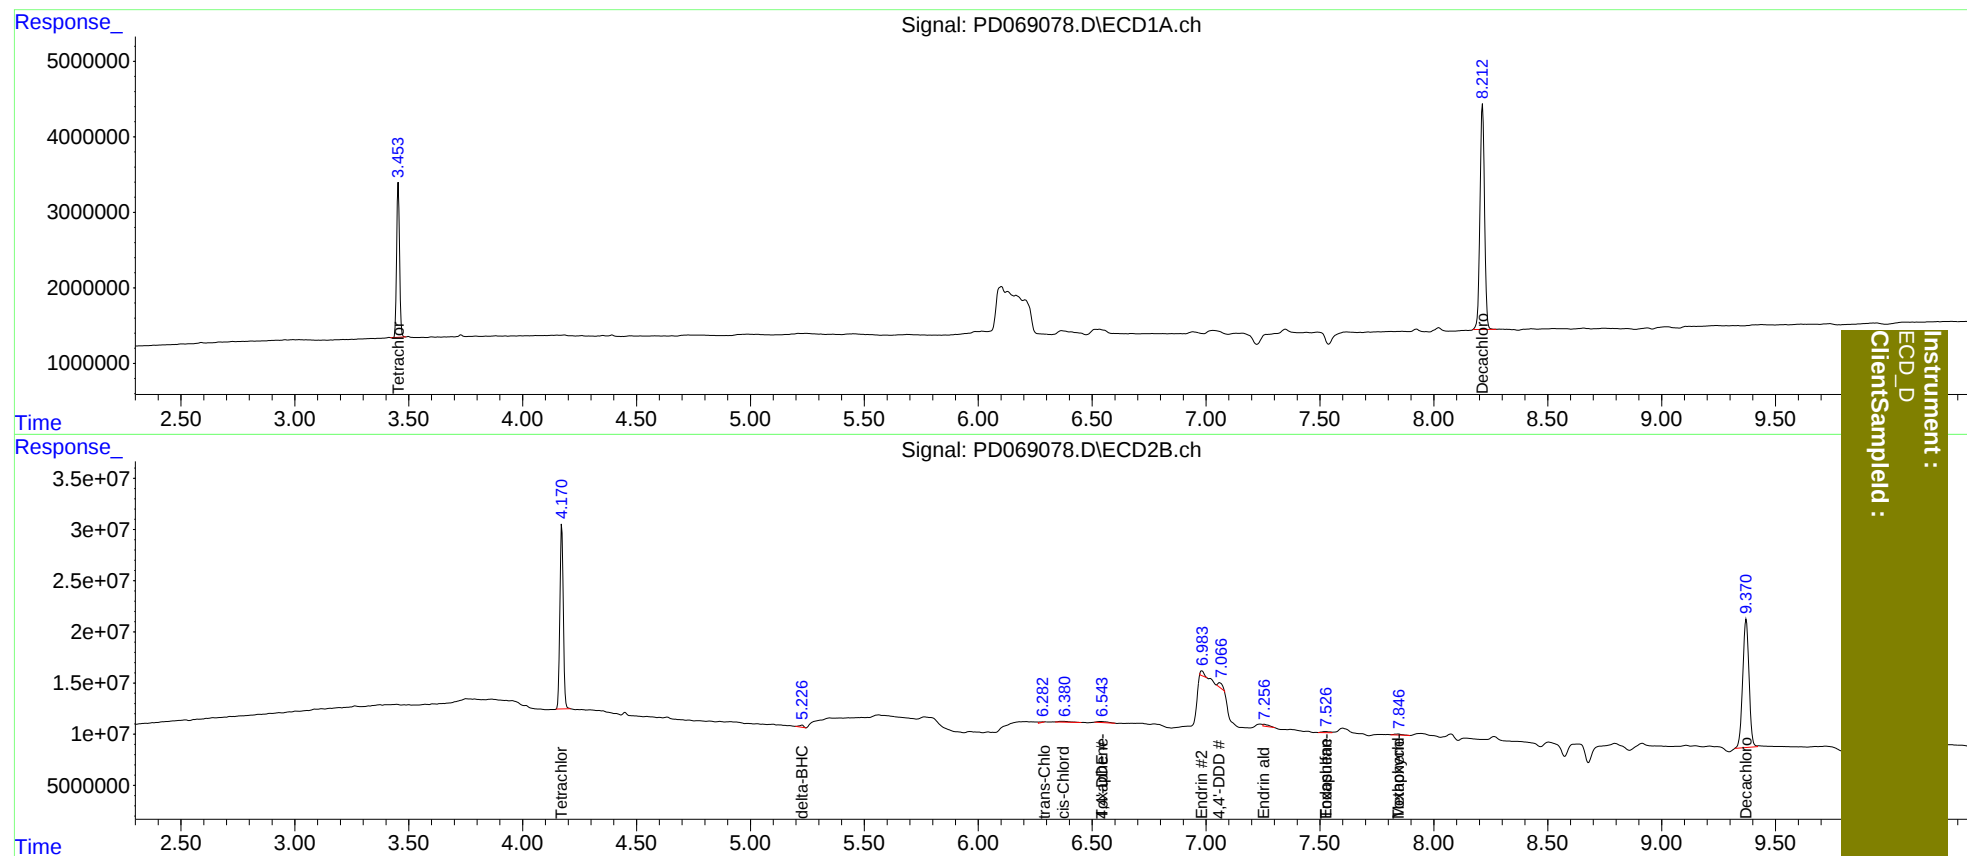


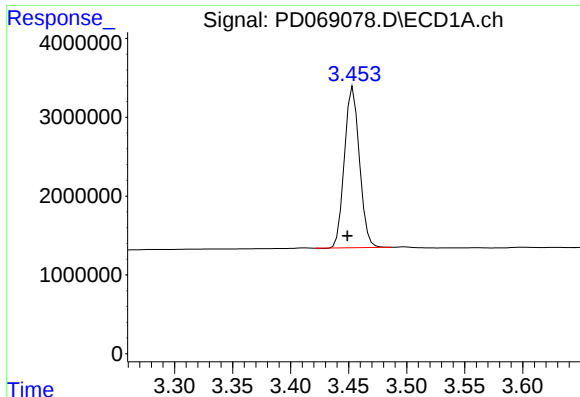

#1 Tetrachloro-m-xylene


R.T.: 3.454 min
Delta R.T.: 0.005 min
Response: 18329051
Conc: 13.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

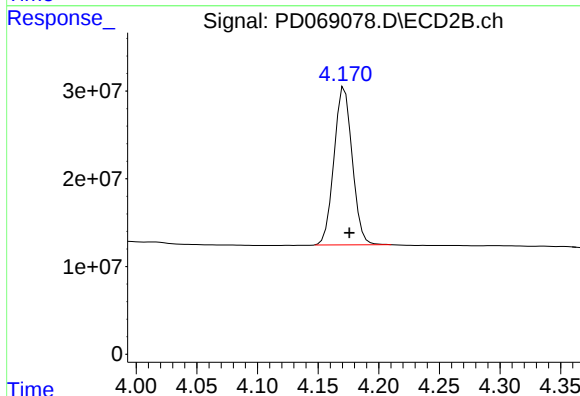


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: -0.004 min
Response: 187954050
Conc: 17.17 ng/ml

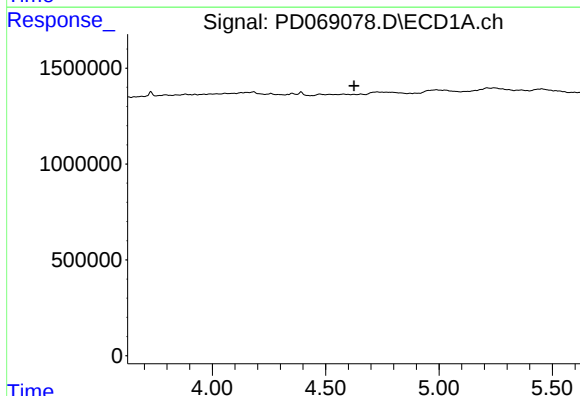


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.625 min
Response: 0
Conc: N.D.

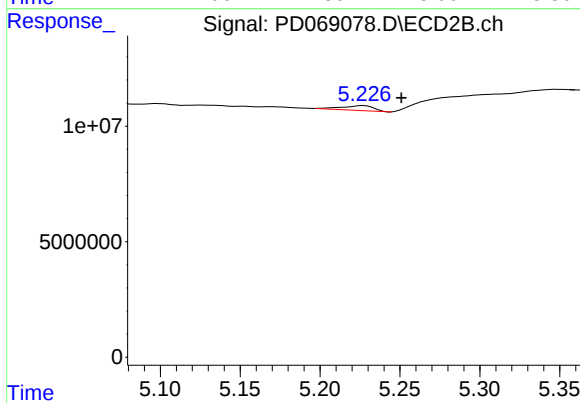

#7 delta-BHC


R.T.: 5.227 min
Delta R.T.: -0.024 min
Response: 2883711
Conc: 0.20 ng/ml

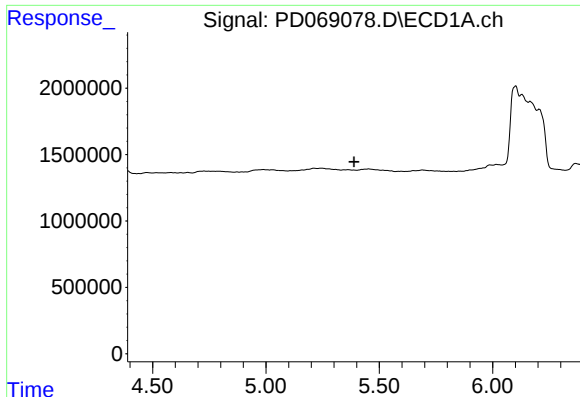

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

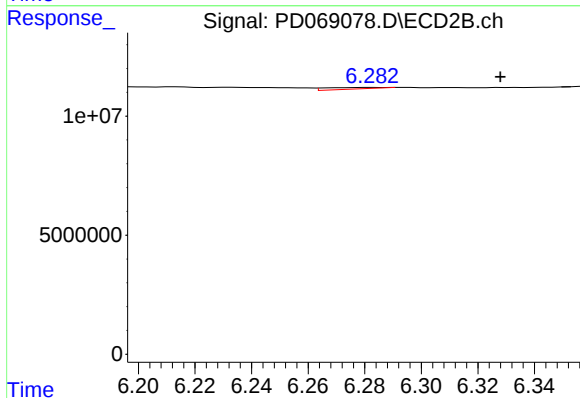


#10 trans-Chlordane

R.T.: 6.283 min
Delta R.T.: -0.045 min
Response: 1767275
Conc: 0.15 ng/ml

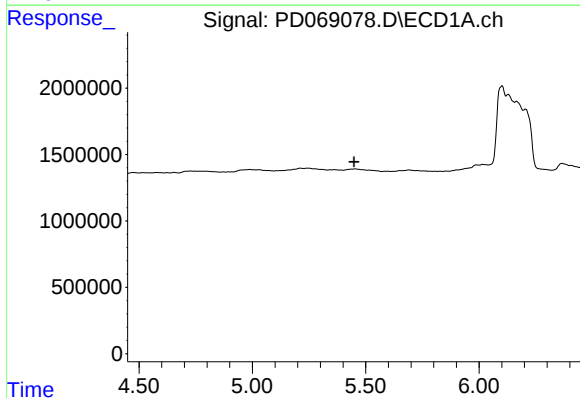


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.448 min
Response: 0
Conc: N.D.

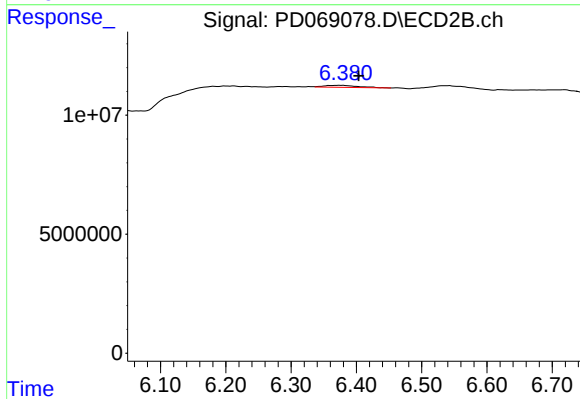

#11 cis-Chlordane


R.T.: 6.375 min
Delta R.T.: -0.028 min
Response: 3031865
Conc: 0.26 ng/ml

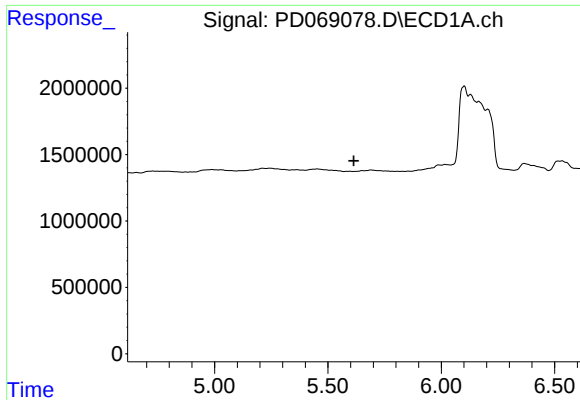

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.614 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

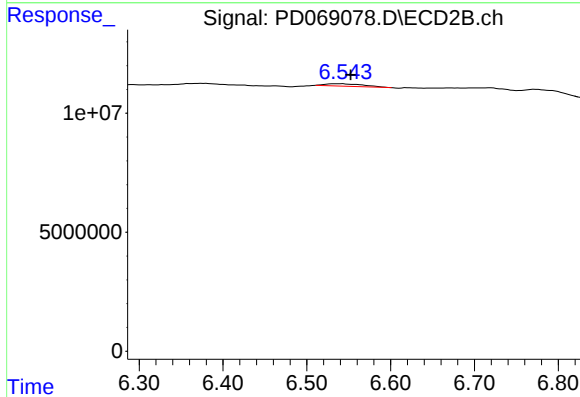


#12 4,4'-DDE

R.T.: 6.543 min
Delta R.T.: -0.009 min
Response: 3137804
Conc: 0.31 ng/ml

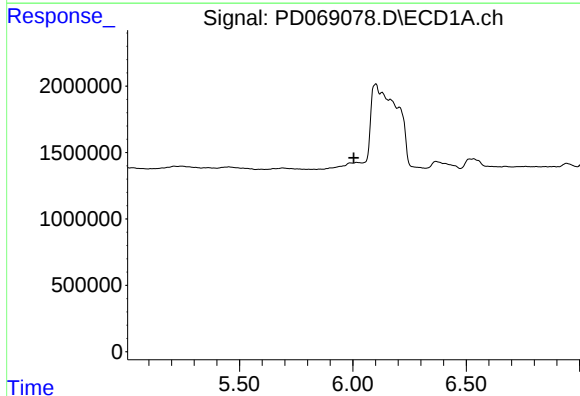


#14 Endrin

R.T.: 6.016 min
Delta R.T.: 0.012 min
Response: -100129
Conc: N.D.

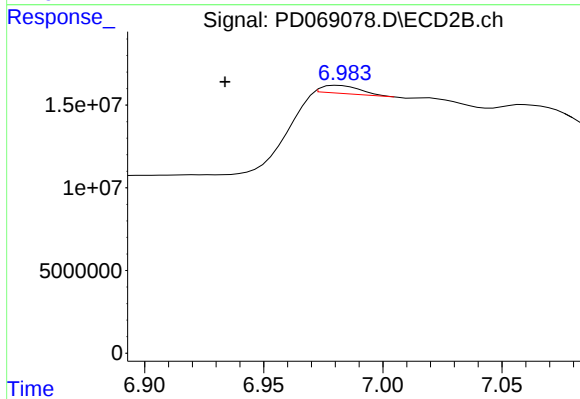

#14 Endrin


R.T.: 6.981 min
Delta R.T.: 0.047 min
Response: 4762338
Conc: 0.56 ng/ml

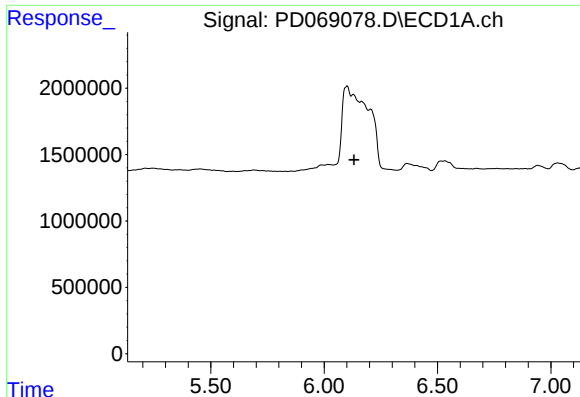

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.132 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

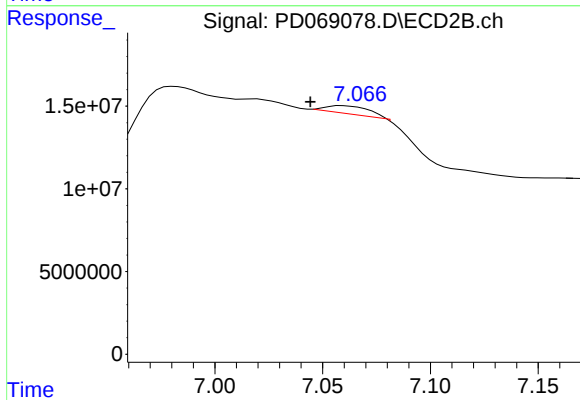


#16 4,4'-DDD

R.T.: 7.059 min
Delta R.T.: 0.015 min
Response: 5787320
Conc: 0.69 ng/ml

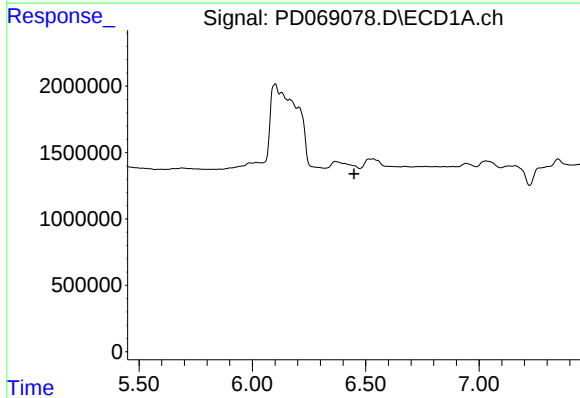


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.449 min
Response: 0
Conc: N.D.

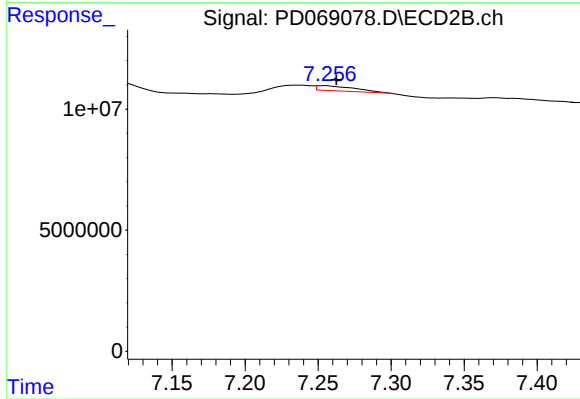

#18 Endrin aldehyde


R.T.: 7.255 min
Delta R.T.: -0.007 min
Response: 3671568
Conc: 0.55 ng/ml

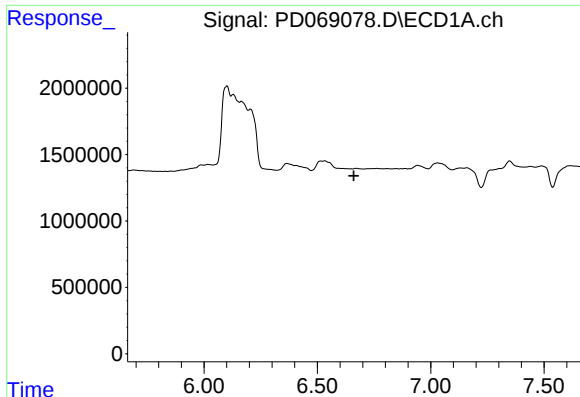

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.661 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

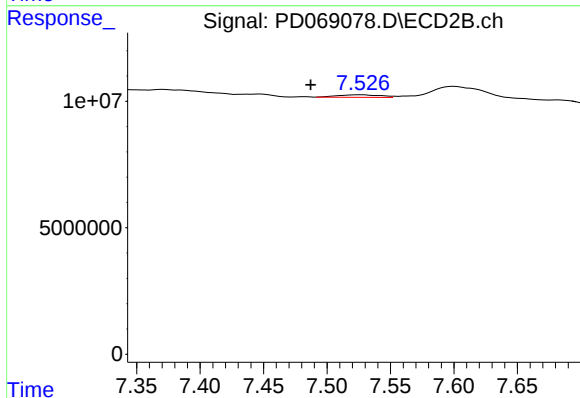


#19 Endosulfan Sulfate

R.T.: 7.527 min
Delta R.T.: 0.039 min
Response: 2345902
Conc: 0.29 ng/ml

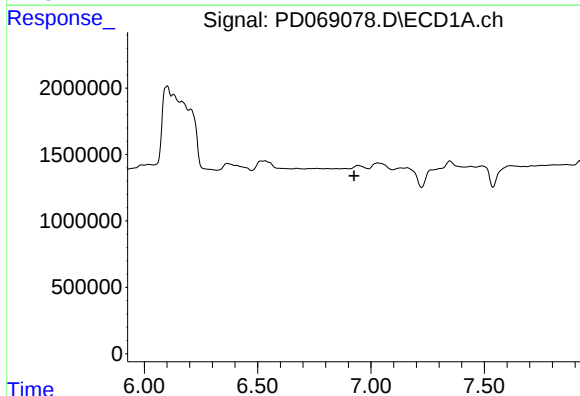


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.925 min
Response: 0
Conc: N.D.

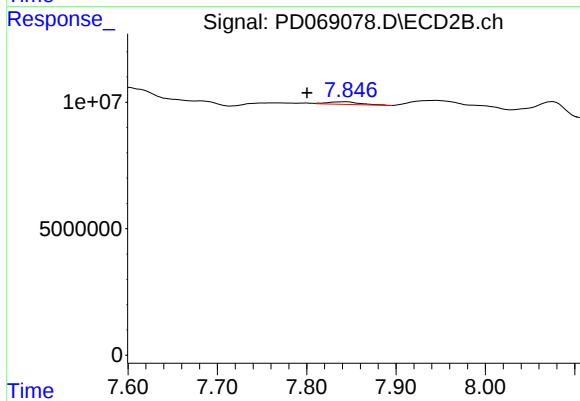

#20 Methoxychlor


R.T.: 7.845 min
Delta R.T.: 0.045 min
Response: 2613422
Conc: 0.75 ng/ml

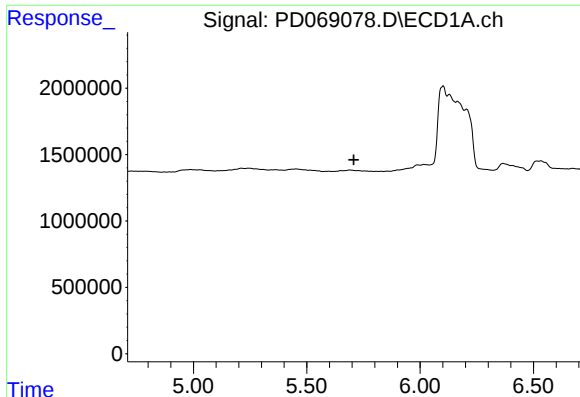

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

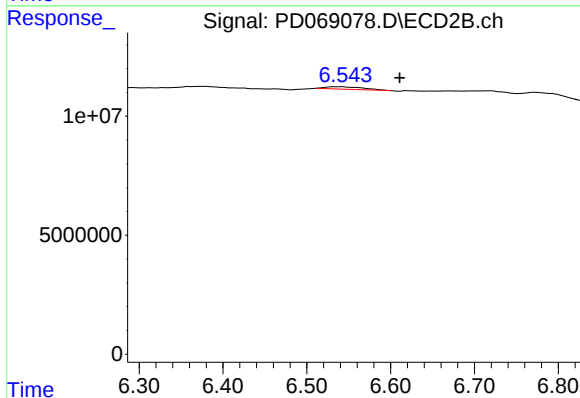


#22 Toxaphene-1

R.T.: 6.543 min
Delta R.T.: -0.068 min
Response: 3137804
Conc: 73.74 ng/ml

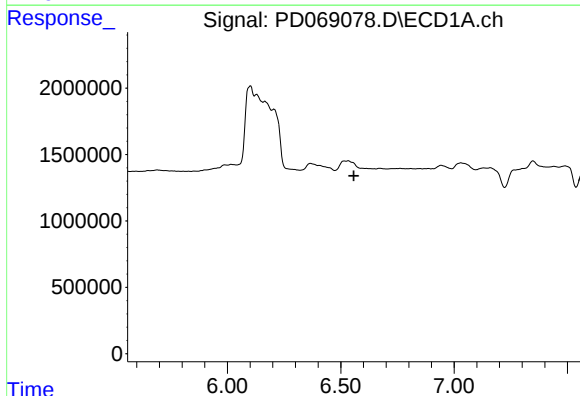


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 6.558 min
Response: 0
Conc: N.D.

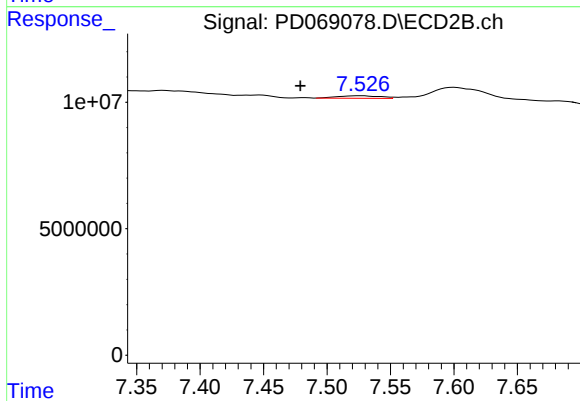

#25 Toxaphene-4


R.T.: 7.527 min
Delta R.T.: 0.047 min
Response: 2345902
Conc: 17.56 ng/ml

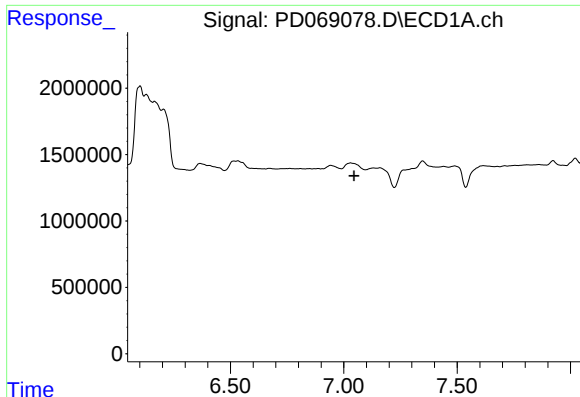

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.045 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

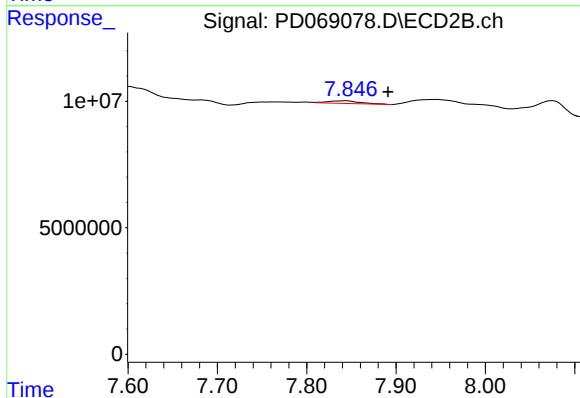


#26 Toxaphene-5

R.T.: 7.845 min
Delta R.T.: -0.046 min
Response: 2613422
Conc: 29.83 ng/ml

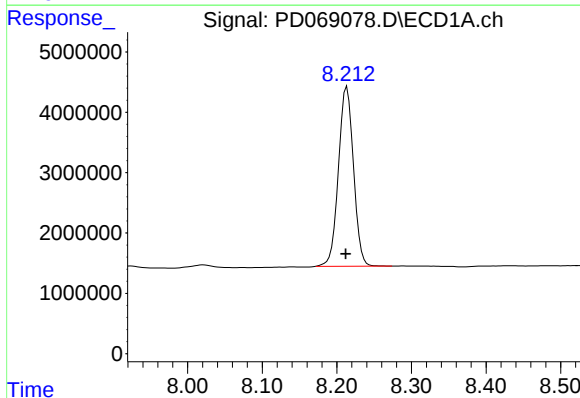

#27 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: 0.001 min
Response: 41672534
Conc: 29.97 ng/ml

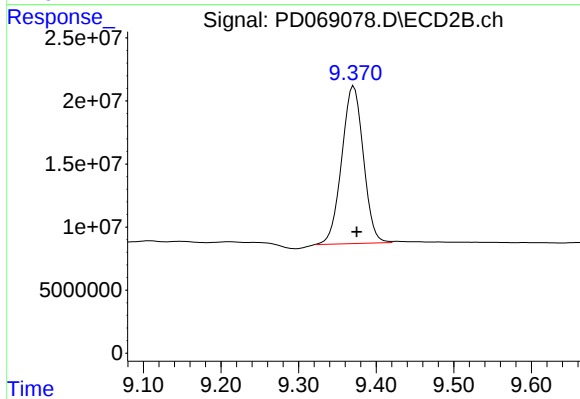

#27 Decachlorobiphenyl

R.T.: 9.371 min
Delta R.T.: -0.004 min
Response: 241295880
Conc: 38.26 ng/ml