

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
 Data File : PD069075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2022 13:12
 Operator : AR\AJ
 Sample : N2353-15 (Sig #1); INDA2-TESTSAMPLE (Sig #2)
 Misc : M03961
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 FLURISIL-CHECK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/12/2022
 Supervised By : mohammad ahmed 04/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 00:51:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 07:24:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.453	4.173	11726954	121.3E6	8.612	11.084 #
27)	SA Decachlor...	8.210	9.370	26542979	142.6E6	19.088	22.604
Target Compounds							
2)	A alpha-BHC	3.893	4.569	15291313	161.5E6	7.988	10.330 #
3)	MA gamma-BHC...	4.176	4.859	15220597	153.7E6	8.385	10.605m#
4)	MA Heptachlor	4.475	5.387	15393887	151.5E6	8.594	11.004 #
9)	A Endosulfan I	5.505	6.451	13276423	117.2E6	8.623	10.770
13)	MA Dieldrin	5.748	6.709	27530376	240.6E6	16.481	21.650 #
14)	MA Endrin	6.006	6.929	24923115	192.5E6	17.629	22.774 #
16)	A 4,4'-DDD	6.134	7.040	21473257	184.1E6	16.337	21.945m#
17)	MA 4,4'-DDT	6.374	7.344	21631596	174.1E6	16.199	22.090 #
20)	A Methoxychlor	6.924	7.797	63844100	417.7E6	90.198	119.236 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041222\
Data File : PD069075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2022 13:12
Operator : AR\AJ
Sample : N2353-15 (Sig #1); INDA2-TESTSAMPLE (Sig #2)
Misc : M03961
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 00:51:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD031322CLP.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 07:24:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

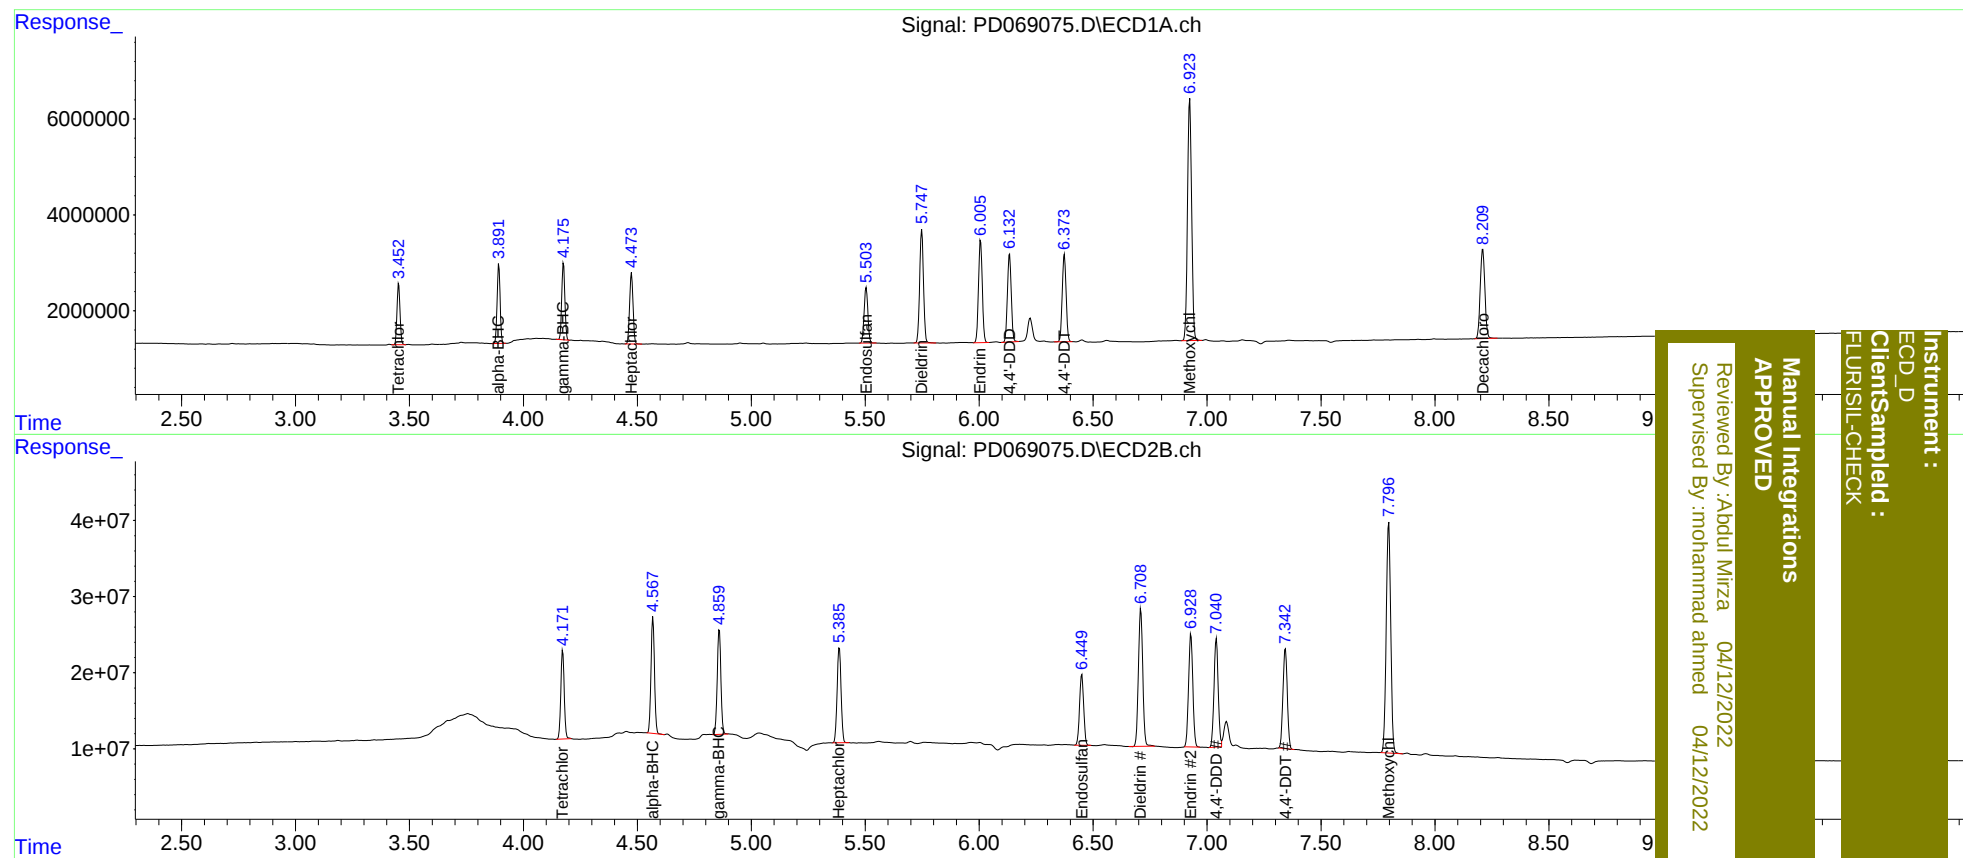

Reviewed By: Abdul Miza 04/12/2022
Supervised By: mohammad ahmed 04/12/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
FLURISIL-CHECK