

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
 Data File : PD082401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2024 12:00
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 12:37:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 12 12:33:07 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.775	121.5E6	340.1E6	75.306	75.196
28)	SA Decachlor...	9.124	7.912	155.0E6	261.8E6	76.152	75.637
Target Compounds							
23)	Chlordane-1	4.735	3.772	63373890	110.2E6	754.642	753.132
24)	Chlordane-2	5.266	4.347	62549043	120.2E6	753.493	751.719
25)	Chlordane-3	5.979	4.977	257.6E6	349.5E6	767.634	753.254
26)	Chlordane-4	6.062	5.041	304.5E6	335.5E6	764.737	751.551
27)	Chlordane-5	6.915	5.936	54615987	120.6E6	765.781	762.923



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
Data File : PD082401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 12:00
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 12:37:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
Quant Title : GC Extractables
QLast Update : Fri Apr 12 12:33:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

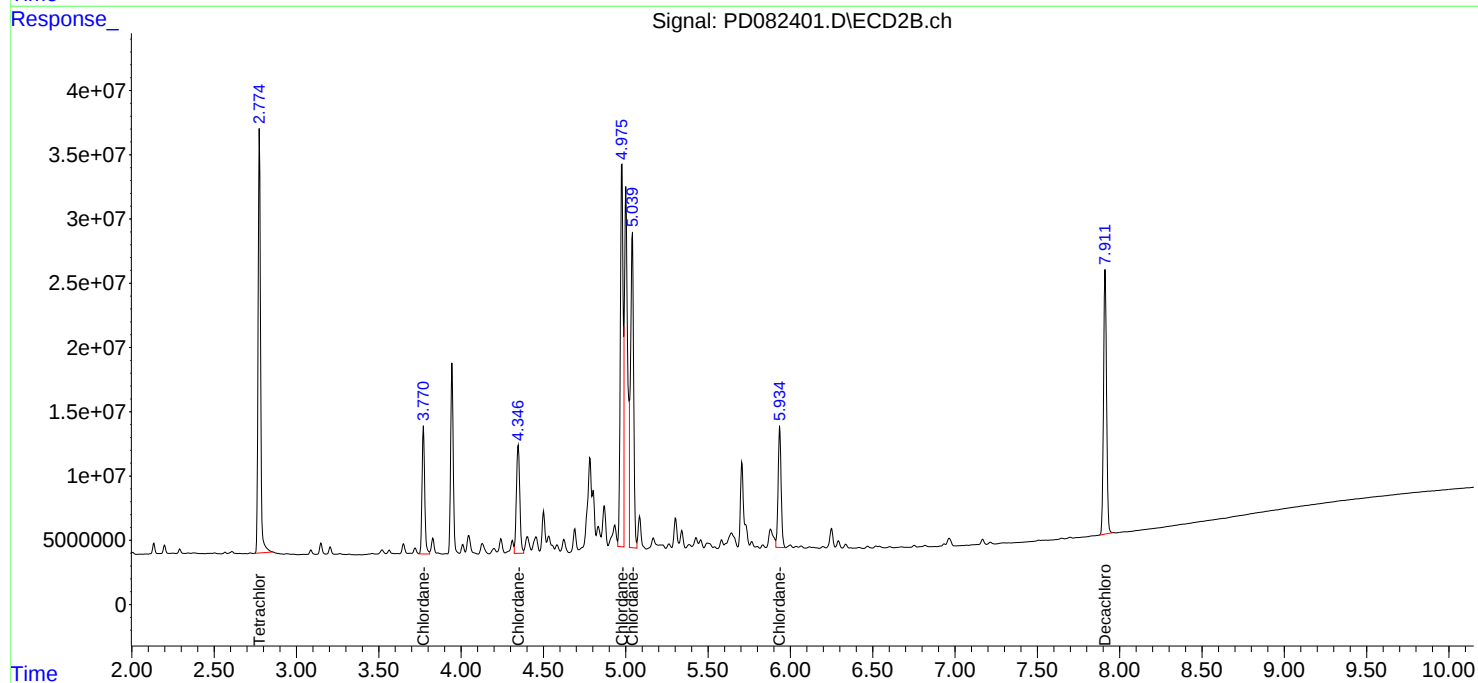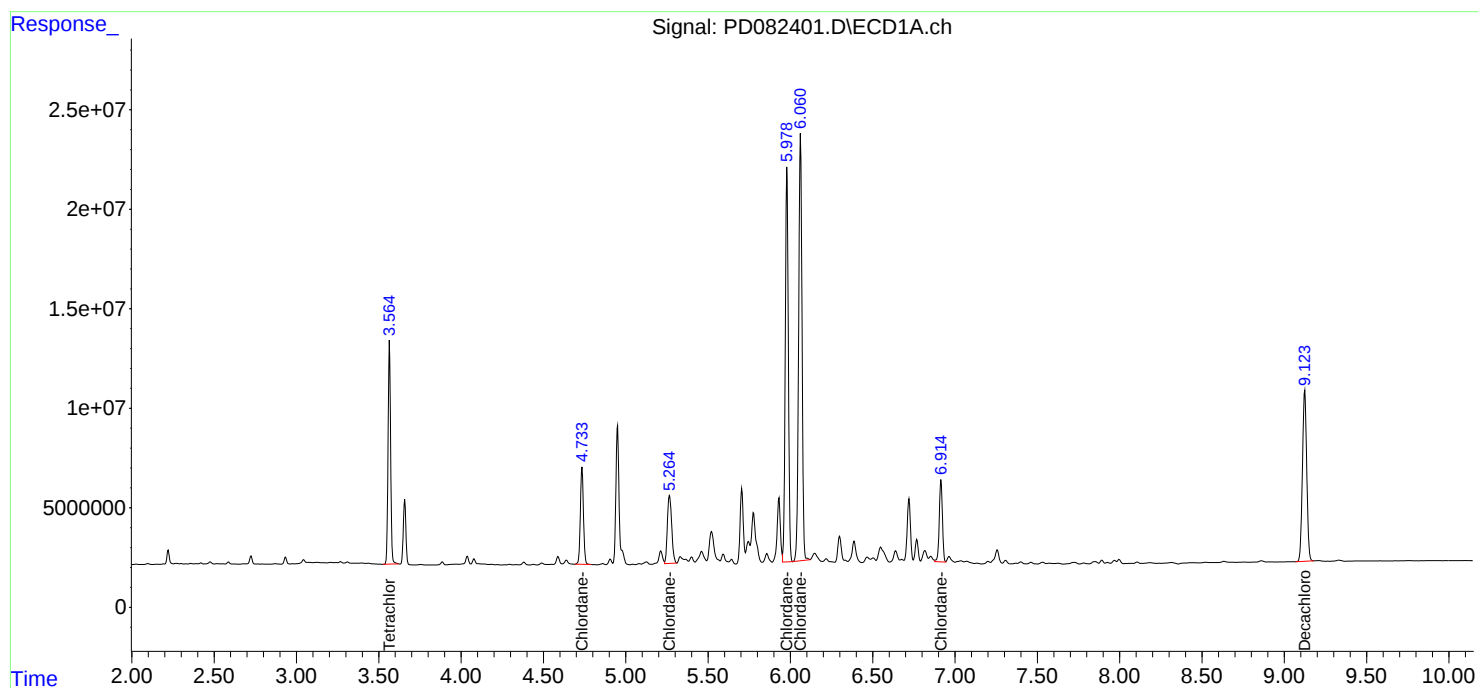


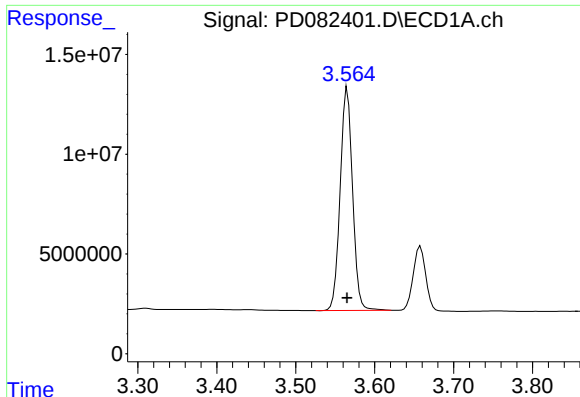

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 121509118
Conc: 75.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

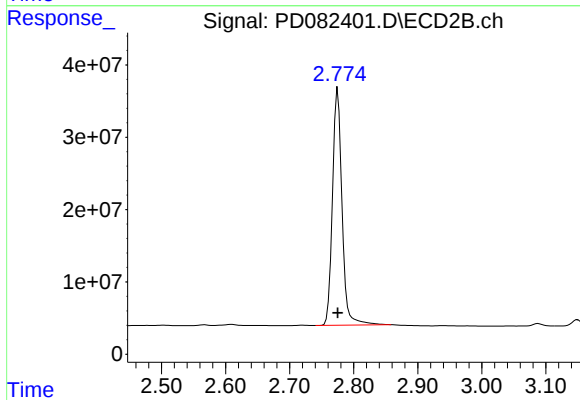


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 340127388
Conc: 75.20 ng/ml

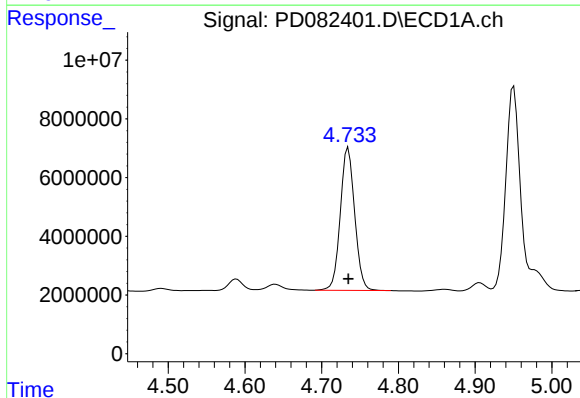


#23 Chlordane-1

R.T.: 4.735 min
Delta R.T.: 0.000 min
Response: 63373890
Conc: 754.64 ng/ml

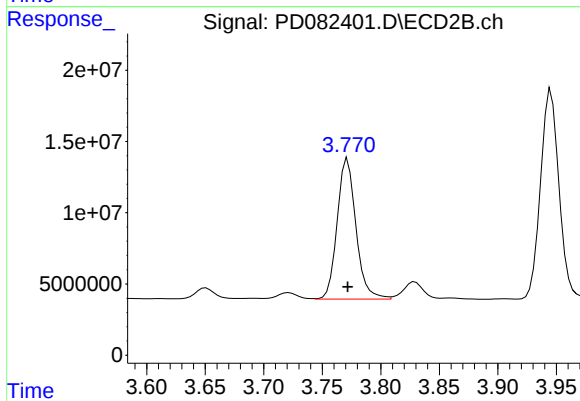

#23 Chlordane-1


R.T.: 3.772 min
Delta R.T.: 0.000 min
Response: 110190707
Conc: 753.13 ng/ml

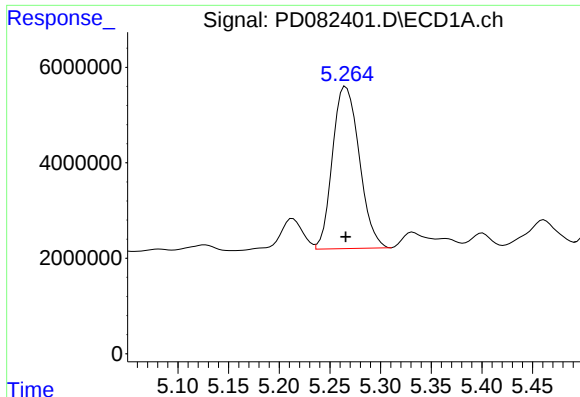

#24 Chlordane-2


R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 62549043
Conc: 753.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

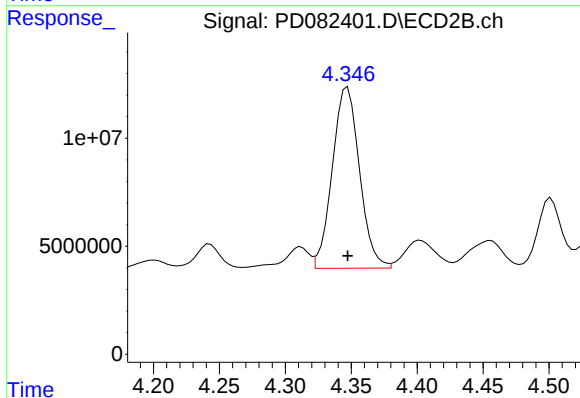


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 120239927
Conc: 751.72 ng/ml

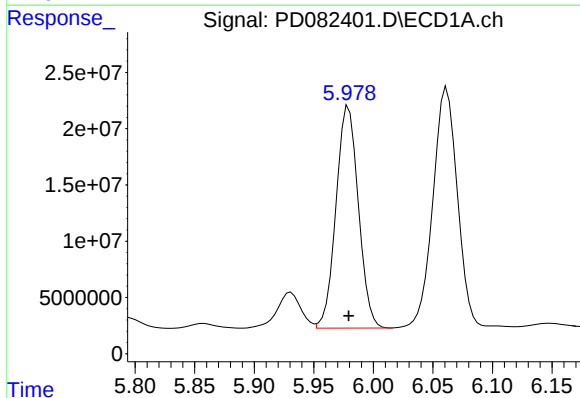


#25 Chlordane-3

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 257631253
Conc: 767.63 ng/ml

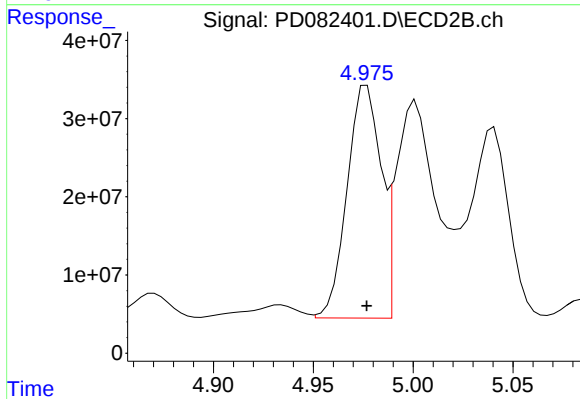

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 349533915
Conc: 753.25 ng/ml

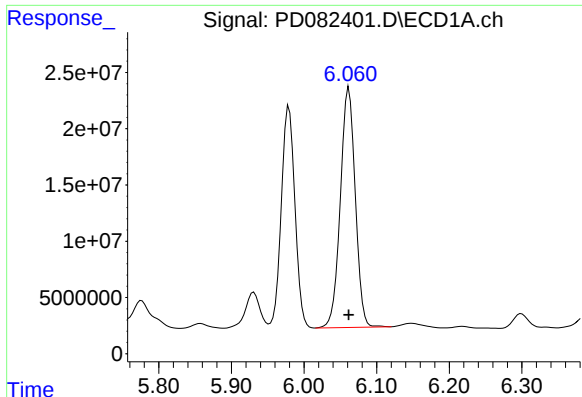

#26 Chlordane-4


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 304508866
Conc: 764.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

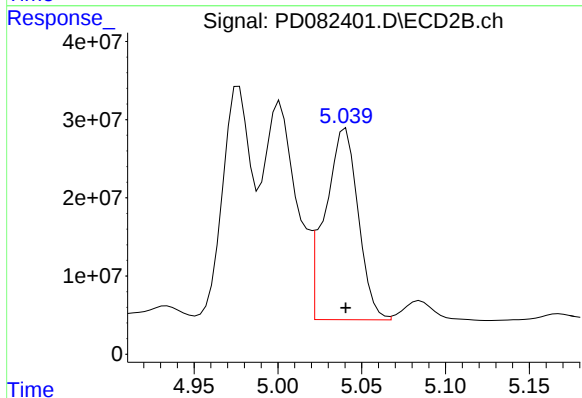


#26 Chlordane-4

R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 335469979
Conc: 751.55 ng/ml

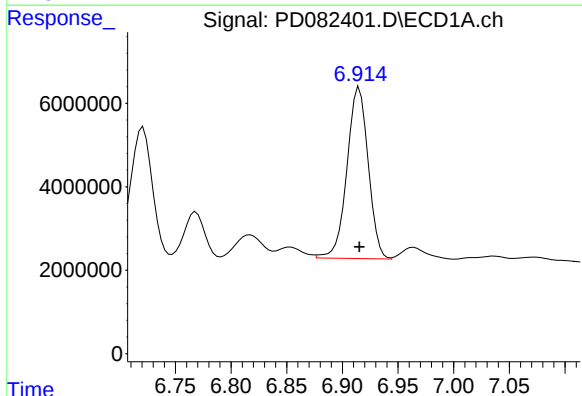


#27 Chlordane-5

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 54615987
Conc: 765.78 ng/ml

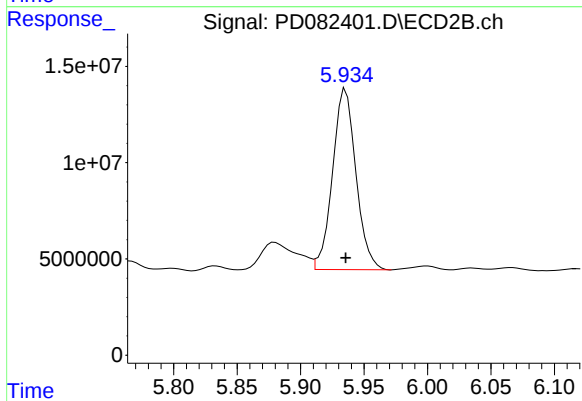

#27 Chlordane-5


R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 120579392
Conc: 762.92 ng/ml

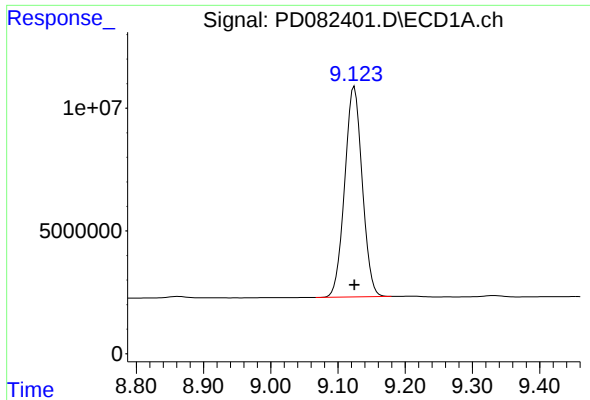

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 15500218
Conc: 76.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

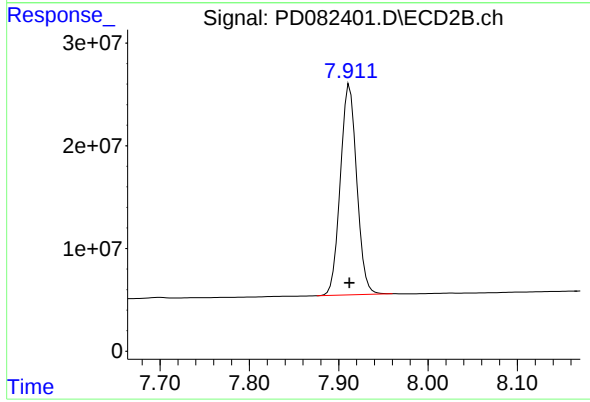

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 261822083
Conc: 75.64 ng/ml