

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
 Data File : PD082403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2024 12:27
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 12:39:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 12 12:39:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.775	40176273	110.1E6	24.925	24.507
28)	SA Decachlor...	9.124	7.913	53393617	87782457	25.913	25.268
Target Compounds							
23)	Chlordane-1	4.734	3.771	20525116	35784204	245.783	245.911
24)	Chlordane-2	5.266	4.347	21730710	41177891	258.730	255.537
25)	Chlordane-3	5.979	4.976	82124529	110.6E6	246.002	241.087
26)	Chlordane-4	6.062	5.040	98092353	106.2E6	247.250	240.776
27)	Chlordane-5	6.914	5.935	17266899	37613584	244.030	240.880



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
Data File : PD082403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 12:27
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 12:39:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
Quant Title : GC Extractables
QLast Update : Fri Apr 12 12:39:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

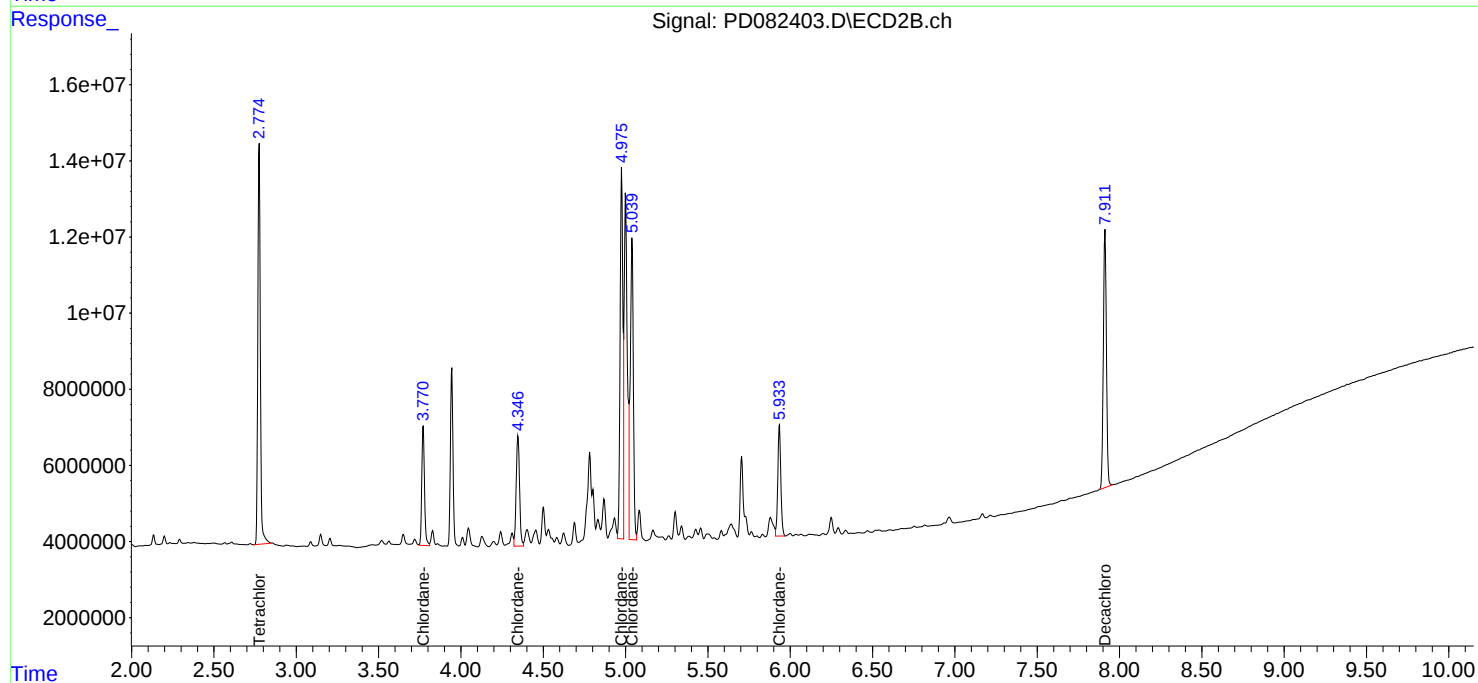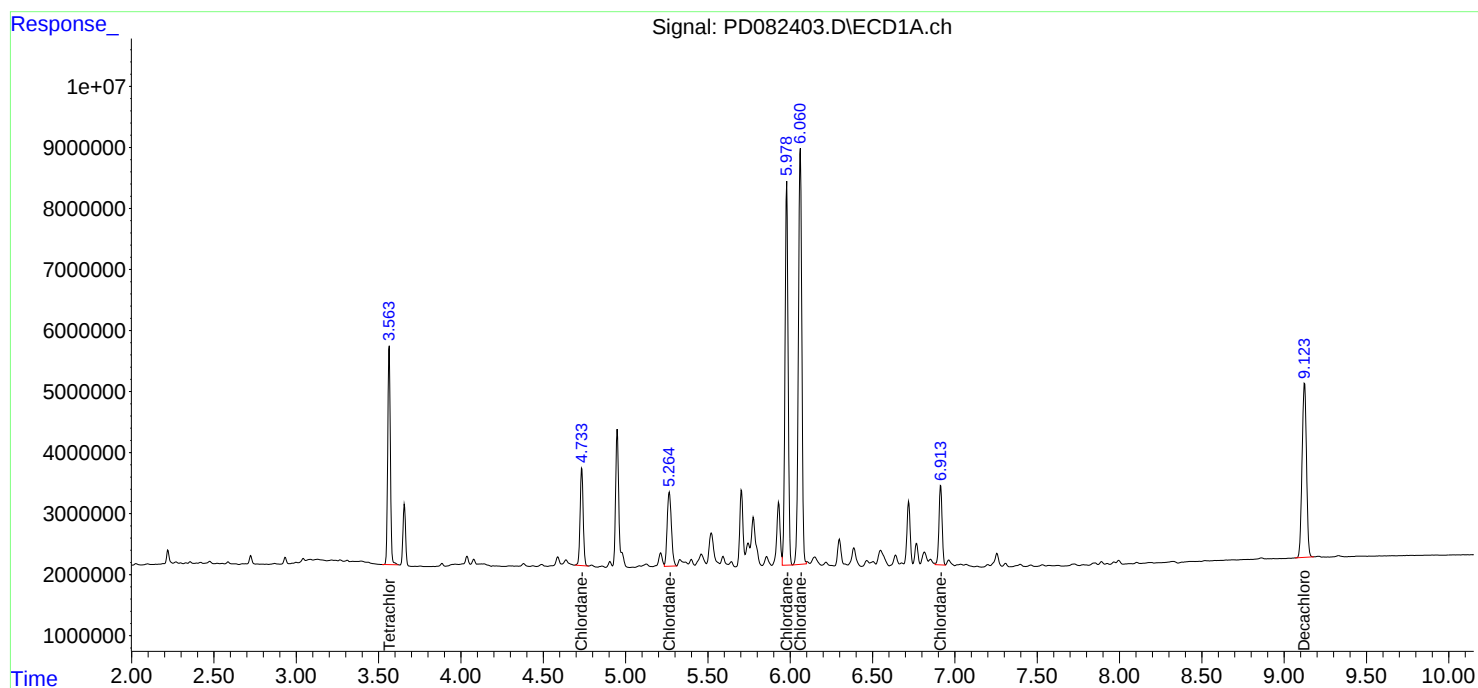


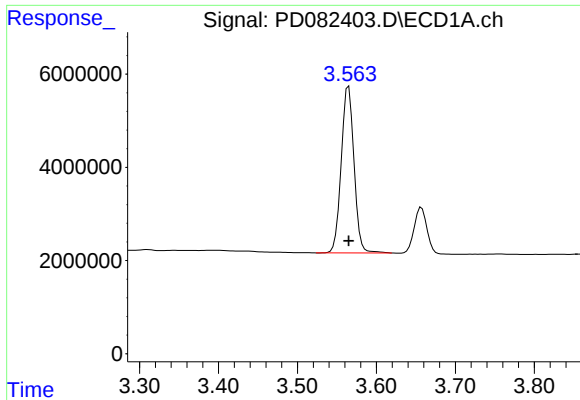

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 40176273
Conc: 24.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

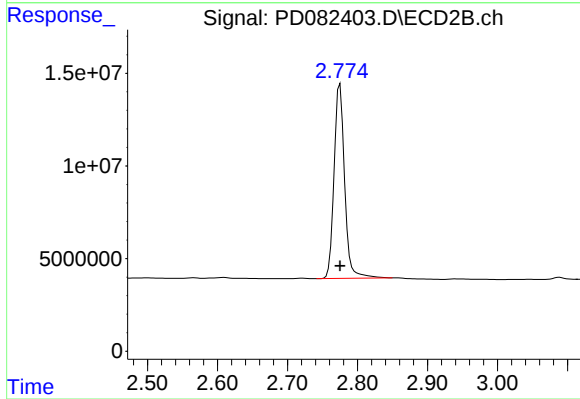


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 110128541
Conc: 24.51 ng/ml

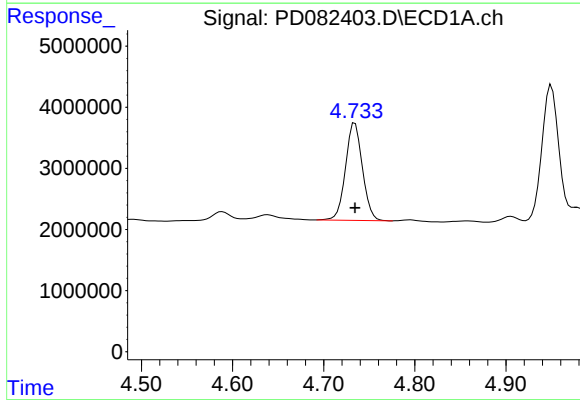


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 20525116
Conc: 245.78 ng/ml

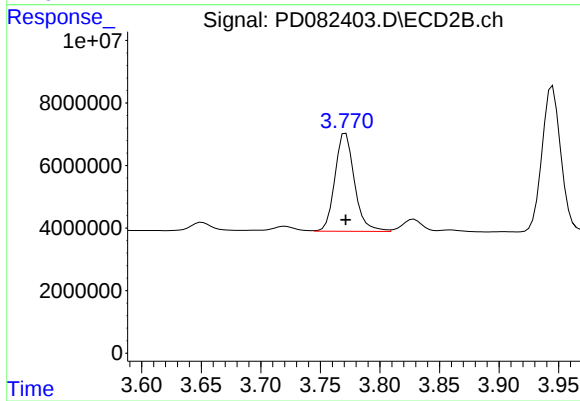

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 35784204
Conc: 245.91 ng/ml

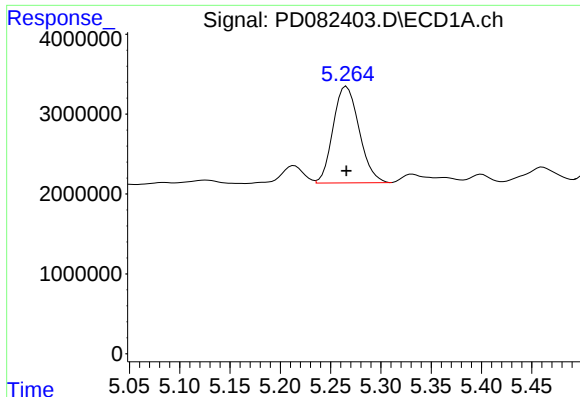

#24 Chlordane-2


R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 21730710
Conc: 258.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

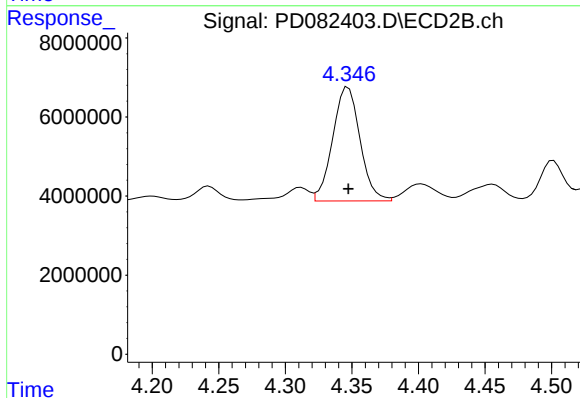


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 41177891
Conc: 255.54 ng/ml

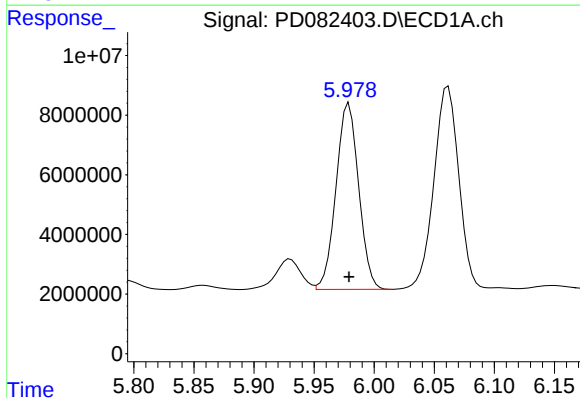


#25 Chlordane-3

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 82124529
Conc: 246.00 ng/ml

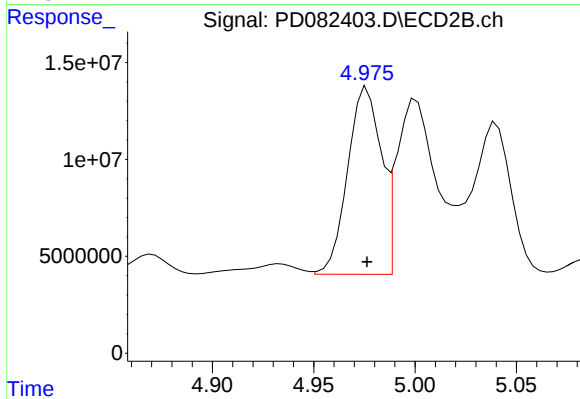

#25 Chlordane-3


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 110558307
Conc: 241.09 ng/ml

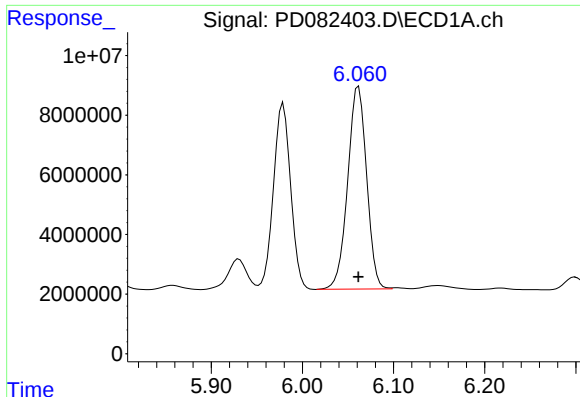

#26 Chlordane-4


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 98092353
Conc: 247.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

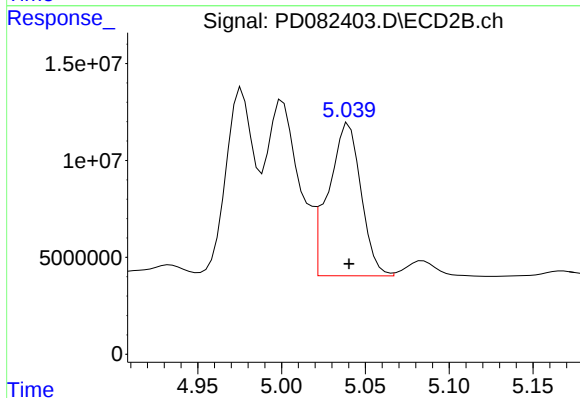


#26 Chlordane-4

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 106169592
Conc: 240.78 ng/ml

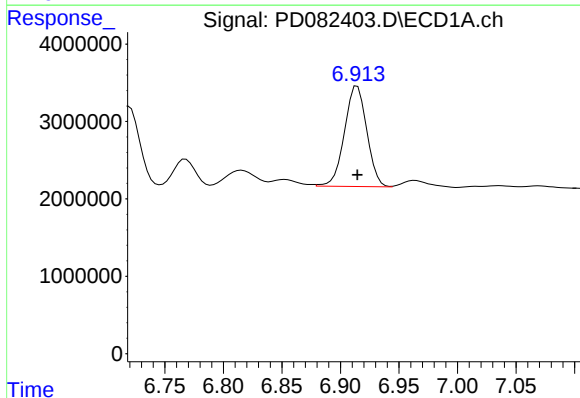


#27 Chlordane-5

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 17266899
Conc: 244.03 ng/ml

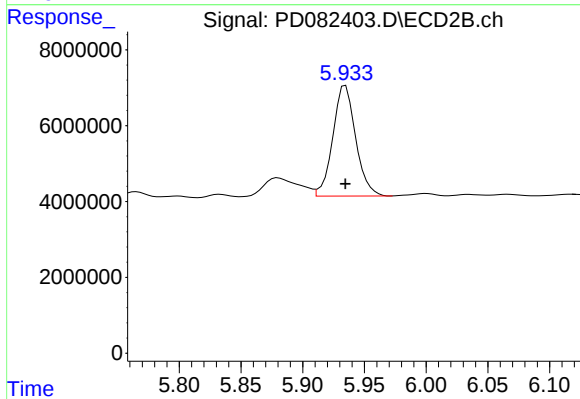

#27 Chlordane-5


R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 37613584
Conc: 240.88 ng/ml

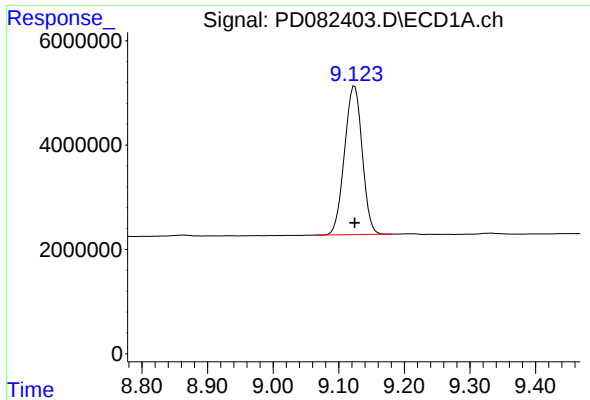

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 53393617
Conc: 25.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

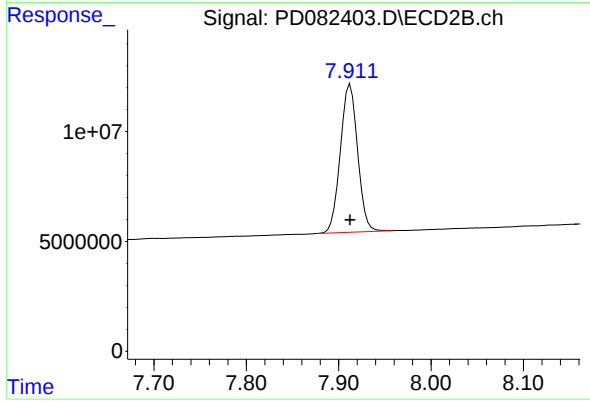

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 87782457
Conc: 25.27 ng/ml