

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
 Data File : PD082402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2024 12:14
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 12:33:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 12 12:33:07 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.775	79413178	222.0E6	50.000	50.000
28)	SA Decachlor...	9.124	7.912	101.8E6	171.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.734	3.771	41089721	71325803	500.000	500.000
24)	Chlordane-2	5.266	4.347	41546049	79817998	500.000	500.000
25)	Chlordane-3	5.979	4.976	163.3E6	225.5E6	500.000	500.000
26)	Chlordane-4	6.062	5.040	194.1E6	216.9E6	500.000	500.000
27)	Chlordane-5	6.915	5.935	34782043	76450834	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
Data File : PD082402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 12:14
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 12:33:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
Quant Title : GC Extractables
QLast Update : Fri Apr 12 12:33:07 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

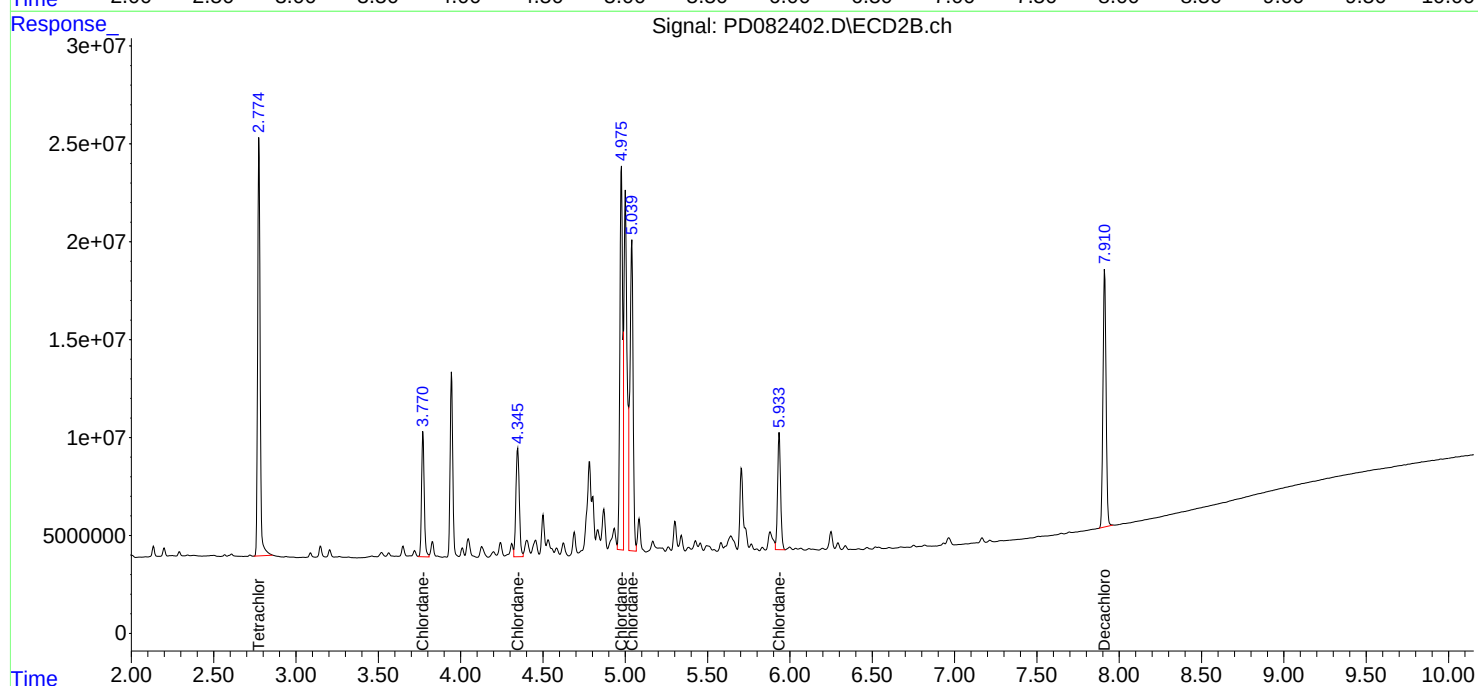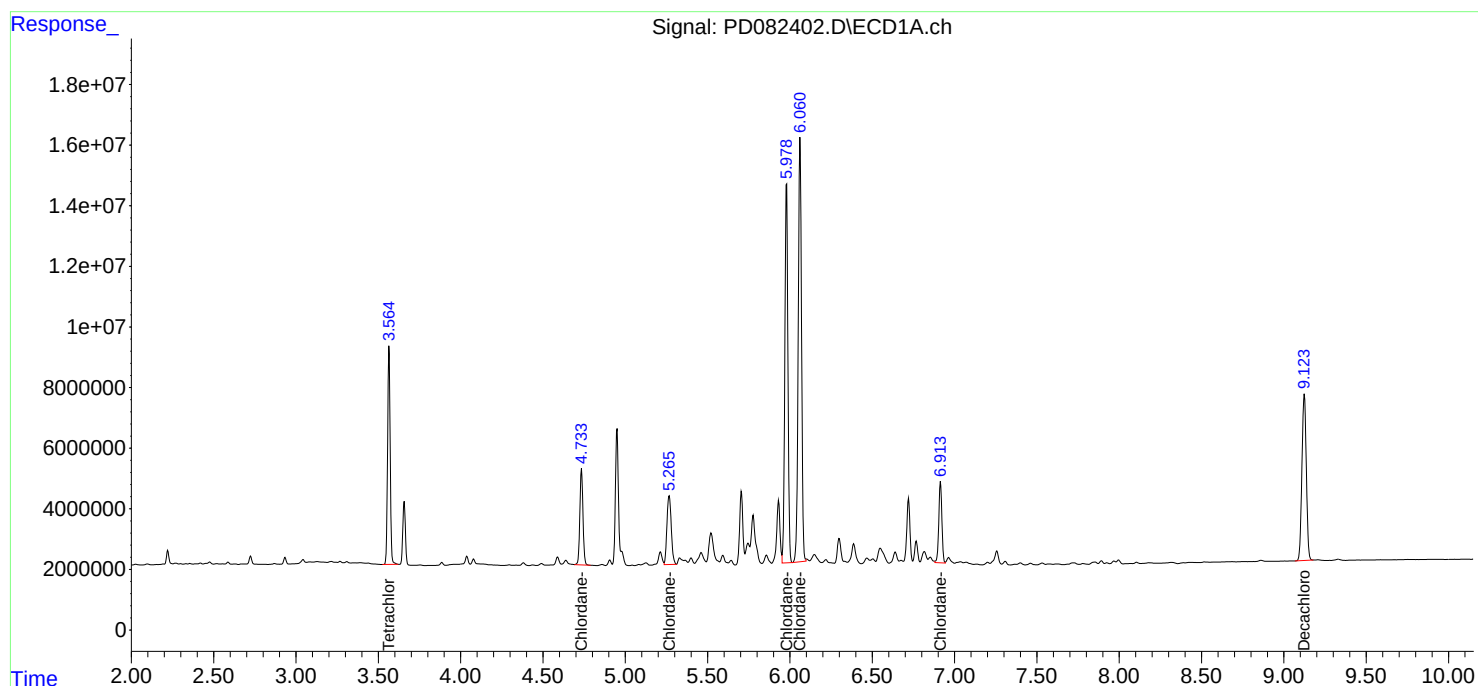


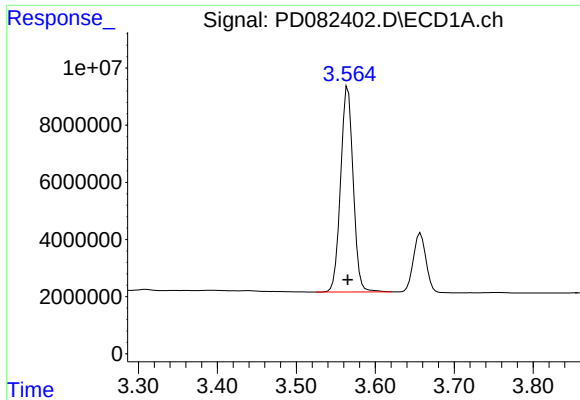

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 79413178
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

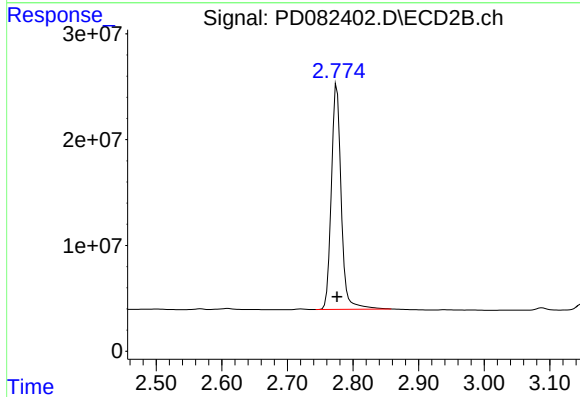


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 221977682
Conc: 50.00 ng/ml

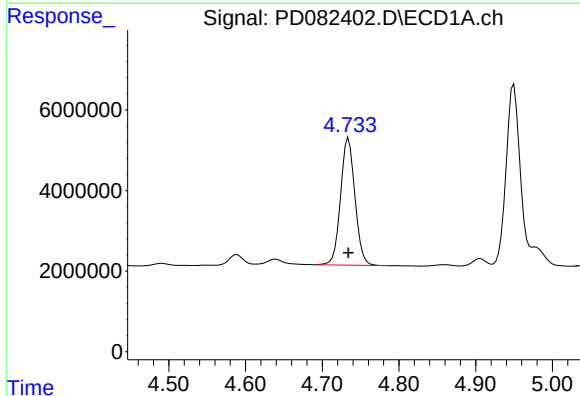


#23 Chlordane-1

R.T.: 4.734 min
Delta R.T.: 0.000 min
Response: 41089721
Conc: 500.00 ng/ml

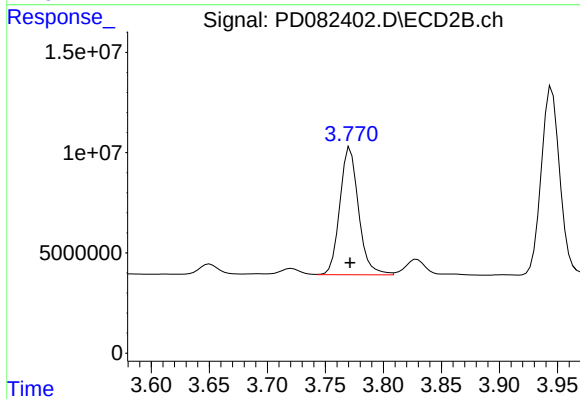

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 71325803
Conc: 500.00 ng/ml

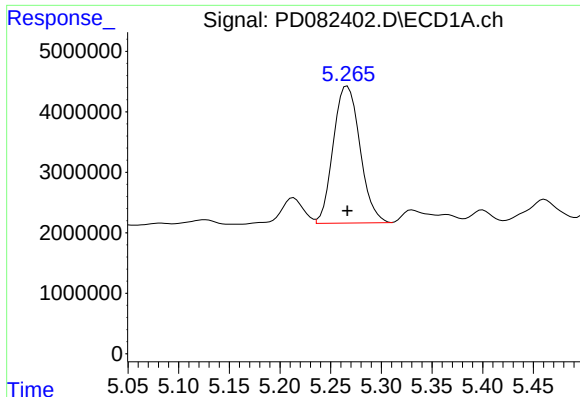

#24 Chlordane-2


R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 41546049
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

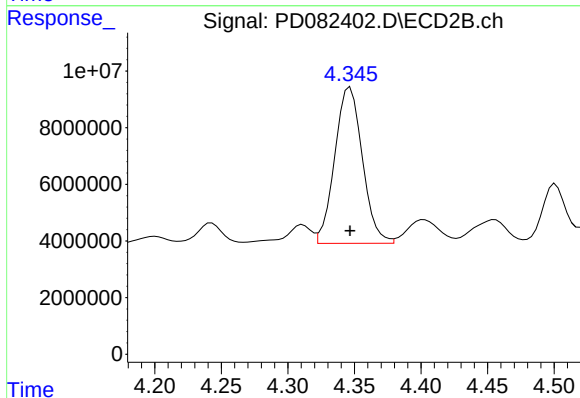


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 79817998
Conc: 500.00 ng/ml

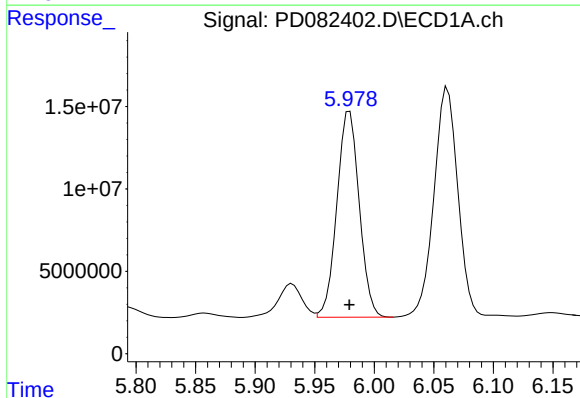


#25 Chlordane-3

R.T.: 5.979 min
Delta R.T.: 0.000 min
Response: 163308751
Conc: 500.00 ng/ml

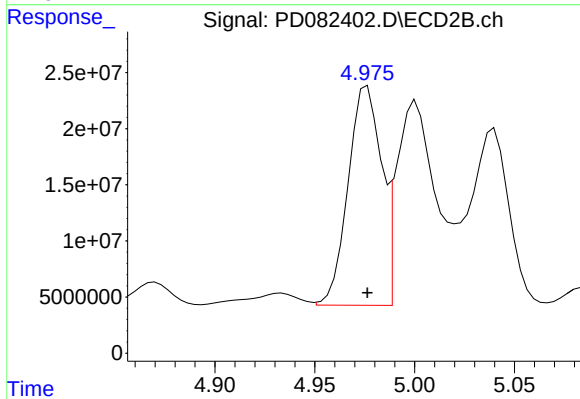

#25 Chlordane-3


R.T.: 4.976 min
Delta R.T.: 0.000 min
Response: 225517030
Conc: 500.00 ng/ml

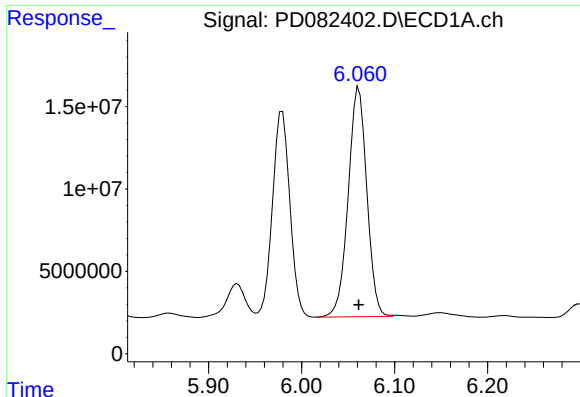

#26 Chlordane-4


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 194050793
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

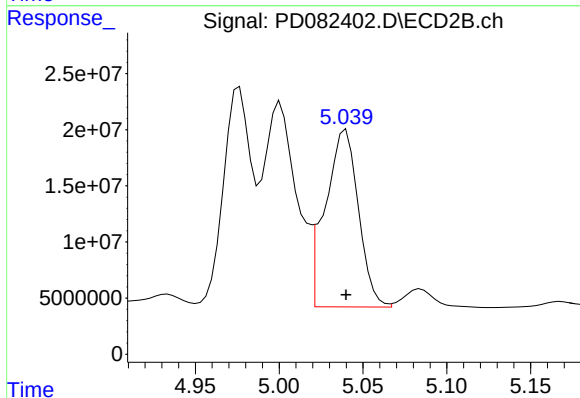


#26 Chlordane-4

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 216868241
Conc: 500.00 ng/ml

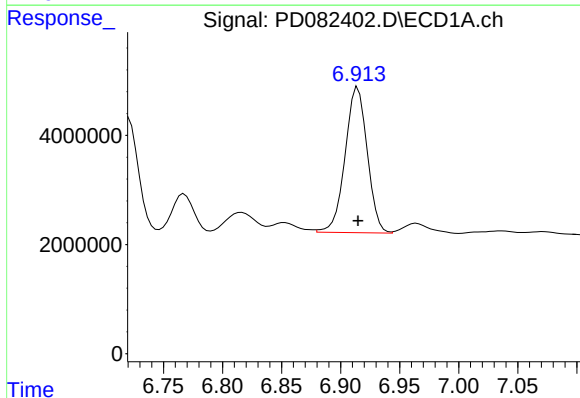


#27 Chlordane-5

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 34782043
Conc: 500.00 ng/ml

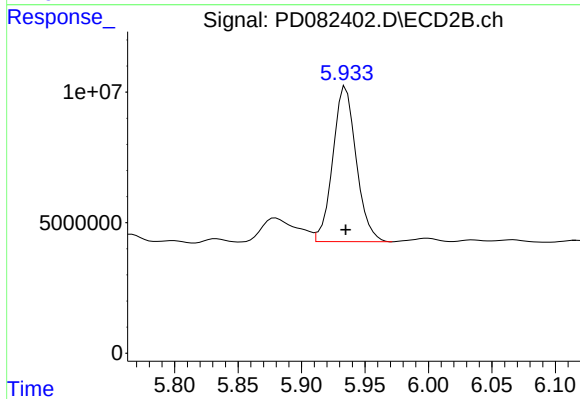

#27 Chlordane-5


R.T.: 5.935 min
Delta R.T.: 0.000 min
Response: 76450834
Conc: 500.00 ng/ml

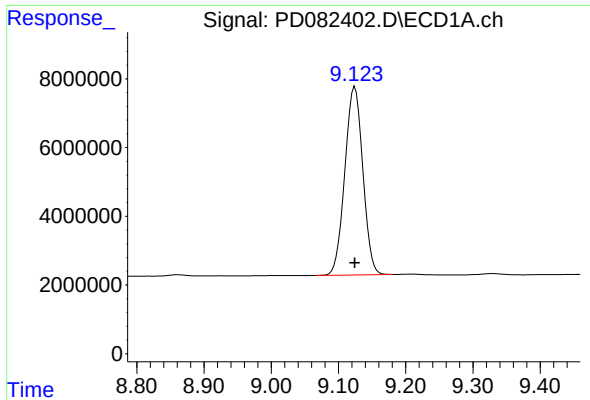

#28 Decachlorobiphenyl

R.T.: 9.124 min
Delta R.T.: 0.000 min
Response: 101755680
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

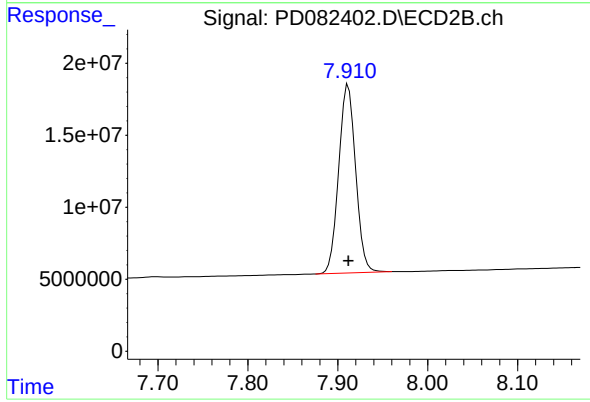

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 171449422
Conc: 50.00 ng/ml