

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
 Data File : PD082432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2024 18:53
 Operator : AR\AJ
 Sample : P2070-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 21:59:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 12 14:27:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.776	20492420	47830232	12.657	11.969
28)	SA Decachlor...	9.123	7.912	22832997	38255920	10.633	11.021
Target Compounds							
17)	MA 4,4'-DDT	7.064	6.031	845440	3099828	0.446	0.884 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041324\
Data File : PD082432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2024 18:53
Operator : AR\AJ
Sample : P2070-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 21:59:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041324.M
Quant Title : GC Extractables
QLast Update : Fri Apr 12 14:27:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

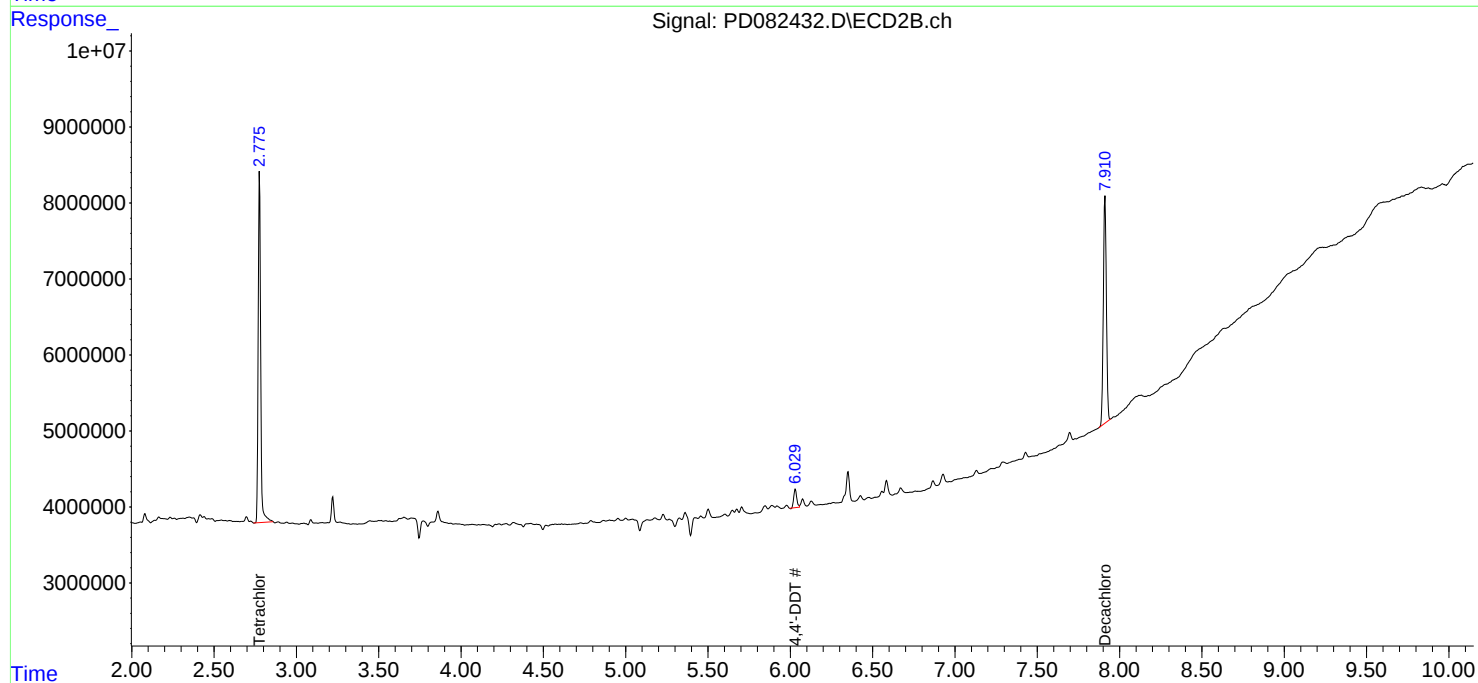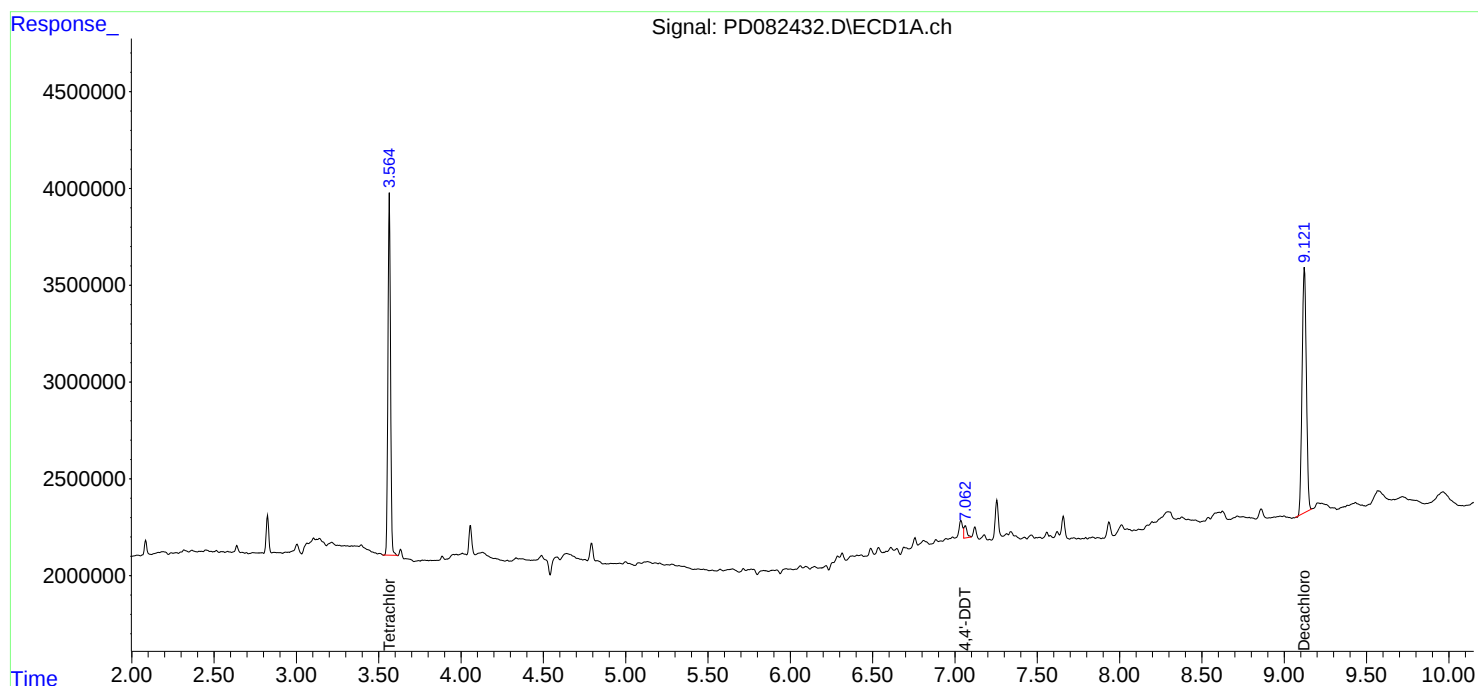


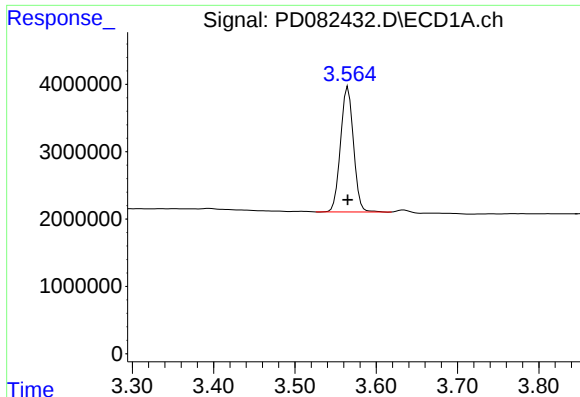

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 20492420
Conc: 12.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3

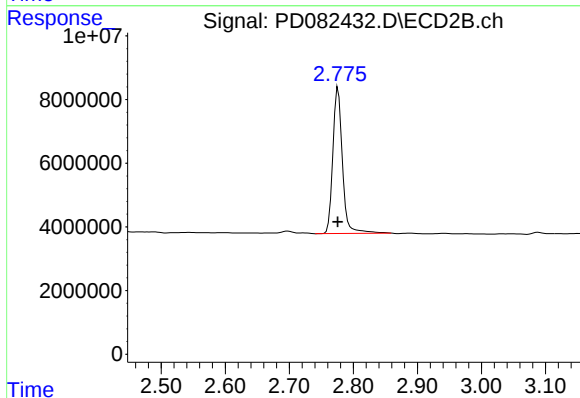


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 47830232
Conc: 11.97 ng/ml

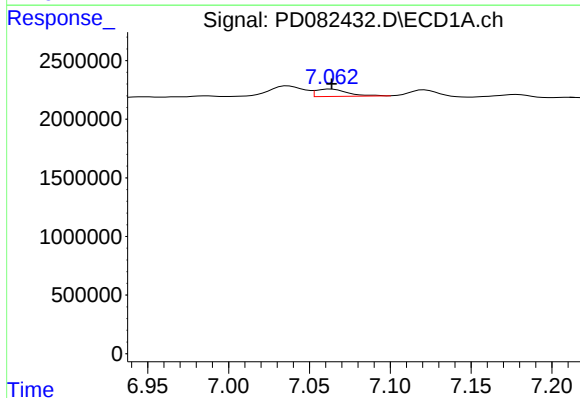


#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: 0.000 min
Response: 845440
Conc: 0.45 ng/ml

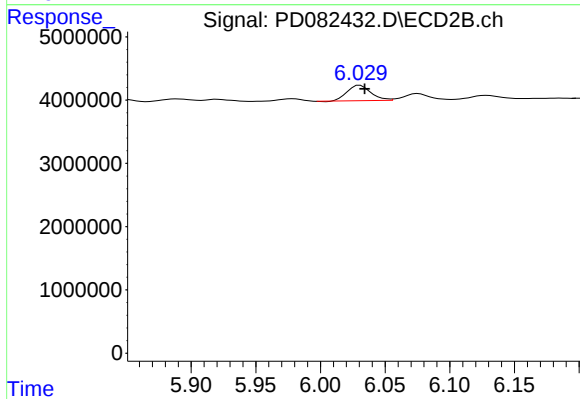

#17 4,4'-DDT


R.T.: 6.031 min
Delta R.T.: -0.004 min
Response: 3099828
Conc: 0.88 ng/ml

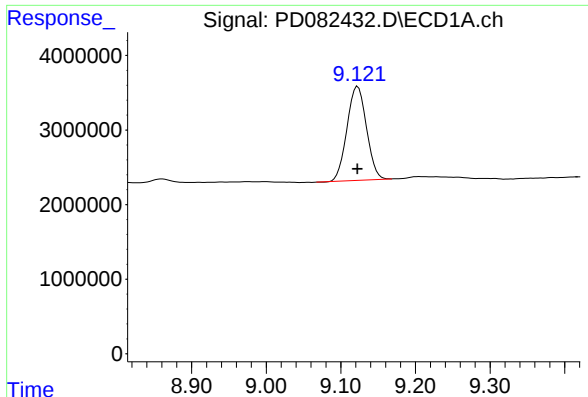

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 22832997
Conc: 10.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-3

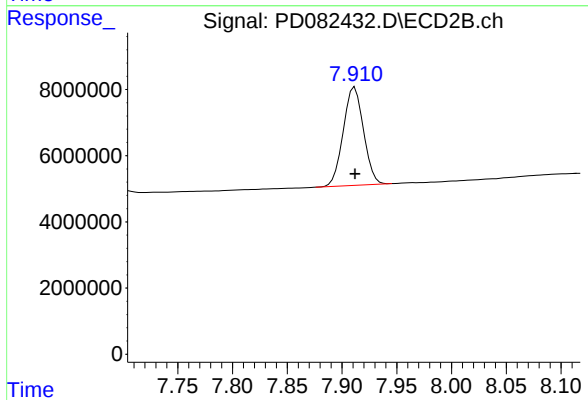

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 38255920
Conc: 11.02 ng/ml