

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041422\
 Data File : PD069114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2022 15:13
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5040

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 02:08:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:08:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.172	96124015	846.8E6	75.869	70.158
27)	SA Decachlor...	8.200	9.365	188.7E6	941.0E6	141.891	133.809
Target Compounds							
2)	A alpha-BHC	3.884	4.567	148.4E6	1246.6E6	83.030	75.828
3)	MA gamma-BHC...	4.167	4.858	139.0E6	1136.7E6	76.874	72.957
4)	MA Heptachlor	4.464	5.385	133.5E6	1080.7E6	78.634	71.384
9)	A Endosulfan I	5.494	6.449	111.5E6	829.2E6	76.390	69.815
13)	MA Dieldrin	5.738	6.708	253.0E6	1733.4E6	162.545	143.708
14)	MA Endrin	5.996	6.928	223.4E6	1405.2E6	159.663	144.494
16)	A 4,4'-DDD	6.124	7.039	196.8E6	1330.3E6	161.441	142.059
17)	MA 4,4'-DDT	6.364	7.342	203.9E6	1310.2E6	166.215	145.545
20)	A Methoxychlor	6.915	7.794	498.5E6	2816.0E6	734.548	683.320

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041422\
Data File : PD069114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2022 15:13
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 02:08:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:08:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

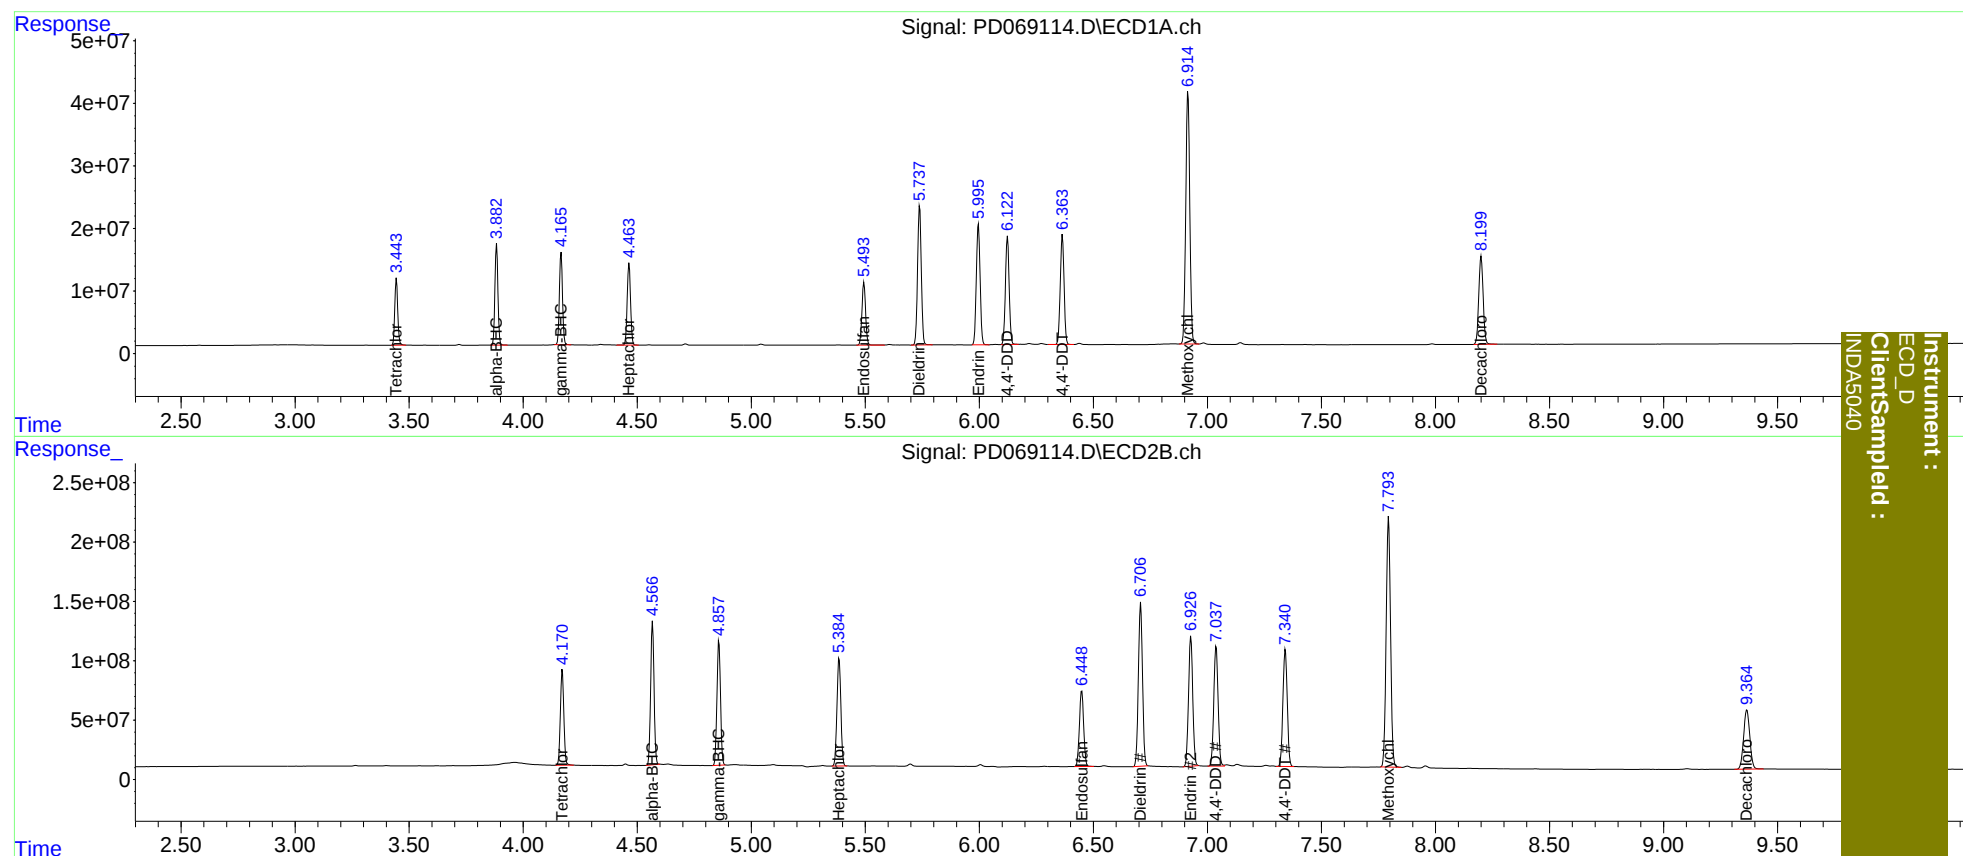

Instrument :
ECD_D
ClientSampled :
INDA5040