

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041423\
 Data File : PD074728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 18:09
 Operator : AR\AJ
 Sample : 02215-02
 Misc : PEST MDL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT2-2023-04

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/14/2023
 Supervised By :Ankita Jodhani 04/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 01:24:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 13 14:14:37 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.771	52649946	28201526	20.622	20.047
27)	SA Decachlor...	9.094	7.922	127.2E6	54671869	41.497	40.508
Target Compounds							
2)	A alpha-BHC	4.006	3.274	4718819	1604127	1.138	0.800 #
3)	MA gamma-BHC...	4.339	3.604	4034924	1638309	1.026	0.845
4)	MA Heptachlor	4.931	3.945	4261171	1650225	1.043	0.869
5)	MB Aldrin	5.275	4.226	4143098	1795750	1.053	0.949
6)	B beta-BHC	4.534	3.898	1445052	796659	0.825	0.899m
7)	B delta-BHC	4.781	4.130	5558718	1721379	1.507	0.880 #
8)	B Heptachlo...	5.699	4.729	4674239	1738279	1.277m	0.999
9)	A Endosulfan I	6.089	5.099	3906435	1488839	1.154	0.955
10)	B trans-Chl...	5.958	4.978	3772011	1728653	1.070	1.012m
11)	B cis-Chlor...	6.038	5.044	3983807	1792068	1.084	1.037
12)	B 4,4'-DDE	6.210	5.233	3466540	1481723	1.004	0.907
13)	MA Dieldrin	6.364	5.364	3867543	1666200	1.035	0.938
14)	MA Endrin	6.595	5.639	3152404	1553661	0.979	0.990m
15)	B Endosulfa...	6.814	5.934	3886215	1595593	1.212	1.056
16)	A 4,4'-DDD	6.727	5.788	2852400	1336322	1.001	0.966
17)	MA 4,4'-DDT	7.043	6.040	3072769	1159846	1.010	0.807
18)	B Endrin al...	6.944	6.113	3246861	1332596	1.241	1.083
19)	B Endosulfa...	7.179	6.336	3689958	1538303	1.204	1.088
20)	A Methoxychlor	7.519	6.616	2189816	812565	1.288	1.105
21)	B Endrin ke...	7.666	6.843	4332553	1725219	1.217	1.024

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041423\
Data File : PD074728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 18:09
Operator : AR\AJ
Sample : 02215-02
Misc : PEST MDL
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 01:24:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041423CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 13 14:14:37 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

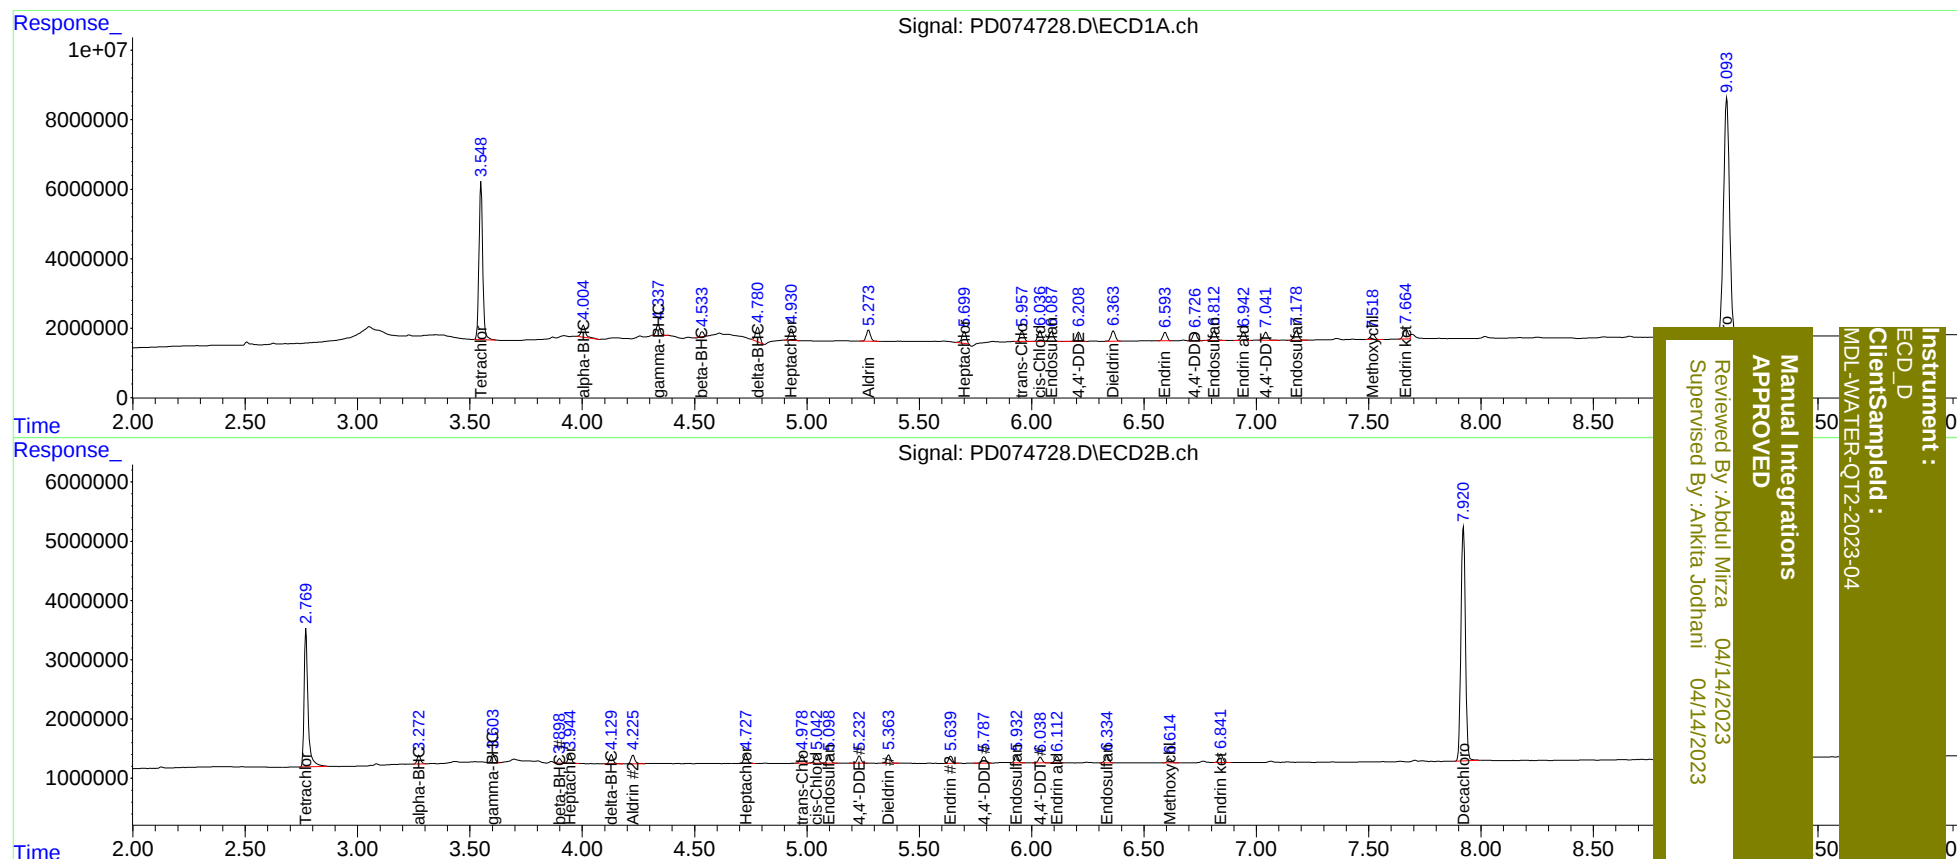

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 04/14/2023
Supervised By: Ankita Jodhani 04/14/2023

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT2-2023-04