

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041519\
 Data File : PD052927.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2019 11:30
 Operator : AJ\SJ
 Sample : PB118826BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 05:29:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.220	4.044	26558008	567.3E6	17.443	17.927
2) SA Decachlor...	7.818	9.167	50861239	596.0E6	36.072	41.334
Target Compounds						
6) B beta-BHC	0.000	4.933f	0 25889039	N.D.	1.324	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041519\
Data File : PD052927.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2019 11:30
Operator : AJ\SJ
Sample : PB118826BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 05:29:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

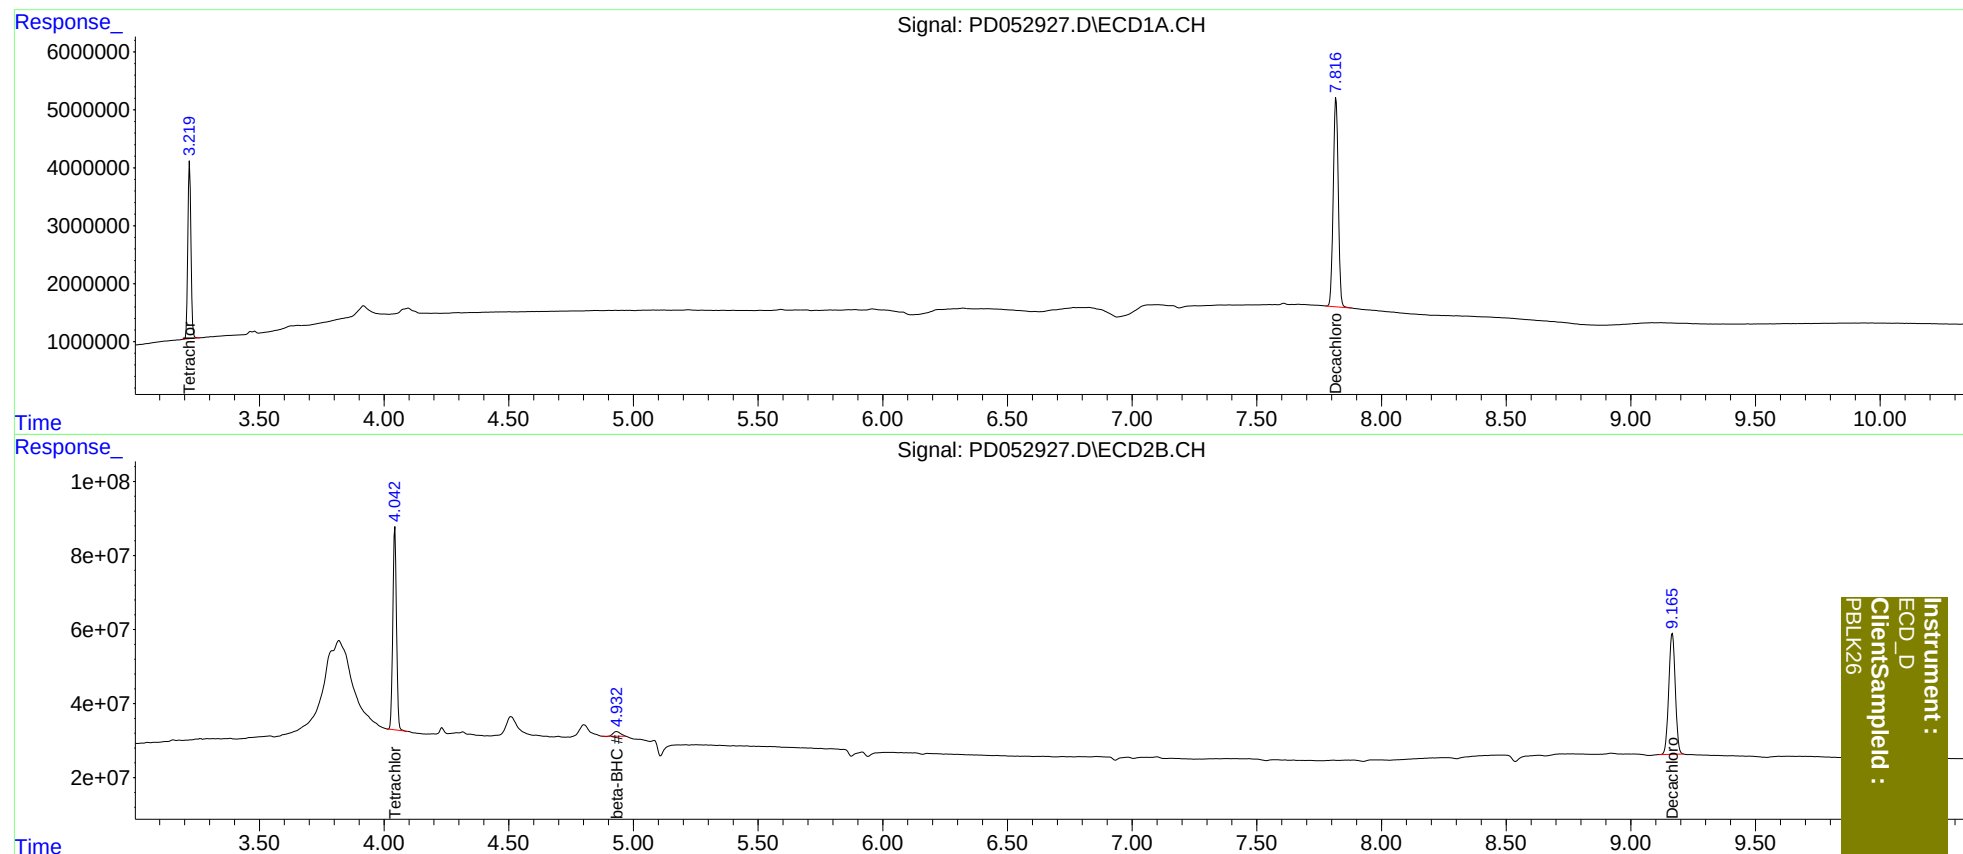


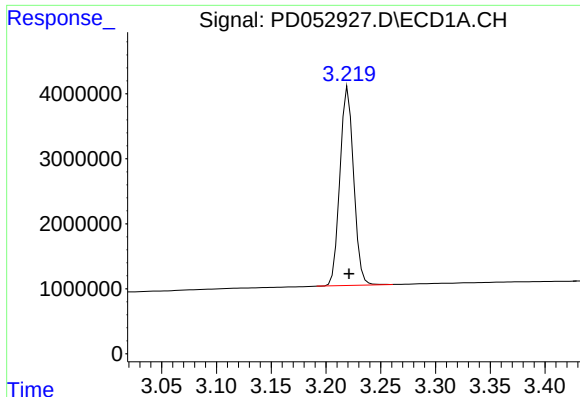

#1 Tetrachloro-m-xylene


R.T.: 3.220 min
Delta R.T.: 0.000 min
Response: 26558008
Conc: 17.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK26

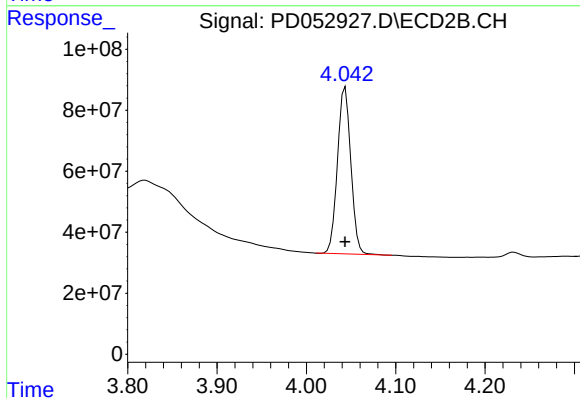


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 567312590
Conc: 17.93 ng/ml

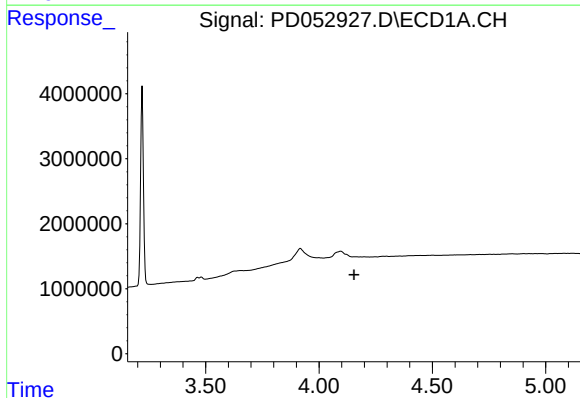


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

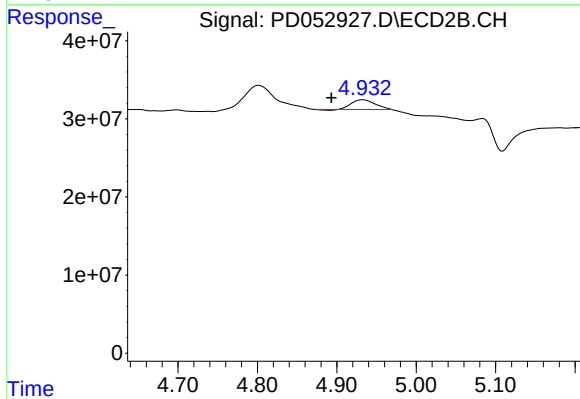

#6 beta-BHC


R.T.: 4.933 min
Delta R.T.: 0.040 min
Response: 25889039
Conc: 1.32 ng/ml

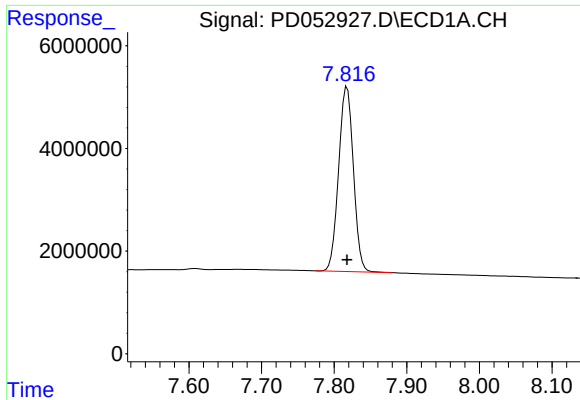

#27 Decachlorobiphenyl

R.T.: 7.818 min
Delta R.T.: 0.000 min
Response: 50861239
Conc: 36.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK26

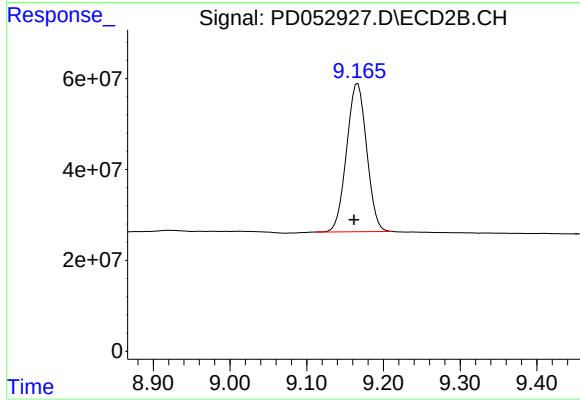

#27 Decachlorobiphenyl

R.T.: 9.167 min
Delta R.T.: 0.005 min
Response: 595990030
Conc: 41.33 ng/ml