

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041519\
 Data File : PD052930.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Apr 2019 12:16
 Operator : AJ\SJ
 Sample : PIBLK44
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK45

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 16 05:29:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Apr 09 07:32:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.223	4.044	29296854	638.6E6	19.242	20.178
2) SA Decachlor...	7.822	9.169	57625731	697.0E6	40.870	48.338
Target Compounds						
6) B beta-BHC	0.000	4.922f	0	50560658	N.D.	2.586

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041519\
Data File : PD052930.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Apr 2019 12:16
Operator : AJ\SJ
Sample : PIBLK44
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 16 05:29:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD040819CLP.M
Quant Title : GC Extractables
QLast Update : Tue Apr 09 07:32:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

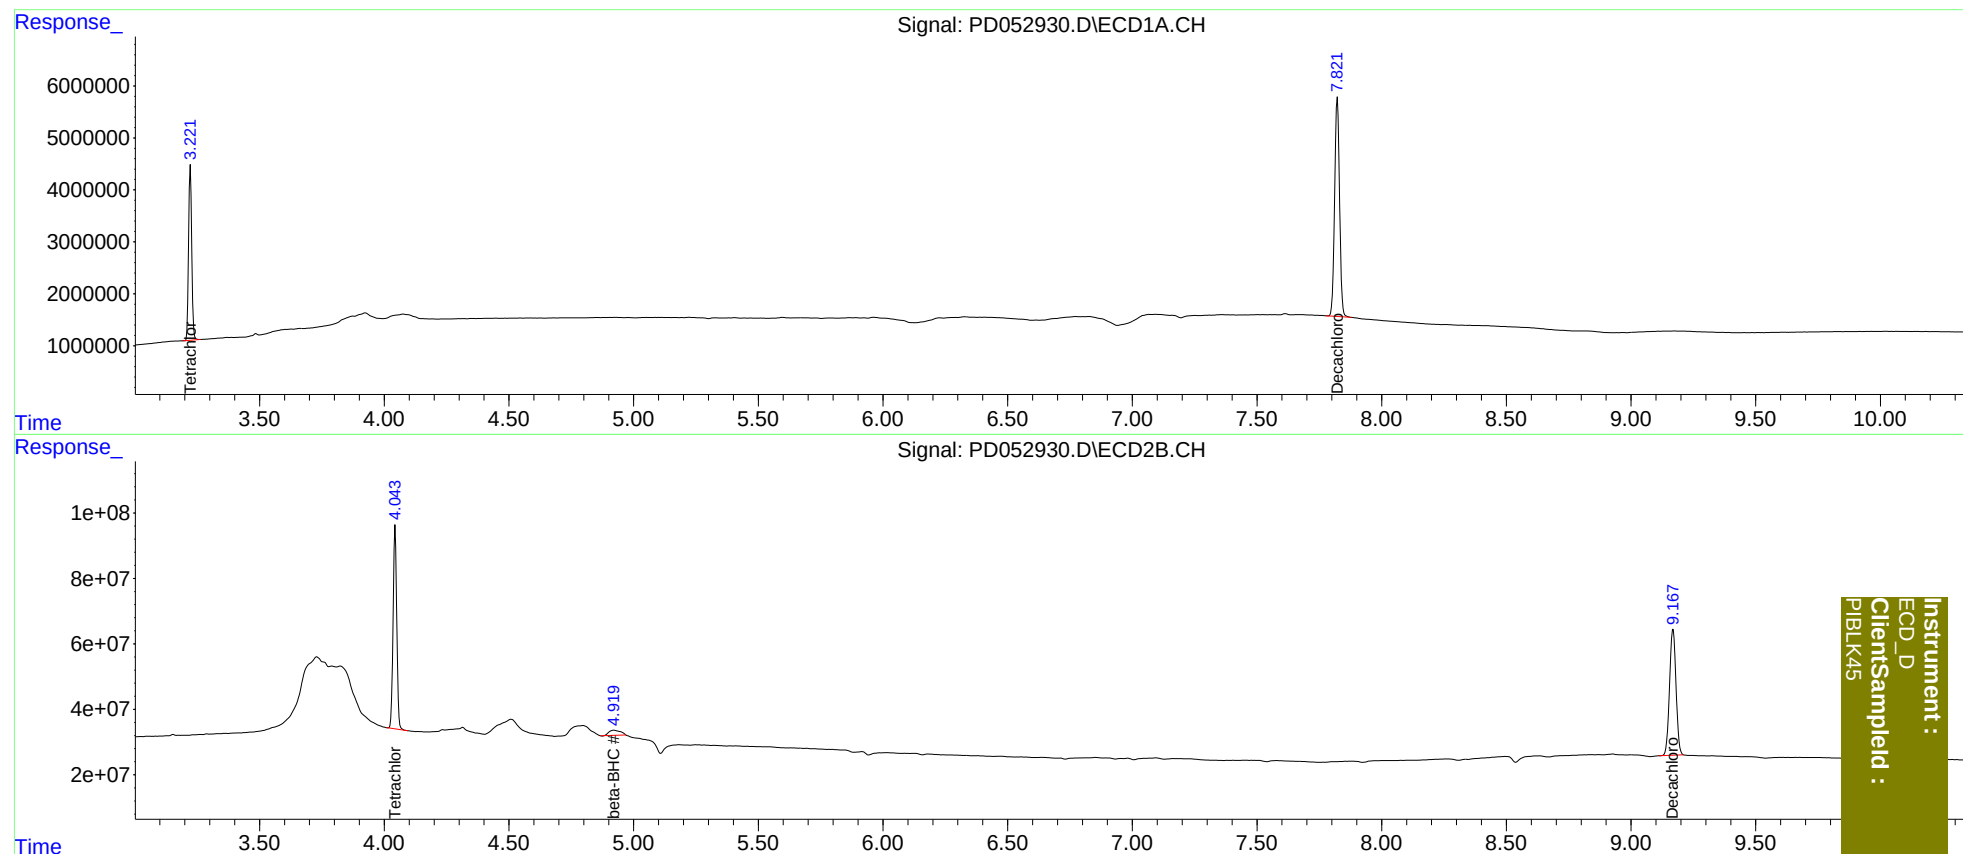


Instrument :
ECD_D
ClientSampleId :
PIBLK45

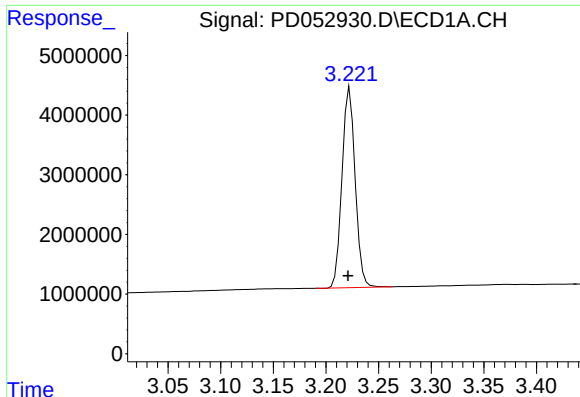

#1 Tetrachloro-m-xylene


R.T.: 3.223 min
Delta R.T.: 0.002 min
Response: 29296854
Conc: 19.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK45

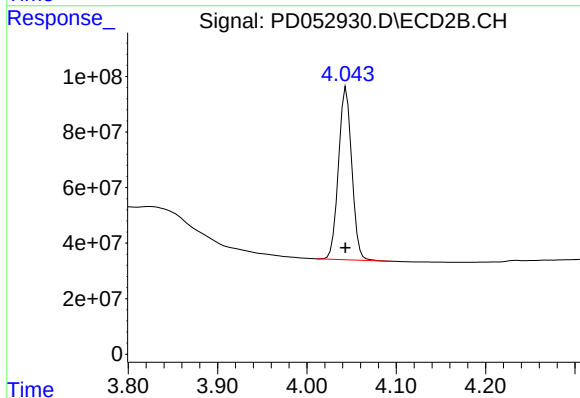


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 638552173
Conc: 20.18 ng/ml

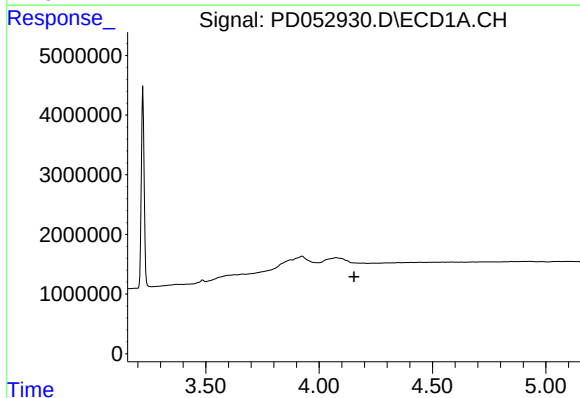


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.155 min
Response: 0
Conc: N.D.

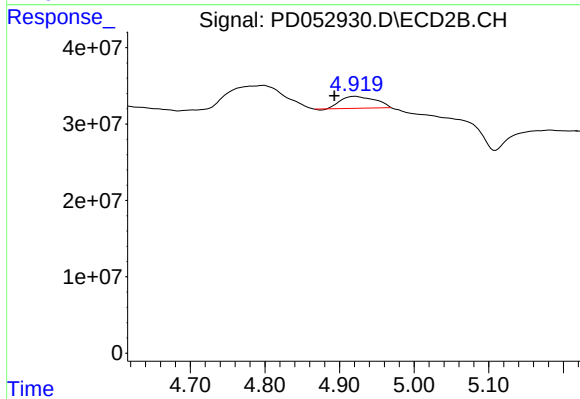

#6 beta-BHC


R.T.: 4.922 min
Delta R.T.: 0.028 min
Response: 50560658
Conc: 2.59 ng/ml

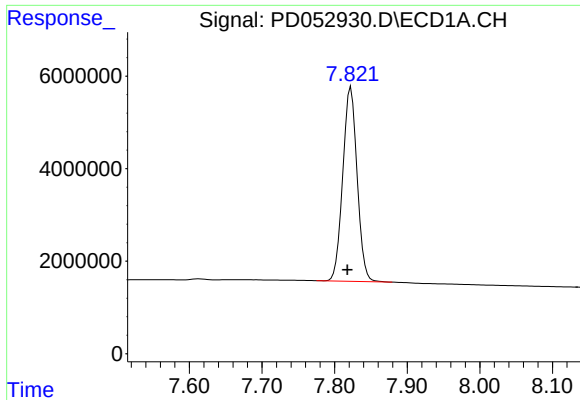

#27 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: 0.005 min
Response: 57625731
Conc: 40.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK45

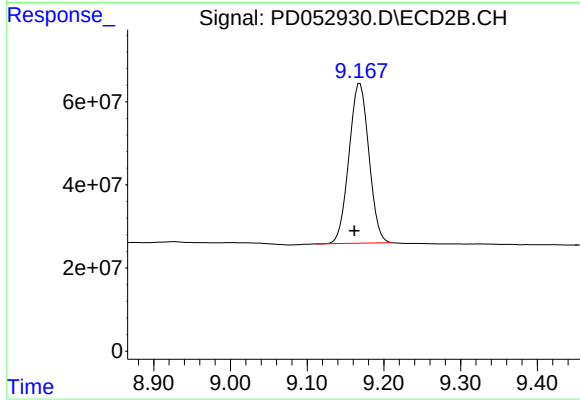

#27 Decachlorobiphenyl

R.T.: 9.169 min
Delta R.T.: 0.007 min
Response: 696971524
Conc: 48.34 ng/ml