

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 11:24
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 06:37:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 15 06:34:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	11937790	6731919	5.201	5.217
27)	SA Decachlor...	9.093	7.920	30757801	13687975	11.507	11.519
Target Compounds							
2)	A alpha-BHC	4.006	3.273	17547848	8628315	4.773	4.810
3)	MA gamma-BHC...	4.339	3.603	16615682	8113866	4.762	4.795
4)	MA Heptachlor	4.931	3.945	16862066	8134002	4.898	4.881
9)	A Endosulfan I	6.088	5.098	14744170	7126830	5.147	5.095
13)	MA Dieldrin	6.364	5.363	30437056	14988001	9.620	9.765
14)	MA Endrin	6.594	5.639	26070574	13476068	9.737	9.950
16)	A 4,4'-DDD	6.727	5.787	23068079	11597314	9.596	9.729
17)	MA 4,4'-DDT	7.042	6.039	25417503	11899463	9.810	9.541
20)	A Methoxychlor	7.518	6.615	76391664	34908074	52.081	53.037

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 11:24
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 06:37:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 15 06:34:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

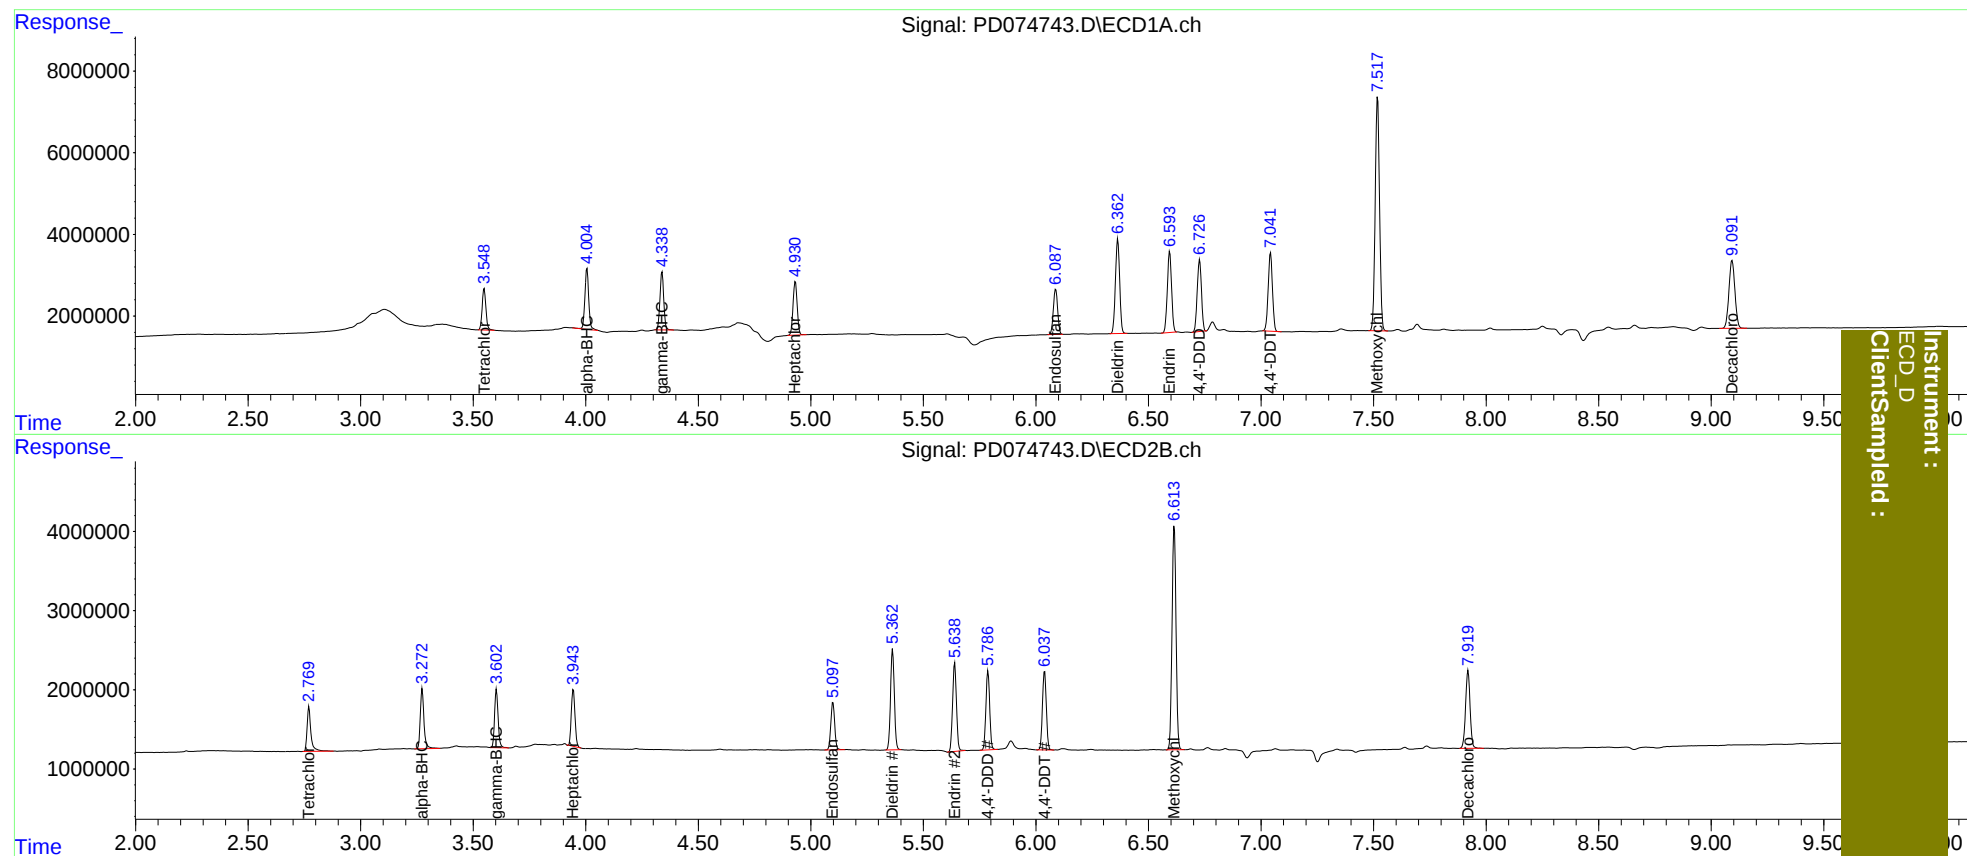


Instrument :
ECD_D
ClientSampled :
INDA101

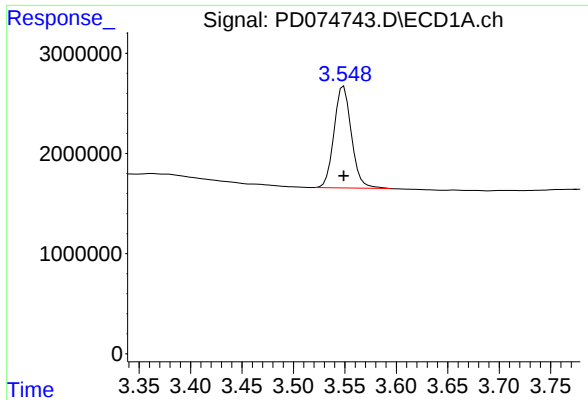

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 11937790
Conc: 5.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

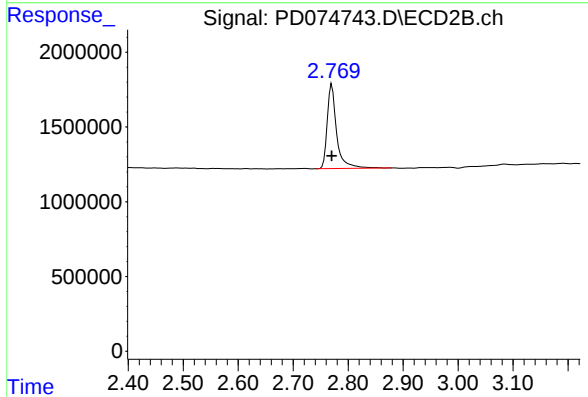


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 6731919
Conc: 5.22 ng/ml

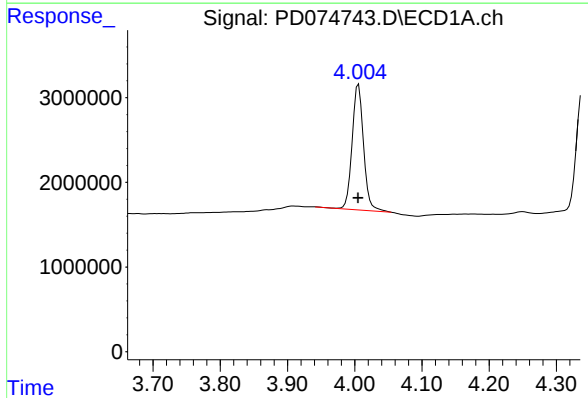


#2 alpha-BHC

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 17547848
Conc: 4.77 ng/ml

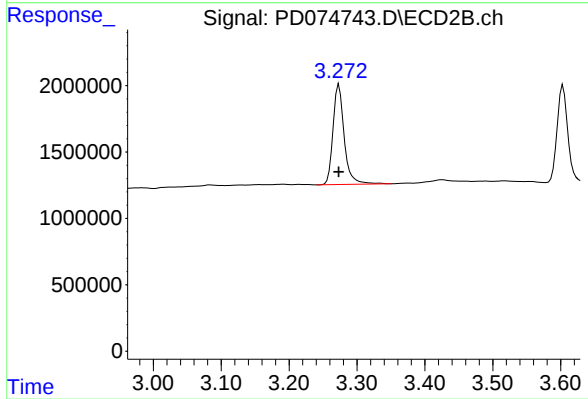

#2 alpha-BHC


R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 8628315
Conc: 4.81 ng/ml

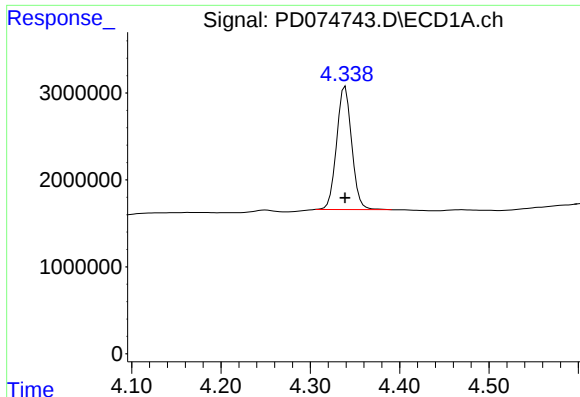

#3 gamma-BHC (Lindane)


R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 16615682
Conc: 4.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

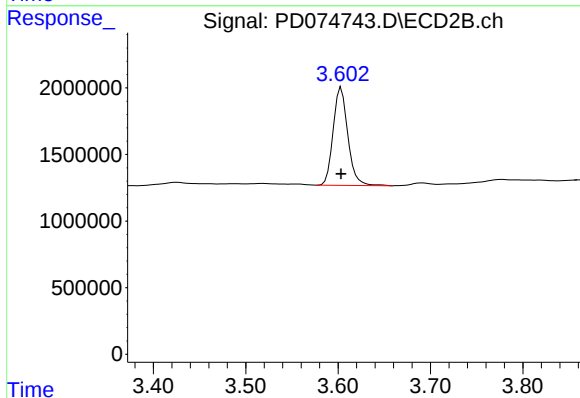


#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.000 min
Response: 8113866
Conc: 4.80 ng/ml

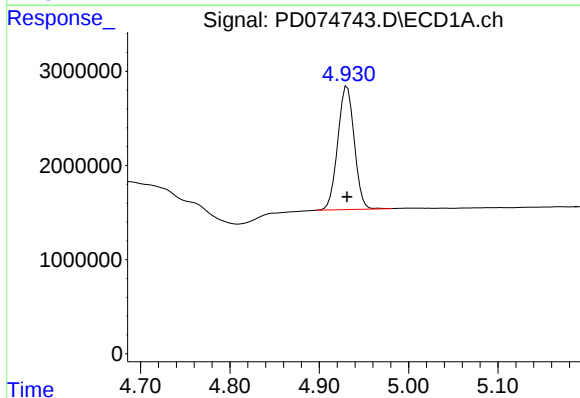


#4 Heptachlor

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 16862066
Conc: 4.90 ng/ml

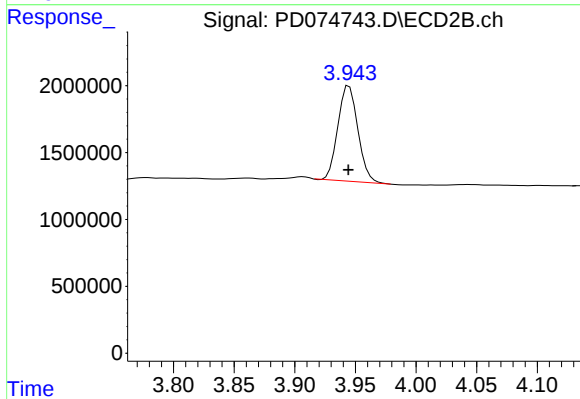

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 8134002
Conc: 4.88 ng/ml

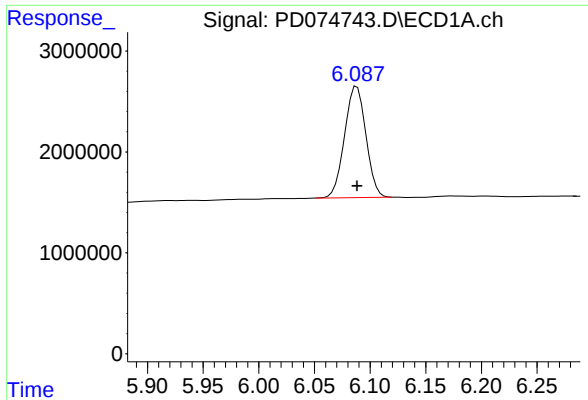

#9 Endosulfan I


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 14744170
Conc: 5.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

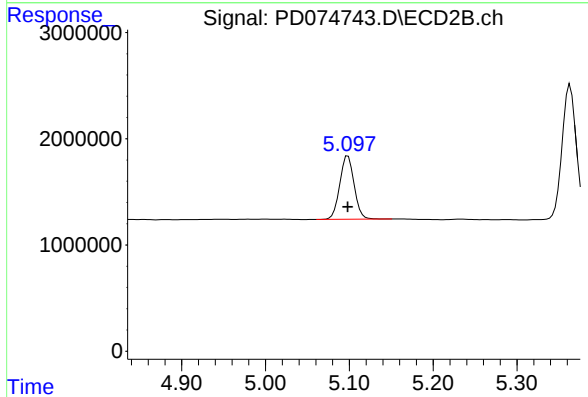


#9 Endosulfan I

R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 7126830
Conc: 5.09 ng/ml

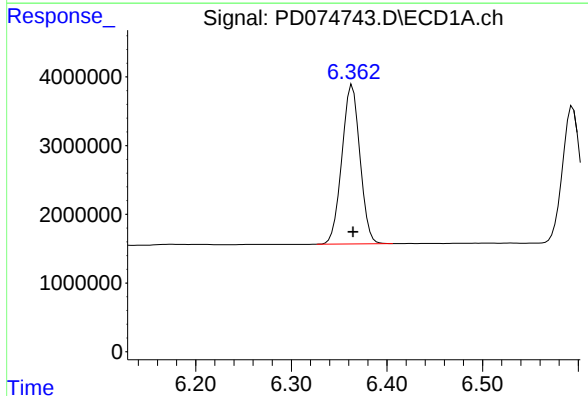


#13 Dieldrin

R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 30437056
Conc: 9.62 ng/ml

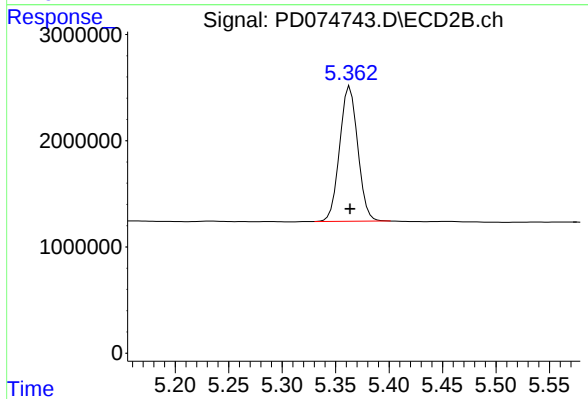

#13 Dieldrin


R.T.: 5.363 min
Delta R.T.: 0.000 min
Response: 14988001
Conc: 9.76 ng/ml

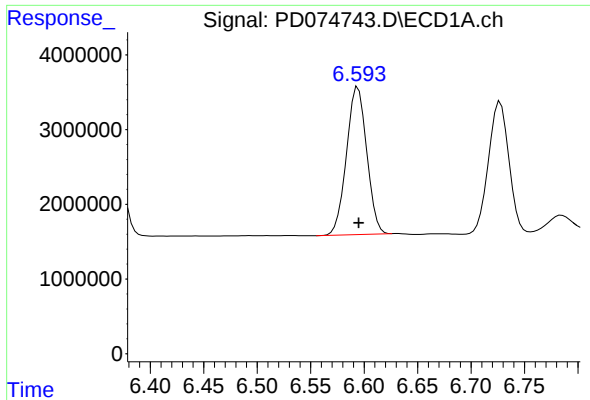

#14 Endrin


R.T.: 6.594 min
Delta R.T.: 0.000 min
Response: 26070574
Conc: 9.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

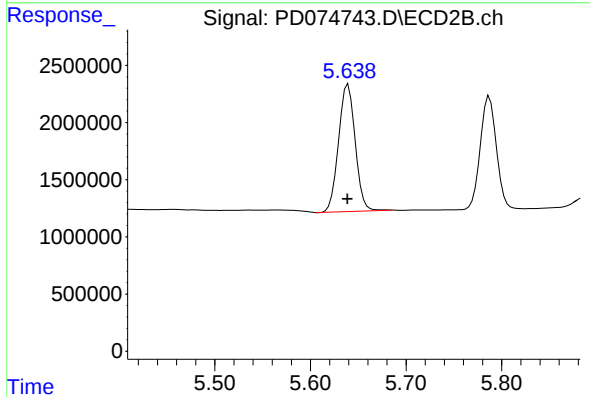


#14 Endrin

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 13476068
Conc: 9.95 ng/ml

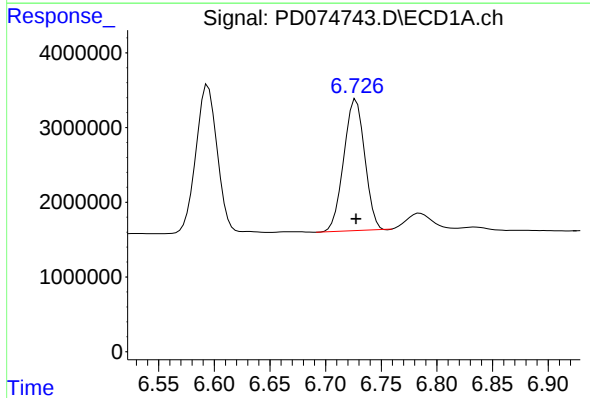


#16 4,4'-DDD

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 23068079
Conc: 9.60 ng/ml

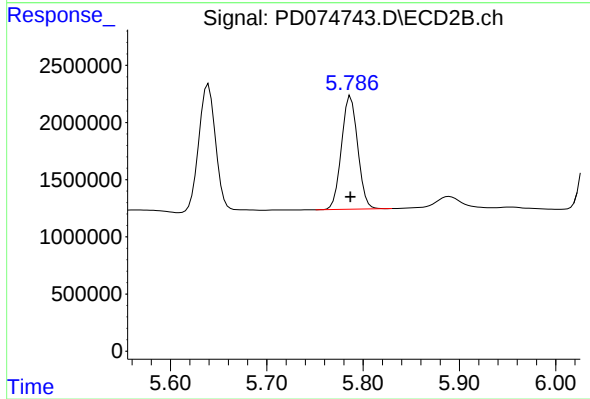

#16 4,4'-DDD


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 11597314
Conc: 9.73 ng/ml

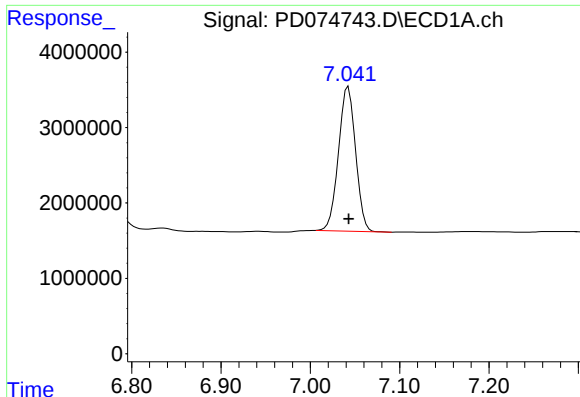

#17 4,4'-DDT


R.T.: 7.042 min
Delta R.T.: 0.000 min
Response: 25417503
Conc: 9.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

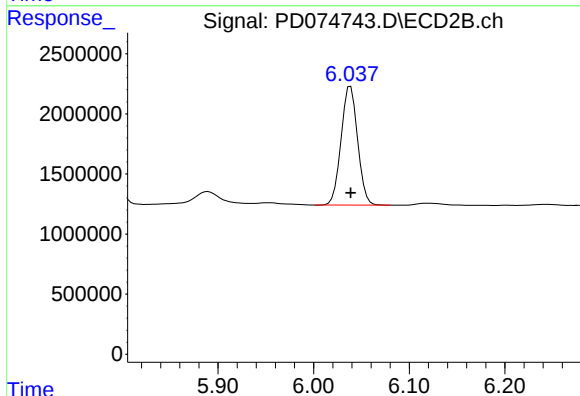


#17 4,4'-DDT

R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 11899463
Conc: 9.54 ng/ml

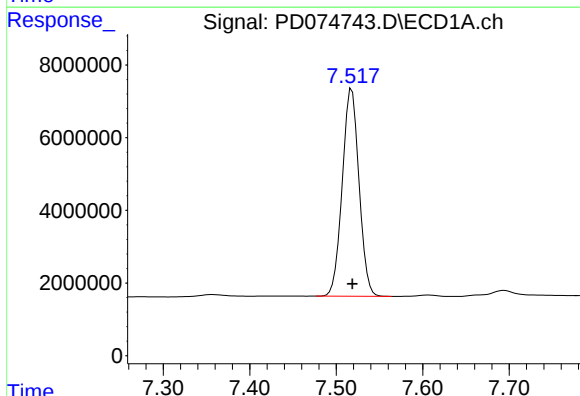


#20 Methoxychlor

R.T.: 7.518 min
Delta R.T.: 0.000 min
Response: 76391664
Conc: 52.08 ng/ml

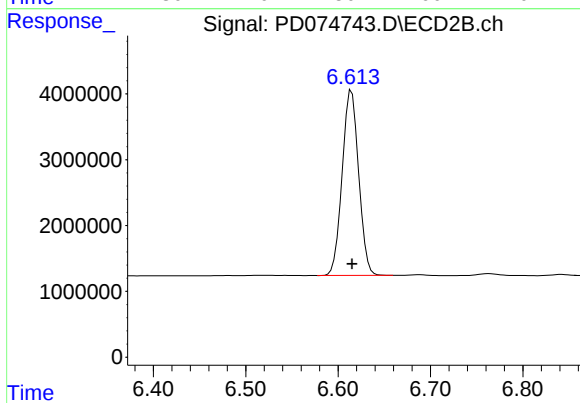

#20 Methoxychlor


R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 34908074
Conc: 53.04 ng/ml

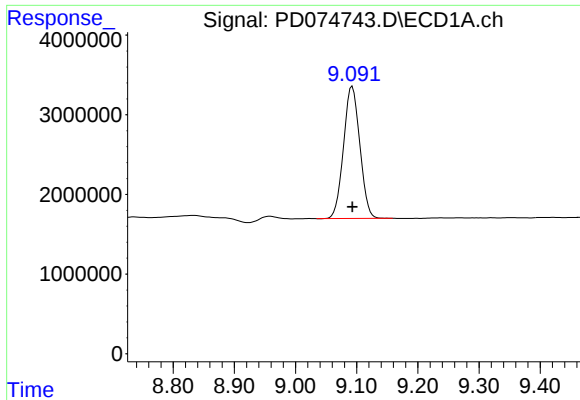

#27 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 30757801
Conc: 11.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

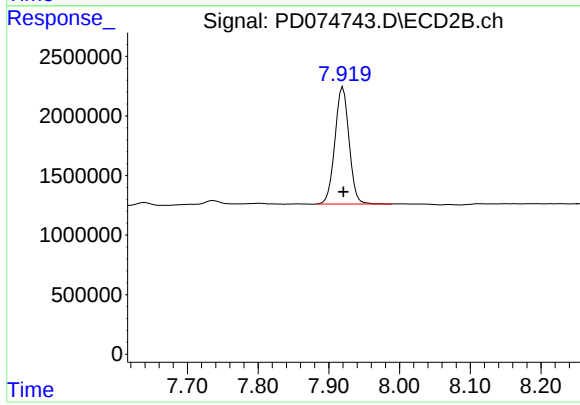

#27 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: 0.000 min
Response: 13687975
Conc: 11.52 ng/ml