

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 11:51
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 06:38:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 15 06:34:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.770	23963978	13478912	10.440	10.445
27)	SA Decachlor...	9.095	7.922	57482058	25463101	21.505	21.429
Target Compounds							
2)	A alpha-BHC	4.005	3.273	35615914	17729886	9.688	9.885
3)	MA gamma-BHC...	4.338	3.603	34359874	16906311	9.848	9.991
4)	MA Heptachlor	4.931	3.944	34632864	16707341	10.059	10.026
9)	A Endosulfan I	6.088	5.098	29301182	14345315	10.229	10.255
13)	MA Dieldrin	6.364	5.364	62269735	30606613	19.681	19.940
14)	MA Endrin	6.595	5.639	52736013	27280635	19.695	20.143
16)	A 4,4'-DDD	6.728	5.787	47607941	23841512	19.805	20.001
17)	MA 4,4'-DDT	7.043	6.039	51241388	24535155	19.776	19.672
20)	A Methoxychlor	7.519	6.615	149.5E6	68849581	101.934	104.606


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 11:51
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 06:38:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 15 06:34:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

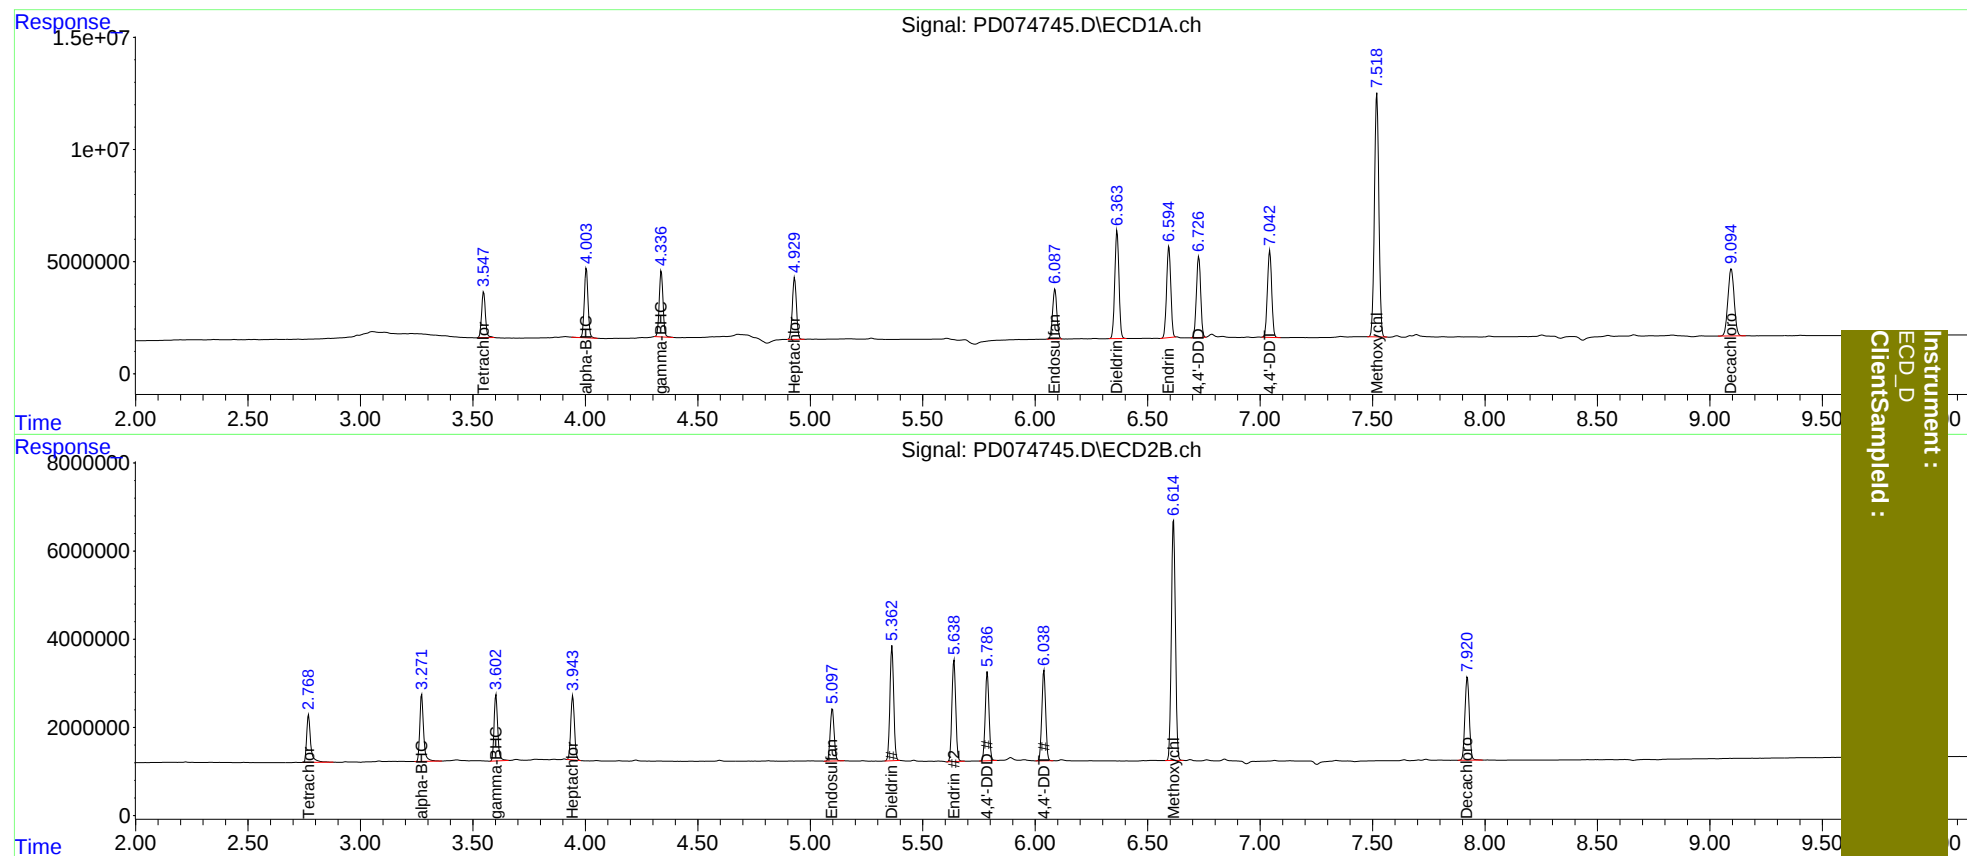


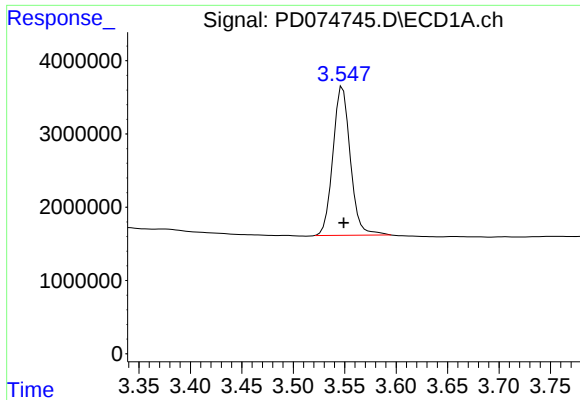

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 23963978
Conc: 10.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

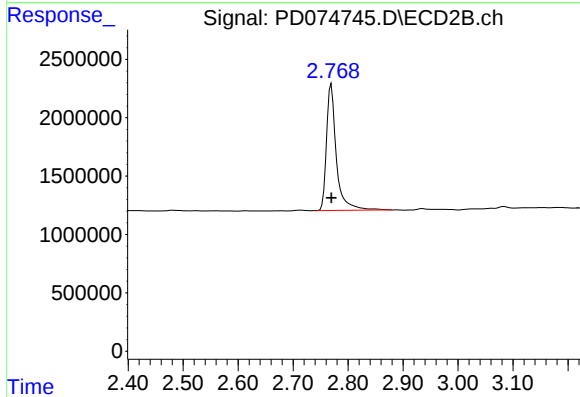


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 13478912
Conc: 10.45 ng/ml

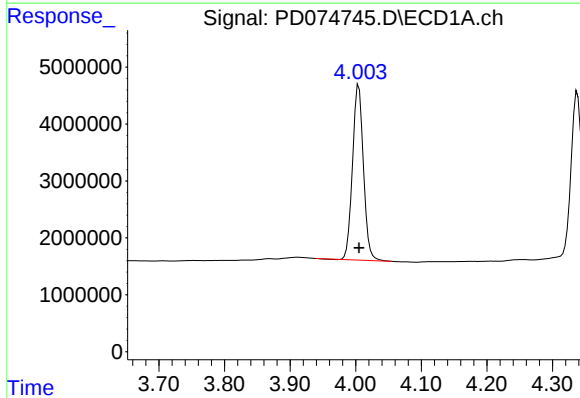


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.000 min
Response: 35615914
Conc: 9.69 ng/ml

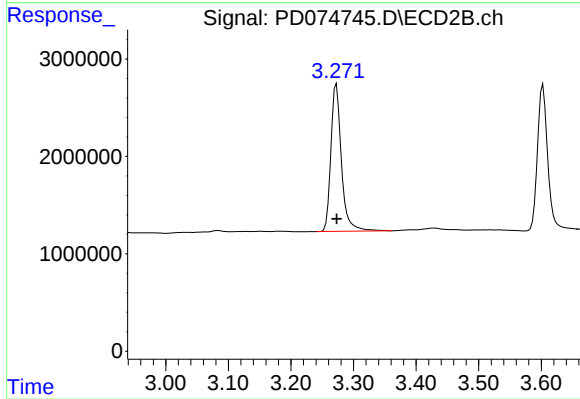

#2 alpha-BHC


R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 17729886
Conc: 9.88 ng/ml

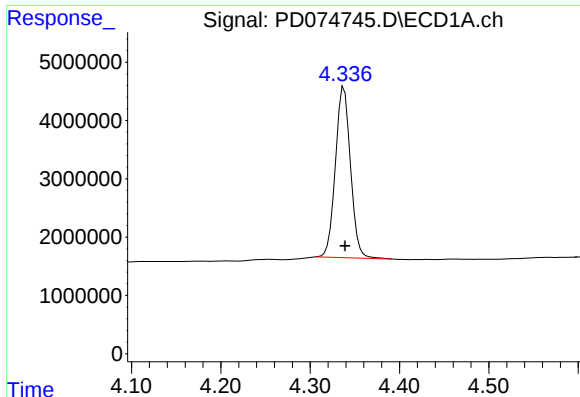

#3 gamma-BHC (Lindane)


R.T.: 4.338 min
Delta R.T.: -0.001 min
Response: 34359874
Conc: 9.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

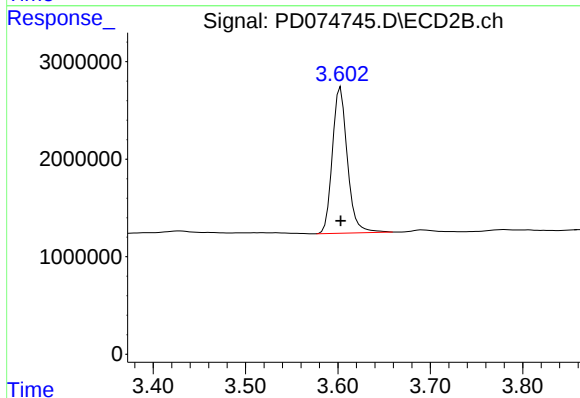


#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.000 min
Response: 16906311
Conc: 9.99 ng/ml

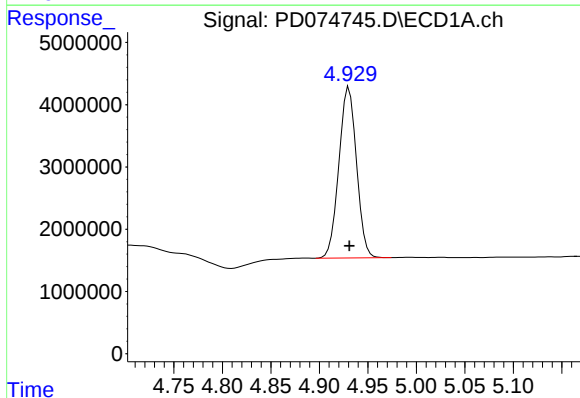


#4 Heptachlor

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 34632864
Conc: 10.06 ng/ml

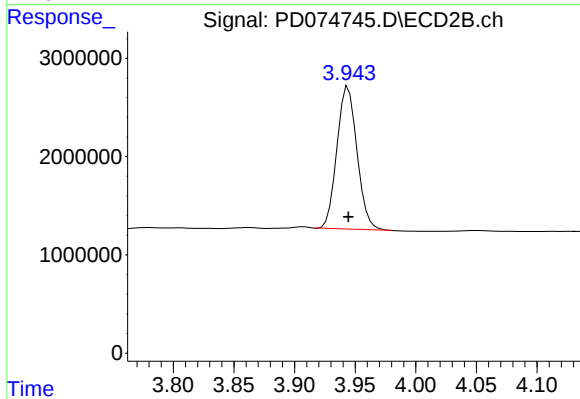

#4 Heptachlor


R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 16707341
Conc: 10.03 ng/ml

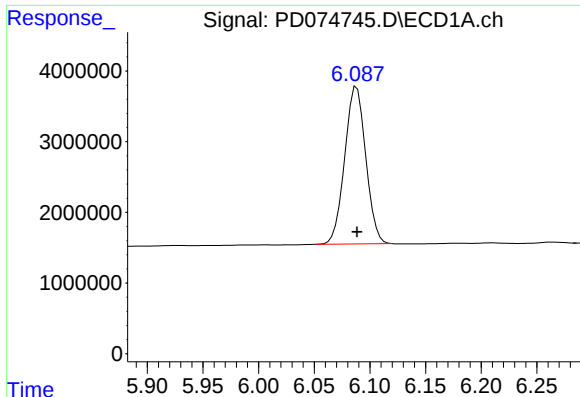

#9 Endosulfan I


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 29301182
Conc: 10.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

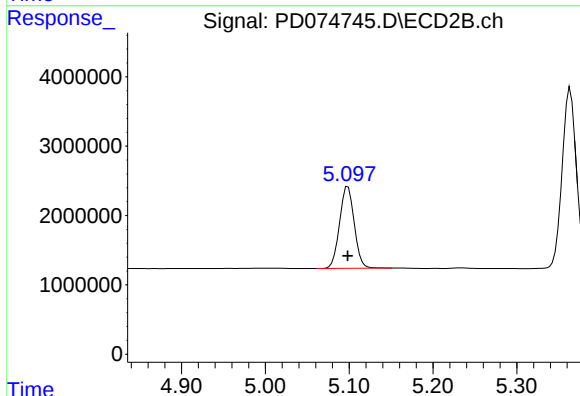


#9 Endosulfan I

R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 14345315
Conc: 10.25 ng/ml

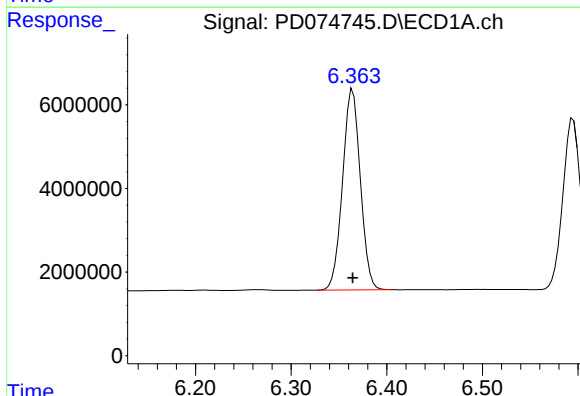


#13 Dieldrin

R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 62269735
Conc: 19.68 ng/ml

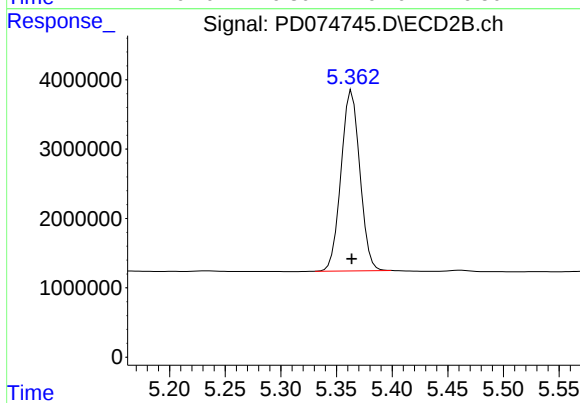

#13 Dieldrin


R.T.: 5.364 min
Delta R.T.: 0.000 min
Response: 30606613
Conc: 19.94 ng/ml

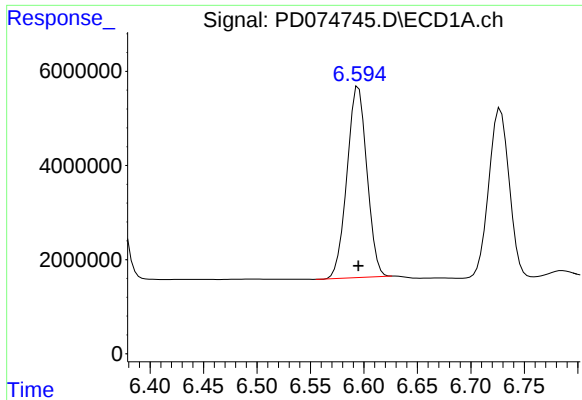

#14 Endrin


R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 52736013
Conc: 19.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

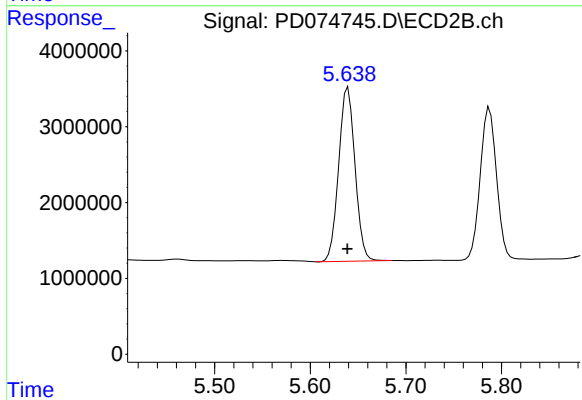


#14 Endrin

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 27280635
Conc: 20.14 ng/ml

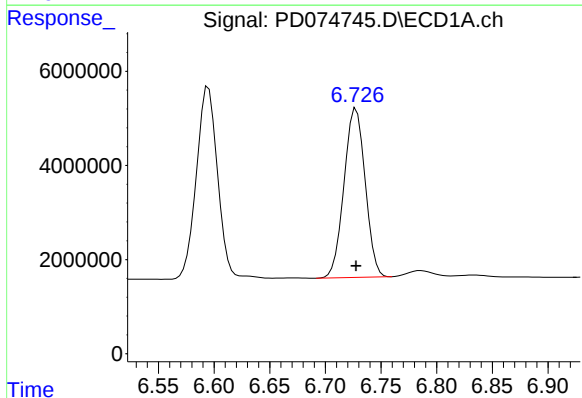


#16 4,4'-DDD

R.T.: 6.728 min
Delta R.T.: 0.000 min
Response: 47607941
Conc: 19.80 ng/ml

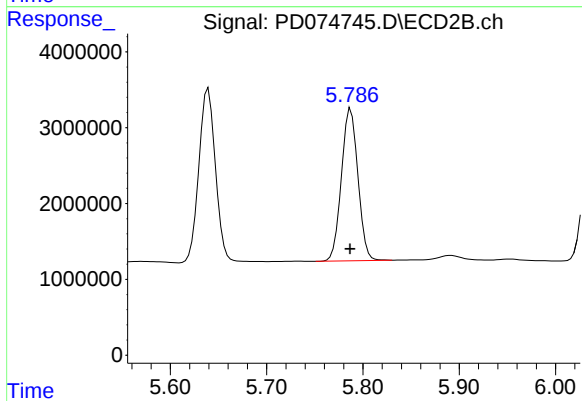

#16 4,4'-DDD


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 23841512
Conc: 20.00 ng/ml

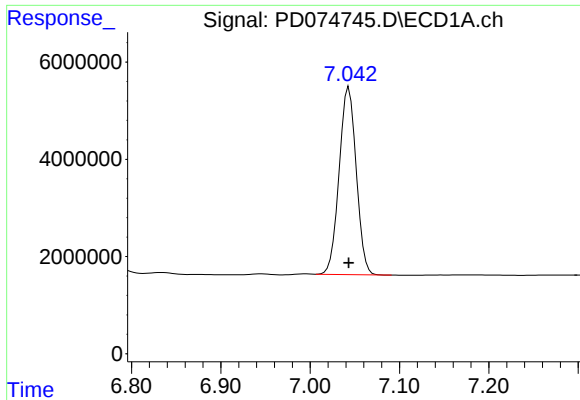

#17 4,4'-DDT


R.T.: 7.043 min
Delta R.T.: 0.000 min
Response: 51241388
Conc: 19.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

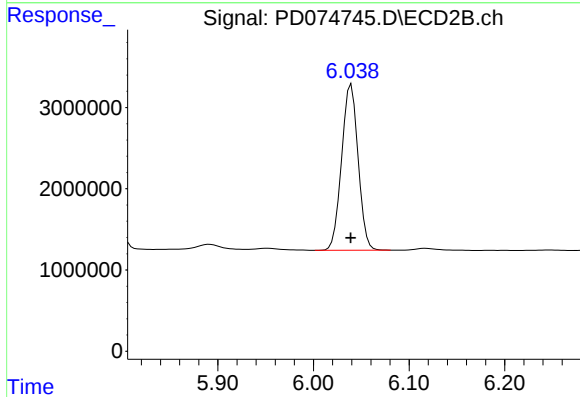


#17 4,4'-DDT

R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 24535155
Conc: 19.67 ng/ml

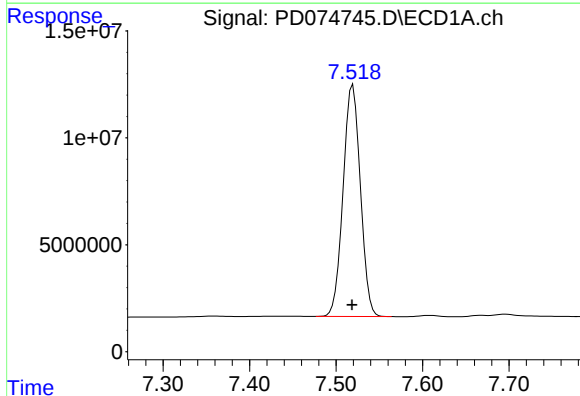


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 149516139
Conc: 101.93 ng/ml

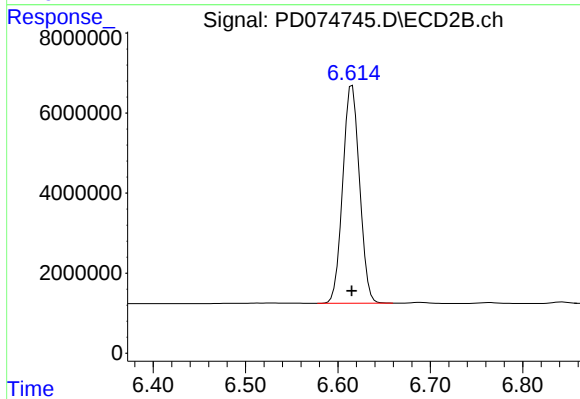

#20 Methoxychlor


R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 68849581
Conc: 104.61 ng/ml

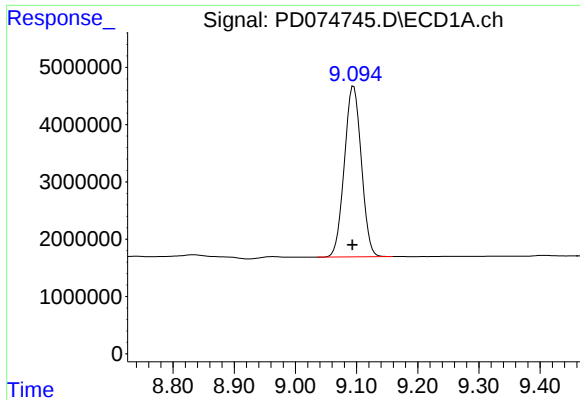

#27 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.002 min
Response: 57482058
Conc: 21.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

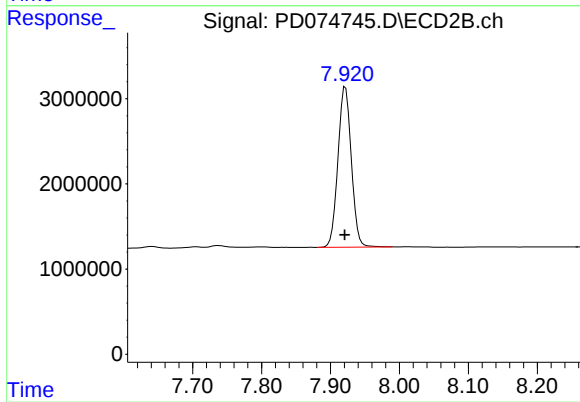

#27 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: 0.000 min
Response: 25463101
Conc: 21.43 ng/ml