

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 12:18
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 06:38:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 15 06:34:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	45907737	25809064	20.000	20.000
27)	SA Decachlor...	9.093	7.921	106.9E6	47529904	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.005	3.273	73526604	35873289	20.000	20.000
3)	MA gamma-BHC...	4.339	3.603	69778106	33841785	20.000	20.000
4)	MA Heptachlor	4.931	3.944	68858680	33328065	20.000	20.000
9)	A Endosulfan I	6.088	5.098	57287914	27977754	20.000	20.000
13)	MA Dieldrin	6.364	5.364	126.6E6	61396528	40.000	40.000
14)	MA Endrin	6.595	5.639	107.1E6	54173065	40.000	40.000
16)	A 4,4'-DDD	6.727	5.787	96155776	47680843	40.000	40.000
17)	MA 4,4'-DDT	7.043	6.039	103.6E6	49887223	40.000	40.000
20)	A Methoxychlor	7.519	6.615	293.4E6	131.6E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 12:18
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 06:38:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 15 06:34:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

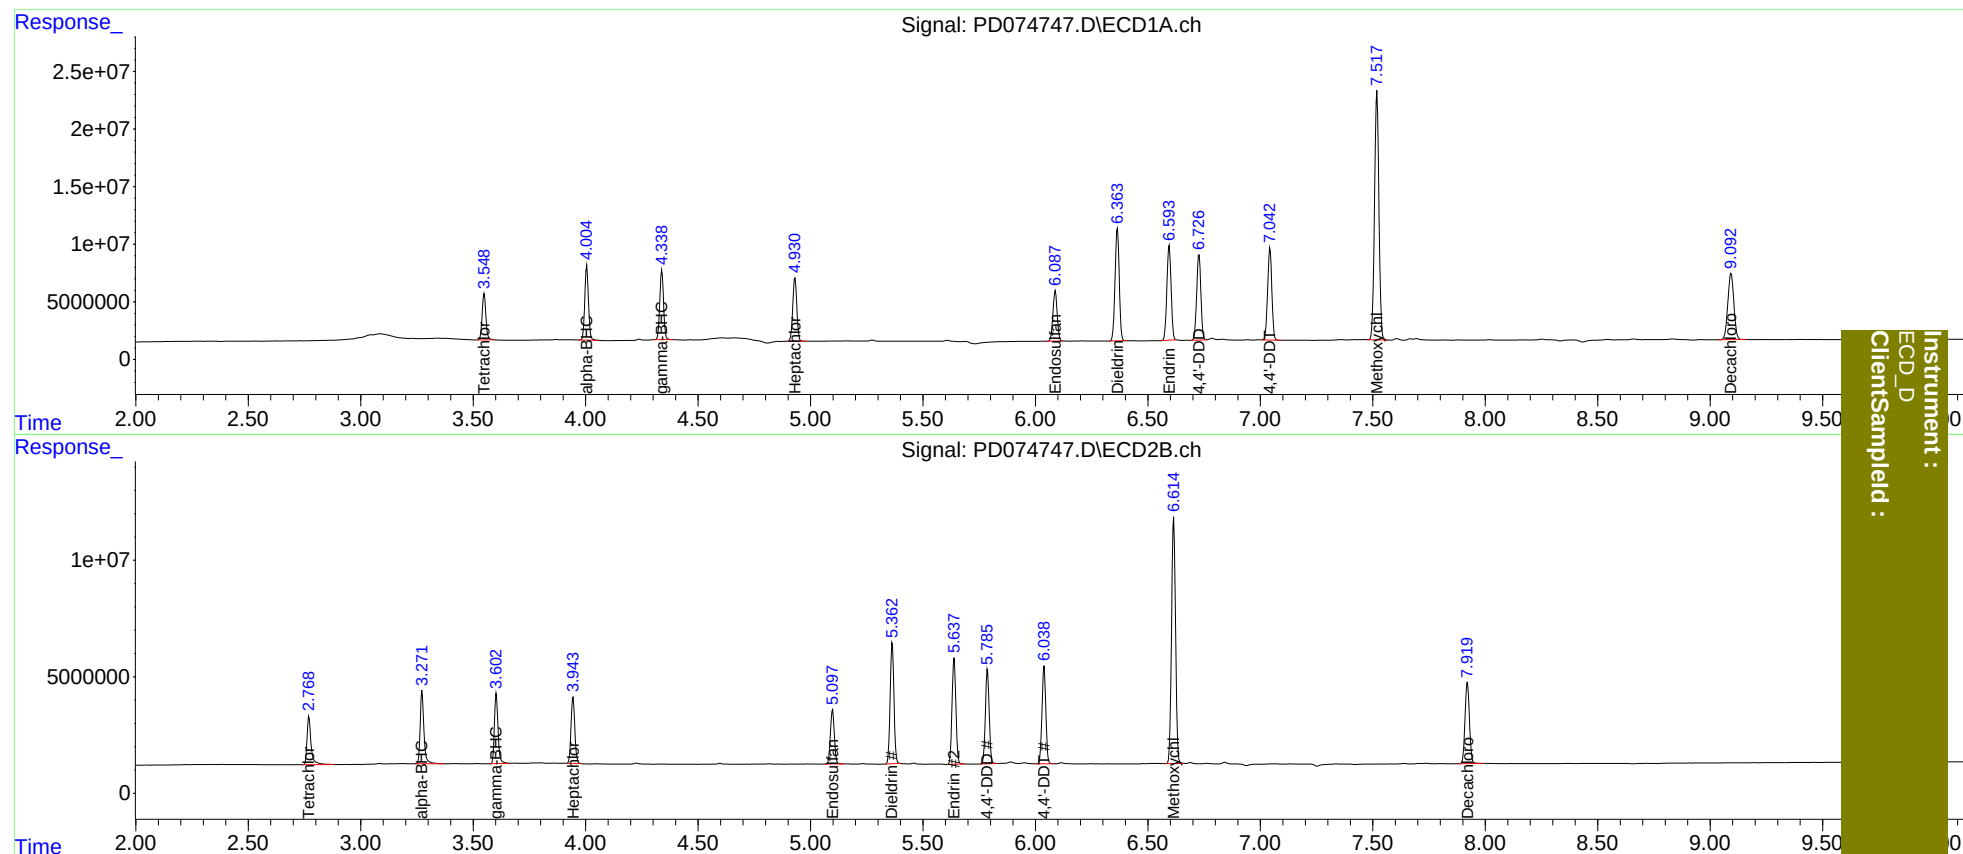


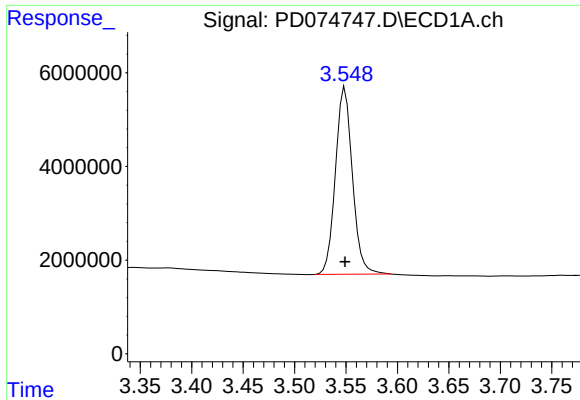

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 45907737
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

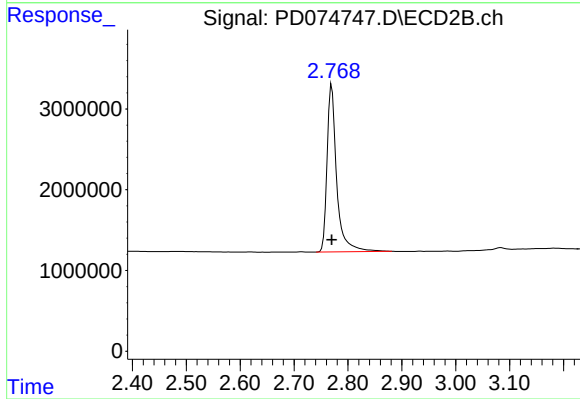


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 25809064
Conc: 20.00 ng/ml

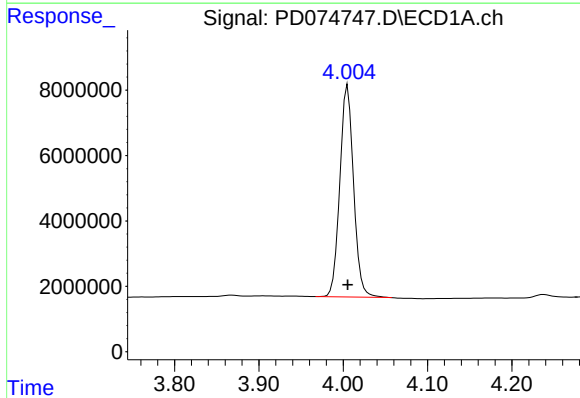


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.000 min
Response: 73526604
Conc: 20.00 ng/ml

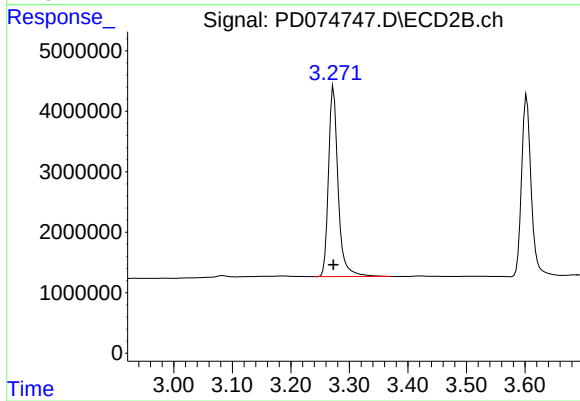

#2 alpha-BHC


R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 35873289
Conc: 20.00 ng/ml

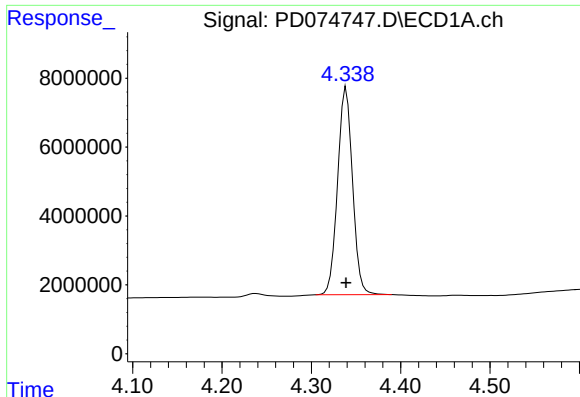

#3 gamma-BHC (Lindane)


R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 69778106
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

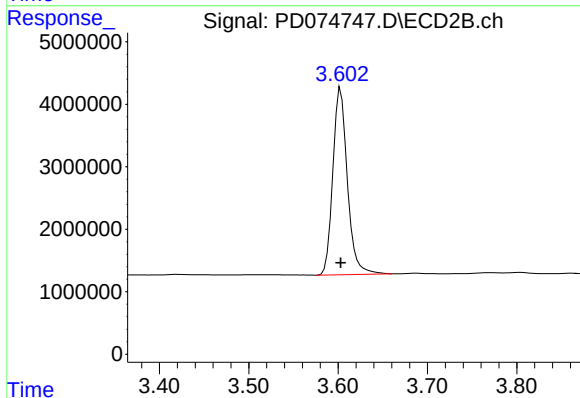


#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.000 min
Response: 33841785
Conc: 20.00 ng/ml

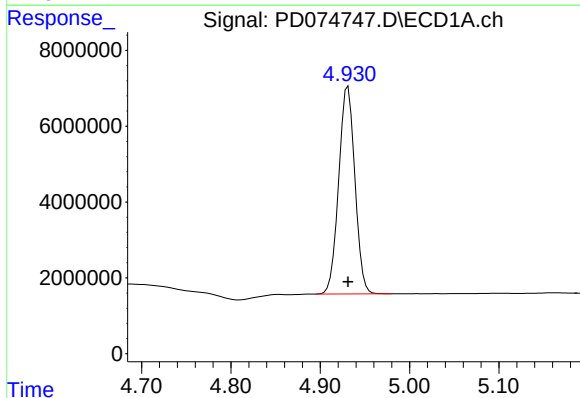


#4 Heptachlor

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 68858680
Conc: 20.00 ng/ml

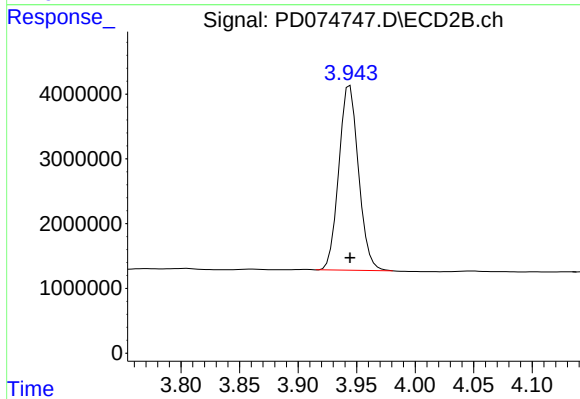

#4 Heptachlor


R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 33328065
Conc: 20.00 ng/ml

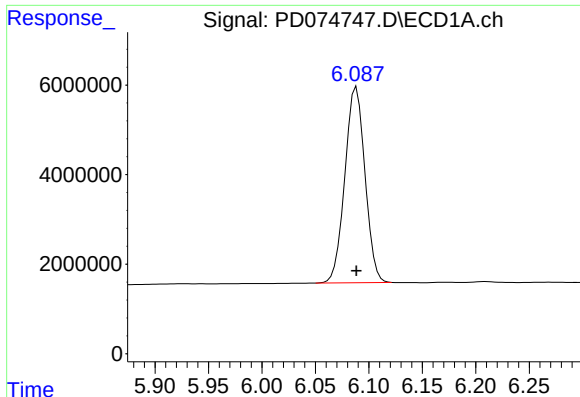

#9 Endosulfan I


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 57287914
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

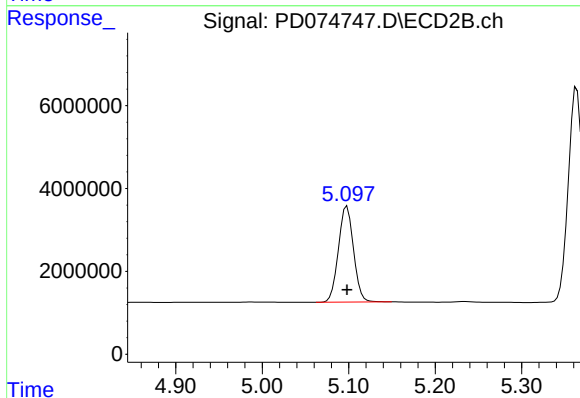


#9 Endosulfan I

R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 27977754
Conc: 20.00 ng/ml

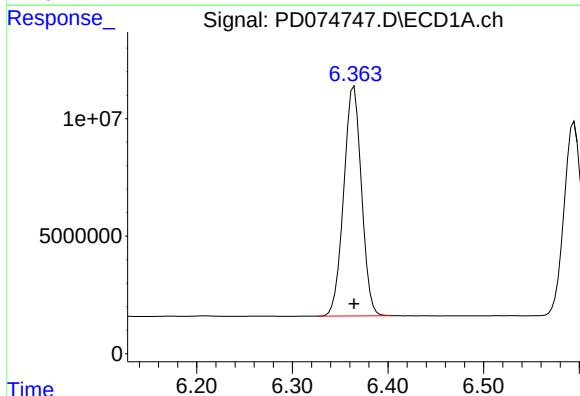


#13 Dieldrin

R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 126556052
Conc: 40.00 ng/ml

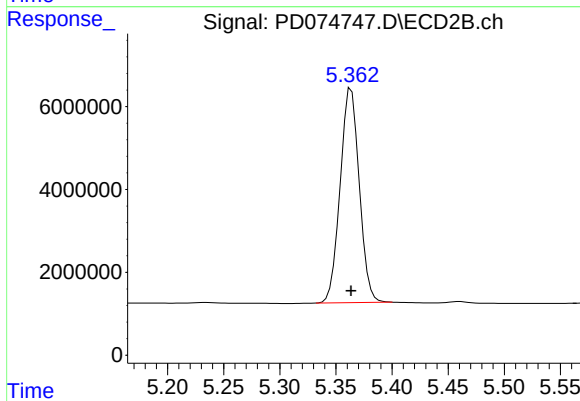

#13 Dieldrin


R.T.: 5.364 min
Delta R.T.: 0.000 min
Response: 61396528
Conc: 40.00 ng/ml

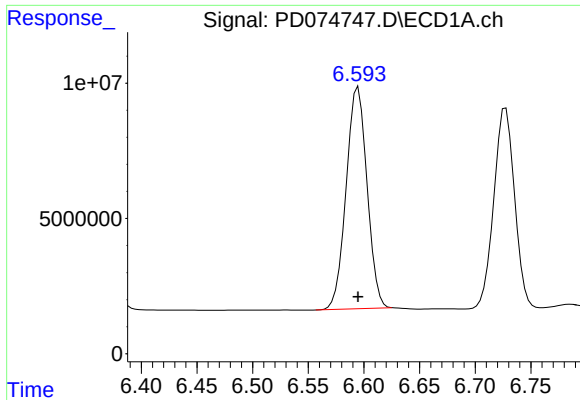

#14 Endrin


R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 107104193
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

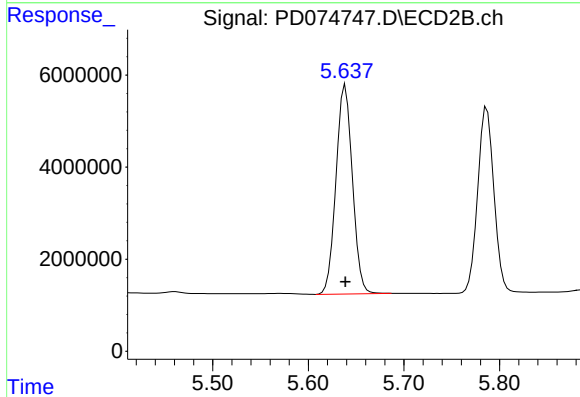


#14 Endrin

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 54173065
Conc: 40.00 ng/ml

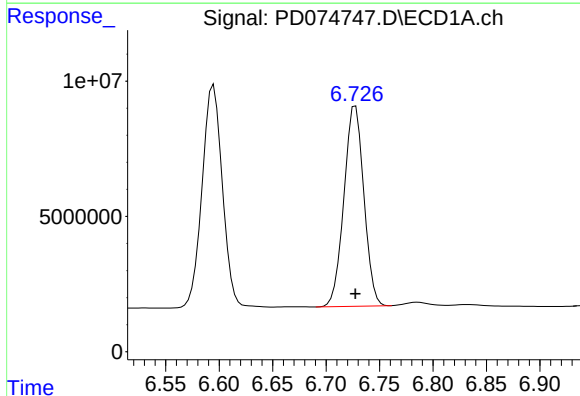


#16 4,4'-DDD

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 96155776
Conc: 40.00 ng/ml

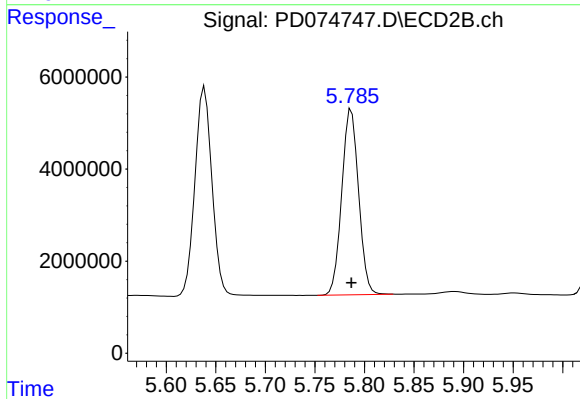

#16 4,4'-DDD


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 47680843
Conc: 40.00 ng/ml

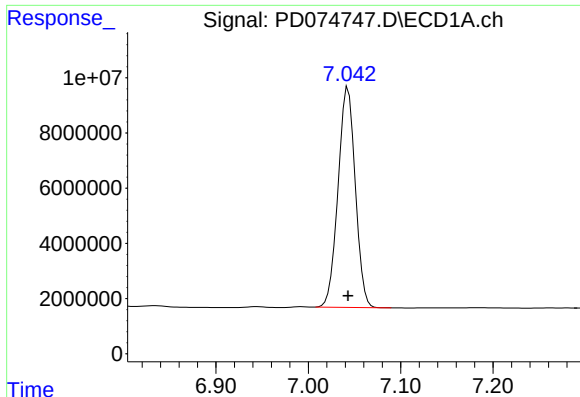

#17 4,4'-DDT


R.T.: 7.043 min
Delta R.T.: 0.000 min
Response: 103643289
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

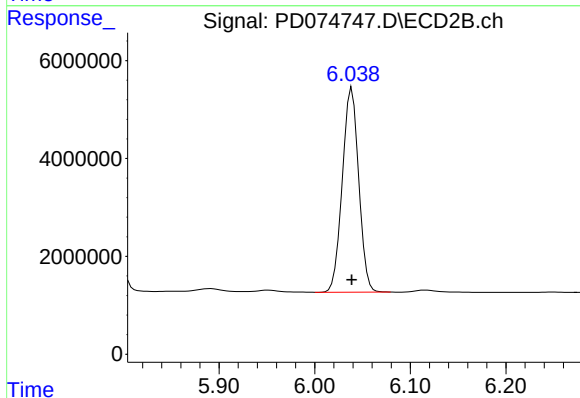


#17 4,4'-DDT

R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 49887223
Conc: 40.00 ng/ml

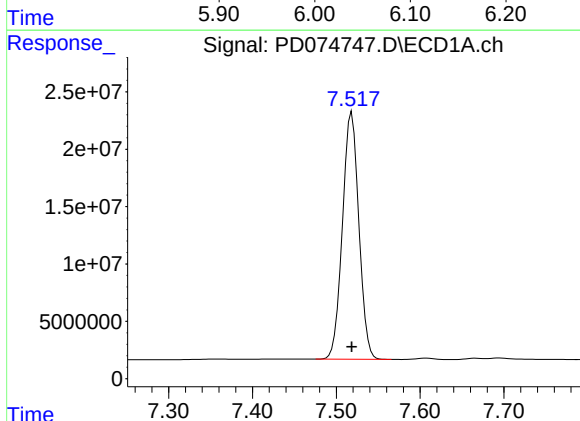


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 293357828
Conc: 200.00 ng/ml

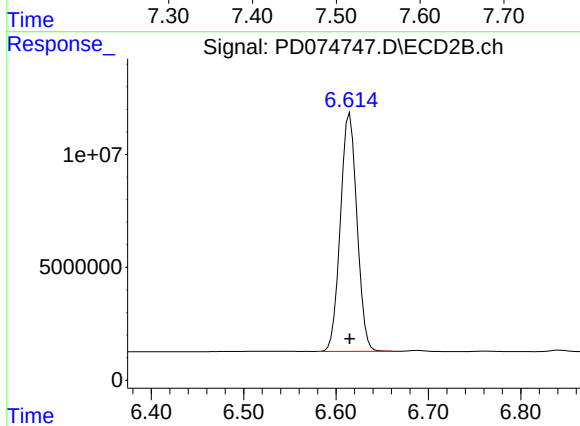

#20 Methoxychlor


R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 131636038
Conc: 200.00 ng/ml

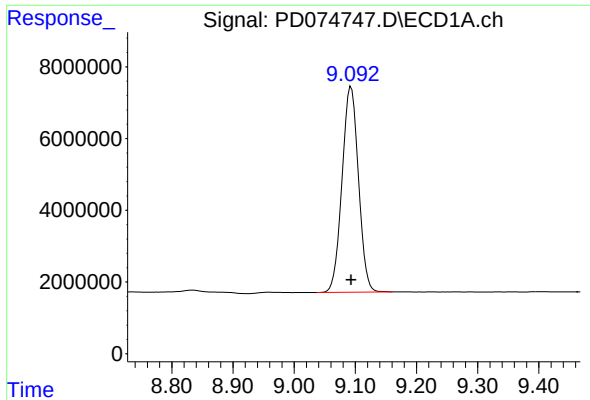

#27 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 106919472
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

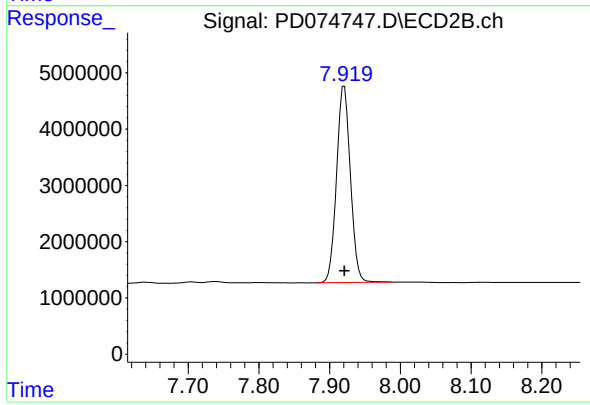

#27 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.000 min
Response: 47529904
Conc: 40.00 ng/ml