

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 12:45
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 06:38:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 15 06:34:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	94549050	52211201	41.191	40.460
27)	SA Decachlor...	9.093	7.920	210.6E6	92459445	78.771	77.812
Target Compounds							
2)	A alpha-BHC	4.005	3.273	161.8E6	76322016	44.002	42.551
3)	MA gamma-BHC...	4.339	3.603	151.4E6	71209051	43.385	42.084
4)	MA Heptachlor	4.931	3.945	150.1E6	69650161	43.610	41.797
9)	A Endosulfan I	6.088	5.098	121.2E6	57506697	42.328	41.109
13)	MA Dieldrin	6.364	5.364	277.3E6	129.2E6	87.631	84.186
14)	MA Endrin	6.595	5.639	234.5E6	113.3E6	87.582	83.664
16)	A 4,4'-DDD	6.727	5.787	209.5E6	99933804	87.160	83.836
17)	MA 4,4'-DDT	7.043	6.039	226.5E6	105.5E6	87.398	84.580
20)	A Methoxychlor	7.518	6.615	612.6E6	259.6E6	417.643	394.387

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 12:45
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 06:38:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 15 06:34:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

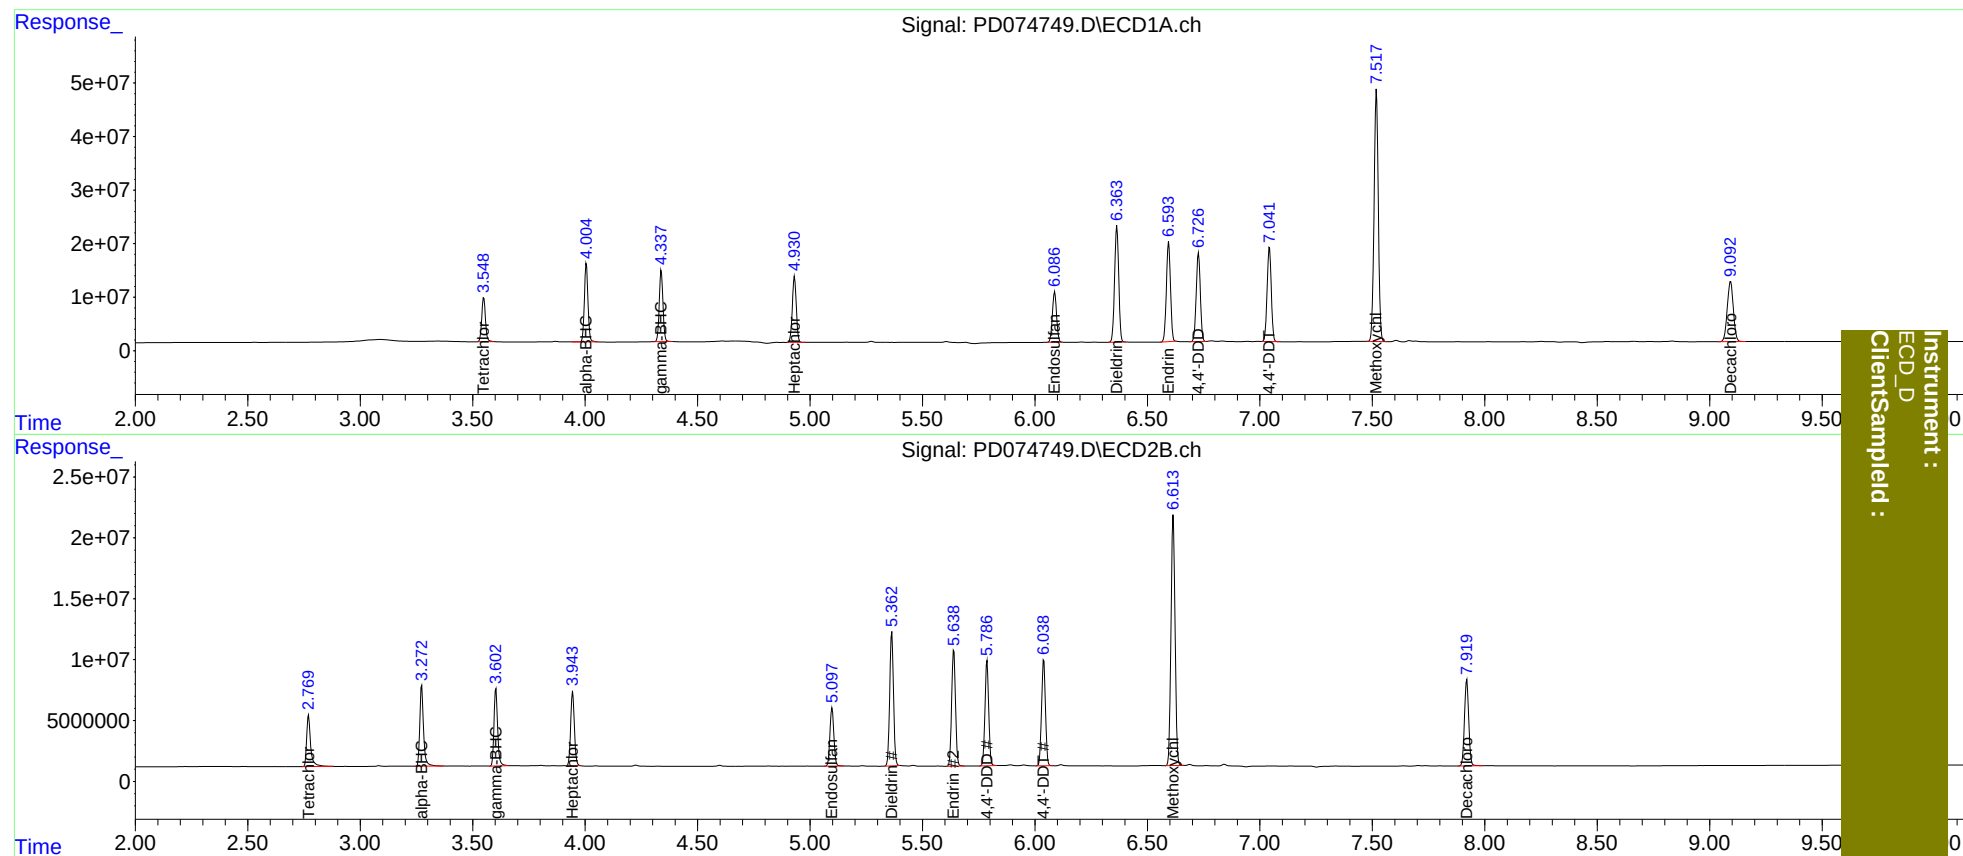


Instrument :
ECD_D
ClientSampled :

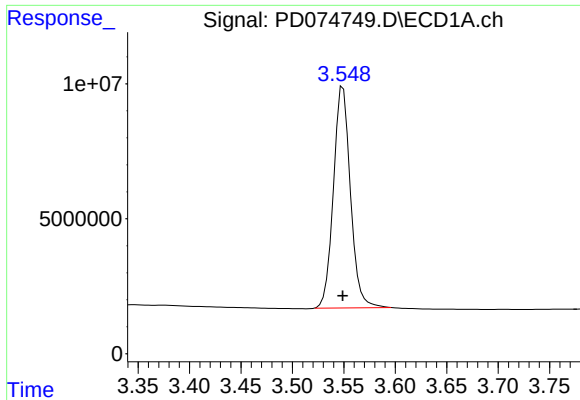

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 94549050
Conc: 41.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

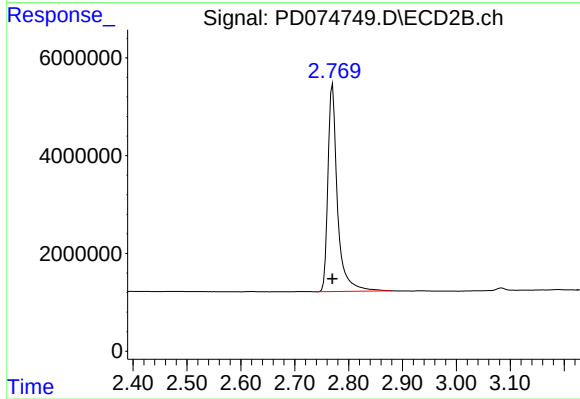


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 52211201
Conc: 40.46 ng/ml

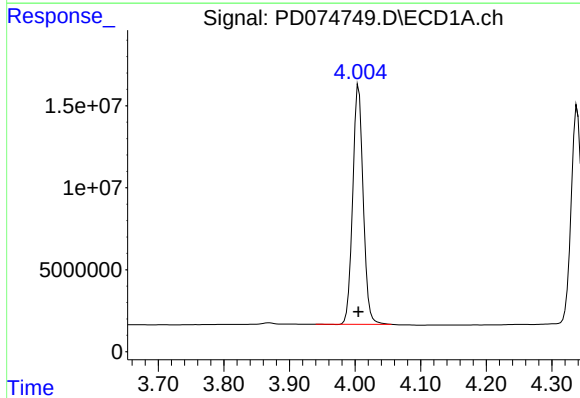


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.000 min
Response: 161764943
Conc: 44.00 ng/ml

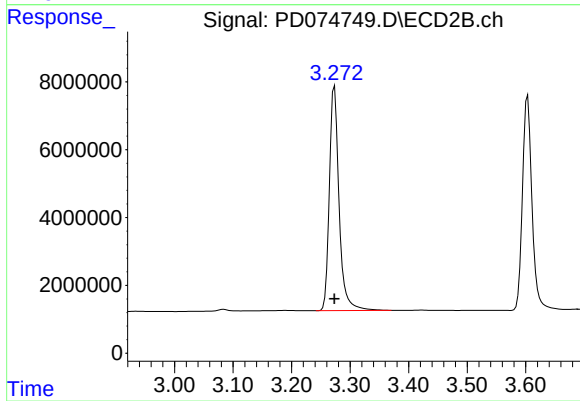

#2 alpha-BHC


R.T.: 3.273 min
Delta R.T.: 0.000 min
Response: 76322016
Conc: 42.55 ng/ml

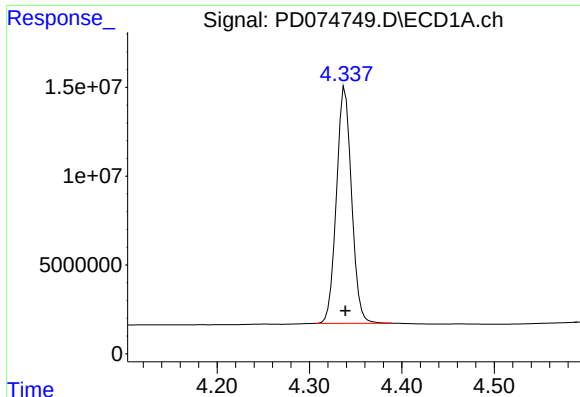

#3 gamma-BHC (Lindane)


R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 151364952
Conc: 43.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

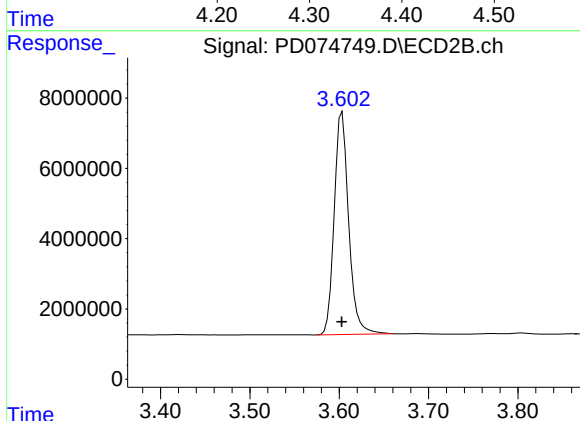


#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.000 min
Response: 71209051
Conc: 42.08 ng/ml

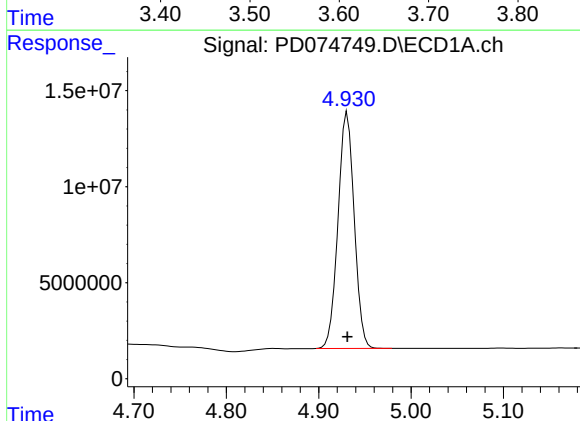


#4 Heptachlor

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 150147322
Conc: 43.61 ng/ml

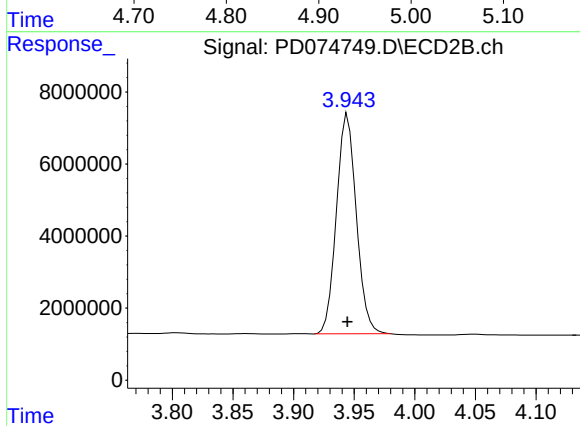

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 69650161
Conc: 41.80 ng/ml

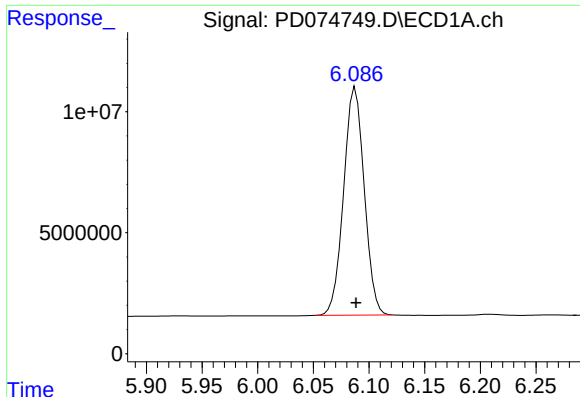

#9 Endosulfan I


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 121243394
Conc: 42.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

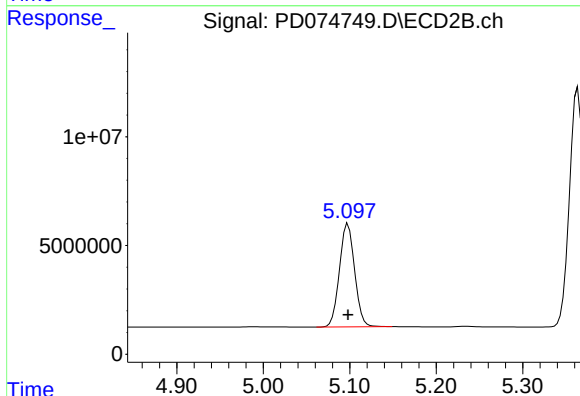


#9 Endosulfan I

R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 57506697
Conc: 41.11 ng/ml

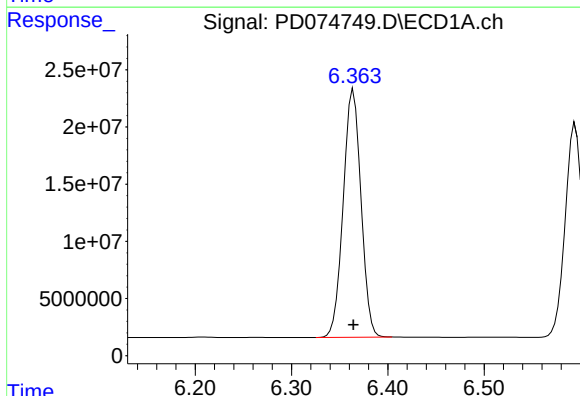


#13 Dieldrin

R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 277254790
Conc: 87.63 ng/ml

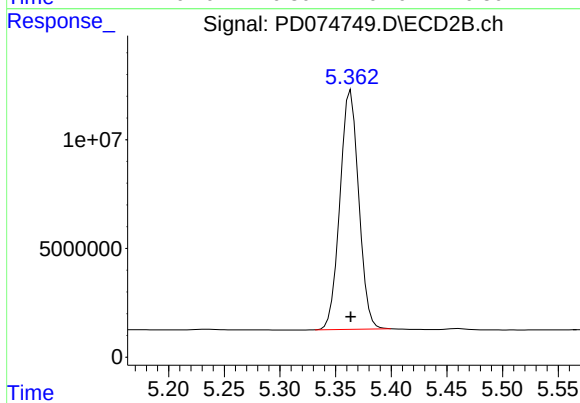

#13 Dieldrin


R.T.: 5.364 min
Delta R.T.: 0.000 min
Response: 129218064
Conc: 84.19 ng/ml

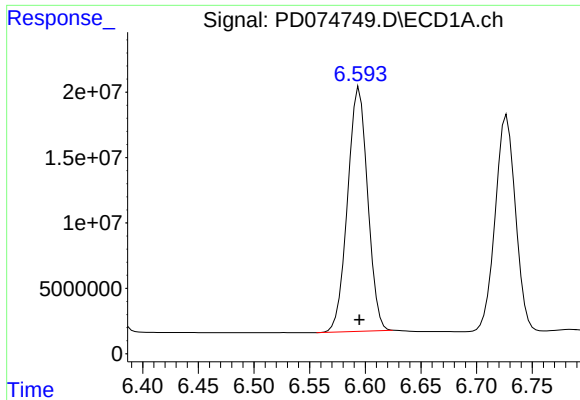

#14 Endrin


R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 234511201
Conc: 87.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

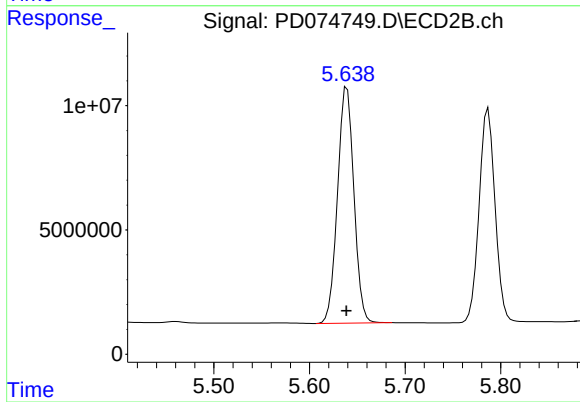


#14 Endrin

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 113308327
Conc: 83.66 ng/ml

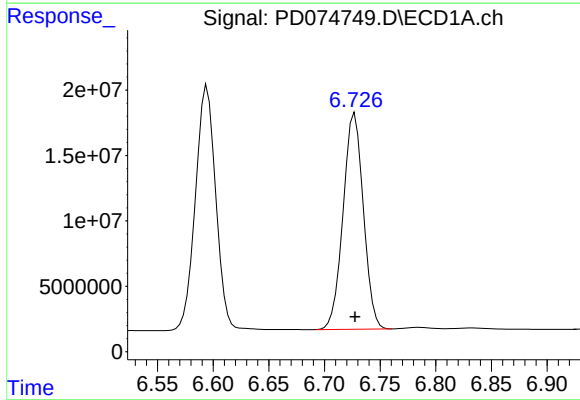


#16 4,4'-DDD

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 209522289
Conc: 87.16 ng/ml

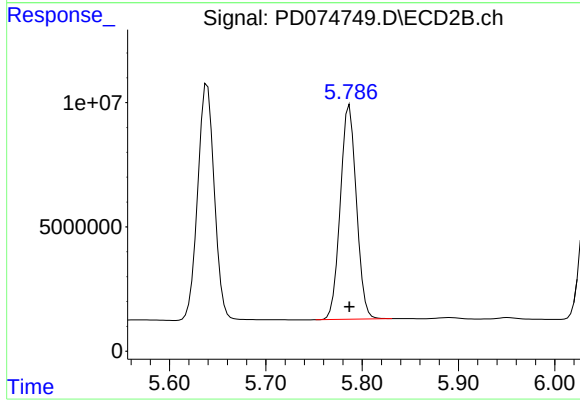

#16 4,4'-DDD


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 99933804
Conc: 83.84 ng/ml

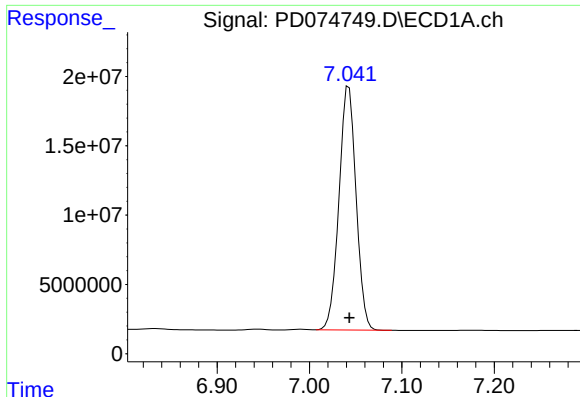

#17 4,4'-DDT


R.T.: 7.043 min
Delta R.T.: 0.000 min
Response: 226455005
Conc: 87.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

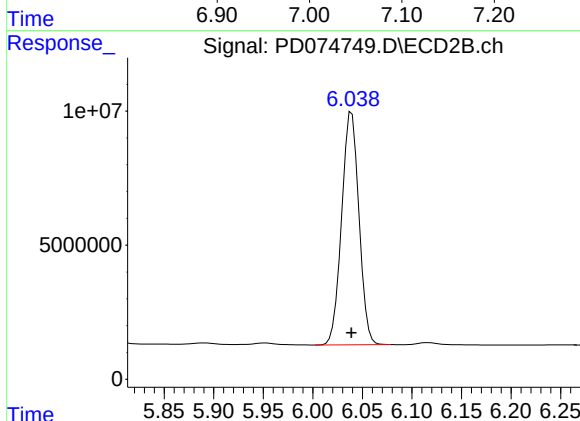


#17 4,4'-DDT

R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 105487067
Conc: 84.58 ng/ml

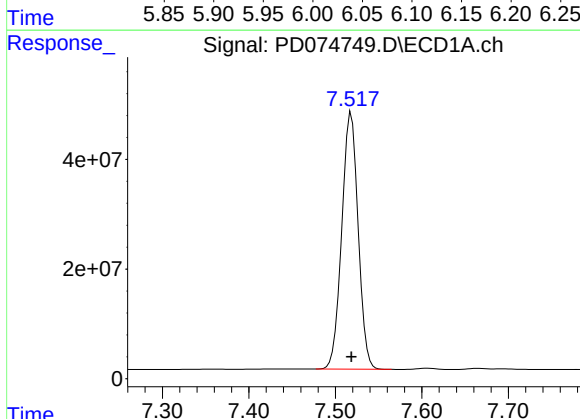


#20 Methoxychlor

R.T.: 7.518 min
Delta R.T.: 0.000 min
Response: 612594677
Conc: 417.64 ng/ml

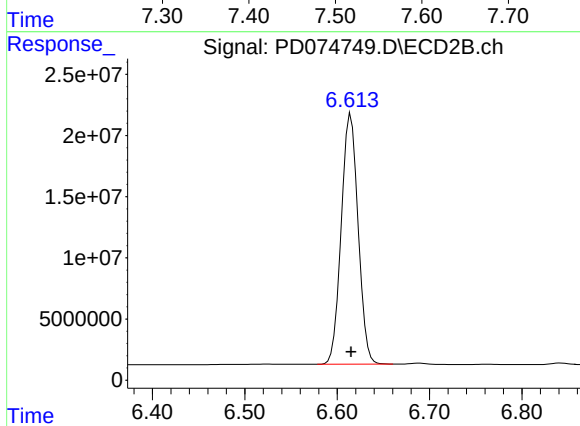

#20 Methoxychlor


R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 259577563
Conc: 394.39 ng/ml

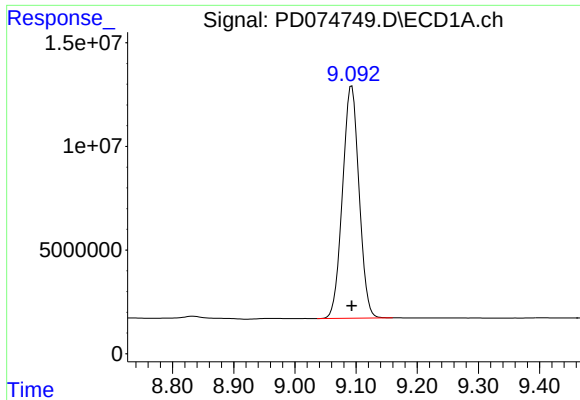

#27 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 210553467
Conc: 78.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

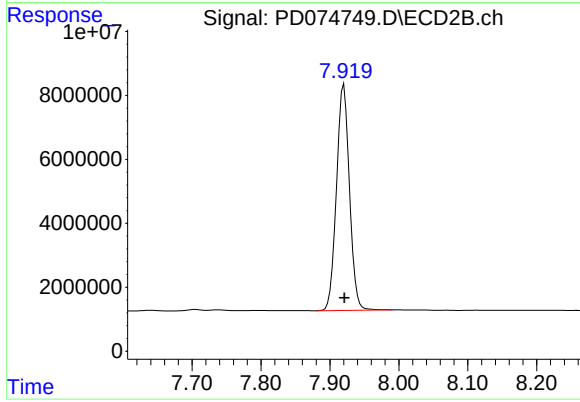

#27 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: 0.000 min
Response: 92459445
Conc: 77.81 ng/ml