

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 12:59
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 01:10:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 17 01:05:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	91538093	50422341	39.663	39.094
27)	SA Decachlor...	9.093	7.921	208.1E6	91441128	76.109	75.318
Target Compounds							
5)	MB Aldrin	5.275	4.226	141.0E6	67225168	41.978	40.184
6)	B beta-BHC	4.534	3.900	61711518	30719776	39.434	38.237
7)	B delta-BHC	4.782	4.130	126.1E6	71279444	43.858	40.849
8)	B Heptachlo...	5.701	4.728	119.8E6	61796202	41.270	39.610
10)	B trans-Chl...	5.958	4.979	123.5E6	60196446	41.128	39.765
11)	B cis-Chlor...	6.038	5.043	126.9E6	61043448	40.659	39.508
12)	B 4,4'-DDE	6.210	5.233	251.1E6	118.2E6	84.837	81.623
15)	B Endosulfa...	6.814	5.933	228.3E6	104.9E6	80.882	79.900
18)	B Endrin al...	6.944	6.112	182.4E6	84748315	80.251	78.240
19)	B Endosulfa...	7.178	6.336	215.1E6	99249959	80.903	78.660
21)	B Endrin ke...	7.665	6.842	249.1E6	118.9E6	80.514	78.797

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 12:59
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 01:10:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 17 01:05:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

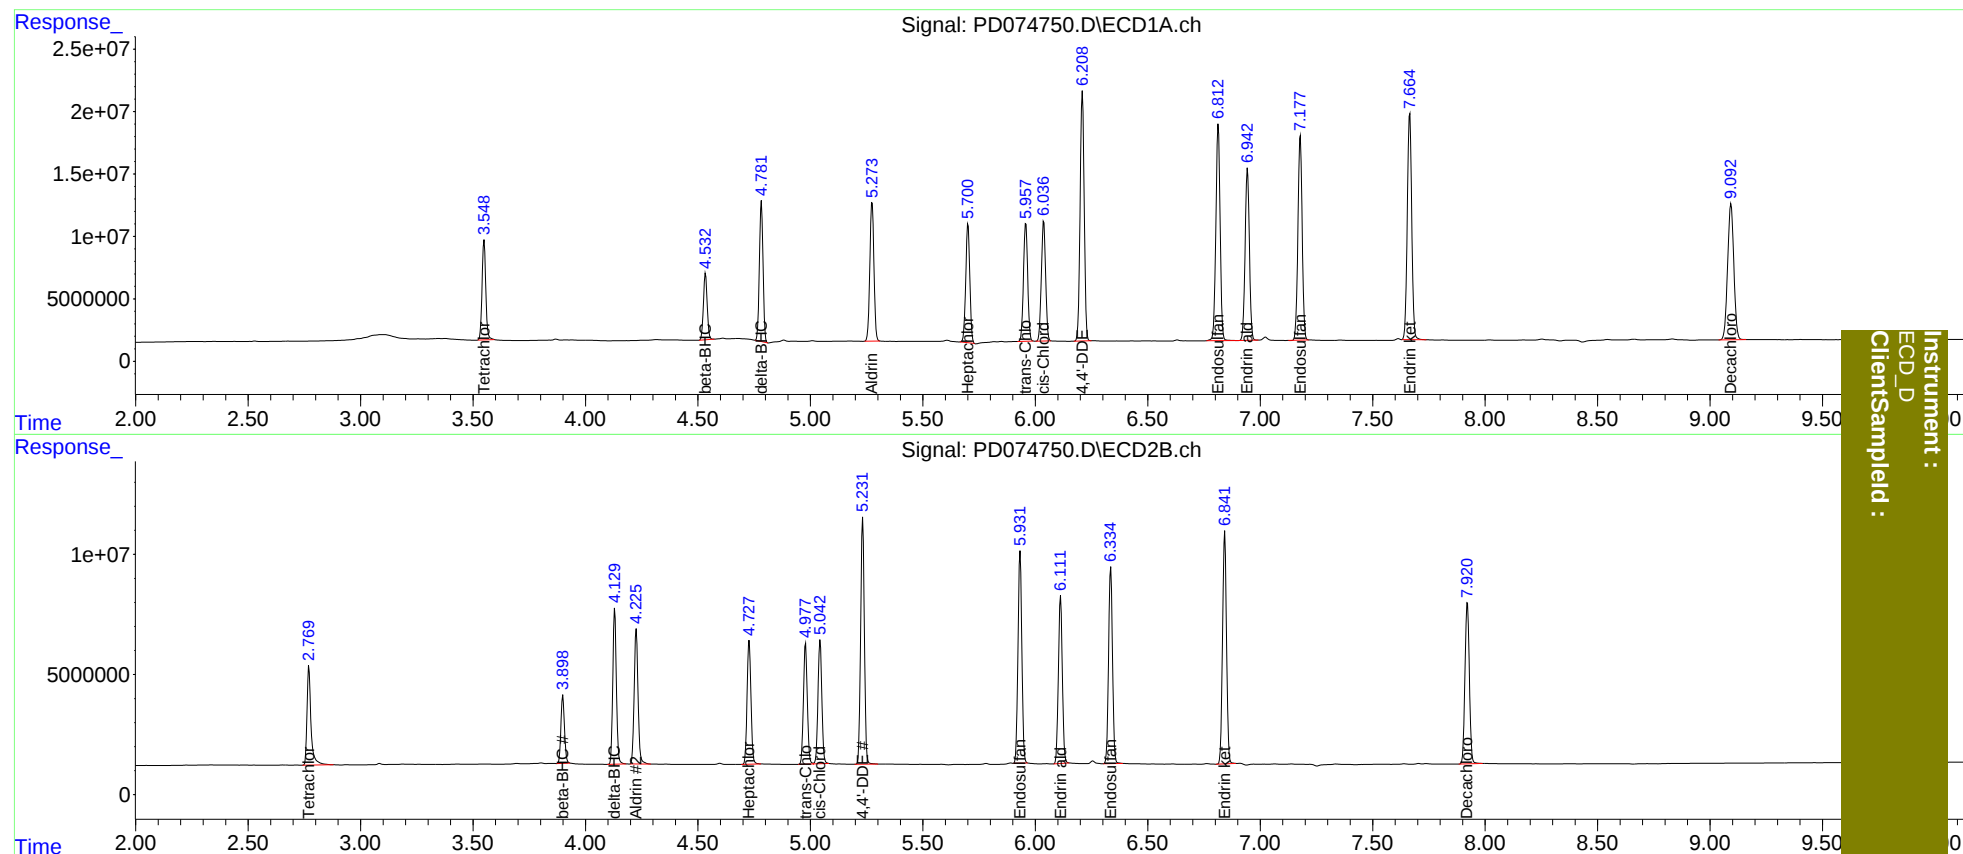


Instrument :
ECD_D
ClientSampled :

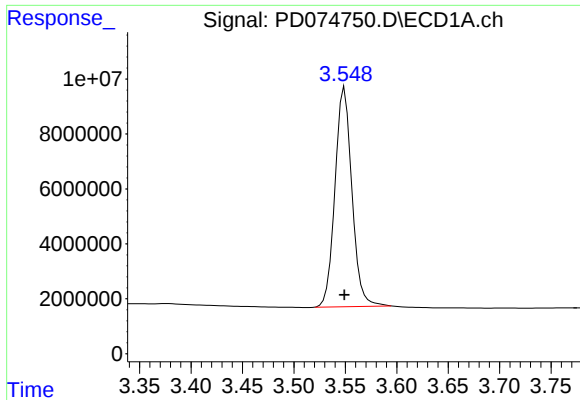

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 91538093
Conc: 39.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

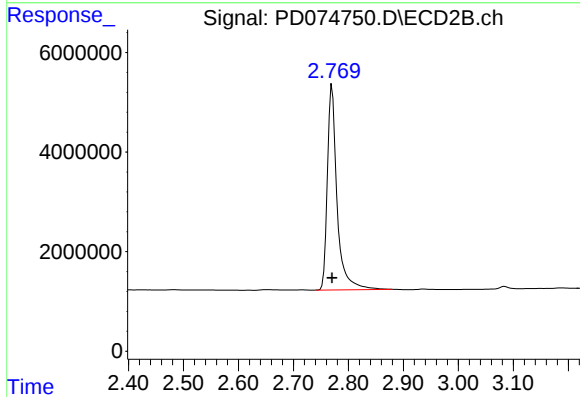


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 50422341
Conc: 39.09 ng/ml

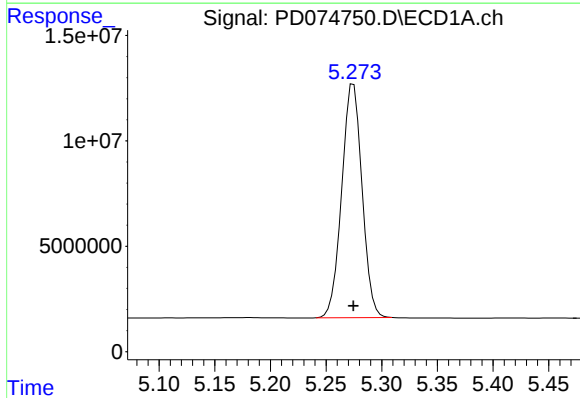


#5 Aldrin

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 141008213
Conc: 41.98 ng/ml

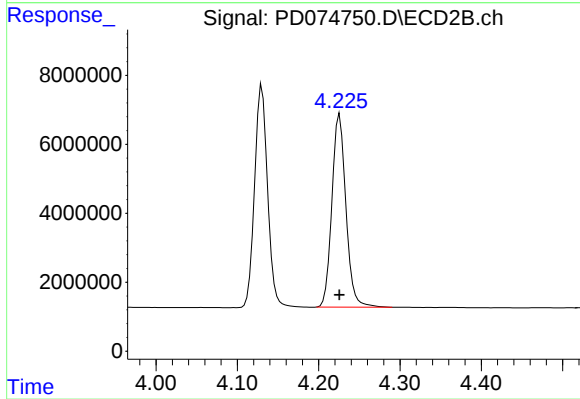

#5 Aldrin


R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 67225168
Conc: 40.18 ng/ml

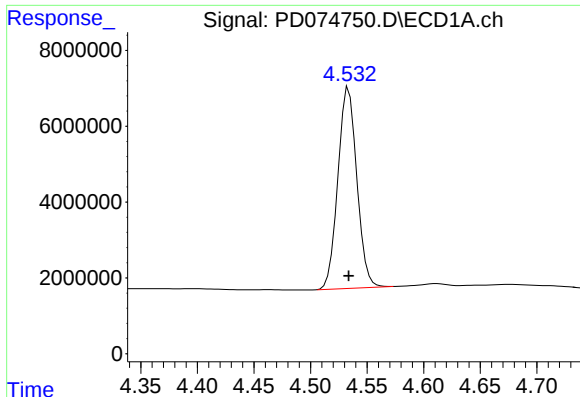

#6 beta-BHC


R.T.: 4.534 min
Delta R.T.: 0.000 min
Response: 61711518
Conc: 39.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

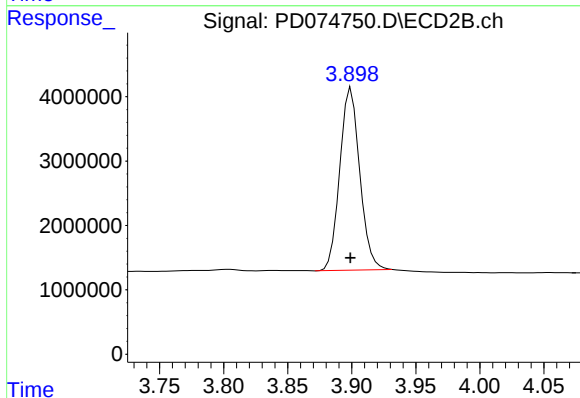


#6 beta-BHC

R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 30719776
Conc: 38.24 ng/ml

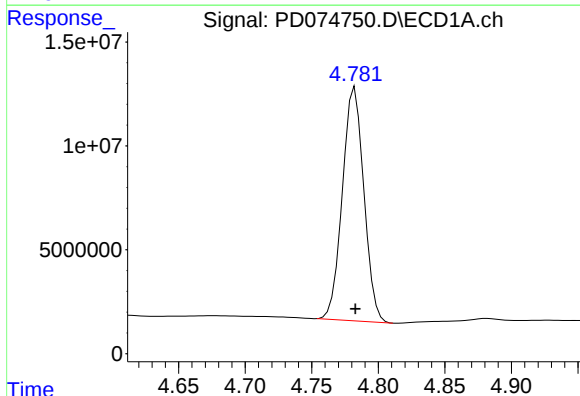


#7 delta-BHC

R.T.: 4.782 min
Delta R.T.: 0.000 min
Response: 126057158
Conc: 43.86 ng/ml

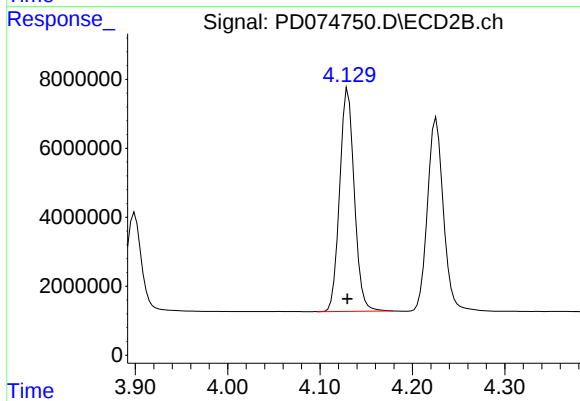

#7 delta-BHC


R.T.: 4.130 min
Delta R.T.: 0.000 min
Response: 71279444
Conc: 40.85 ng/ml

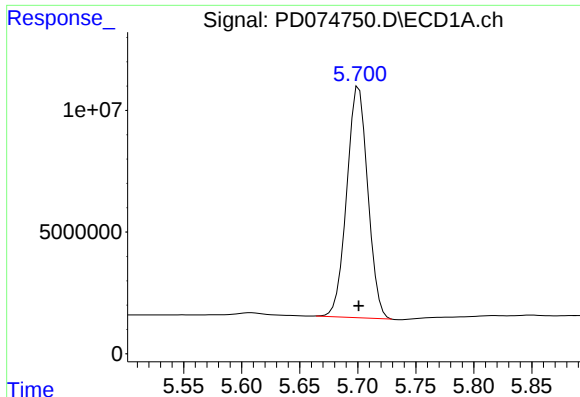

#8 Heptachlor epoxide


R.T.: 5.701 min
Delta R.T.: 0.000 min
Response: 119778861
Conc: 41.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

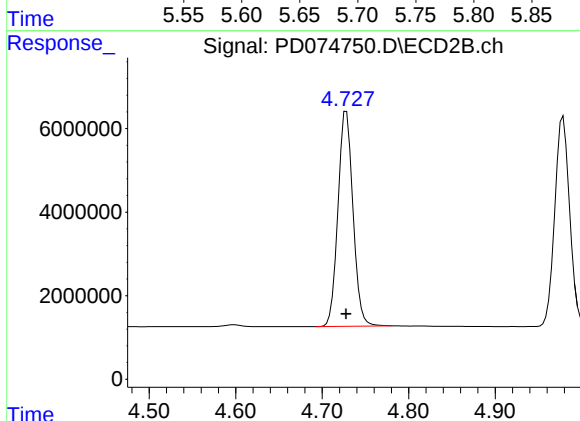


#8 Heptachlor epoxide

R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 61796202
Conc: 39.61 ng/ml

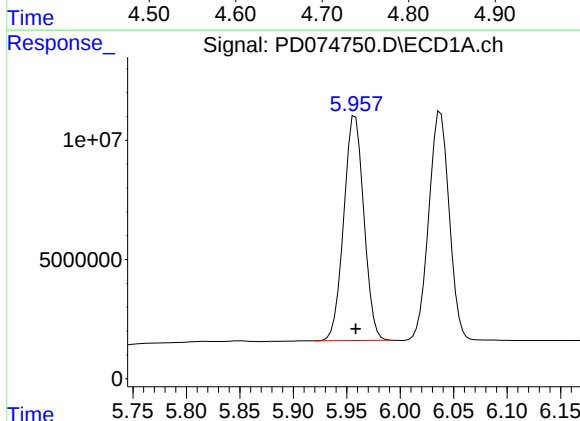


#10 trans-Chlordane

R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 123516706
Conc: 41.13 ng/ml

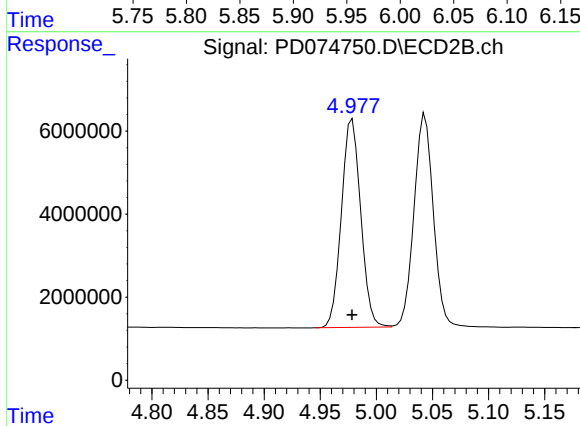

#10 trans-Chlordane


R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 60196446
Conc: 39.77 ng/ml

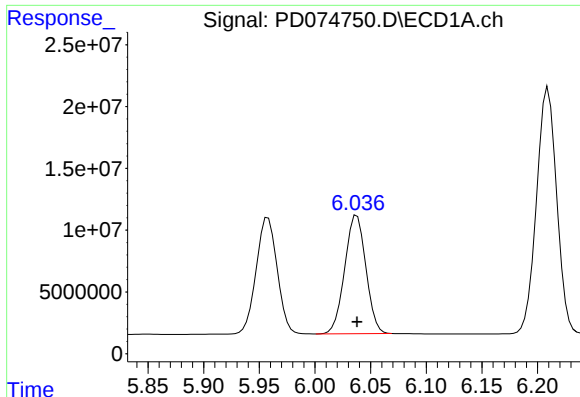

#11 cis-Chlordane


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 126930577
Conc: 40.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

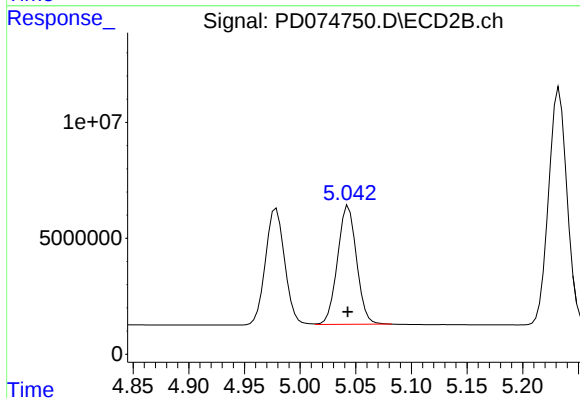


#11 cis-Chlordane

R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 61043448
Conc: 39.51 ng/ml

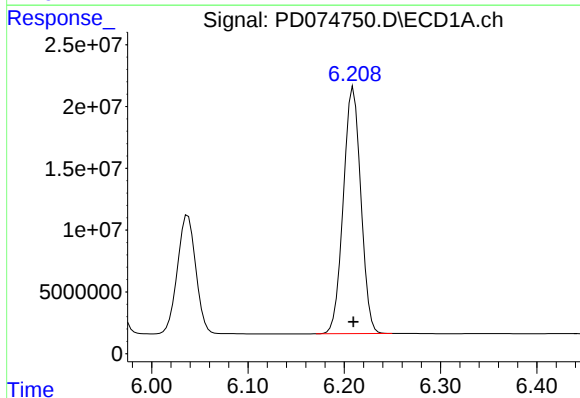


#12 4,4'-DDE

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 251055862
Conc: 84.84 ng/ml

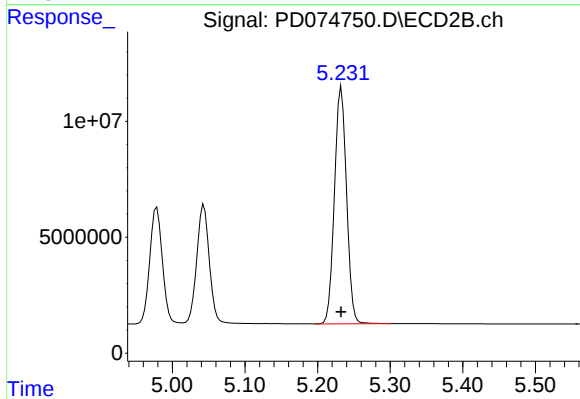

#12 4,4'-DDE


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 118216324
Conc: 81.62 ng/ml

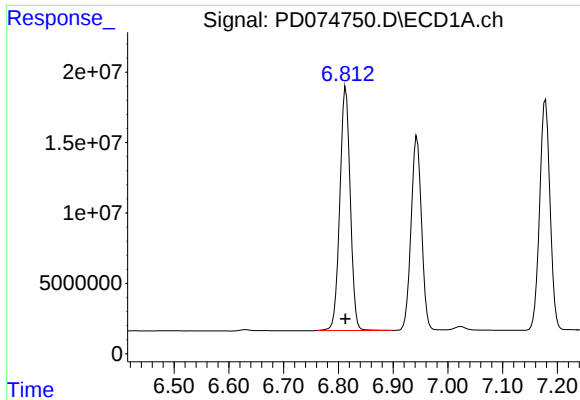

#15 Endosulfan II


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 228328164
Conc: 80.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

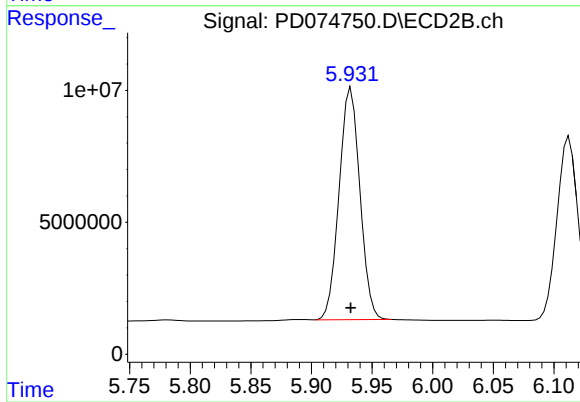


#15 Endosulfan II

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 104876727
Conc: 79.90 ng/ml

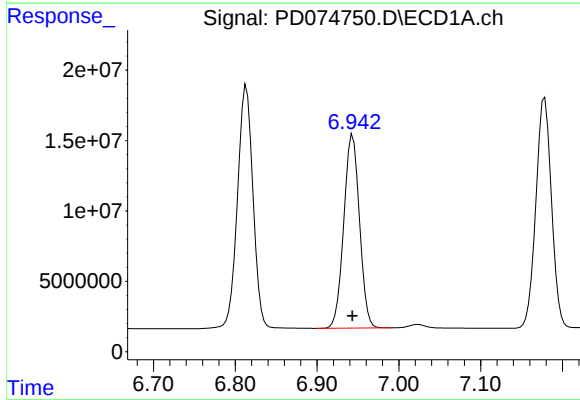


#18 Endrin aldehyde

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 182441463
Conc: 80.25 ng/ml

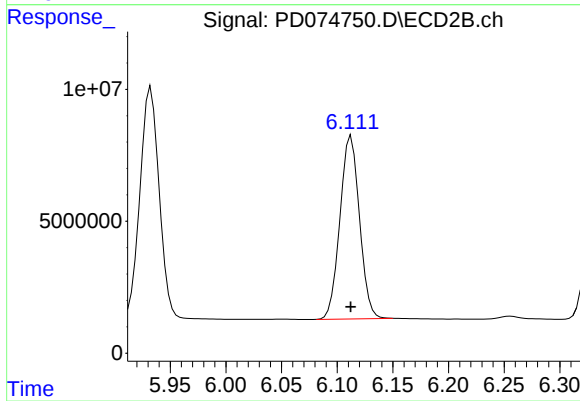

#18 Endrin aldehyde


R.T.: 6.112 min
Delta R.T.: 0.000 min
Response: 84748315
Conc: 78.24 ng/ml

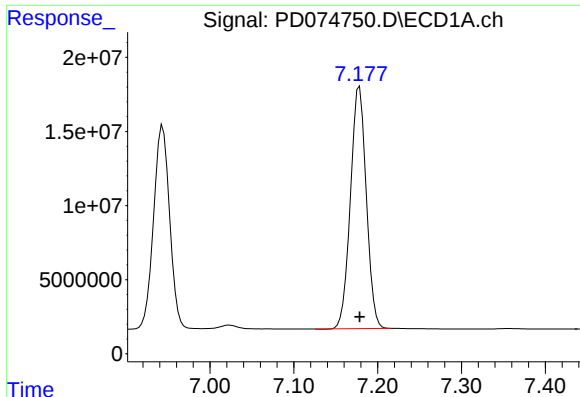

#19 Endosulfan Sulfate


R.T.: 7.178 min
Delta R.T.: 0.000 min
Response: 215052955
Conc: 80.90 ng/ml

Instrument :
ECD_D
ClientSampleId :

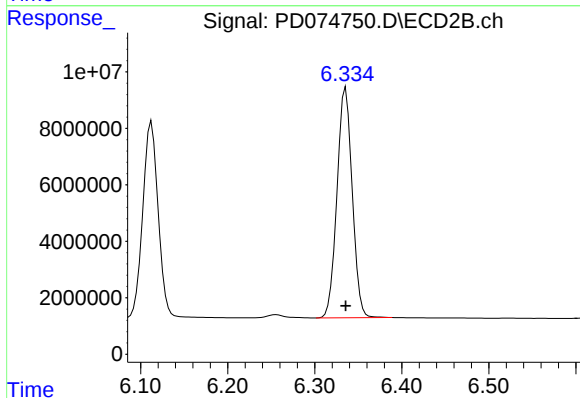


#19 Endosulfan Sulfate

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 99249959
Conc: 78.66 ng/ml

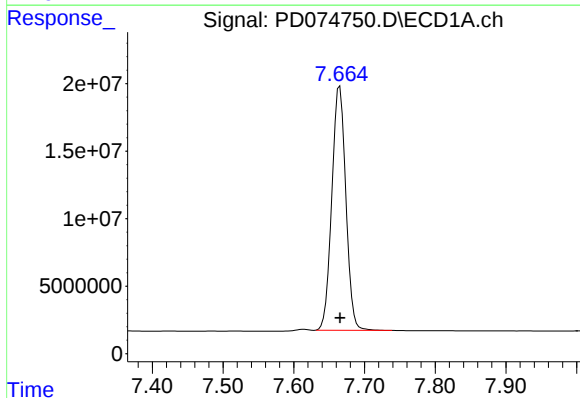


#21 Endrin ketone

R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 249107223
Conc: 80.51 ng/ml

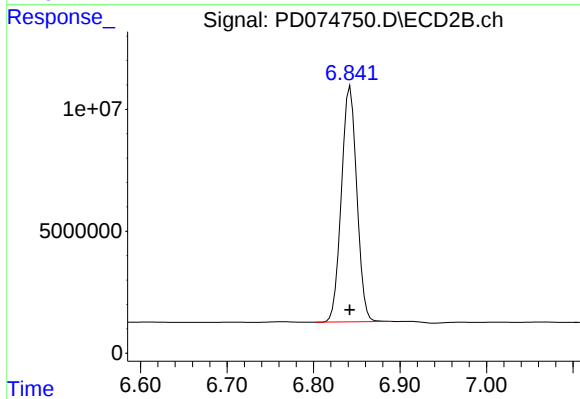

#21 Endrin ketone


R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 118890849
Conc: 78.80 ng/ml

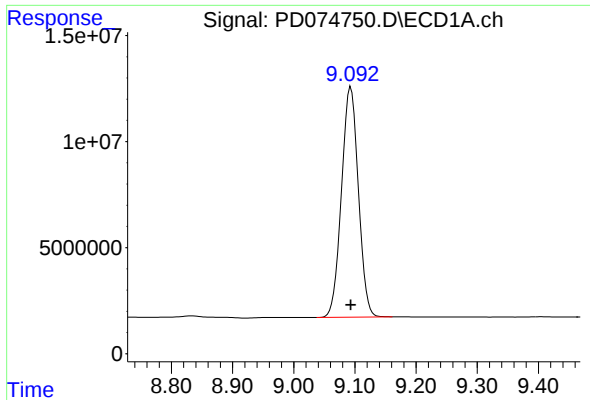

#27 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: 0.000 min
Response: 208064019
Conc: 76.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

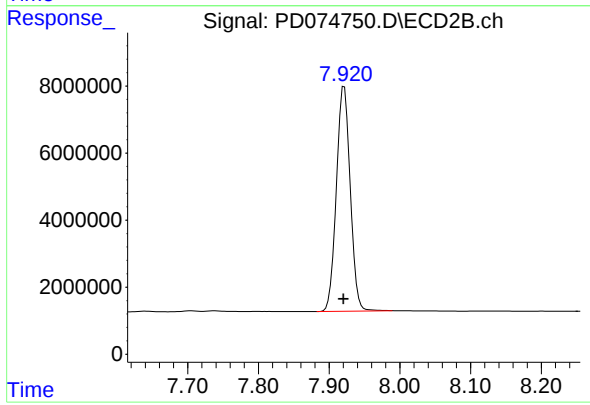

#27 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.001 min
Response: 91441128
Conc: 75.32 ng/ml