

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 13:13
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 06:38:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 15 06:34:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.770	186.3E6	100.8E6	81.157	78.093
27)	SA Decachlor...	9.093	7.921	399.5E6	174.7E6	149.446	146.983
Target Compounds							
2)	A alpha-BHC	4.006	3.274	336.2E6	154.6E6	91.452	86.215
3)	MA gamma-BHC...	4.339	3.604	311.3E6	142.5E6	89.238	84.189
4)	MA Heptachlor	4.932	3.945	308.7E6	138.9E6	89.649	83.332
9)	A Endosulfan I	6.089	5.099	243.9E6	113.7E6	85.149	81.298
13)	MA Dieldrin	6.364	5.364	568.0E6	256.9E6	179.535	167.376
14)	MA Endrin	6.595	5.639	478.2E6	223.9E6	178.590	165.294
16)	A 4,4'-DDD	6.727	5.788	429.5E6	198.8E6	178.668	166.806
17)	MA 4,4'-DDT	7.043	6.040	465.5E6	211.0E6	179.655	169.195
20)	A Methoxychlor	7.518	6.615	1202.7E6	478.4E6	819.974	726.892


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 13:13
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 06:38:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 15 06:34:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

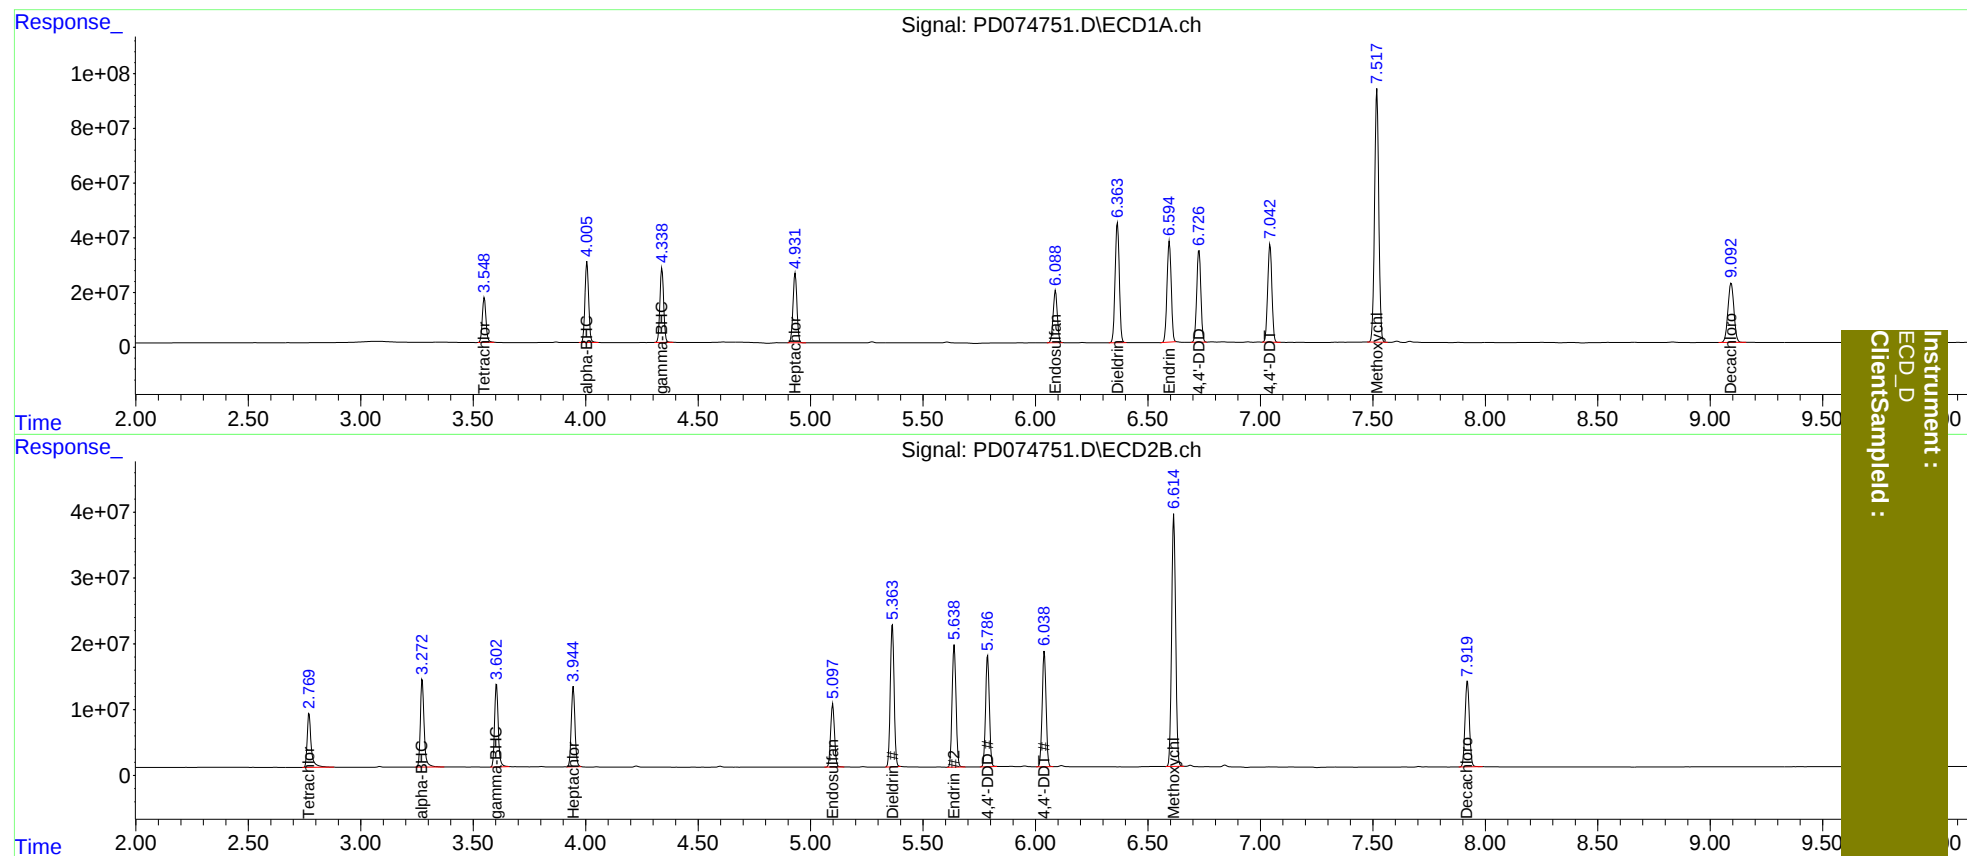


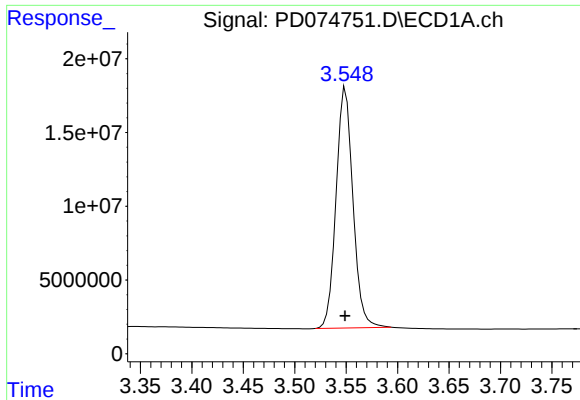

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 186286267
Conc: 81.16 ng/ml

Instrument :
ECD_D
ClientSampleId :

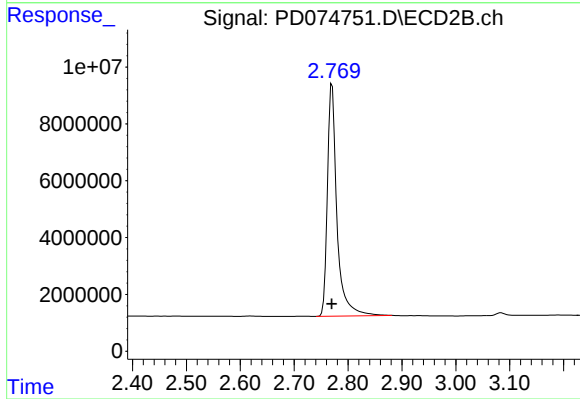


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 100775637
Conc: 78.09 ng/ml

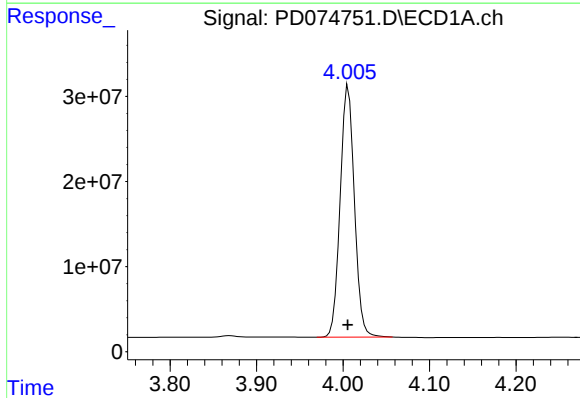


#2 alpha-BHC

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 336208476
Conc: 91.45 ng/ml

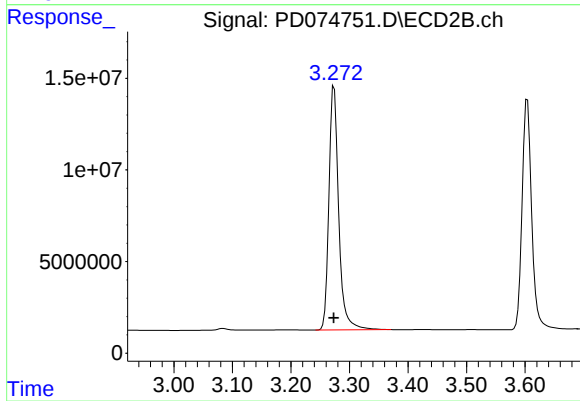

#2 alpha-BHC


R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 154641279
Conc: 86.22 ng/ml

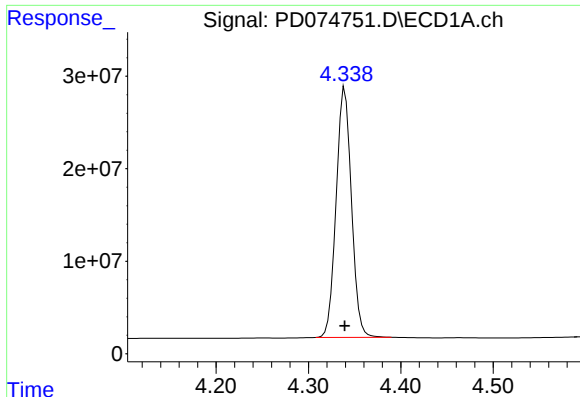

#3 gamma-BHC (Lindane)


R.T.: 4.339 min
Delta R.T.: 0.000 min
Response: 311343417
Conc: 89.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

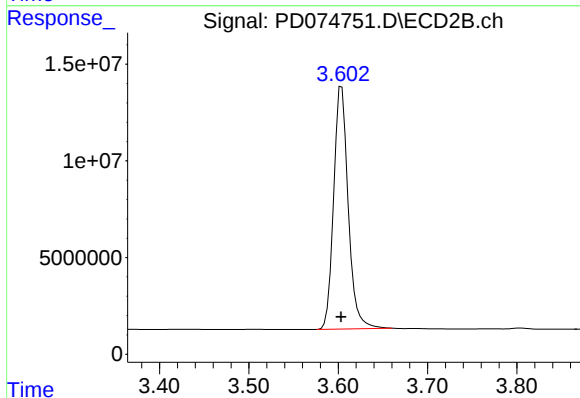


#3 gamma-BHC (Lindane)

R.T.: 3.604 min
Delta R.T.: 0.000 min
Response: 142455060
Conc: 84.19 ng/ml

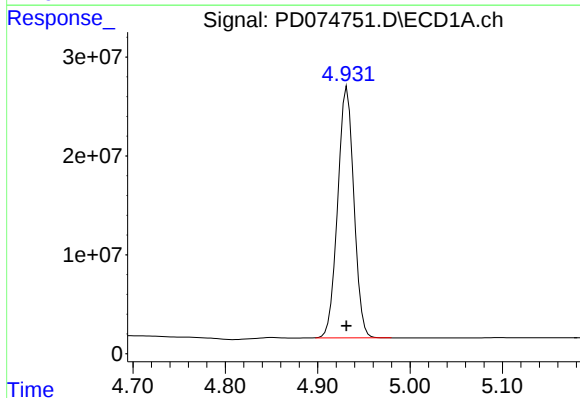


#4 Heptachlor

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 308655344
Conc: 89.65 ng/ml

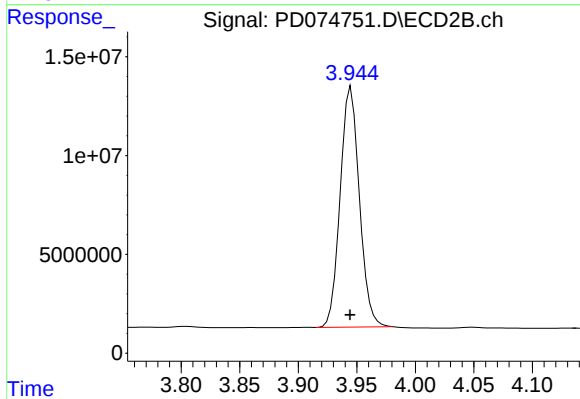

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 138865031
Conc: 83.33 ng/ml

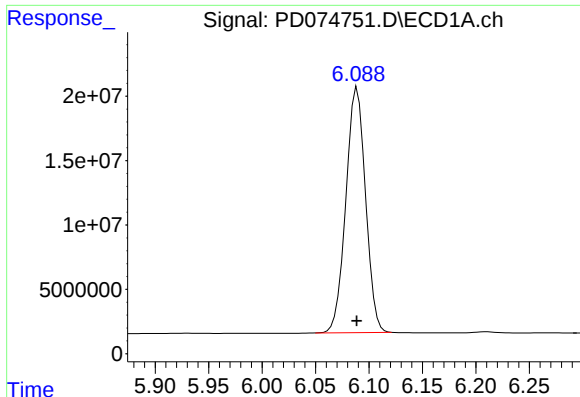

#9 Endosulfan I


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 243899995
Conc: 85.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

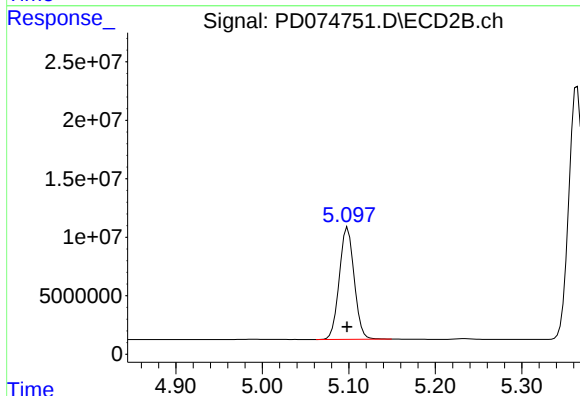


#9 Endosulfan I

R.T.: 5.099 min
Delta R.T.: 0.000 min
Response: 113727339
Conc: 81.30 ng/ml

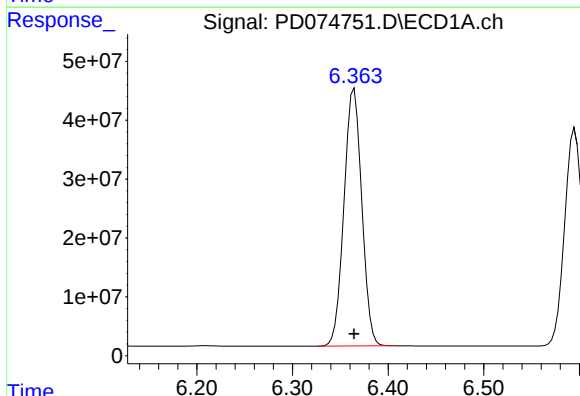


#13 Dieldrin

R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 568029617
Conc: 179.53 ng/ml

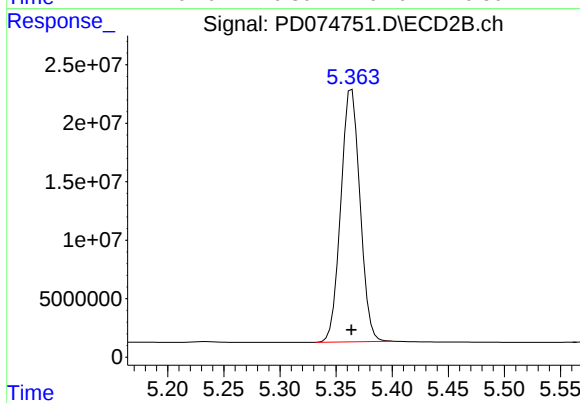

#13 Dieldrin


R.T.: 5.364 min
Delta R.T.: 0.000 min
Response: 256907971
Conc: 167.38 ng/ml

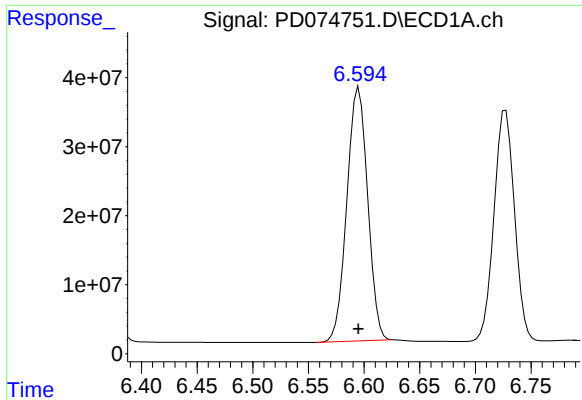

#14 Endrin


R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 478192860
Conc: 178.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

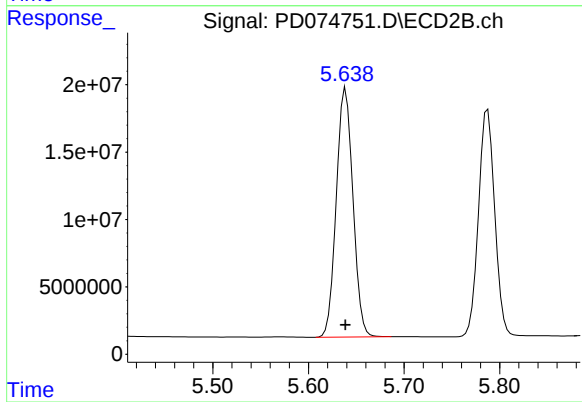


#14 Endrin

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 223862234
Conc: 165.29 ng/ml

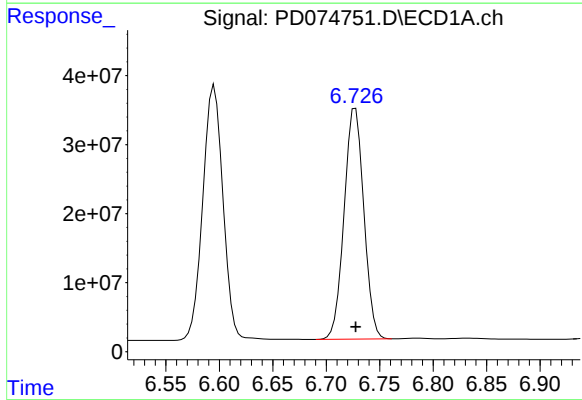


#16 4,4'-DDD

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 429499921
Conc: 178.67 ng/ml

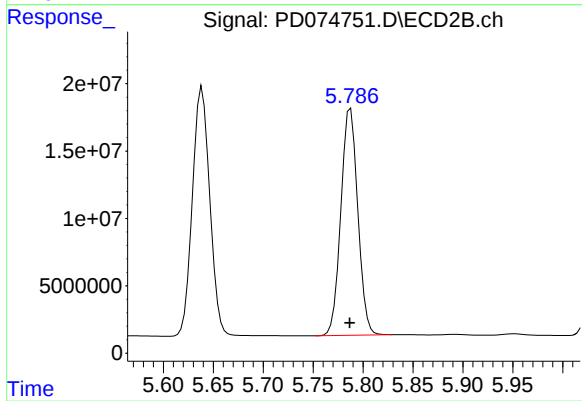

#16 4,4'-DDD


R.T.: 5.788 min
Delta R.T.: 0.000 min
Response: 198836602
Conc: 166.81 ng/ml

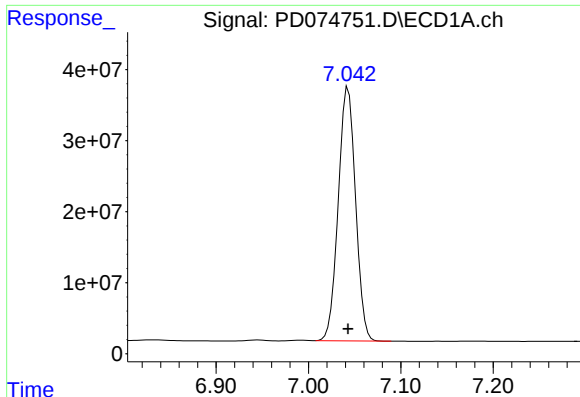

#17 4,4'-DDT


R.T.: 7.043 min
Delta R.T.: 0.000 min
Response: 465500898
Conc: 179.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

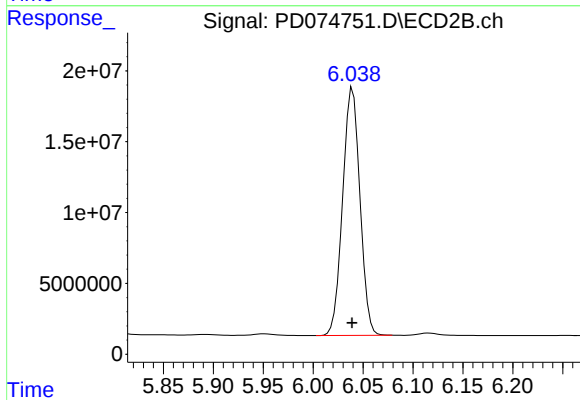


#17 4,4'-DDT

R.T.: 6.040 min
Delta R.T.: 0.000 min
Response: 211016649
Conc: 169.19 ng/ml

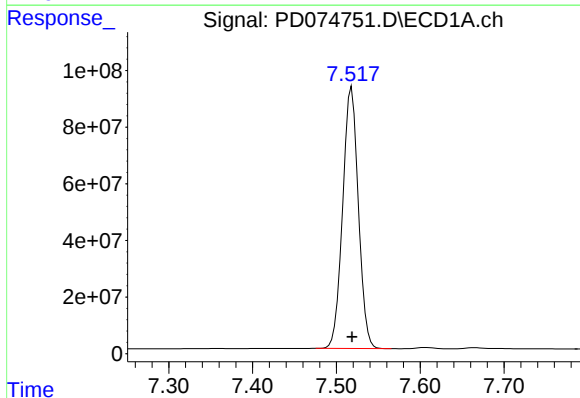


#20 Methoxychlor

R.T.: 7.518 min
Delta R.T.: 0.000 min
Response: 1202729243
Conc: 819.97 ng/ml

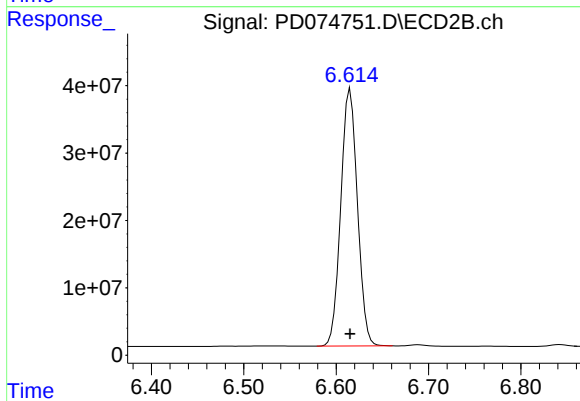

#20 Methoxychlor

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 478425737
Conc: 726.89 ng/ml

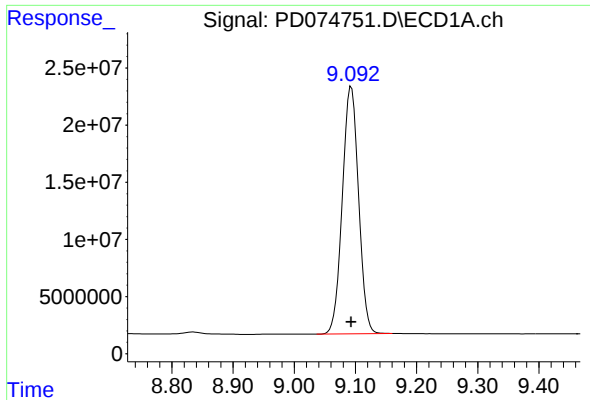

#27 Decachlorobiphenyl


R.T.: 9.093 min

Delta R.T.: 0.000 min

Response: 399467538

Conc: 149.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

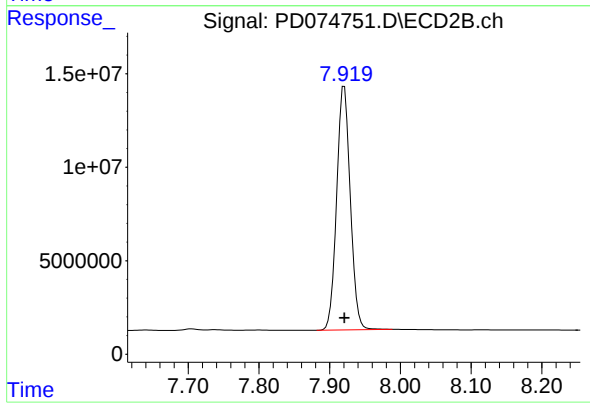

#27 Decachlorobiphenyl

R.T.: 7.921 min

Delta R.T.: 0.000 min

Response: 174652545

Conc: 146.98 ng/ml