

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074752.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 13:26
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 01:10:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 17 01:05:36 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	181.6E6	98572945	78.696	76.426
27)	SA Decachlor...	9.093	7.921	397.1E6	173.7E6	145.271	143.073
Target Compounds							
5)	MB Aldrin	5.275	4.226	292.7E6	135.7E6	87.125	81.101
6)	B beta-BHC	4.534	3.899	121.6E6	59023134	77.672	73.466
7)	B delta-BHC	4.783	4.130	269.5E6	145.5E6	93.762	83.381
8)	B Heptachlo...	5.702	4.728	245.9E6	122.6E6	84.724	78.591
10)	B trans-Chl...	5.958	4.979	254.4E6	120.8E6	84.713	79.810
11)	B cis-Chlor...	6.038	5.043	258.7E6	121.2E6	82.876	78.464
12)	B 4,4'-DDE	6.210	5.233	523.2E6	239.1E6	176.794	165.108
15)	B Endosulfa...	6.814	5.933	460.8E6	207.5E6	163.231	158.091
18)	B Endrin al...	6.944	6.113	363.1E6	164.4E6	159.711	151.754
19)	B Endosulfa...	7.179	6.336	432.1E6	194.9E6	162.555	154.474
21)	B Endrin ke...	7.666	6.842	496.9E6	231.9E6	160.588	153.726


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074752.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 13:26
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 01:10:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 17 01:05:36 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

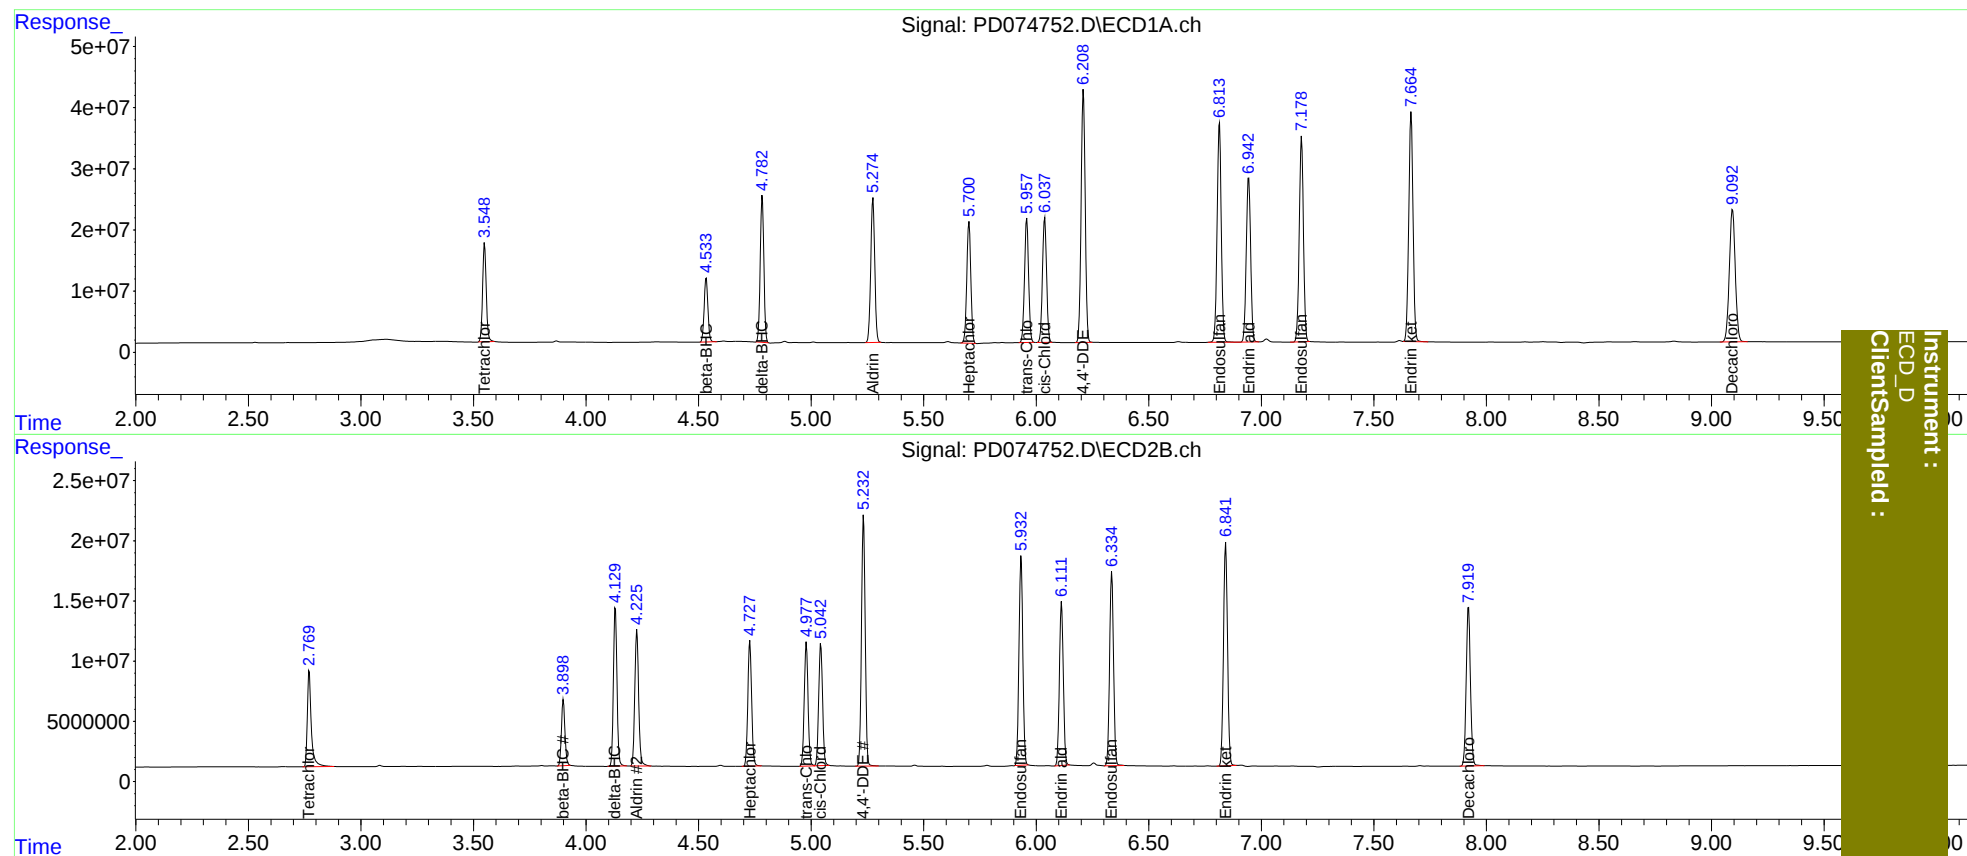


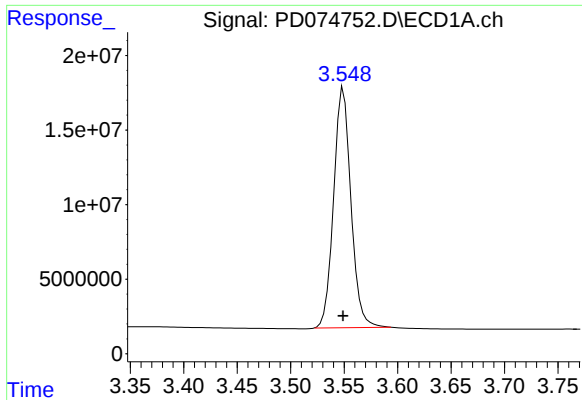

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 181623988
Conc: 78.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

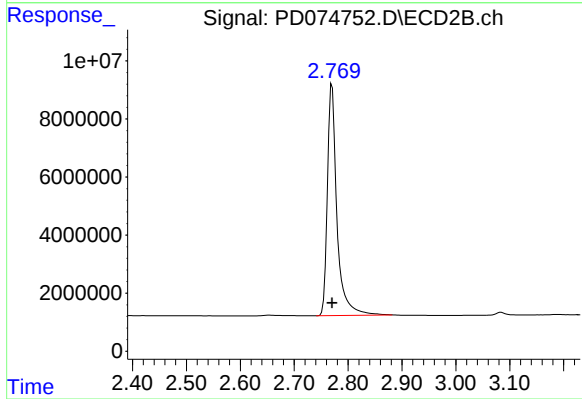


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 98572945
Conc: 76.43 ng/ml

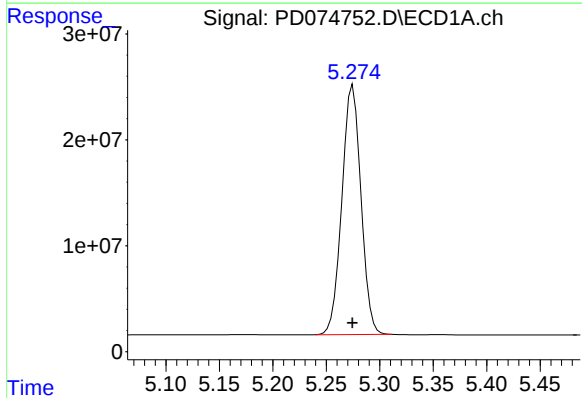


#5 Aldrin

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 292662609
Conc: 87.13 ng/ml

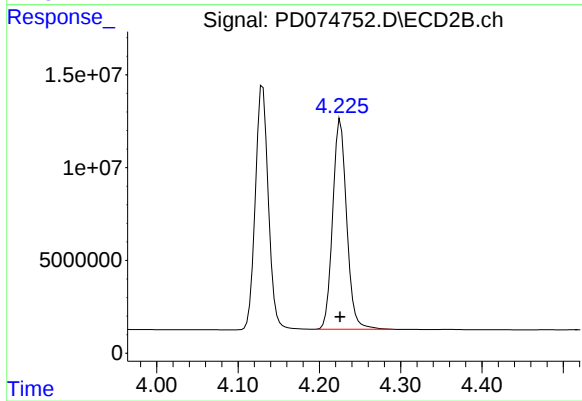

#5 Aldrin


R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 135676566
Conc: 81.10 ng/ml

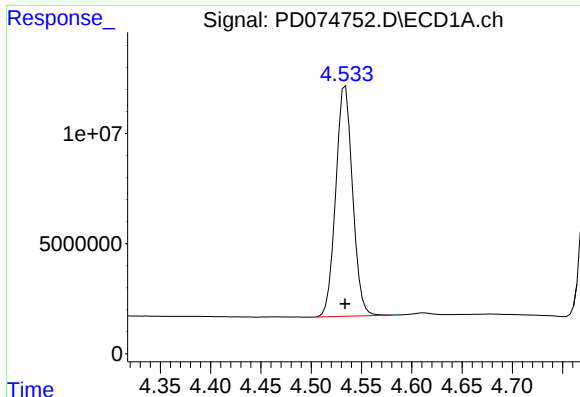

#6 beta-BHC


R.T.: 4.534 min
Delta R.T.: 0.000 min
Response: 121551035
Conc: 77.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

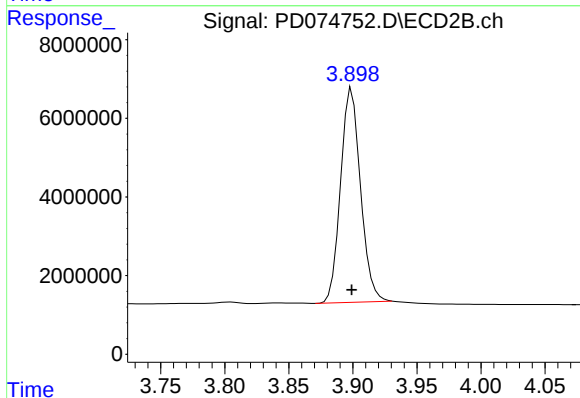


#6 beta-BHC

R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 59023134
Conc: 73.47 ng/ml

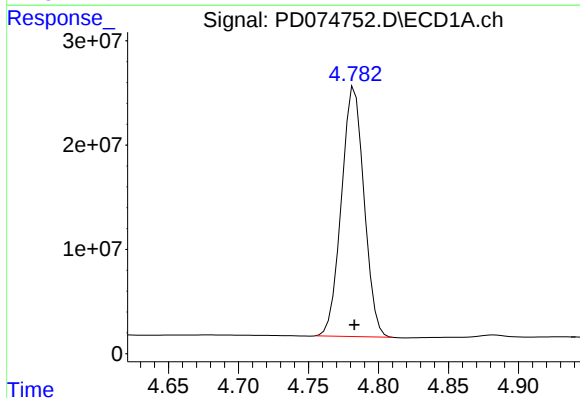


#7 delta-BHC

R.T.: 4.783 min
Delta R.T.: 0.000 min
Response: 269493125
Conc: 93.76 ng/ml

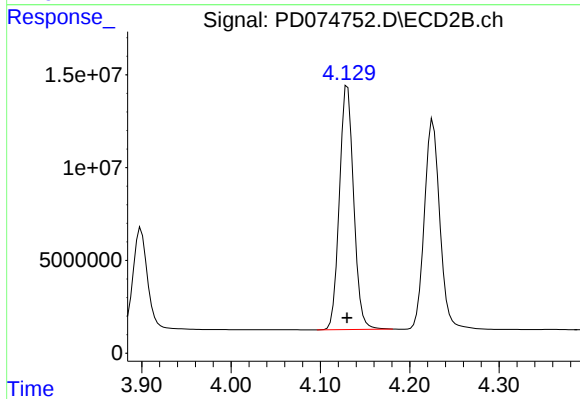

#7 delta-BHC


R.T.: 4.130 min
Delta R.T.: 0.000 min
Response: 145495205
Conc: 83.38 ng/ml

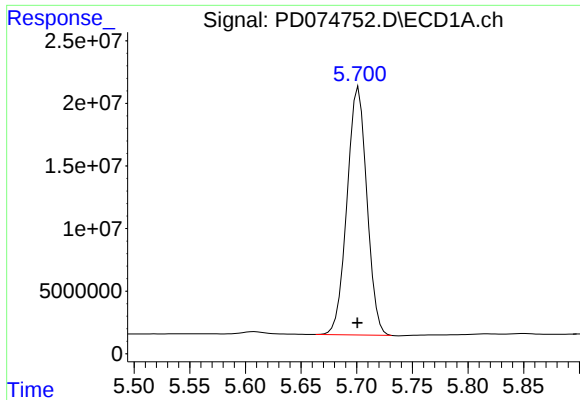

#8 Heptachlor epoxide


R.T.: 5.702 min
Delta R.T.: 0.000 min
Response: 245897382
Conc: 84.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

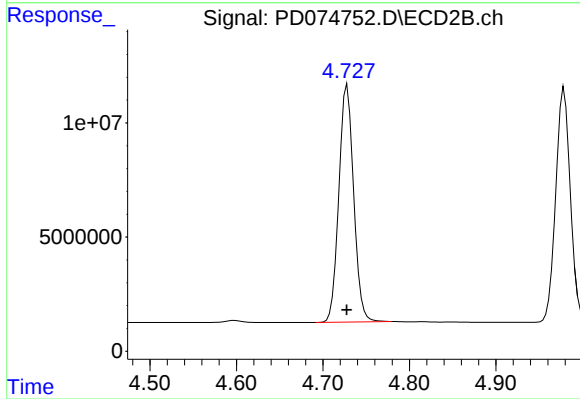


#8 Heptachlor epoxide

R.T.: 4.728 min
Delta R.T.: 0.000 min
Response: 122612612
Conc: 78.59 ng/ml

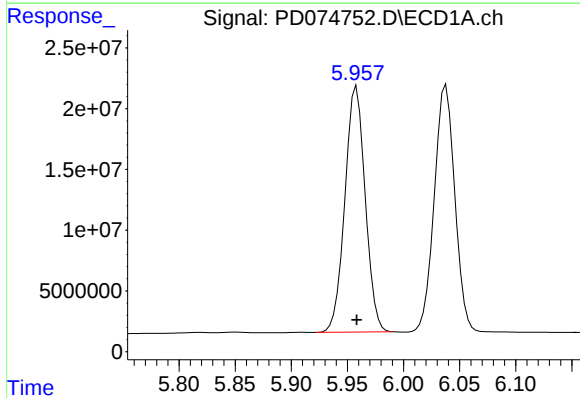


#10 trans-Chlordane

R.T.: 5.958 min
Delta R.T.: 0.000 min
Response: 254412950
Conc: 84.71 ng/ml

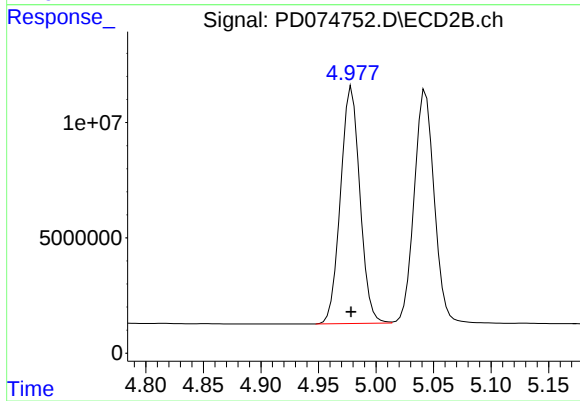

#10 trans-Chlordane


R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 120816210
Conc: 79.81 ng/ml

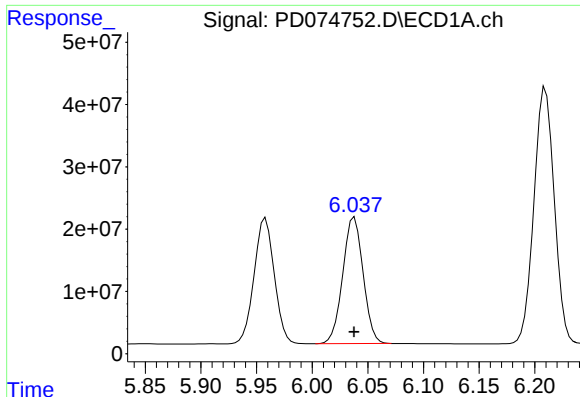

#11 cis-Chlordane


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 258725951
Conc: 82.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

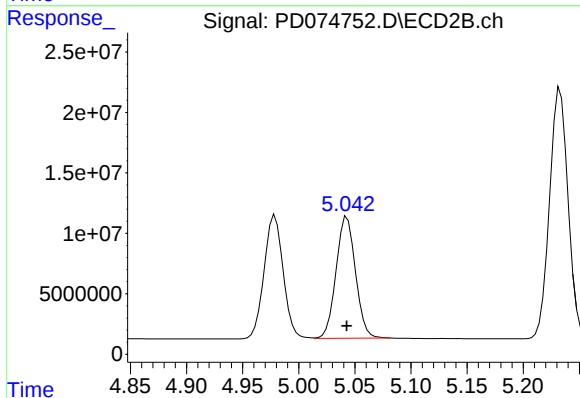


#11 cis-Chlordane

R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 121233044
Conc: 78.46 ng/ml

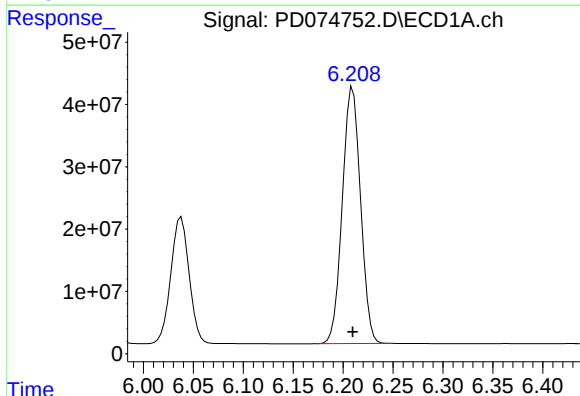


#12 4,4'-DDE

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 523180990
Conc: 176.79 ng/ml

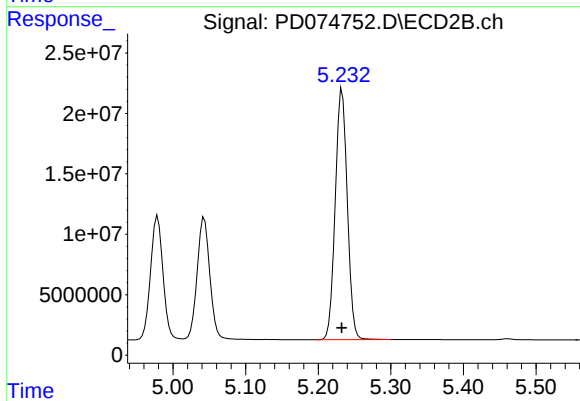

#12 4,4'-DDE


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 239128390
Conc: 165.11 ng/ml

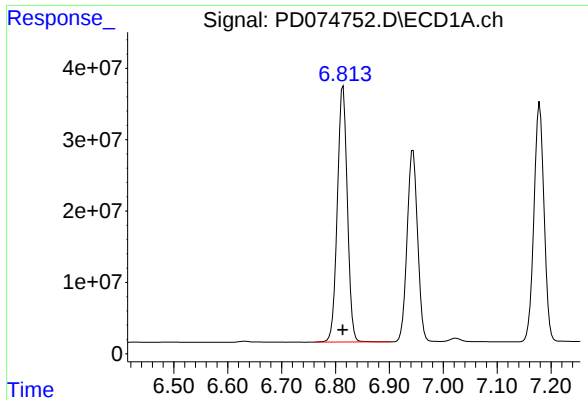

#15 Endosulfan II


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 460798362
Conc: 163.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

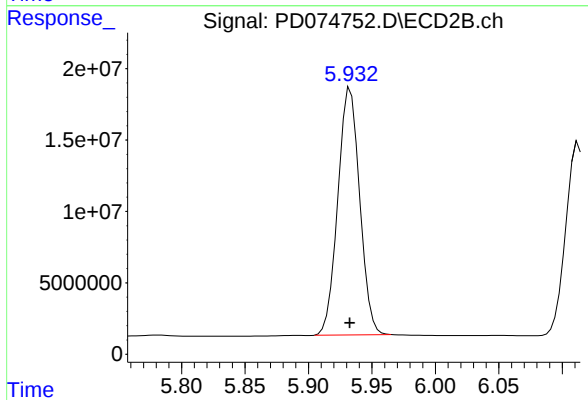


#15 Endosulfan II

R.T.: 5.933 min
Delta R.T.: 0.000 min
Response: 207509548
Conc: 158.09 ng/ml

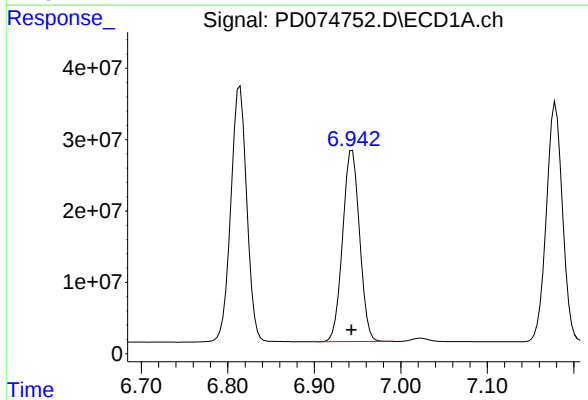


#18 Endrin aldehyde

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 363085160
Conc: 159.71 ng/ml

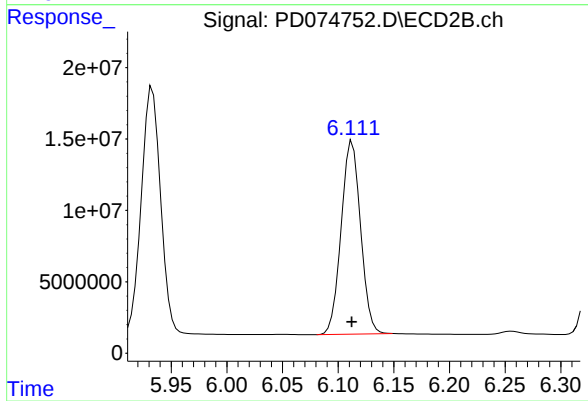

#18 Endrin aldehyde


R.T.: 6.113 min
Delta R.T.: 0.000 min
Response: 164377865
Conc: 151.75 ng/ml

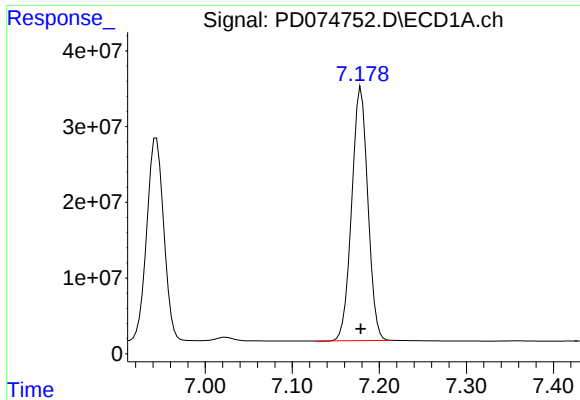

#19 Endosulfan Sulfate


R.T.: 7.179 min
Delta R.T.: 0.000 min
Response: 432094985
Conc: 162.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

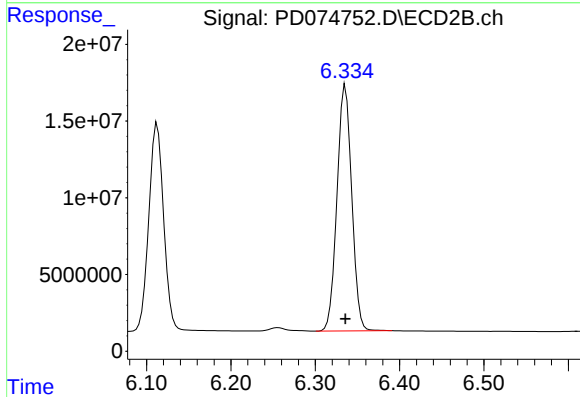


#19 Endosulfan Sulfate

R.T.: 6.336 min
Delta R.T.: 0.000 min
Response: 194909813
Conc: 154.47 ng/ml

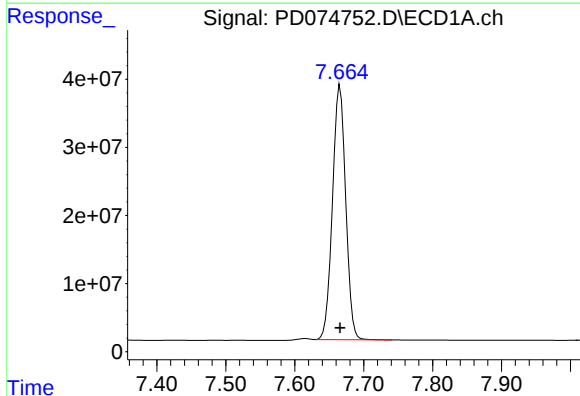


#21 Endrin ketone

R.T.: 7.666 min
Delta R.T.: 0.000 min
Response: 496851795
Conc: 160.59 ng/ml

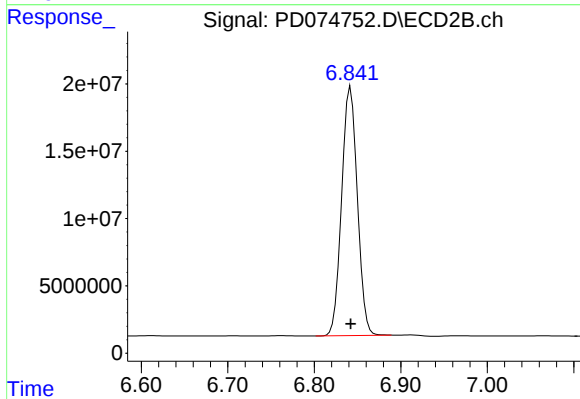

#21 Endrin ketone

R.T.: 6.842 min
Delta R.T.: 0.000 min
Response: 231944637
Conc: 153.73 ng/ml

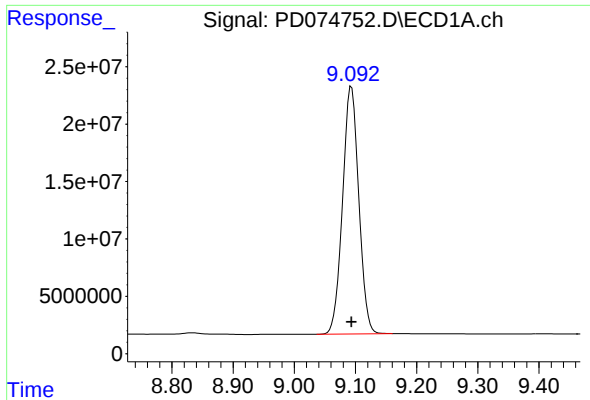

#27 Decachlorobiphenyl


R.T.: 9.093 min

Delta R.T.: 0.000 min

Response: 397135483

Conc: 145.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

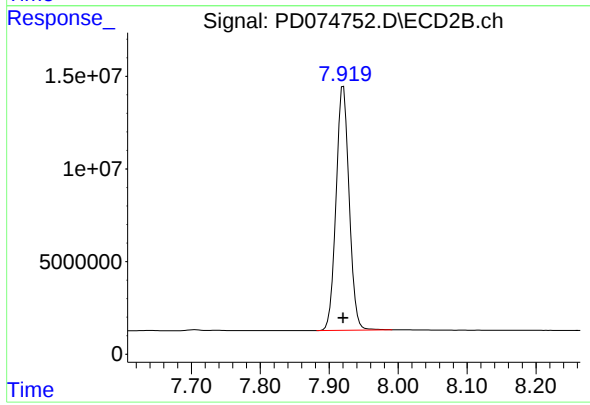

#27 Decachlorobiphenyl

R.T.: 7.921 min

Delta R.T.: 0.000 min

Response: 173700555

Conc: 143.07 ng/ml