

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 13:40
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 06:38:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 15 06:34:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.770	372.9E6	199.3E6	162.458	154.445
27)	SA Decachlor...	9.094	7.921	778.8E6	340.9E6	291.360	286.880
Target Compounds							
2)	A alpha-BHC	4.006	3.274	694.6E6	314.0E6	188.951	175.070
3)	MA gamma-BHC...	4.340	3.603	637.0E6	287.8E6	182.580	170.111
4)	MA Heptachlor	4.932	3.945	630.1E6	277.5E6	183.005	166.548
9)	A Endosulfan I	6.089	5.099	491.5E6	225.8E6	171.582	161.434
13)	MA Dieldrin	6.365	5.364	1144.2E6	504.6E6	361.636	328.762
14)	MA Endrin	6.595	5.640	965.8E6	439.4E6	360.683	324.465
16)	A 4,4'-DDD	6.727	5.787	866.6E6	392.5E6	360.482	329.302
17)	MA 4,4'-DDT	7.043	6.039	944.3E6	420.3E6	364.433	337.003
20)	A Methoxychlor	7.519	6.615	2353.7E6	881.2E6	1604.648	1338.793


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 13:40
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 06:38:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 15 06:34:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

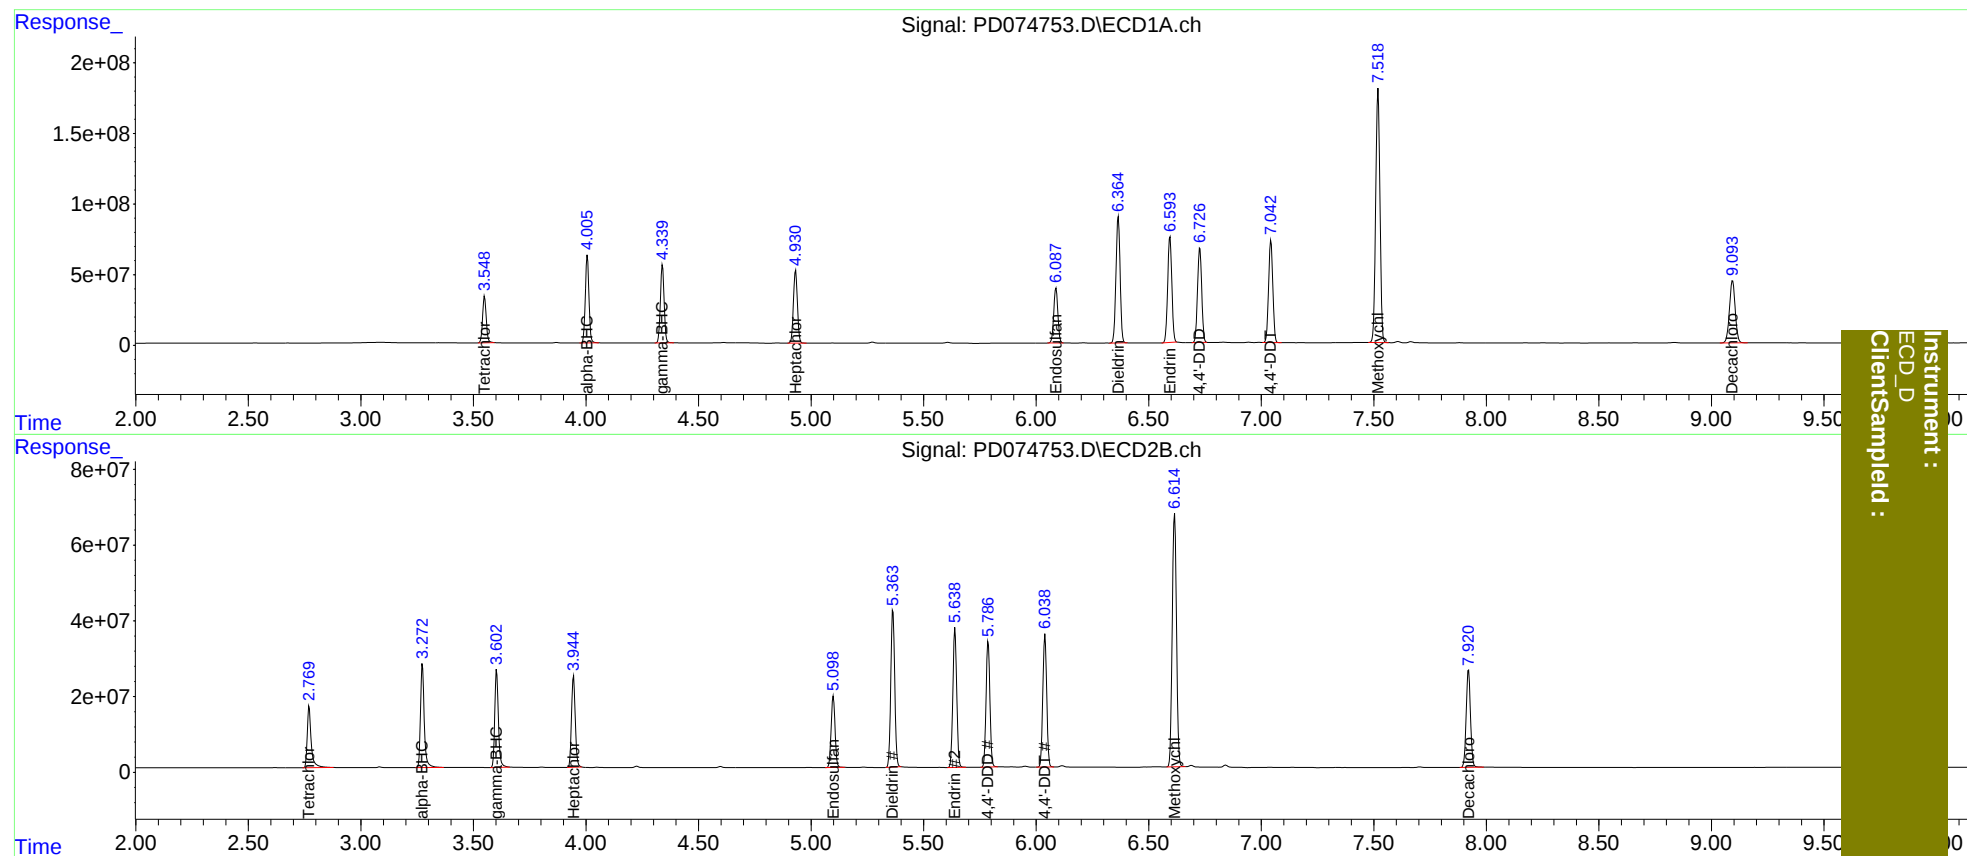


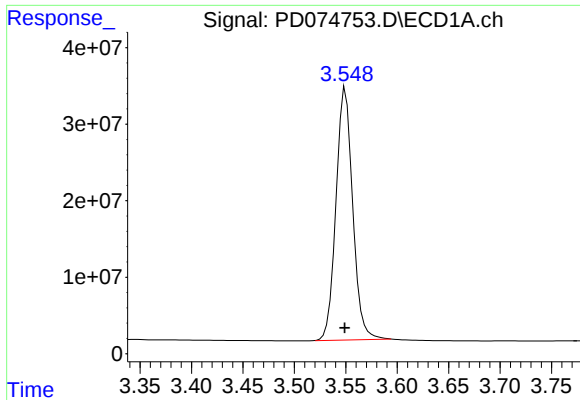

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 372903499
Conc: 162.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

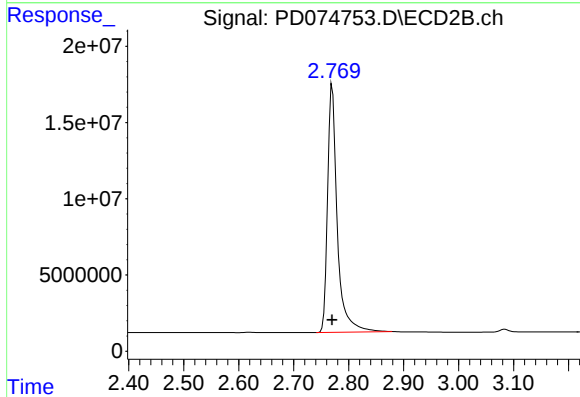


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 199304106
Conc: 154.45 ng/ml

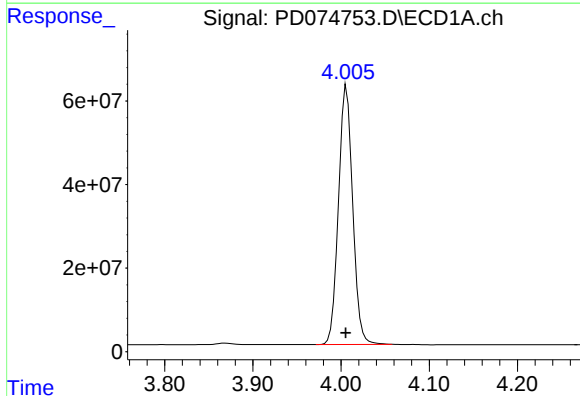


#2 alpha-BHC

R.T.: 4.006 min
Delta R.T.: 0.001 min
Response: 694645339
Conc: 188.95 ng/ml

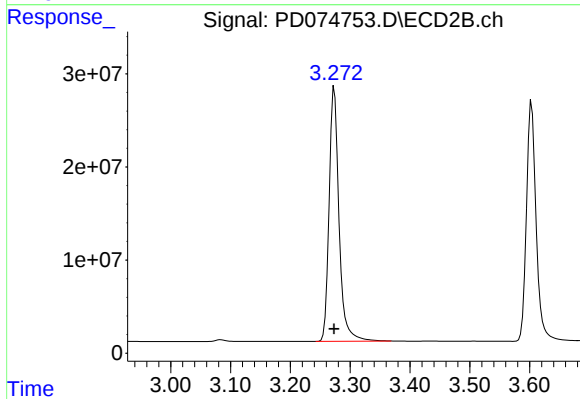

#2 alpha-BHC


R.T.: 3.274 min
Delta R.T.: 0.000 min
Response: 314016800
Conc: 175.07 ng/ml

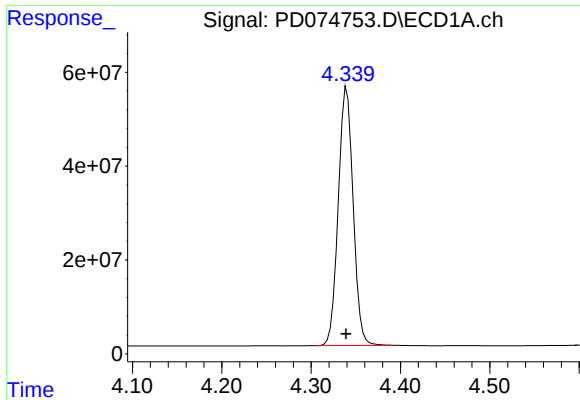

#3 gamma-BHC (Lindane)


R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 637004789
Conc: 182.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

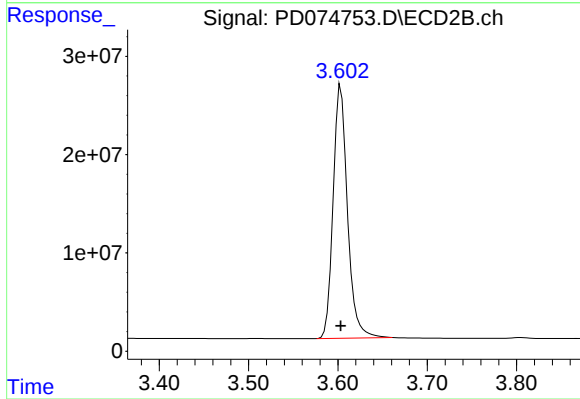


#3 gamma-BHC (Lindane)

R.T.: 3.603 min
Delta R.T.: 0.000 min
Response: 287843132
Conc: 170.11 ng/ml

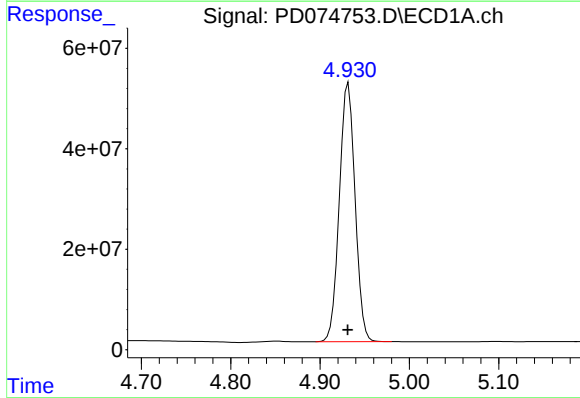


#4 Heptachlor

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 630074779
Conc: 183.01 ng/ml

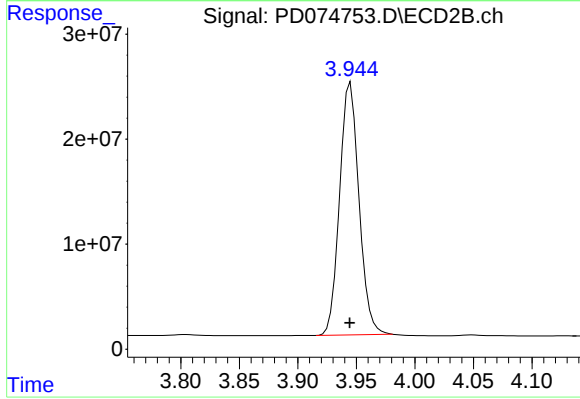

#4 Heptachlor


R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 277536940
Conc: 166.55 ng/ml

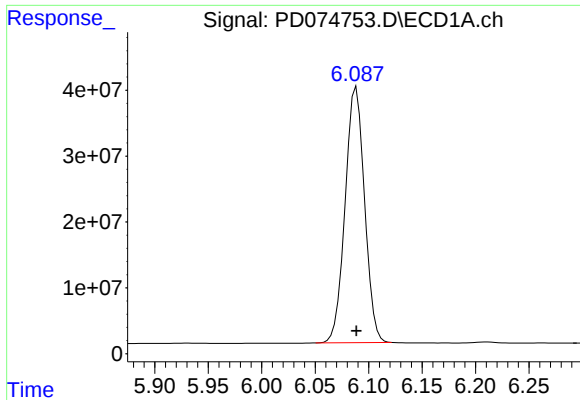

#9 Endosulfan I


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 491479871
Conc: 171.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

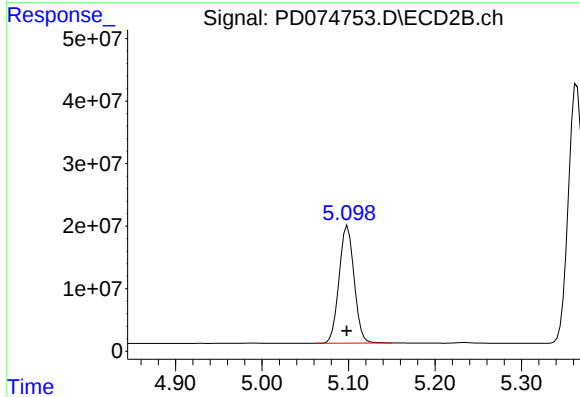


#9 Endosulfan I

R.T.: 5.099 min
Delta R.T.: 0.000 min
Response: 225828619
Conc: 161.43 ng/ml

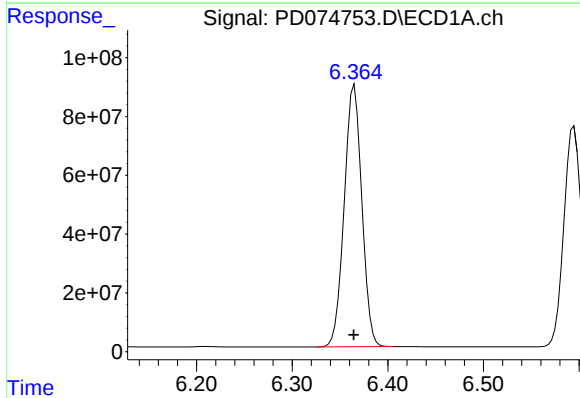


#13 Dieldrin

R.T.: 6.365 min
Delta R.T.: 0.000 min
Response: 1144181588
Conc: 361.64 ng/ml

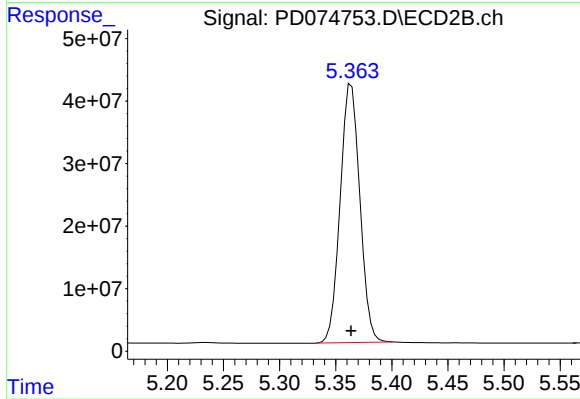

#13 Dieldrin


R.T.: 5.364 min
Delta R.T.: 0.000 min
Response: 504620645
Conc: 328.76 ng/ml

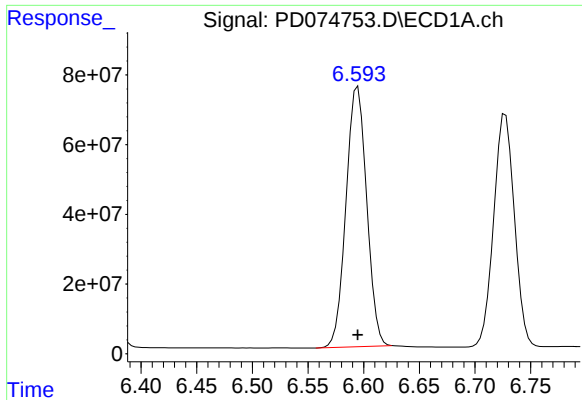

#14 Endrin


R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 965767310
Conc: 360.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

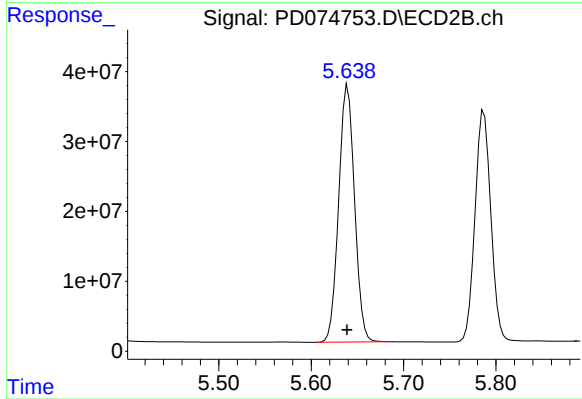


#14 Endrin

R.T.: 5.640 min
Delta R.T.: 0.000 min
Response: 439431876
Conc: 324.47 ng/ml

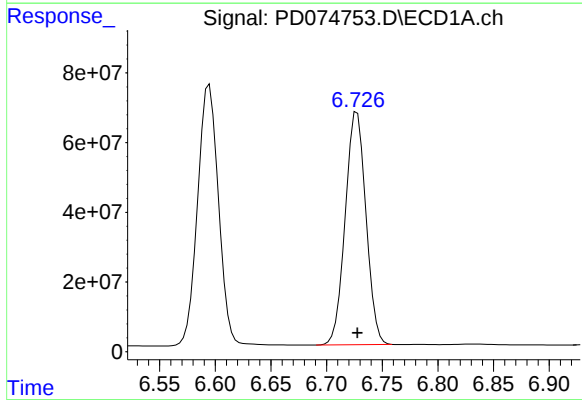


#16 4,4'-DDD

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 866560205
Conc: 360.48 ng/ml

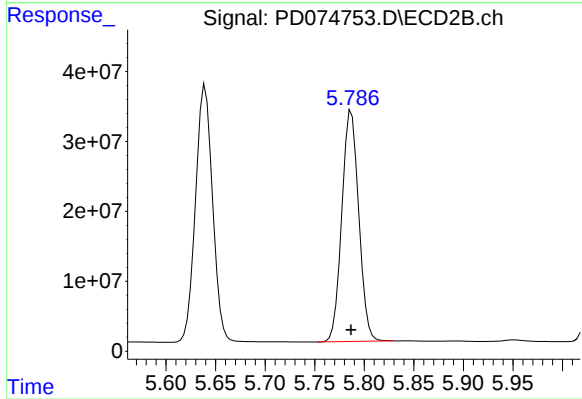

#16 4,4'-DDD


R.T.: 5.787 min
Delta R.T.: 0.000 min
Response: 392535354
Conc: 329.30 ng/ml

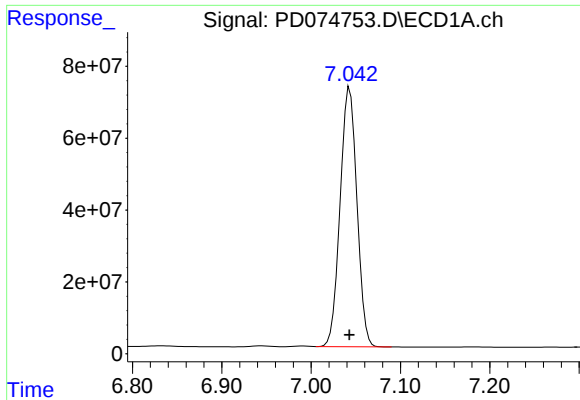

#17 4,4'-DDT


R.T.: 7.043 min
Delta R.T.: 0.000 min
Response: 944275876
Conc: 364.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

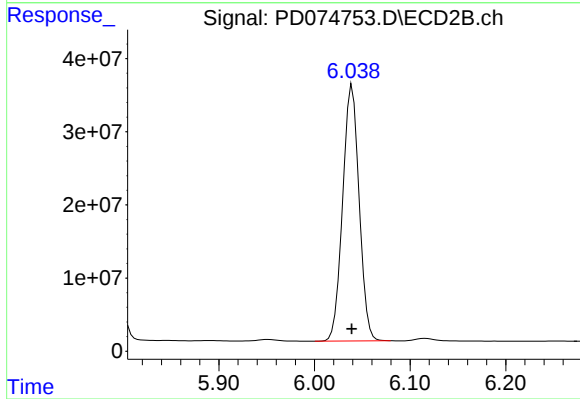


#17 4,4'-DDT

R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 420304194
Conc: 337.00 ng/ml

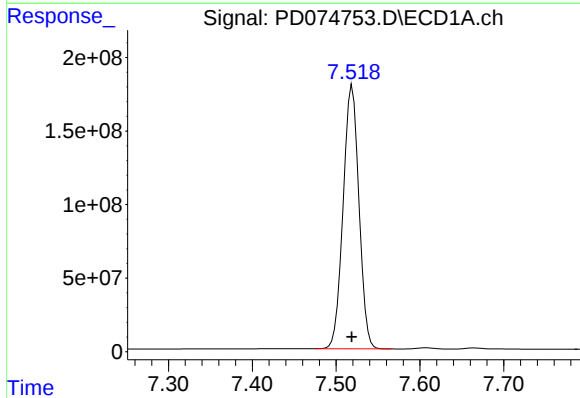


#20 Methoxychlor

R.T.: 7.519 min
Delta R.T.: 0.000 min
Response: 2353680248
Conc: 1604.65 ng/ml

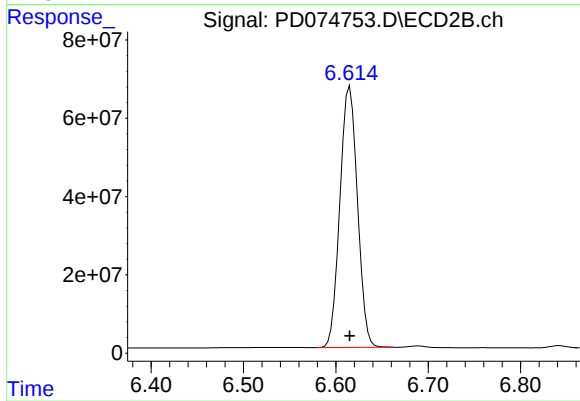

#20 Methoxychlor

R.T.: 6.615 min
Delta R.T.: 0.000 min
Response: 881167187
Conc: 1338.79 ng/ml

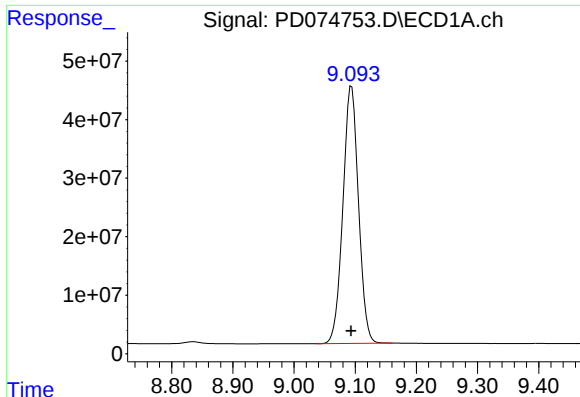

#27 Decachlorobiphenyl


R.T.: 9.094 min

Delta R.T.: 0.000 min

Response: 778801830

Conc: 291.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

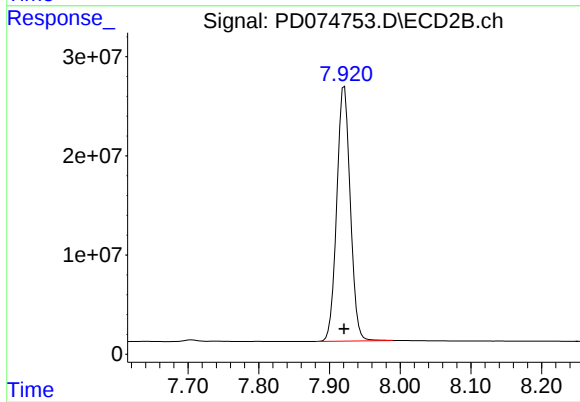

#27 Decachlorobiphenyl

R.T.: 7.921 min

Delta R.T.: 0.000 min

Response: 340883908

Conc: 286.88 ng/ml