

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 13:40
 Operator : AR\AJ
 Sample : INDA601
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA6065

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 06:56:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 15 06:56:30 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.770	372.9E6	199.3E6	158.657	153.402
27)	SA Decachlor...	9.094	7.921	778.8E6	340.9E6	288.709	286.345
Target Compounds							
2)	A alpha-BHC	4.006	3.274	694.6E6	314.0E6	178.605	169.800
3)	MA gamma-BHC...	4.340	3.603	637.0E6	287.8E6	174.480	166.617
4)	MA Heptachlor	4.932	3.945	630.1E6	277.5E6	173.189	163.648
9)	A Endosulfan I	6.089	5.099	491.5E6	225.8E6	164.789	158.858
13)	MA Dieldrin	6.365	5.364	1144.2E6	504.6E6	344.762	323.410
14)	MA Endrin	6.595	5.640	965.8E6	439.4E6	343.698	319.406
16)	A 4,4'-DDD	6.727	5.787	866.6E6	392.5E6	344.271	324.302
17)	MA 4,4'-DDT	7.043	6.039	944.3E6	420.3E6	345.765	331.175
20)	A Methoxychlor	7.519	6.615	2353.7E6	881.2E6	1569.865	1375.913

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 13:40
Operator : AR\AJ
Sample : INDA601
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 06:56:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Sat Apr 15 06:56:30 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

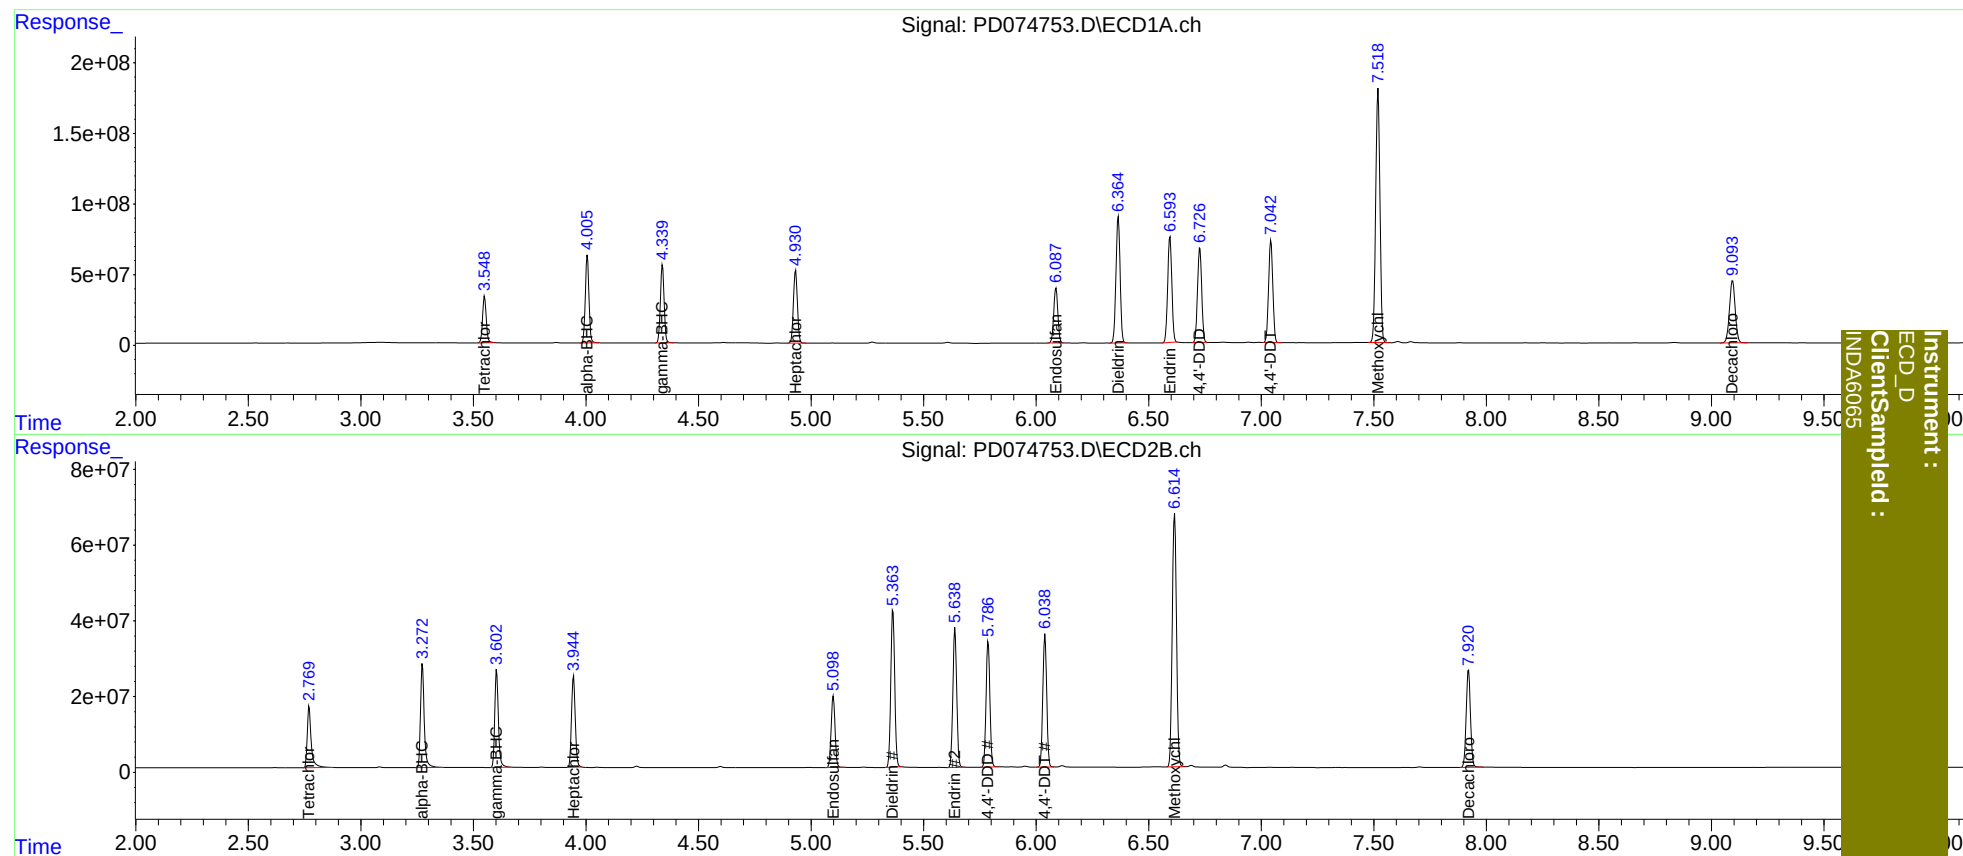

Instrument :
ECD_D
ClientSampled :
INDA6065