

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 15:08
 Operator : AR\AJ
 Sample : PB152088BS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS088

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/17/2023
 Supervised By : Ankita Jodhani 04/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 04:21:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 17 04:00:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.771	45540984	24384801	19.376	18.769
27)	SA Decachlor...	9.095	7.922	110.3E6	47376802	40.896	39.797
Target Compounds							
2)	A alpha-BHC	4.006	3.274	16528219	7718158	4.250	4.173
3)	MA gamma-BHC...	4.339	3.604	15659936	7235235	4.289	4.188
4)	MA Heptachlor	4.932	3.946	17017945	7582349	4.678	4.466
5)	MB Aldrin	5.275	4.226	17208849	7893372	4.922	4.674
6)	B beta-BHC	4.534	3.900	7632727	3665944	4.853	4.468
7)	B delta-BHC	4.782	4.130	12510228	6370920	4.239	3.585
8)	B Heptachlo...	5.701	4.728	16321841	7307310	5.561	4.668
9)	A Endosulfan I	6.089	5.099	14712982	6567077	4.933	4.620
10)	B trans-Chl...	5.958	4.979	15289381	7254784	4.916	4.736
11)	B cis-Chlor...	6.038	5.044	16102313	7305770	5.011	4.700
12)	B 4,4'-DDE	6.209	5.233	26374586	12955229	8.582	8.868
13)	MA Dieldrin	6.365	5.364	30983952	14184528	9.336	9.091
14)	MA Endrin	6.594	5.640	25720211	13094013	9.153m	9.518
15)	B Endosulfa...	6.814	5.933	27947237	12265478	9.575	9.357
16)	A 4,4'-DDD	6.727	5.786	23286976	12155581	9.252m	10.043m
17)	MA 4,4'-DDT	7.043	6.039	25972012	11516237	9.510	9.074
18)	B Endrin al...	6.944	6.113	20414278	9584145	8.818	8.891
19)	B Endosulfa...	7.180	6.336	26485344	12066526	9.725	9.587
20)	A Methoxychlor	7.520	6.616	75584663	33666954	50.414	52.570
21)	B Endrin ke...	7.665	6.843	31713881	14757649	10.015m	9.892

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 15:08
Operator : AR\AJ
Sample : PB152088BS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:21:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 17 04:00:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

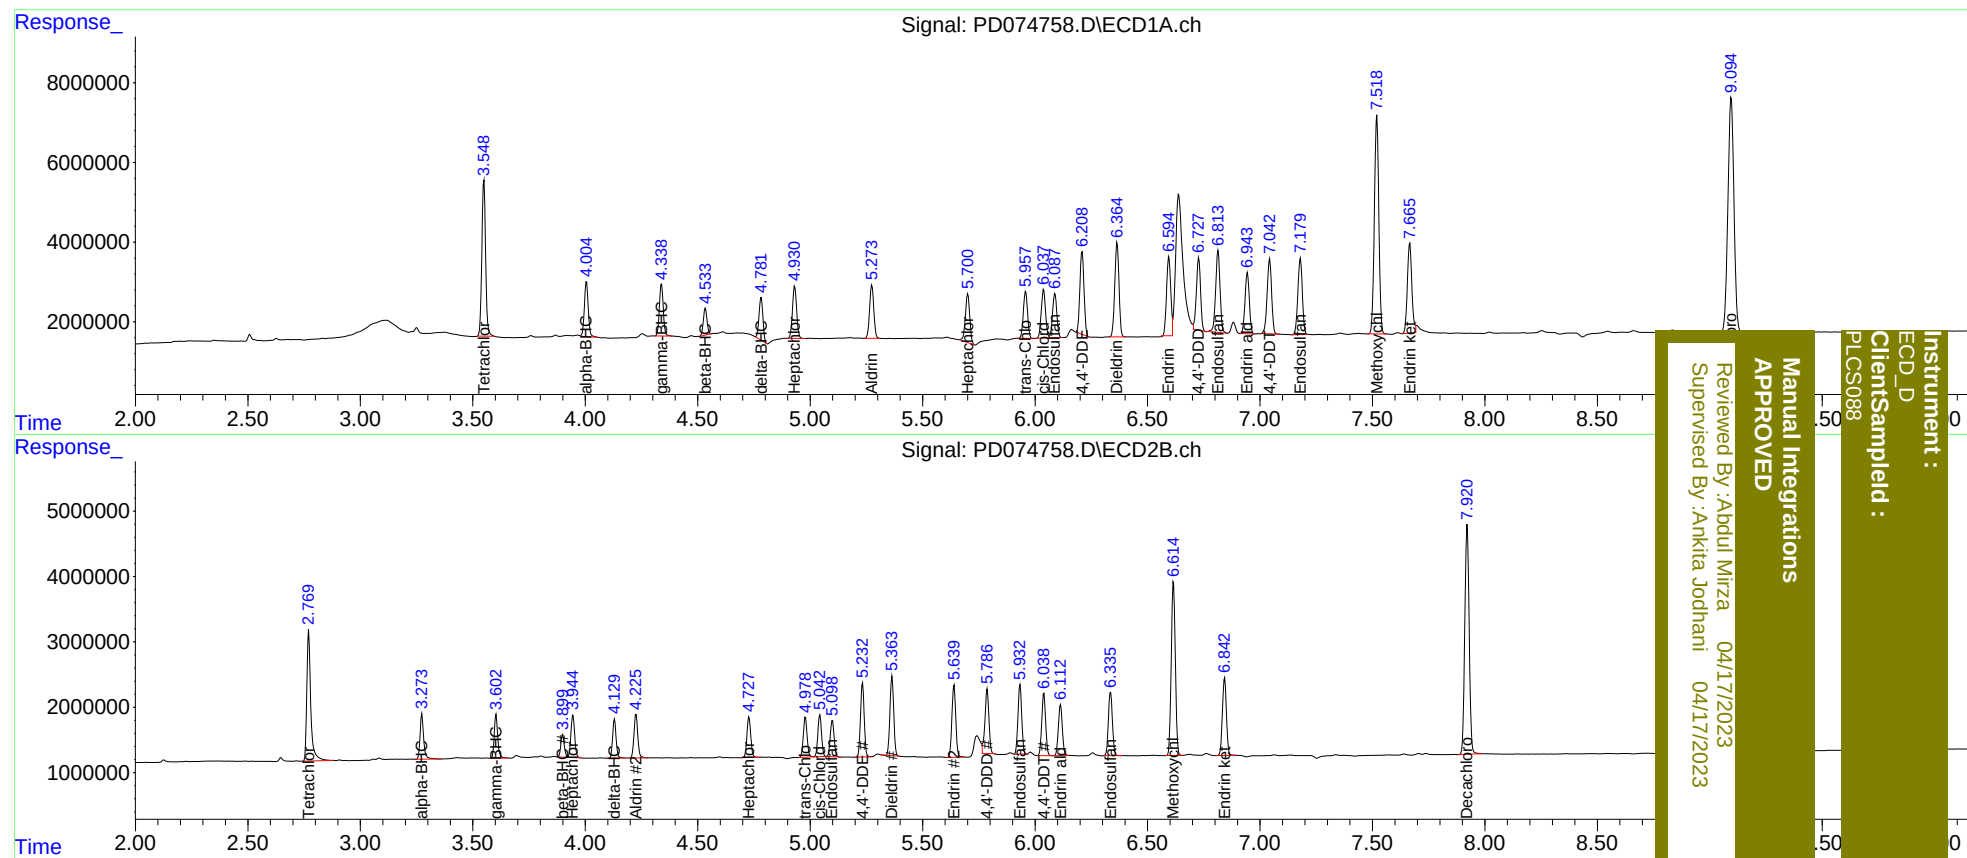

Instrument :
ECD_D
ClientSampled :
PLCS088

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 04/17/2023
Supervised By: Ankita Jodhani 04/17/2023