

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 09:19
 Operator : AR\AJ
 Sample : RESC354
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC007

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 04:19:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 17 04:00:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.770	47159524	27404650	20.065	21.093
27)	SA Decachlor...	9.094	7.921	110.4E6	49255411	40.927	41.375
Target Compounds							
2)	A alpha-BHC	4.006	3.273	34723519	18183115	8.928	9.832
3)	MA gamma-BHC...	4.339	3.603	32834964	17039444	8.994	9.863
4)	MA Heptachlor	4.931	3.945	31004538	16735782	8.522	9.858
5)	MB Aldrin	5.275	4.226	33024681	17441404	9.446	10.328
6)	B beta-BHC	4.534	3.899	16669130	8849564	10.598	10.786
7)	B delta-BHC	4.782	4.130	24387051	17733464	8.263	9.980
8)	B Heptachlo...	5.701	4.728	24696246	15903295	8.415	10.160
9)	A Endosulfan I	6.089	5.099	27100929	13377672	9.087	9.410
10)	B trans-Chl...	5.958	4.979	28471340	15403033	9.155	10.055
11)	B cis-Chlor...	6.038	5.043	30408327	15438092	9.463	9.932
12)	B 4,4'-DDE	6.210	5.233	55981738	28751595	18.215	19.680
13)	MA Dieldrin	6.365	5.364	58855463	29436972	17.734	18.866
14)	MA Endrin	6.595	5.640	50147229	26037680	17.846	18.926
15)	B Endosulfa...	6.814	5.933	64066471	27321219	21.950	20.843
16)	A 4,4'-DDD	6.728	5.788	45042538	22585160	17.895	18.659
17)	MA 4,4'-DDT	7.043	6.040	50358661	23578531	18.440	18.579
18)	B Endrin al...	6.945	6.113	47363450	22732709	20.459	21.089
19)	B Endosulfa...	7.179	6.336	55861662	25995009	20.511	20.653
20)	A Methoxychlor	7.519	6.616	149.4E6	67557457	99.654	105.489
21)	B Endrin ke...	7.665	6.843	65752972	31366033	20.763	21.024

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 09:19
Operator : AR\AJ
Sample : RESC354
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:19:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 17 04:00:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

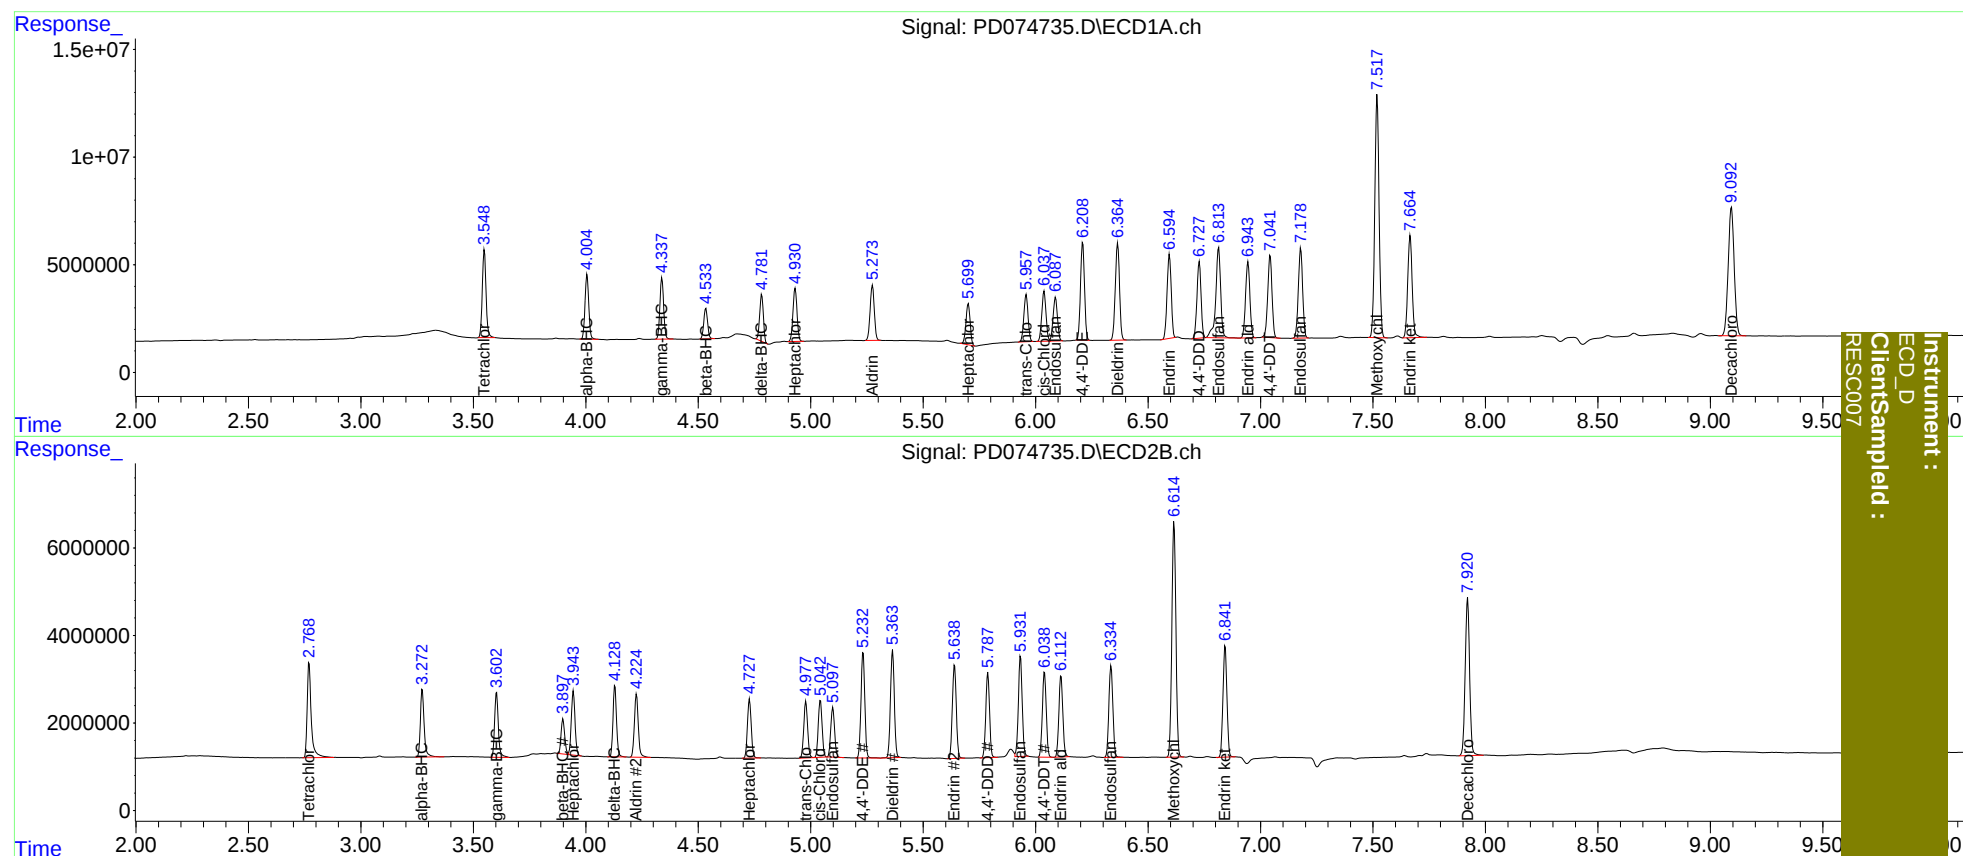

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074735.D
Acq On : 14 Apr 2023 09:19
Operator : AR\AJ
Sample : RESC354
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Title : GC Extractables
Last Update : Mon Apr 17 04:00:38 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.549	4.006	100.00%
4.006	4.339	100.00%
4.339	4.534	100.00%
4.534	4.782	100.00%
4.782	4.931	100.00%
4.931	5.275	100.00%
5.275	5.701	100.00%
5.701	5.958	100.00%
5.958	6.038	100.00%
6.038	6.089	97.80%
6.089	6.210	100.00%
6.210	6.365	100.00%
6.365	6.595	100.00%
6.595	6.728	100.00%
6.728	6.814	100.00%
6.814	6.945	100.00%
6.945	7.043	100.00%
7.043	7.179	100.00%
7.179	7.519	100.00%
7.519	7.666	100.00%
7.666	9.094	100.00%

Signal #2


2.770	3.273	100.00%
3.273	3.603	100.00%
3.603	3.899	100.00%
3.899	3.945	98.89%
3.945	4.130	100.00%
4.130	4.226	100.00%
4.226	4.728	100.00%
4.728	4.979	100.00%
4.979	5.043	100.00%
5.043	5.099	100.00%
5.099	5.233	100.00%
5.233	5.364	100.00%
5.364	5.640	100.00%
5.640	5.788	100.00%
5.788	5.933	100.00%
5.933	6.040	100.00%
6.040	6.113	100.00%
6.113	6.336	100.00%
6.336	6.616	100.00%
6.616	6.843	100.00%
6.843	7.921	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 09:19
Operator : AR\AJ
Sample : RESC354
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:19:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 17 04:00:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

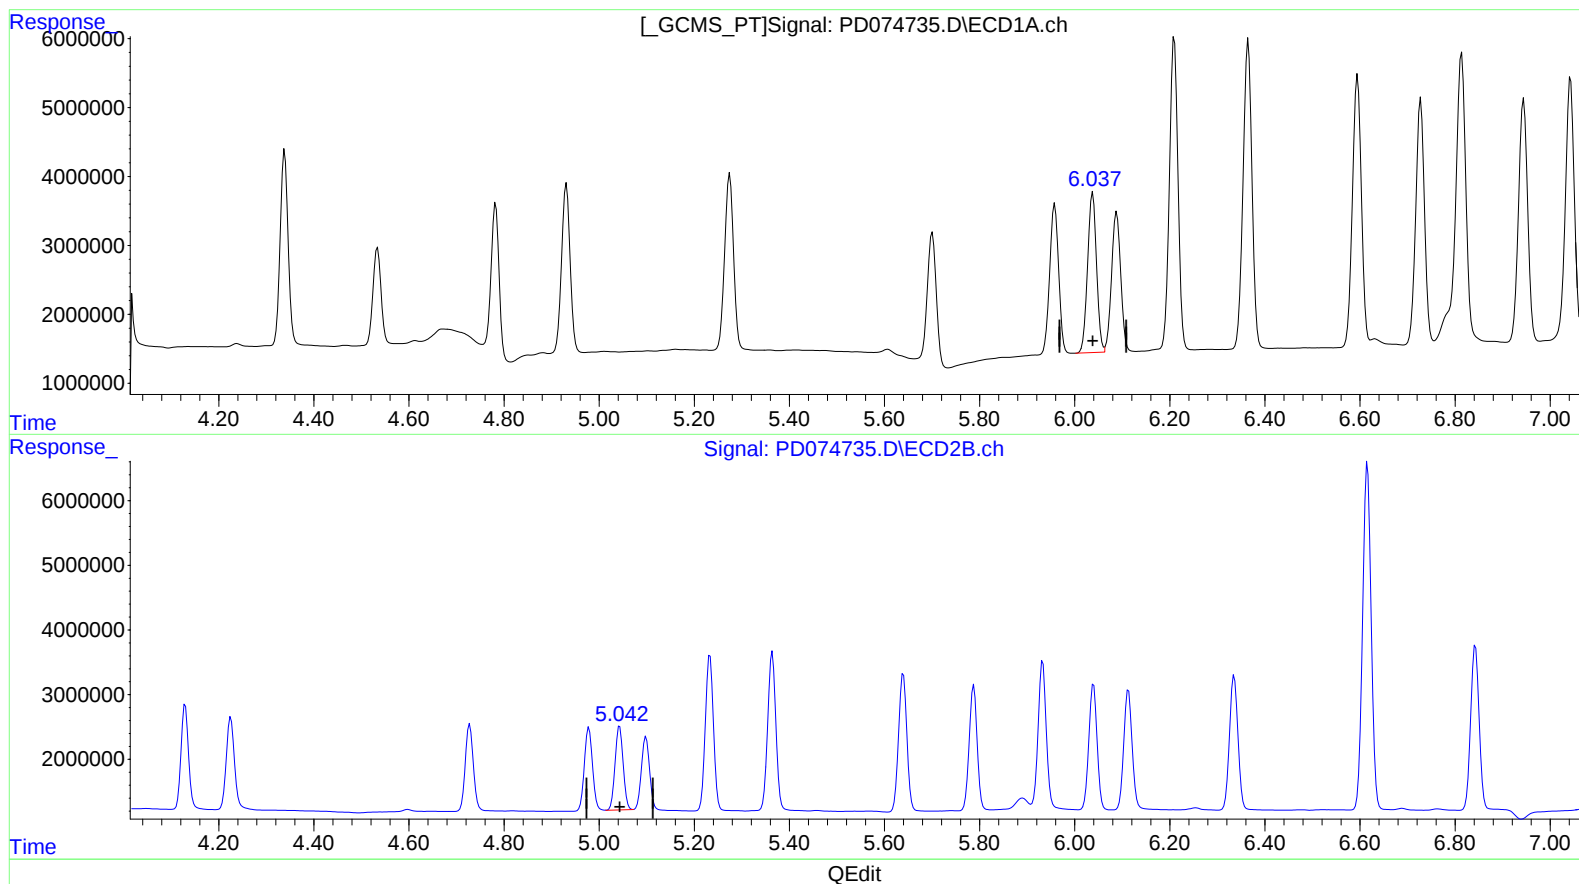

(11) cis-Chlordane (B)

6.038min 9.463 ng/ml

response 30408327

(11) cis-Chlordane #2 (B)

5.043min 9.932 ng/ml


response 15438092

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 09:19
Operator : AR\AJ
Sample : RESC354
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC007

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:19:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 17 04:00:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

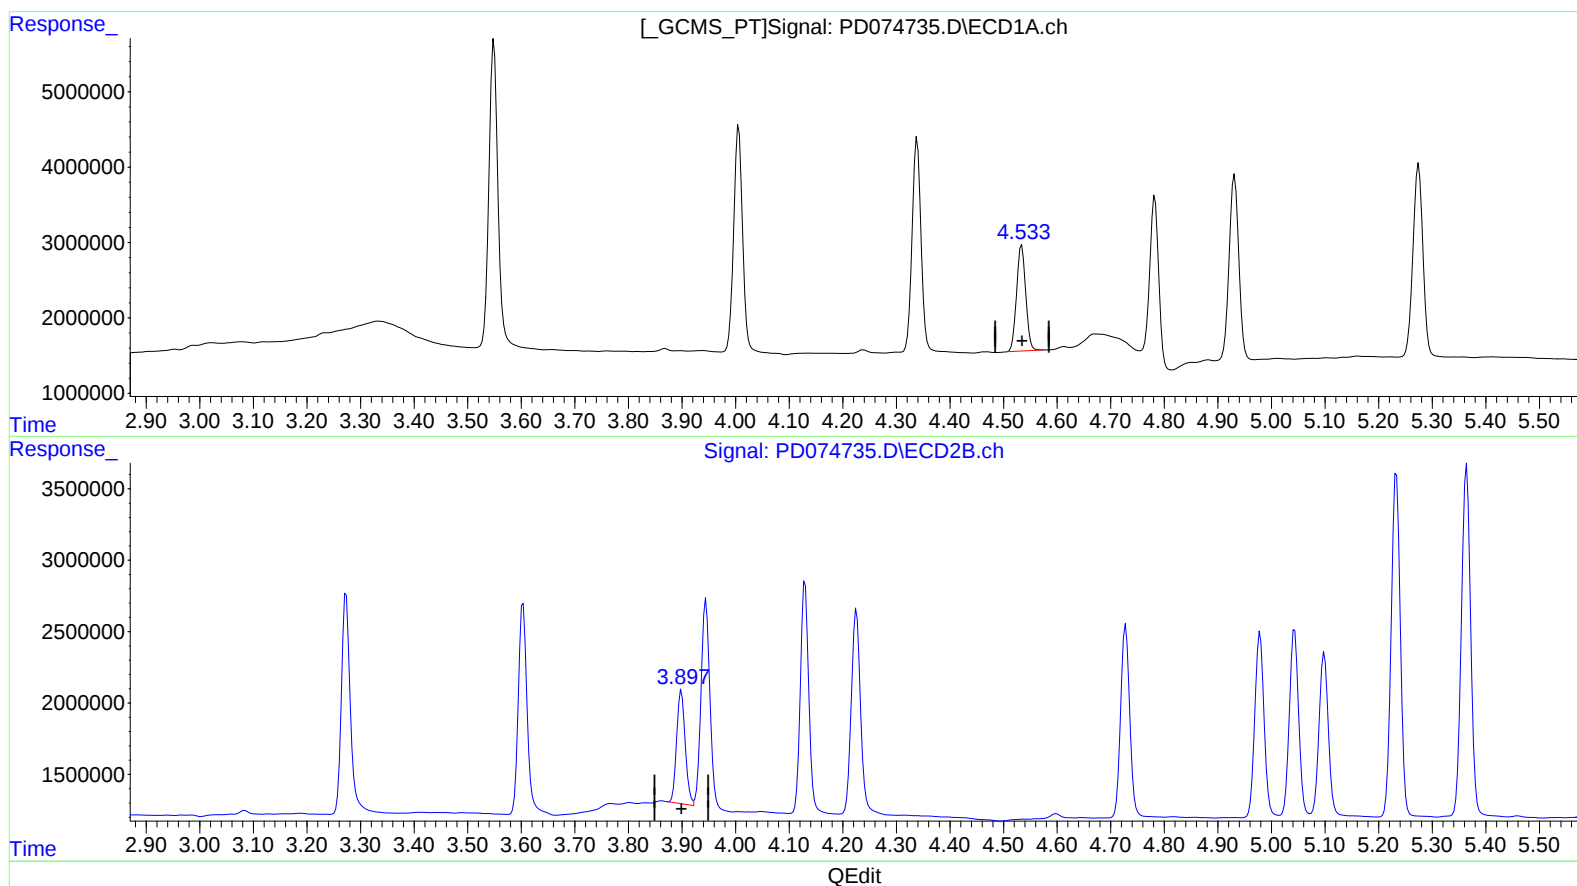

(6) beta-BHC (B)
4.534min 10.598 ng/ml
response 16669130

(6) beta-BHC #2 (B)
3.899min 10.786 ng/ml
response 8849564