

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
 Data File : PD074761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2023 15:49
 Operator : AR\AJ
 Sample : 02255-02MS 10X (Sig #1); 02255-02MS (Sig #2)
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AN5MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 17 04:15:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 17 04:00:38 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.771	51754923	26573298	22.020	20.453
2)	SA Decachlor...	9.095	7.922	118.6E6	50837199	43.959	42.704
Target Compounds							
2)	A alpha-BHC	4.006	3.274	200.9E6	92232586	51.642	49.873
3)	MA gamma-BHC...	4.339	3.604	184.3E6	83009440	50.486	48.050
4)	MA Heptachlor	4.932	3.945	181.2E6	81520469	49.818	48.017
5)	MB Aldrin	5.276	4.226	189.5E6	86575368	54.194	51.268
6)	B beta-BHC	4.534	3.899	75596746	35546972	48.062	43.326
7)	B delta-BHC	4.783	4.130	129.8E6	67737340	43.970	38.120
8)	B Heptachlo...	5.702	4.729	156.0E6	76261655	53.152	48.721
9)	A Endosulfan I	6.089	5.099	152.6E6	67721250	51.163	47.638
10)	B trans-Chl...	5.959	4.979	162.1E6	75658167	52.119	49.390
11)	B cis-Chlor...	6.039	5.043	166.6E6	74668441	51.856	48.037
12)	B 4,4'-DDE	6.211	5.233	327.5E6	150.5E6	106.568	103.028
13)	MA Dieldrin	6.365	5.364	359.7E6	162.2E6	108.371	103.930
14)	MA Endrin	6.596	5.640	300.9E6	142.6E6	107.075	103.679
15)	B Endosulfa...	6.815	5.934	291.6E6	132.8E6	99.914	101.324
16)	A 4,4'-DDD	6.729	5.788	263.5E6	122.7E6	104.686	101.338
17)	MA 4,4'-DDT	7.044	6.040	300.1E6	132.2E6	109.884	104.201
18)	B Endrin al...	6.944	6.114	208.7E6	95160506	90.133	88.280
19)	B Endosulfa...	7.179	6.336	264.2E6	119.4E6	97.019	94.828
20)	A Methoxychlor	7.520	6.616	767.1E6	314.8E6	511.616	491.597
21)	B Endrin ke...	7.667	6.844	318.7E6	149.1E6	100.629	99.929

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041523\
Data File : PD074761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2023 15:49
Operator : AR\AJ
Sample : 02255-02MS 10X (Sig #1); 02255-02MS (Sig #2)
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 17 04:15:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041523CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Mon Apr 17 04:00:38 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

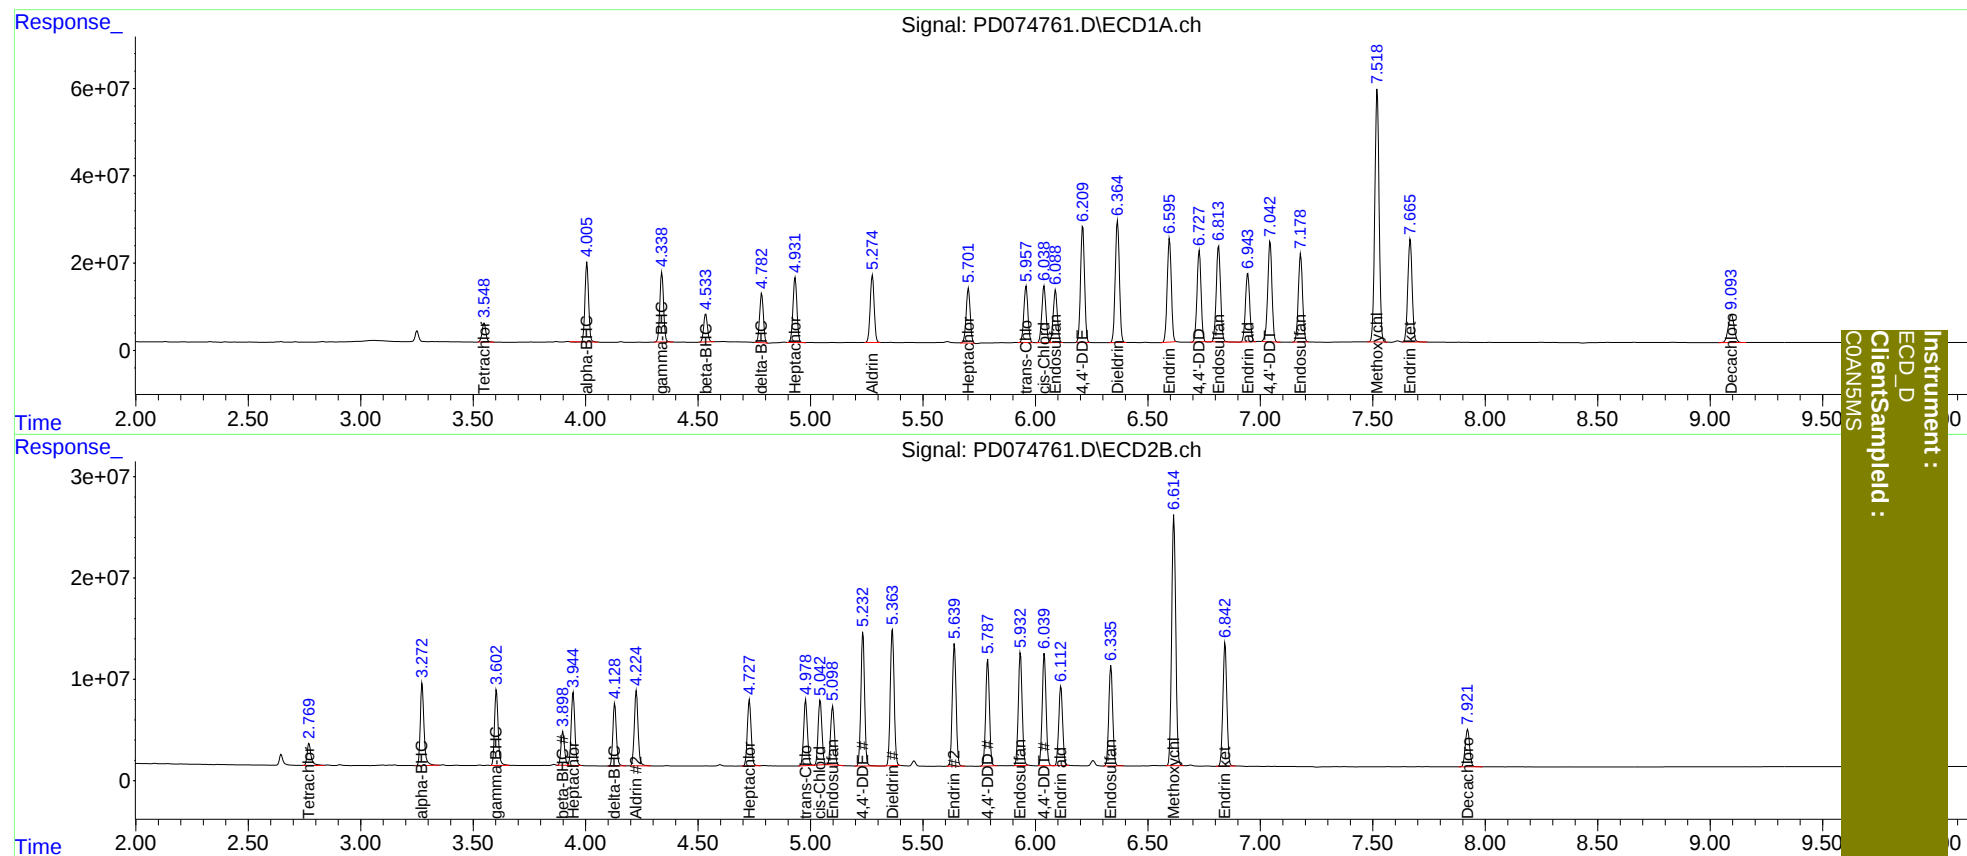

Instrument :
ECD_D
ClientSampled :
COAN5MS