

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041719\
 Data File : PD052962.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Apr 2019 8:16
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 01:09:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 29 13:06:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.219	4.041	30830687	639.2E6	22.094	22.054
28)	SA Decachlor...	7.814	9.159	32389722	349.9E6	24.303	22.500
Target Compounds							
3)	MA gamma-BHC...	3.929f	0.000	1070056	0	0.489	N.D. #
4)	MA Heptachlor	0.000	5.245	0	1178370	N.D.	0.030 #
8)	B Heptachlo...	4.867f	5.919	697338	13642312	0.367	0.423
10)	B gamma-Chl...	0.000	6.165	0	84218031	N.D.	2.632 #
12)	B 4,4'-DDE	0.000	6.421f	0	3753049	N.D.	0.123 #
14)	MA Endrin	0.000	6.763	0	22940614	N.D.	0.915 #
22)	Mirex	0.000	8.253	0	15749963	N.D.	1.221 #
25)	Chlordane-3	0.000	6.165	0	84218031	N.D.	19.085 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041719\
Data File : PD052962.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Apr 2019 8:16
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 01:09:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032919.M
Quant Title : GC Extractables
QLast Update : Fri Mar 29 13:06:45 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

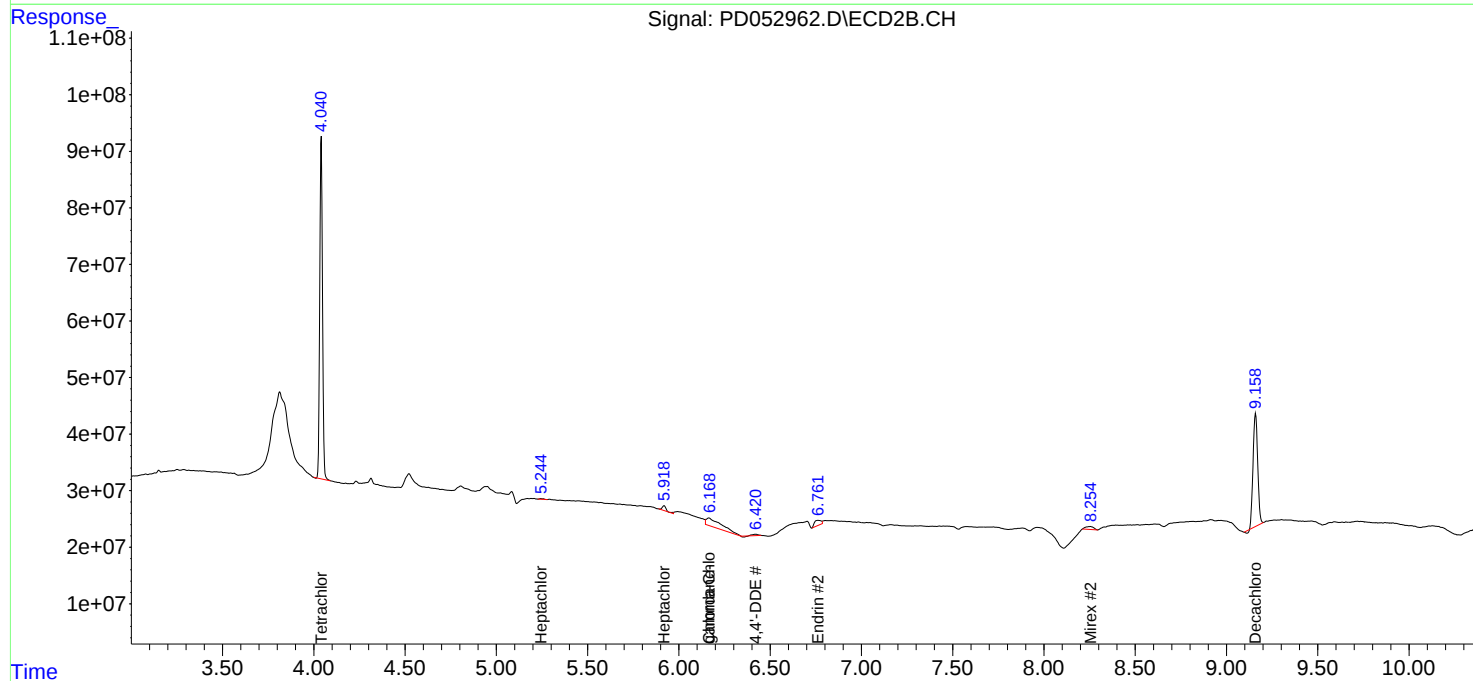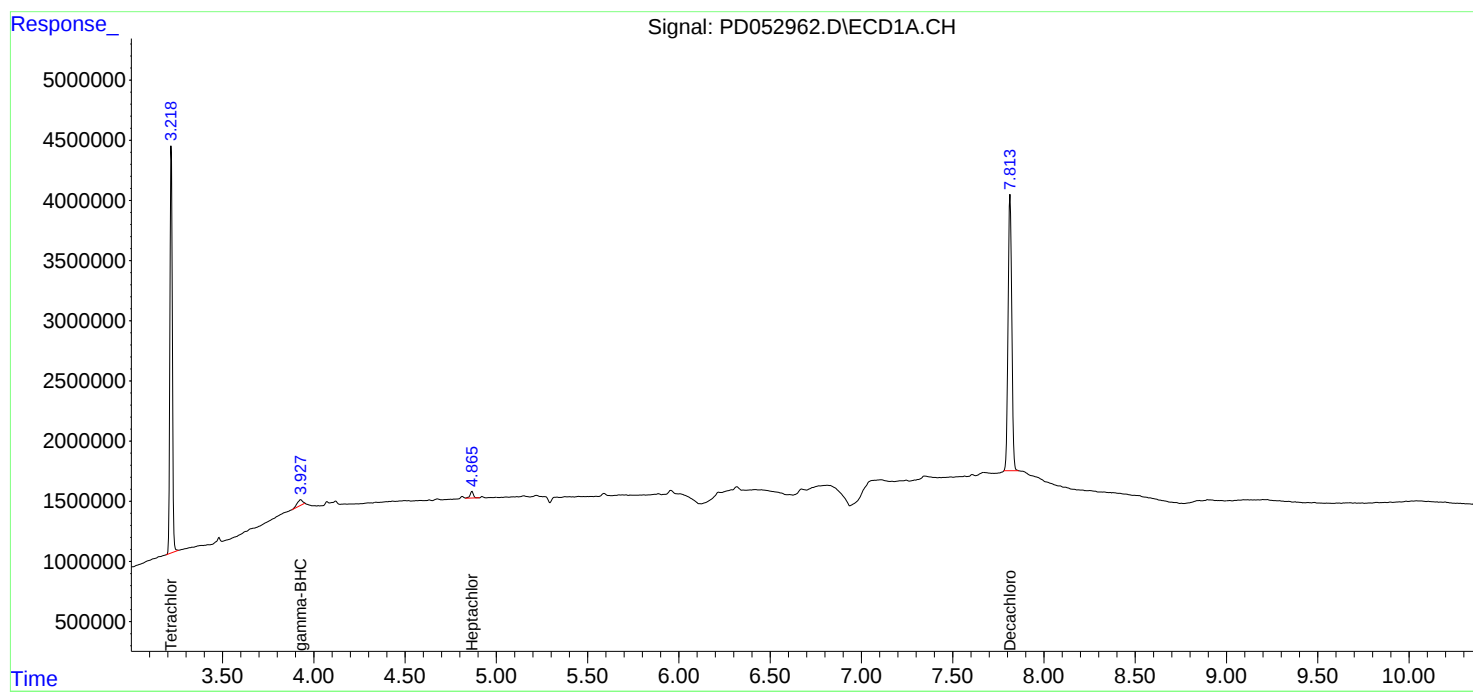


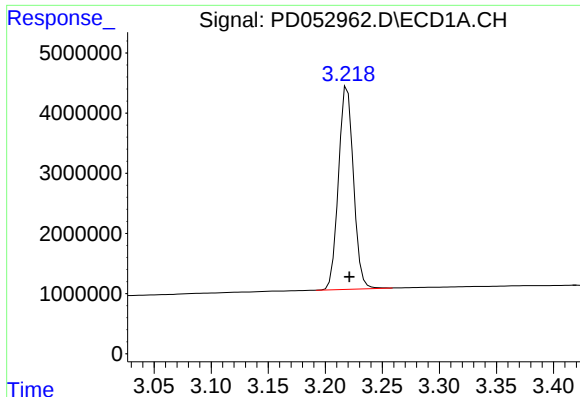

#1 Tetrachloro-m-xylene


R.T.: 3.219 min
Delta R.T.: -0.002 min
Response: 30830687
Conc: 22.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

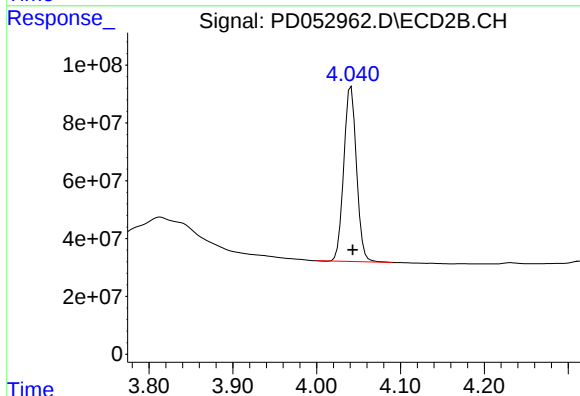


#1 Tetrachloro-m-xylene

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 639203491
Conc: 22.05 ng/ml

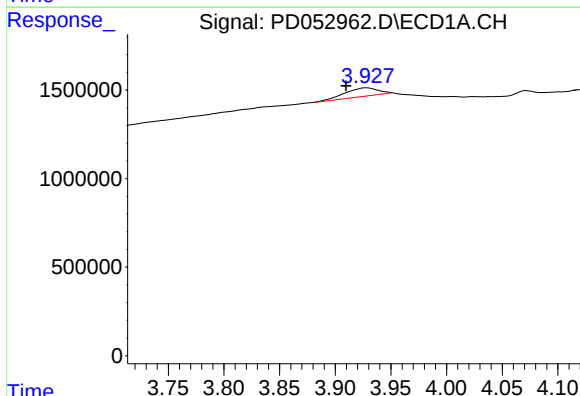


#3 gamma-BHC (Lindane)

R.T.: 3.929 min
Delta R.T.: 0.019 min
Response: 1070056
Conc: 0.49 ng/ml

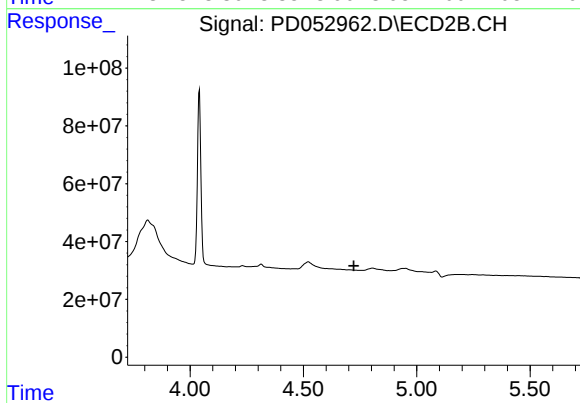

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

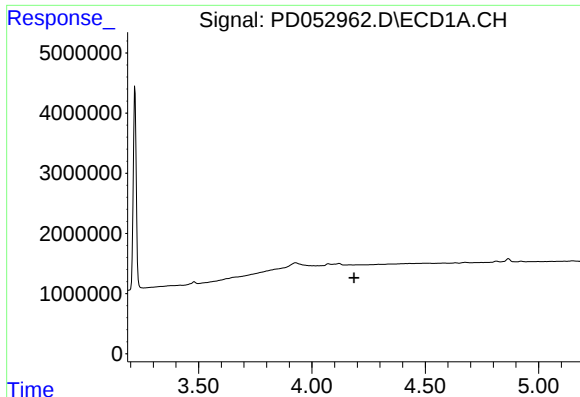

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.187 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

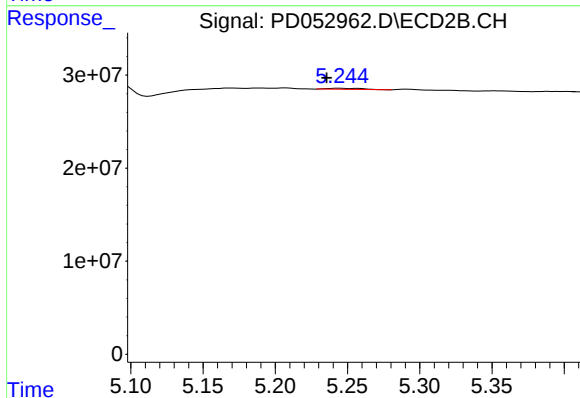


#4 Heptachlor

R.T.: 5.245 min
Delta R.T.: 0.009 min
Response: 1178370
Conc: 0.03 ng/ml

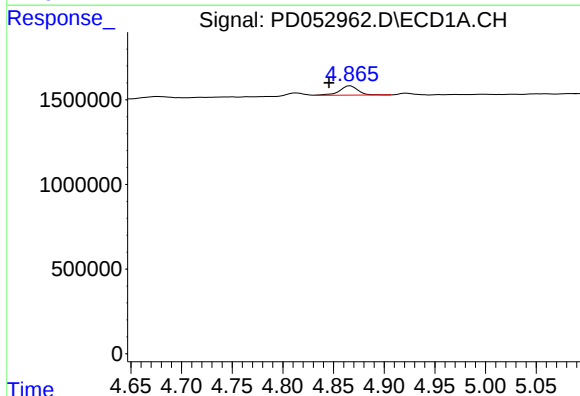


#8 Heptachlor epoxide

R.T.: 4.867 min
Delta R.T.: 0.021 min
Response: 697338
Conc: 0.37 ng/ml

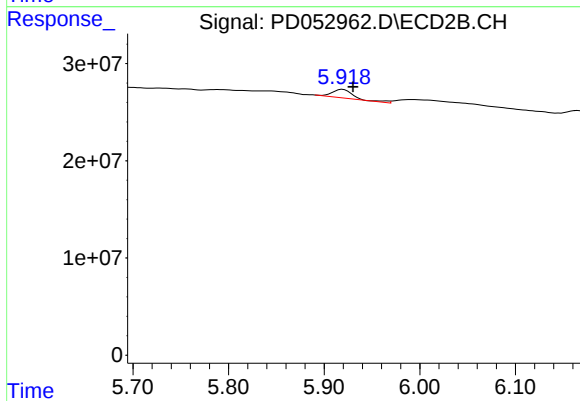

#8 Heptachlor epoxide


R.T.: 5.919 min
Delta R.T.: -0.011 min
Response: 13642312
Conc: 0.42 ng/ml

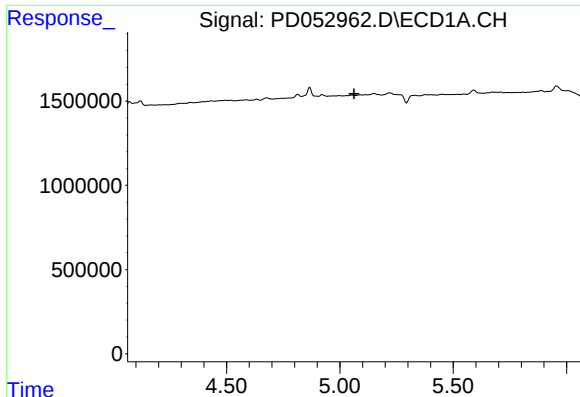

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.063 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

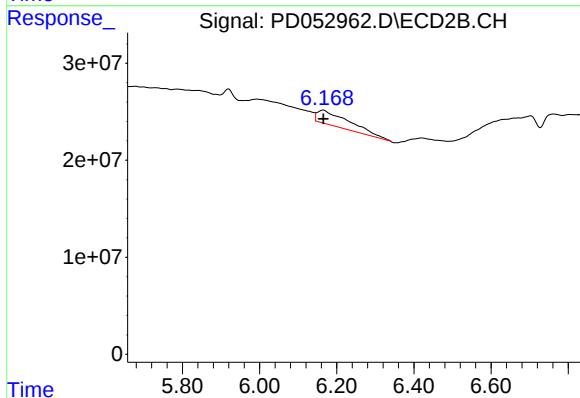


#10 gamma-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 84218031
Conc: 2.63 ng/ml

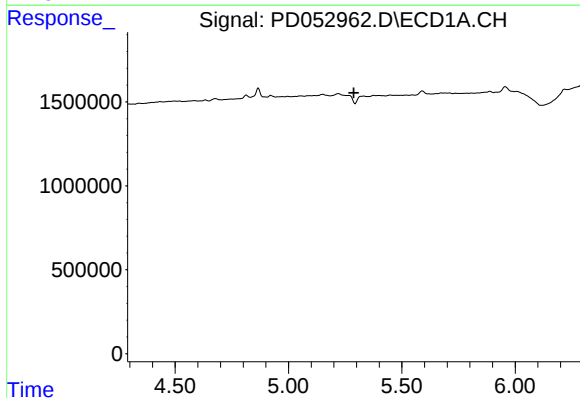


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.288 min
Response: 0
Conc: N.D.

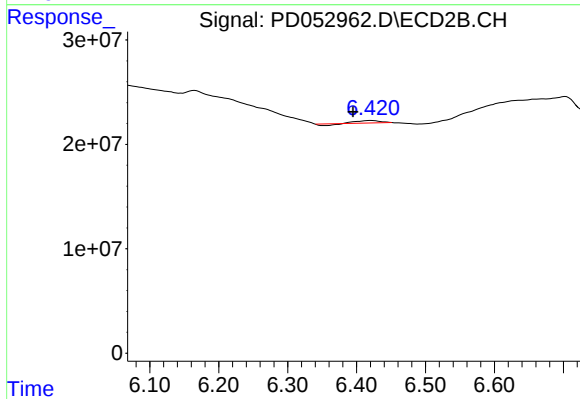

#12 4,4'-DDE


R.T.: 6.421 min
Delta R.T.: 0.026 min
Response: 3753049
Conc: 0.12 ng/ml

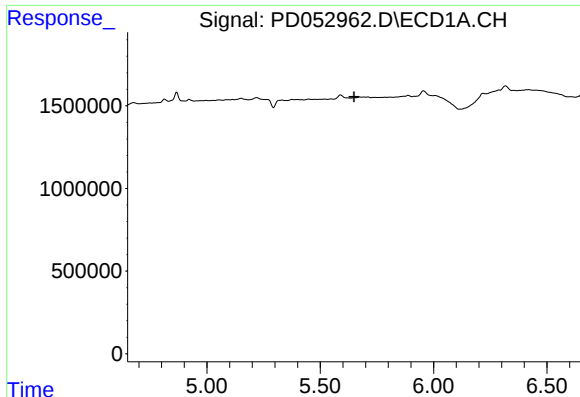

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.650 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

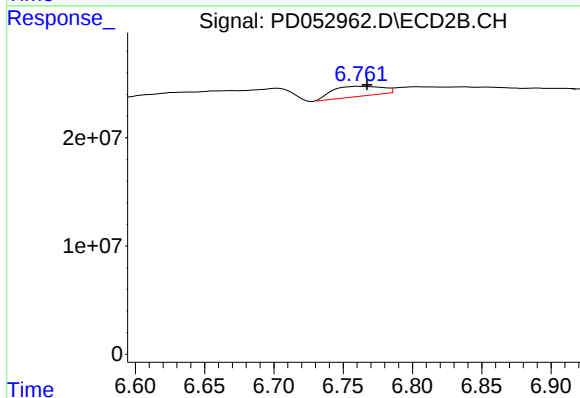


#14 Endrin

R.T.: 6.763 min
Delta R.T.: -0.005 min
Response: 22940614
Conc: 0.92 ng/ml

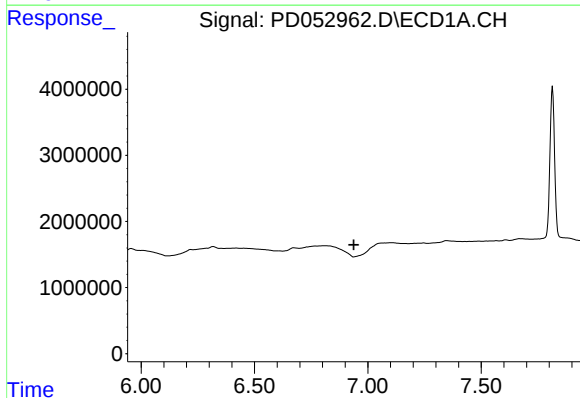


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 6.938 min
Response: 0
Conc: N.D.

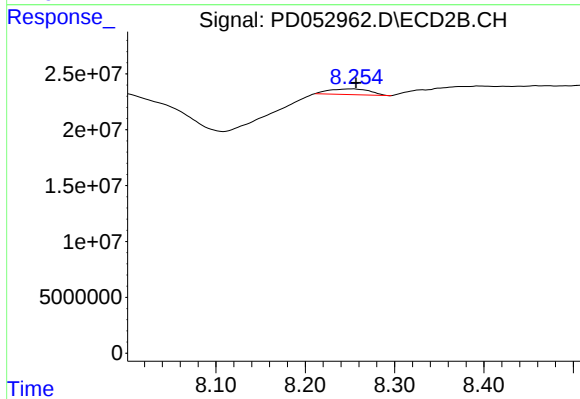

#22 Mirex


R.T.: 8.253 min
Delta R.T.: -0.004 min
Response: 15749963
Conc: 1.22 ng/ml

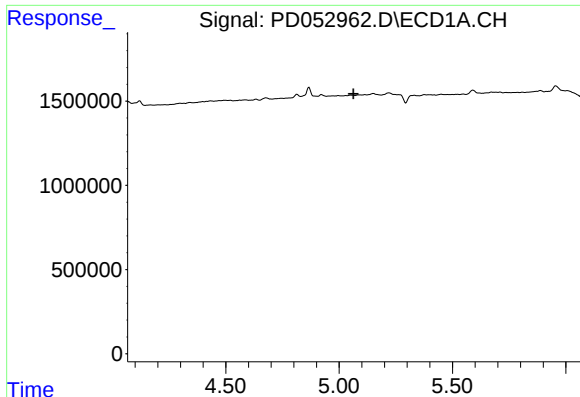

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

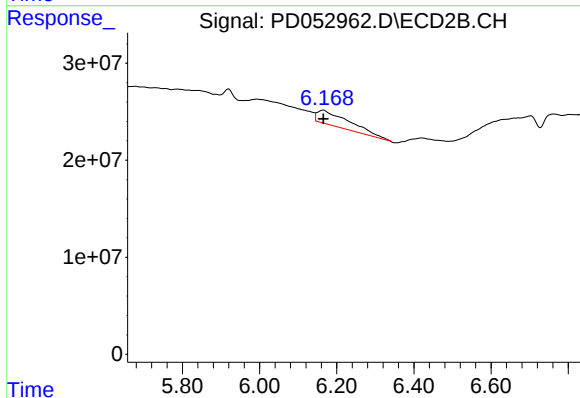


#25 Chlordane-3

R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 84218031
Conc: 19.08 ng/ml

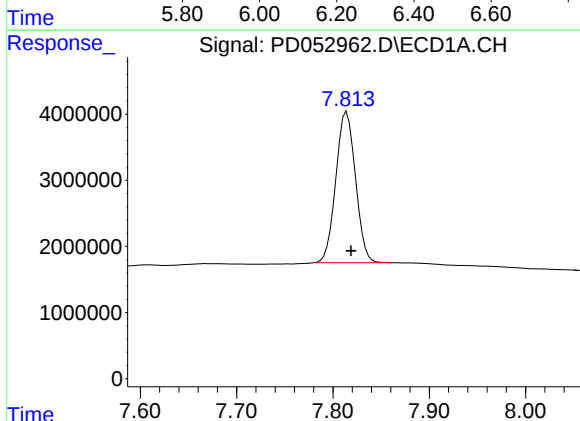

#28 Decachlorobiphenyl

R.T.: 7.814 min
Delta R.T.: -0.004 min
Response: 32389722
Conc: 24.30 ng/ml

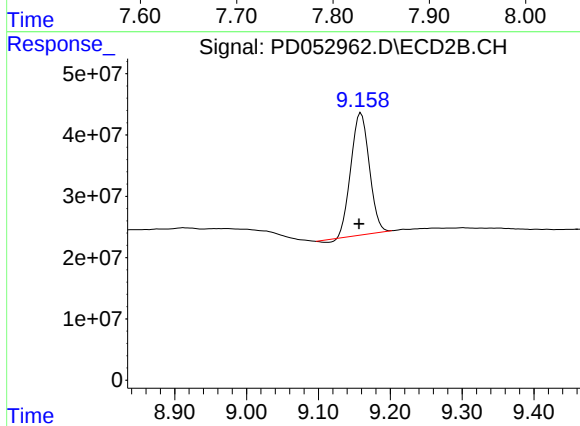

#28 Decachlorobiphenyl

R.T.: 9.159 min
Delta R.T.: 0.003 min
Response: 349899227
Conc: 22.50 ng/ml