

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
 Data File : PD069121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 09:11
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 16:20:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 15 16:15:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.171	28381350	284.8E6	25.567	26.559
28)	SA Decachlor...	8.201	9.365	31094152	172.7E6	24.902	26.387
Target Compounds							
9)	A Endosulfan I	5.494	6.447	16181874	154.2E6	12.539	14.277
10)	B gamma-Chl...	5.381	6.322	17907143	175.1E6	12.882	15.034
12)	B 4,4'-DDE	5.606	6.547	31018466	277.8E6	24.514	25.721
13)	MA Dieldrin	5.738	6.706	33700454	294.1E6	24.976	26.386
19)	B Endosulfa...	6.652	7.480	27621384	206.1E6	22.835	24.144
20)	A Methoxychlor	6.914	7.793	72586493	473.9E6	114.264	109.920
21)	B Endrin ke...	7.145	7.955	34166063	233.6E6	24.266	25.835



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
Data File : PD069121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 09:11
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 16:20:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Fri Apr 15 16:15:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

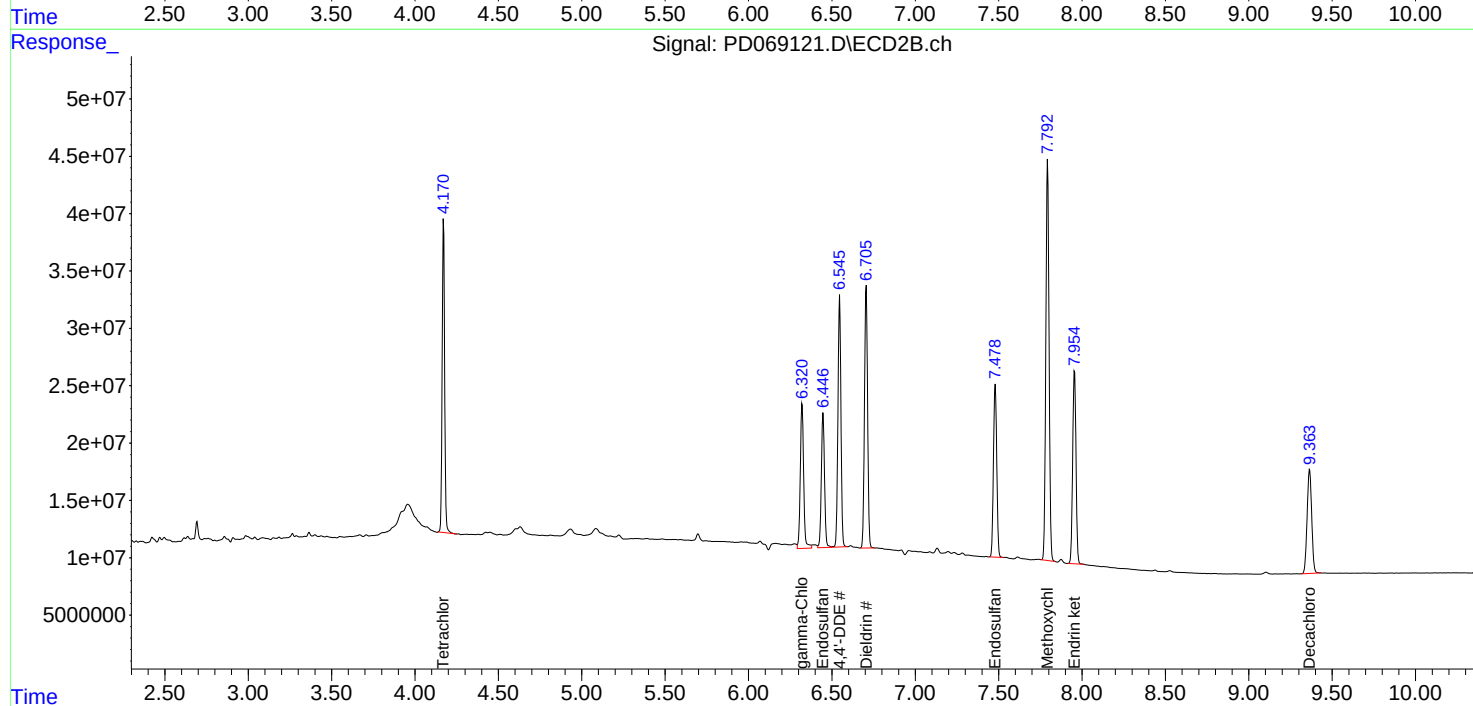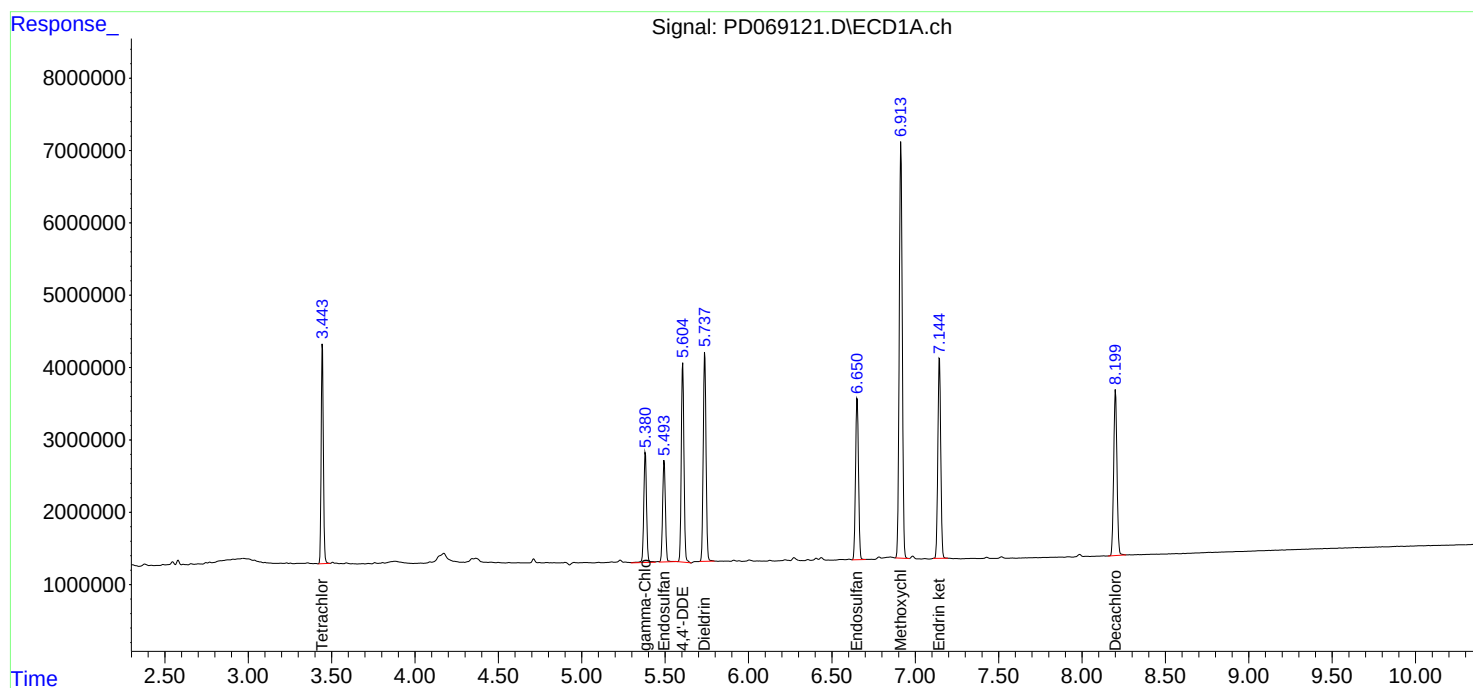


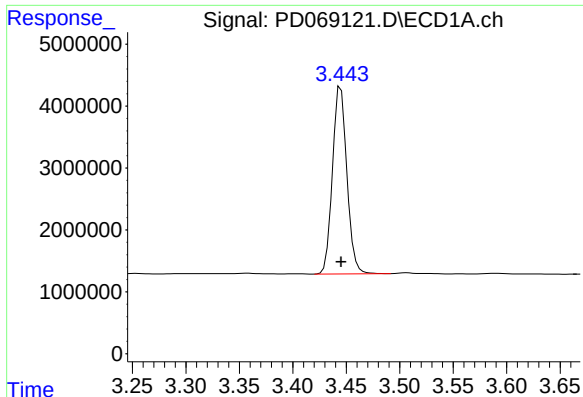

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 28381350
Conc: 25.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

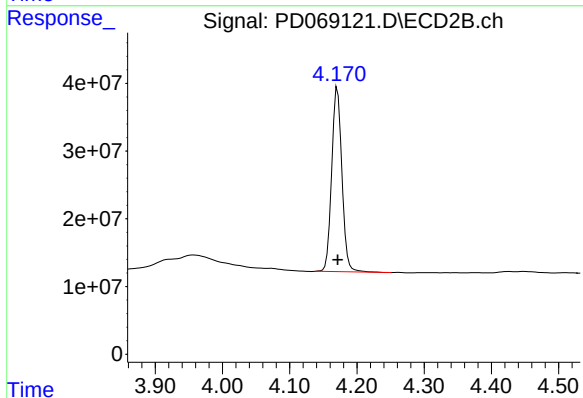


#1 Tetrachloro-m-xylene

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 284753952
Conc: 26.56 ng/ml

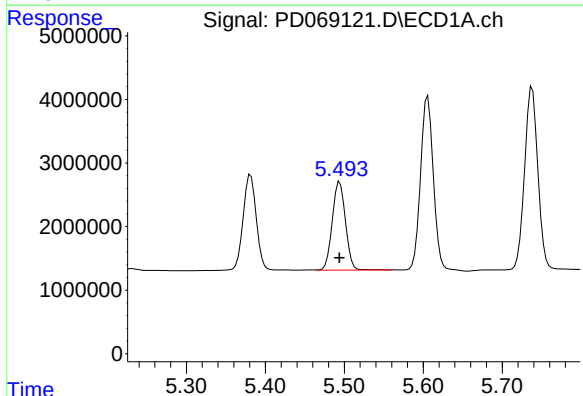


#9 Endosulfan I

R.T.: 5.494 min
Delta R.T.: 0.000 min
Response: 16181874
Conc: 12.54 ng/ml

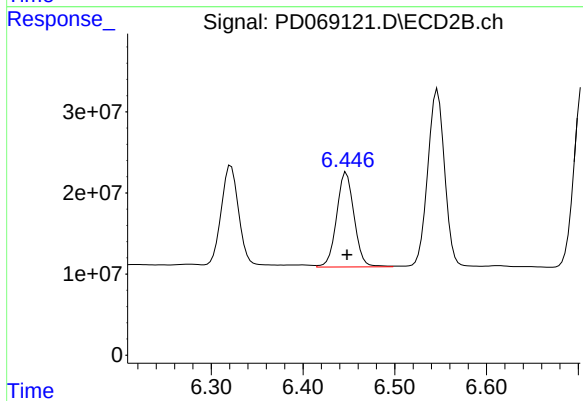

#9 Endosulfan I


R.T.: 6.447 min
Delta R.T.: 0.000 min
Response: 154198066
Conc: 14.28 ng/ml

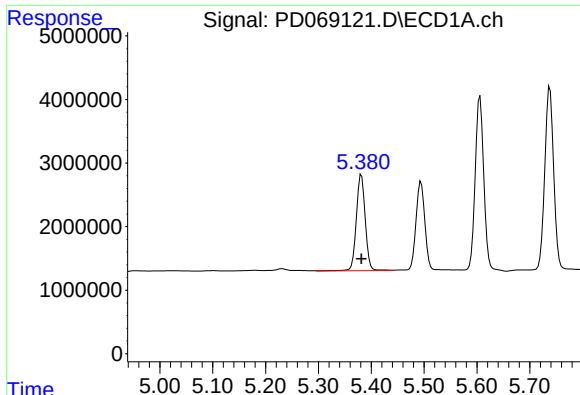

#10 gamma-Chlordane


R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 17907143
Conc: 12.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

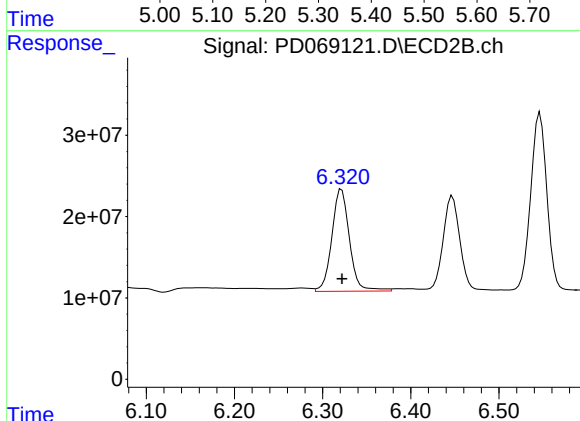


#10 gamma-Chlordane

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 175054808
Conc: 15.03 ng/ml

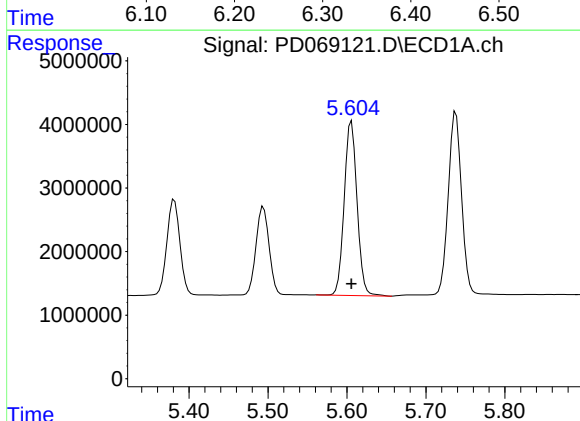


#12 4,4'-DDE

R.T.: 5.606 min
Delta R.T.: 0.000 min
Response: 31018466
Conc: 24.51 ng/ml

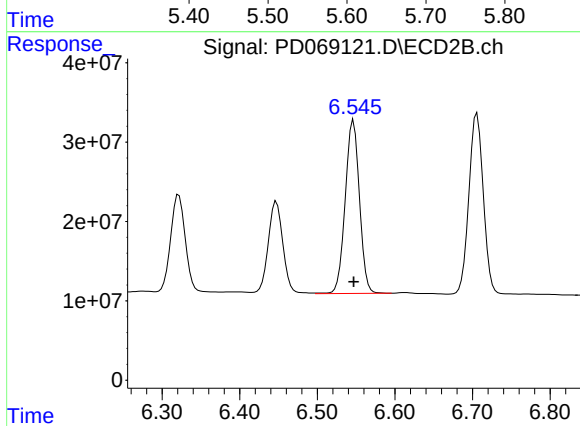

#12 4,4'-DDE


R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 277847555
Conc: 25.72 ng/ml

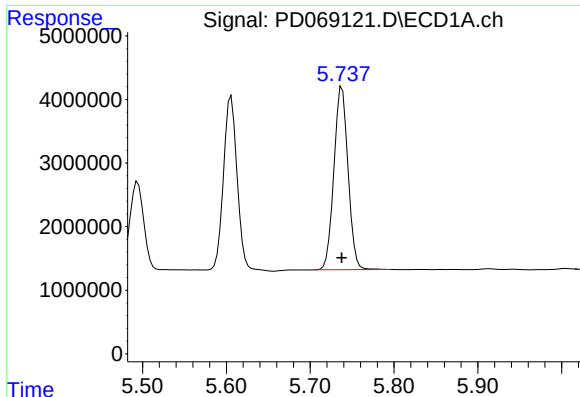

#13 Dieldrin


R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 33700454
Conc: 24.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

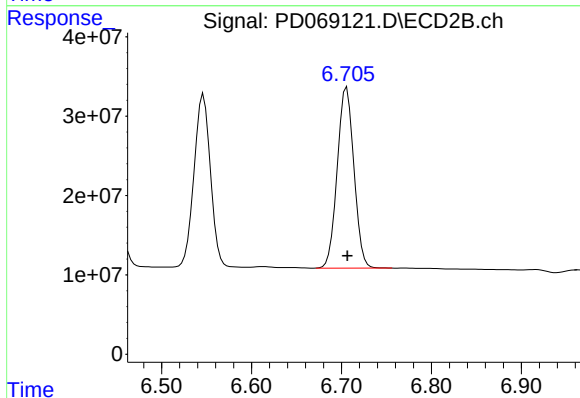


#13 Dieldrin

R.T.: 6.706 min
Delta R.T.: 0.000 min
Response: 294146130
Conc: 26.39 ng/ml

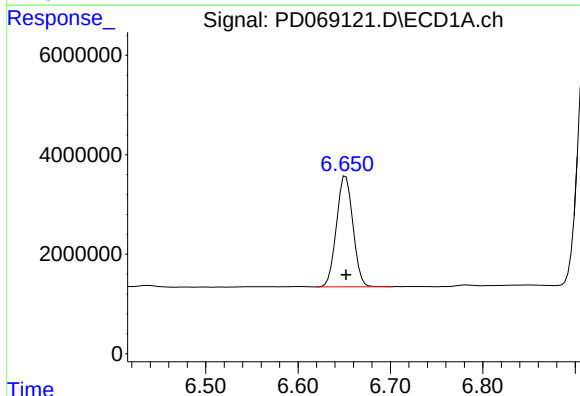


#19 Endosulfan Sulfate

R.T.: 6.652 min
Delta R.T.: 0.000 min
Response: 27621384
Conc: 22.83 ng/ml

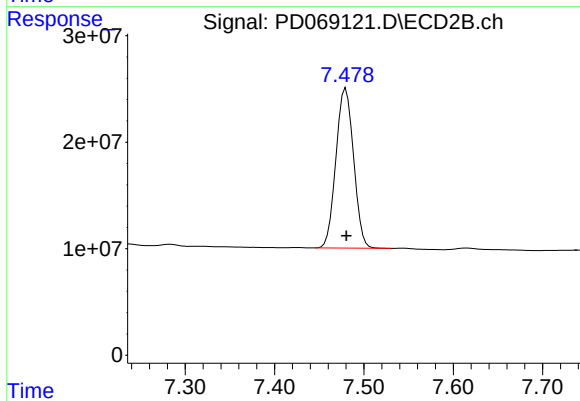

#19 Endosulfan Sulfate


R.T.: 7.480 min
Delta R.T.: 0.000 min
Response: 206105782
Conc: 24.14 ng/ml

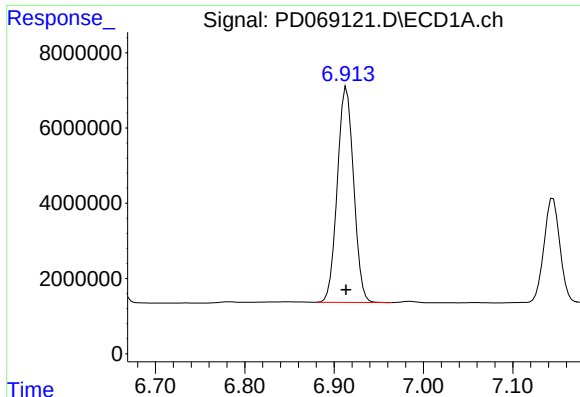

#20 Methoxychlor


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 72586493
Conc: 114.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

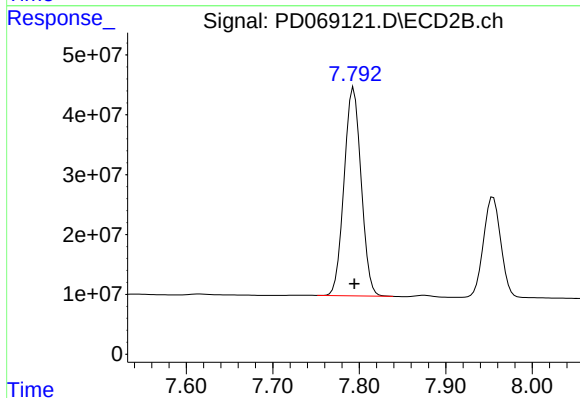


#20 Methoxychlor

R.T.: 7.793 min
Delta R.T.: -0.001 min
Response: 473876078
Conc: 109.92 ng/ml

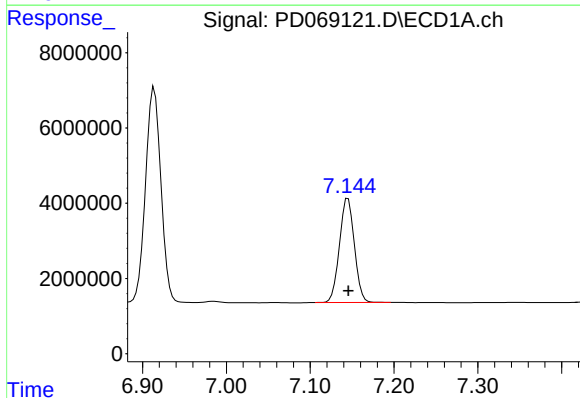


#21 Endrin ketone

R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 34166063
Conc: 24.27 ng/ml

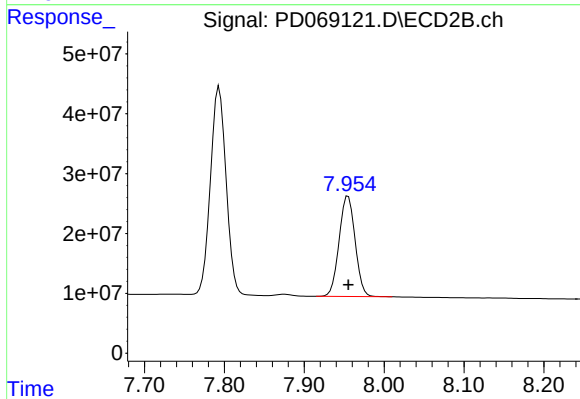

#21 Endrin ketone


R.T.: 7.955 min
Delta R.T.: 0.000 min
Response: 233584240
Conc: 25.83 ng/ml

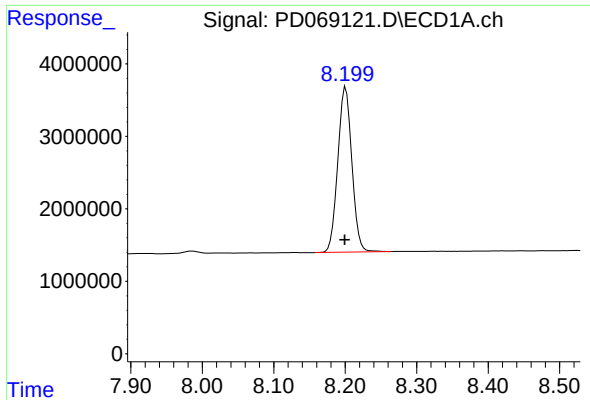

#28 Decachlorobiphenyl

R.T.: 8.201 min
Delta R.T.: 0.001 min
Response: 31094152
Conc: 24.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

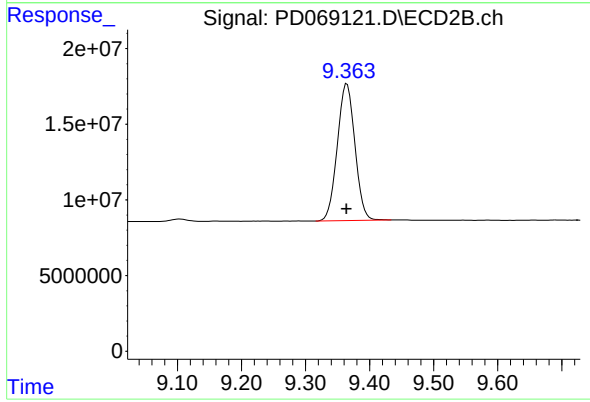

#28 Decachlorobiphenyl

R.T.: 9.365 min
Delta R.T.: 0.000 min
Response: 172673763
Conc: 26.39 ng/ml