

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
 Data File : PD069127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Apr 2022 10:42
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 23:57:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 15 23:57:03 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.172	133.6E6	1046.5E6	112.899	97.135
28)	SA Decachlor...	8.207	9.368	121.6E6	618.2E6	97.797	93.988
Target Compounds							
23)	Chlordane-1	4.320	5.194	41562064	429.6E6	1020.258	974.881
24)	Chlordane-2	4.822	5.667	47270757	403.1E6	996.020	962.060
25)	Chlordane-3	5.390	6.324	140.3E6	1514.6E6	1033.138	988.151
26)	Chlordane-4	5.448	6.400	116.4E6	1753.6E6	1030.556	979.786
27)	Chlordane-5	6.285	7.212	48603732	335.4E6	1030.131	975.997



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041622\
Data File : PD069127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Apr 2022 10:42
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 23:57:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041622.M
Quant Title : GC Extractables
QLast Update : Fri Apr 15 23:57:03 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

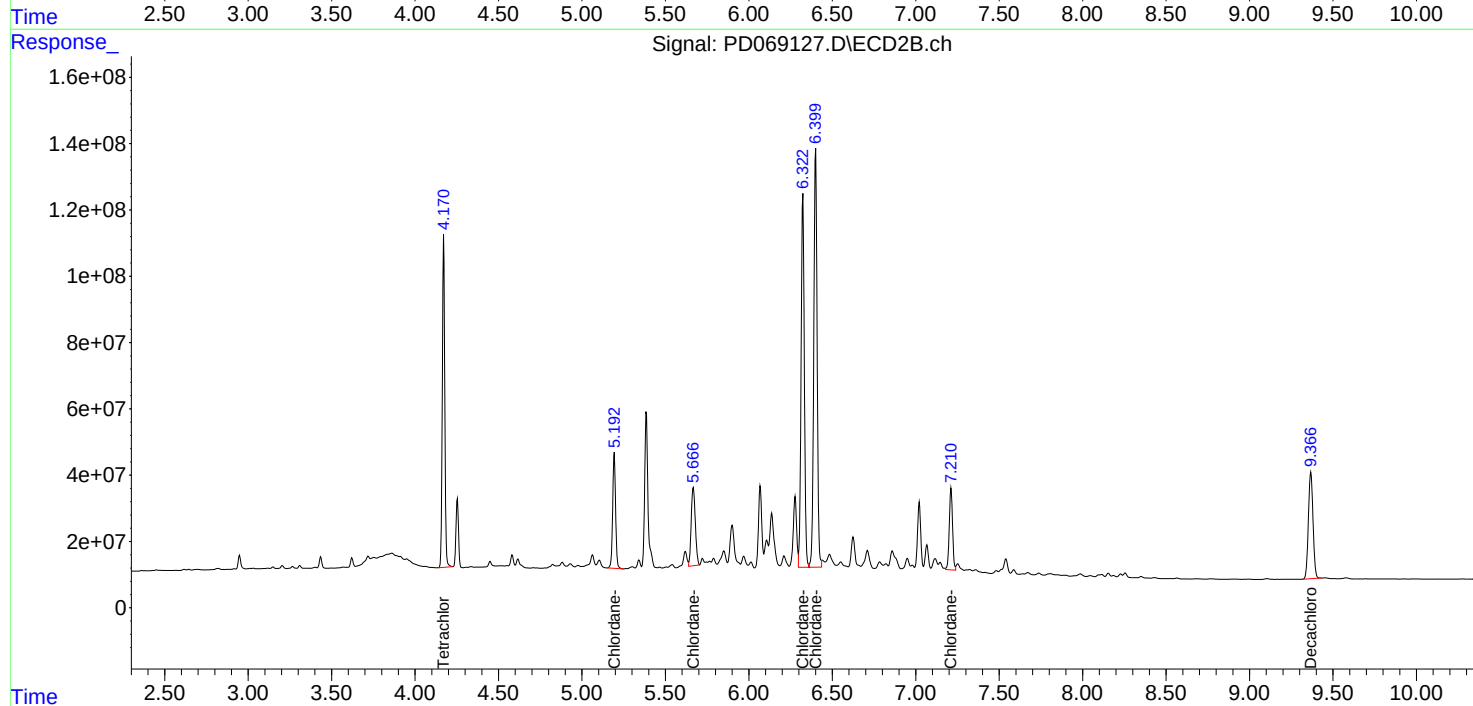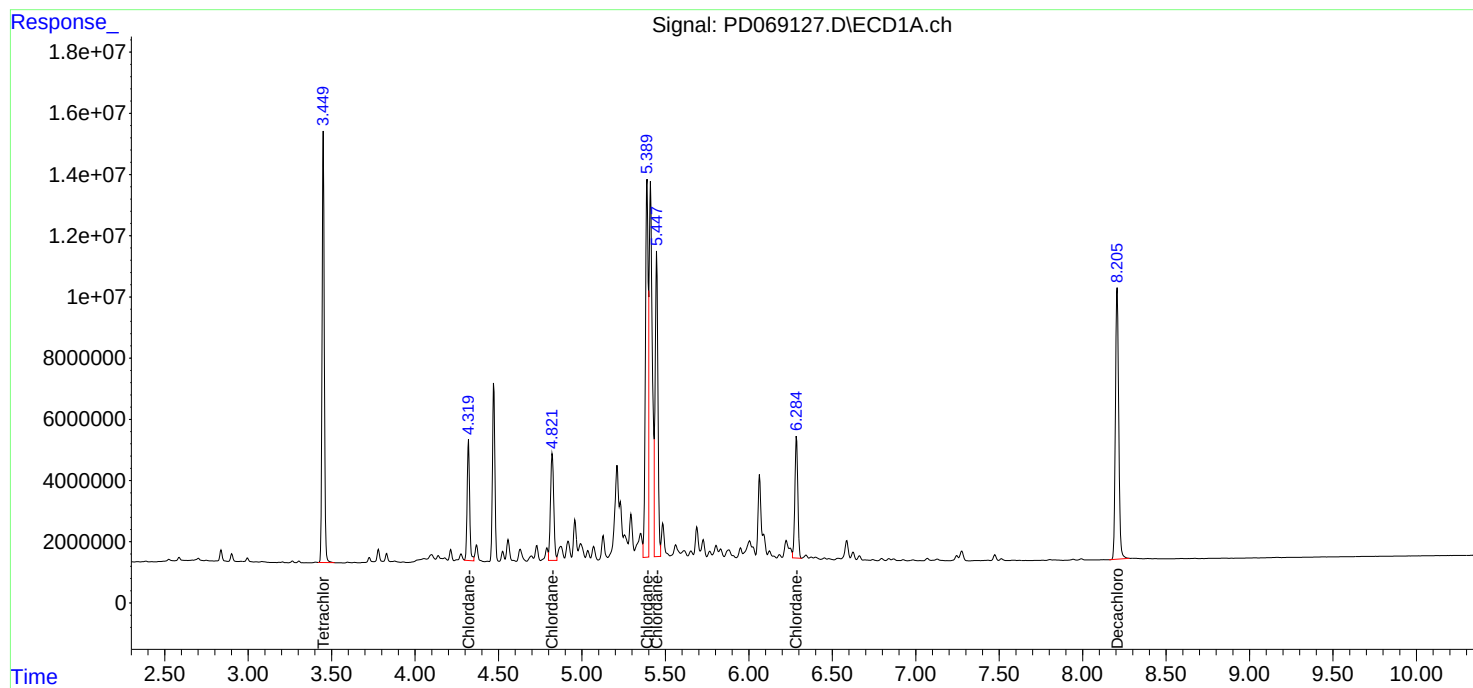


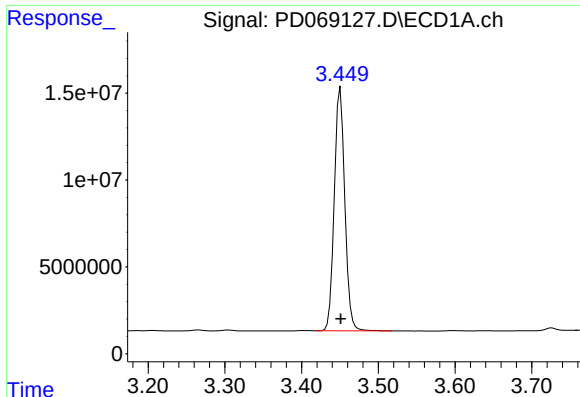

#1 Tetrachloro-m-xylene


R.T.: 3.451 min
Delta R.T.: 0.000 min
Response: 133580876
Conc: 112.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

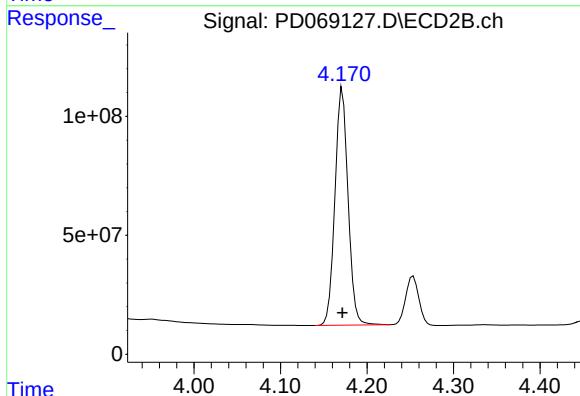


#1 Tetrachloro-m-xylene

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 1046487274
Conc: 97.14 ng/ml

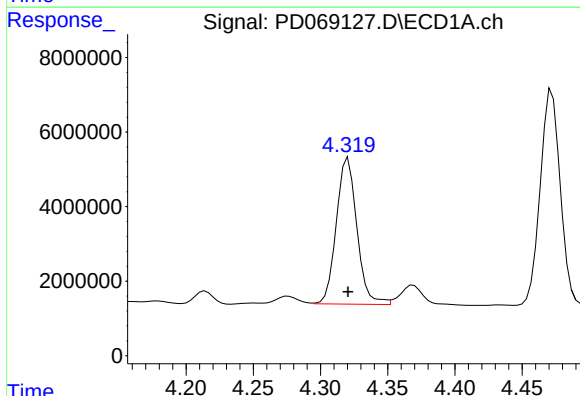


#23 Chlordane-1

R.T.: 4.320 min
Delta R.T.: 0.000 min
Response: 41562064
Conc: 1020.26 ng/ml

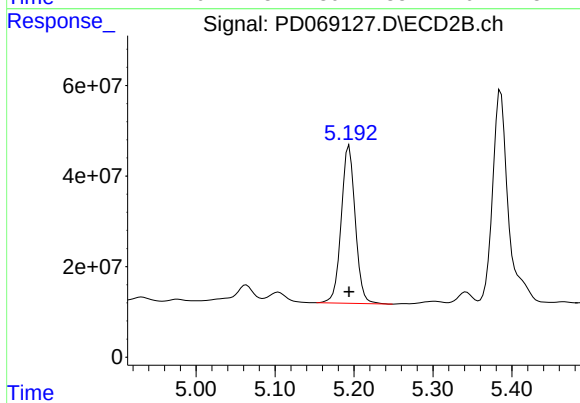

#23 Chlordane-1


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 429649269
Conc: 974.88 ng/ml

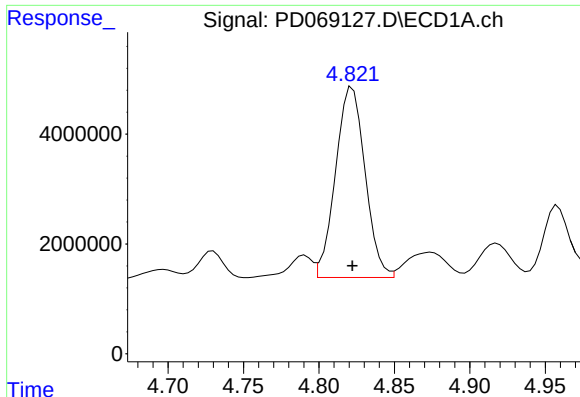

#24 Chlordane-2


R.T.: 4.822 min
Delta R.T.: 0.000 min
Response: 47270757
Conc: 996.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

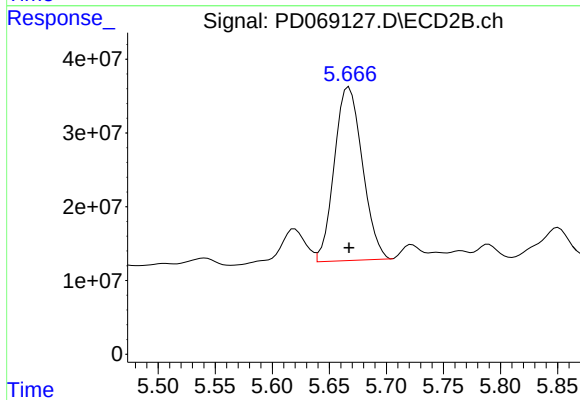


#24 Chlordane-2

R.T.: 5.667 min
Delta R.T.: 0.000 min
Response: 403116423
Conc: 962.06 ng/ml

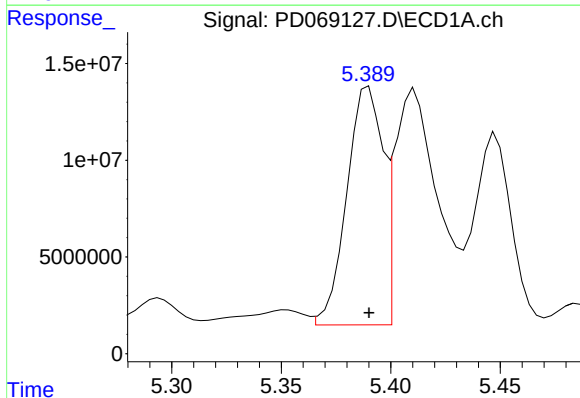


#25 Chlordane-3

R.T.: 5.390 min
Delta R.T.: 0.000 min
Response: 140330155
Conc: 1033.14 ng/ml

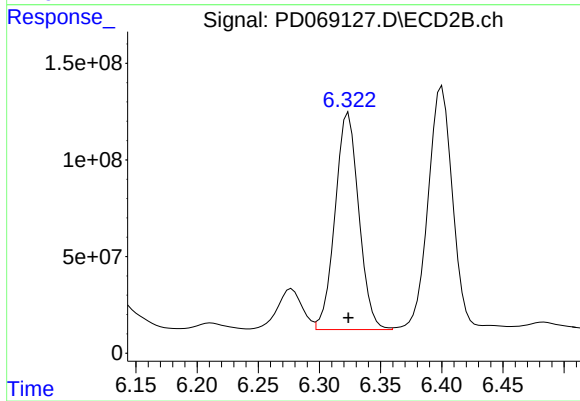

#25 Chlordane-3


R.T.: 6.324 min
Delta R.T.: 0.000 min
Response: 1514642333
Conc: 988.15 ng/ml

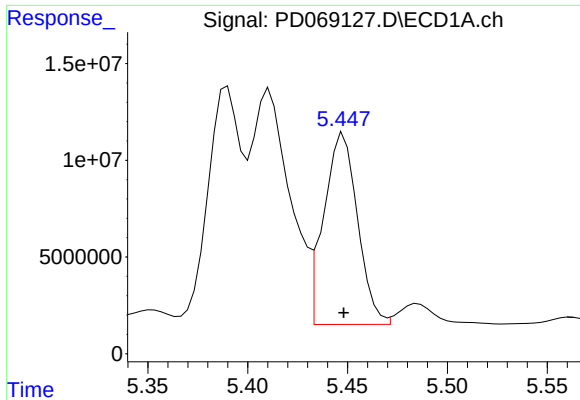

#26 Chlordane-4


R.T.: 5.448 min
Delta R.T.: 0.000 min
Response: 116357939
Conc: 1030.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

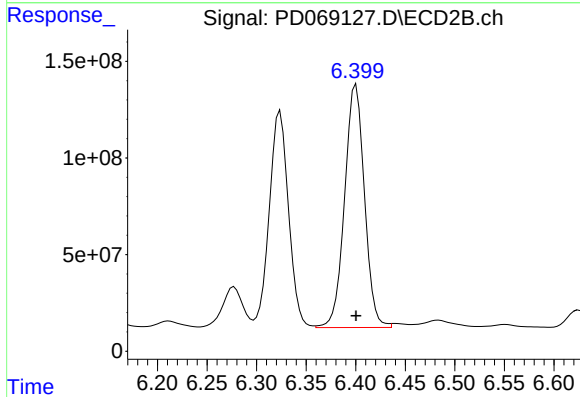


#26 Chlordane-4

R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 1753574820
Conc: 979.79 ng/ml

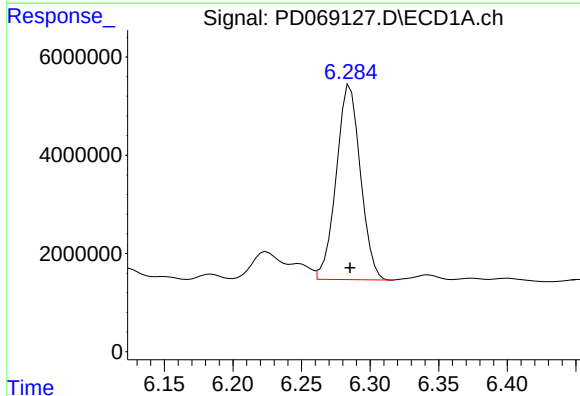


#27 Chlordane-5

R.T.: 6.285 min
Delta R.T.: 0.000 min
Response: 48603732
Conc: 1030.13 ng/ml

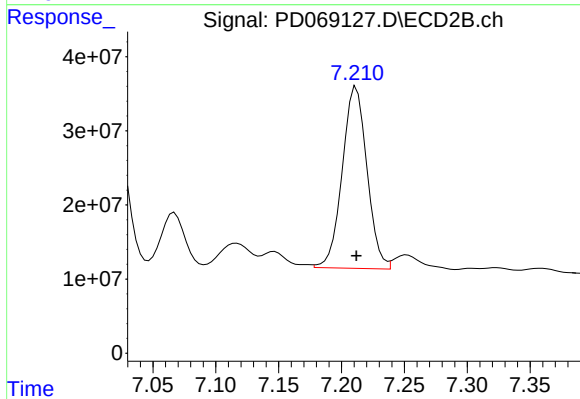

#27 Chlordane-5


R.T.: 7.212 min
Delta R.T.: 0.000 min
Response: 335410612
Conc: 976.00 ng/ml

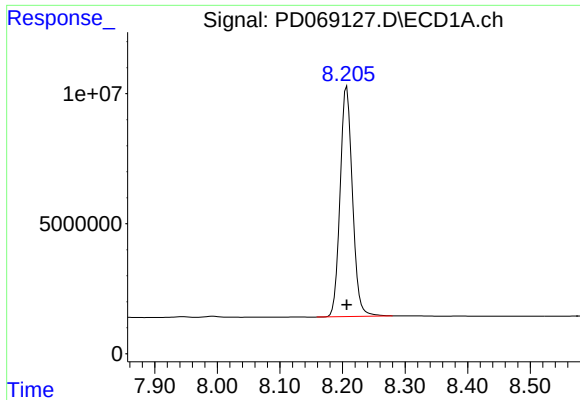

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 121648651
Conc: 97.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

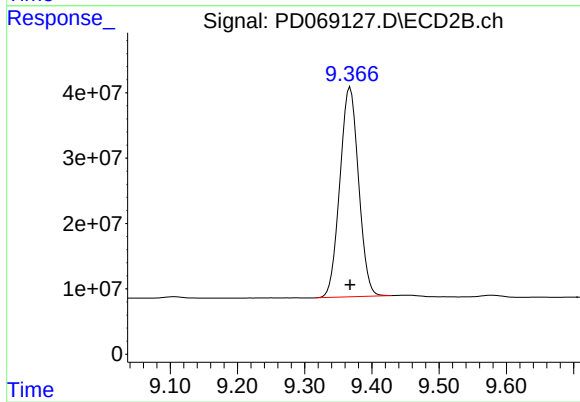

#28 Decachlorobiphenyl

R.T.: 9.368 min
Delta R.T.: 0.000 min
Response: 618171208
Conc: 93.99 ng/ml